
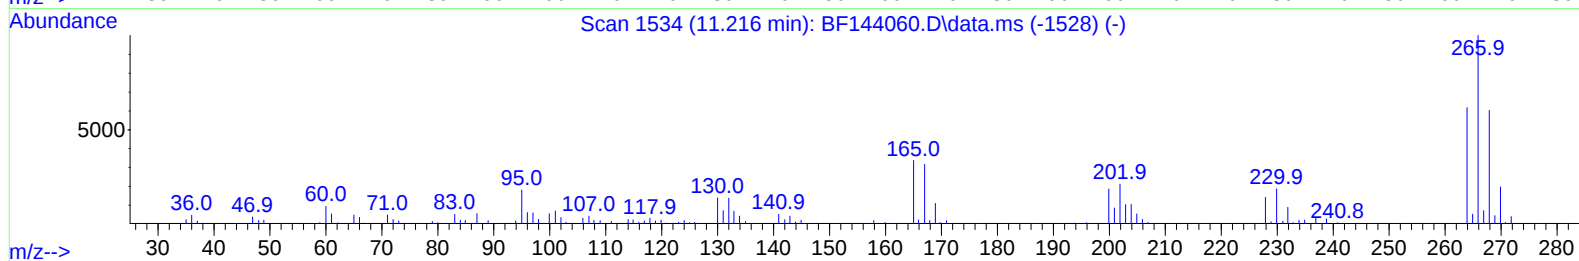
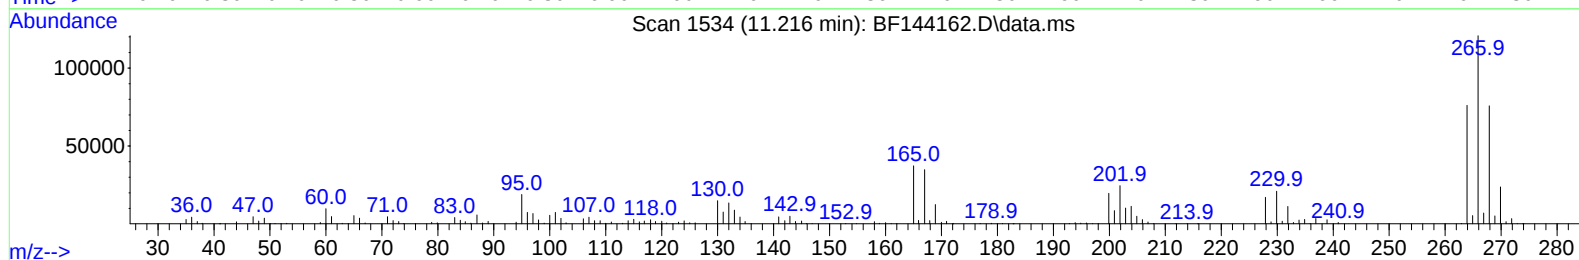


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110325\
Data File : BF144162.D
Acq On : 03 Nov 2025 15:42
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 04 10:13:17 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 24 17:30:25 2025
Response via : Initial Calibration

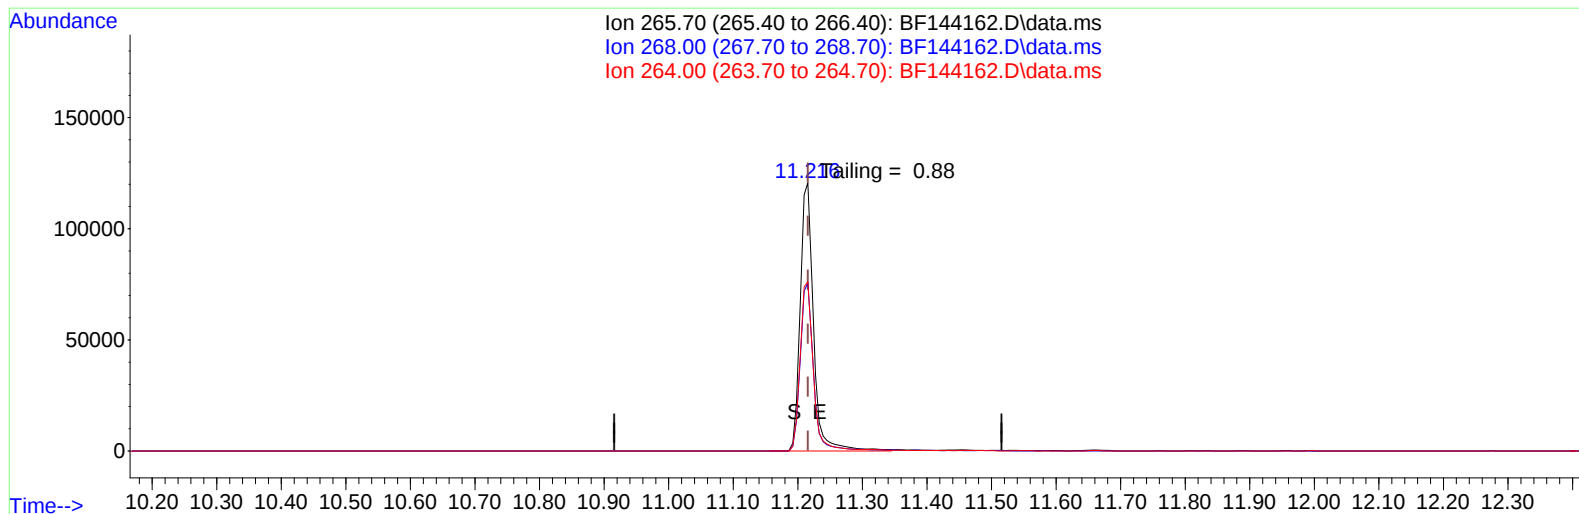

TIC: BF144162.D\data.ms

(70) Pentachlorophenol (C)




11.216min (-0.000) 42346.37 ng

response 175188

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	60.30	62.74
264.00	61.70	63.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110325\
Data File : BF144162.D
Acq On : 03 Nov 2025 15:42
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 04 10:13:17 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 24 17:30:25 2025
Response via : Initial Calibration

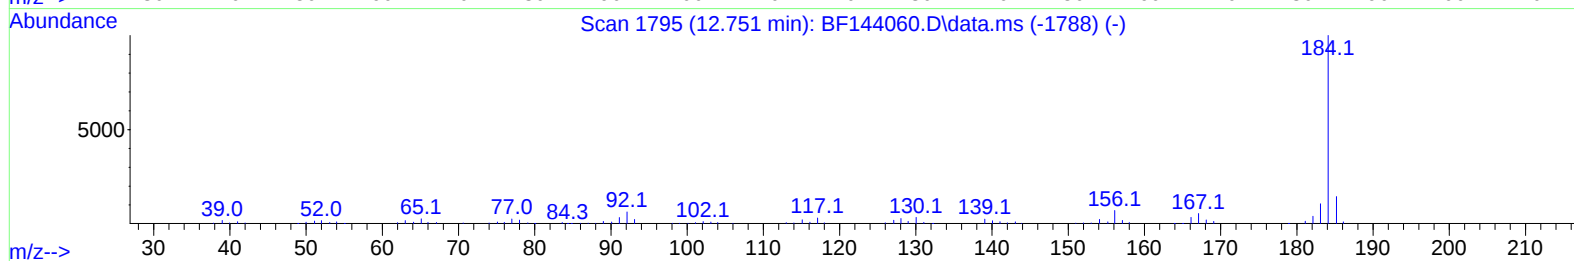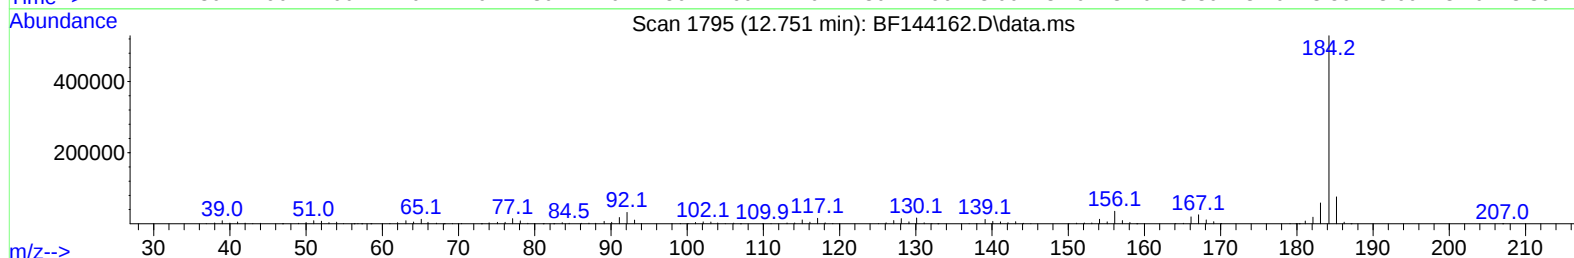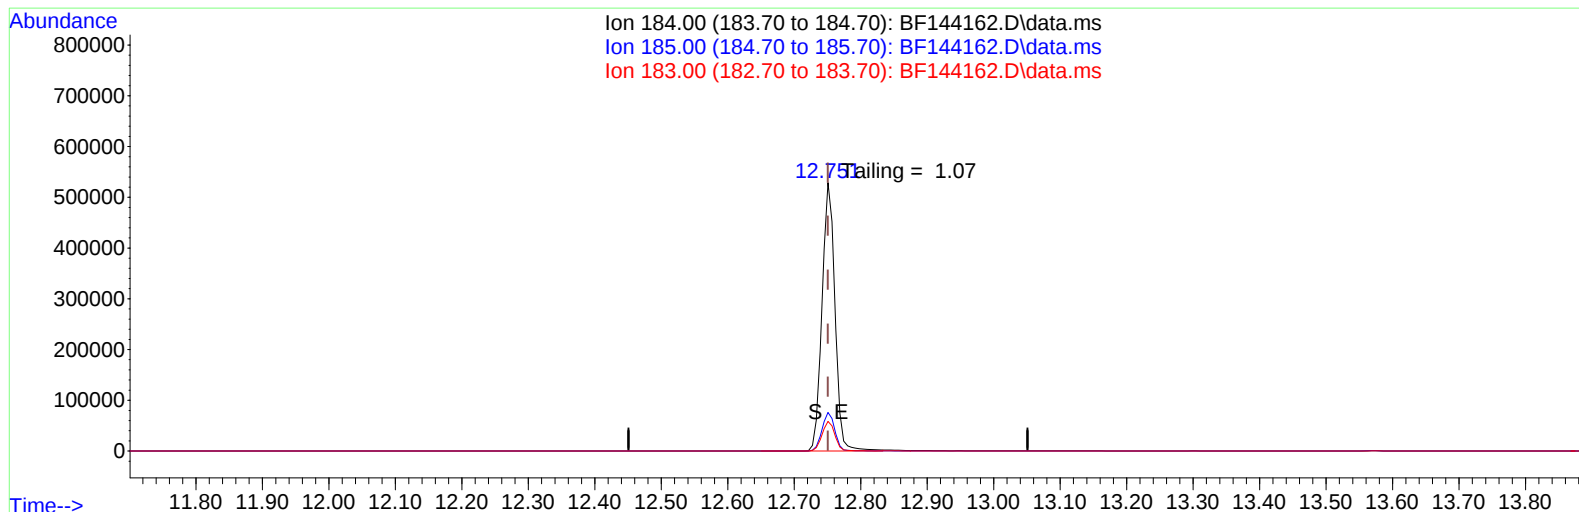

TIC: BF144162.D\data.ms

(77) Benzidine

12.751min (-0.000) 0.00 ng

response 719483

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.36
183.00	10.60	11.06
0.00	0.00	0.00