


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110325\
Data File : BF144162.D
Acq On : 03 Nov 2025 15:42
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Oct 24 17:30:25 2025

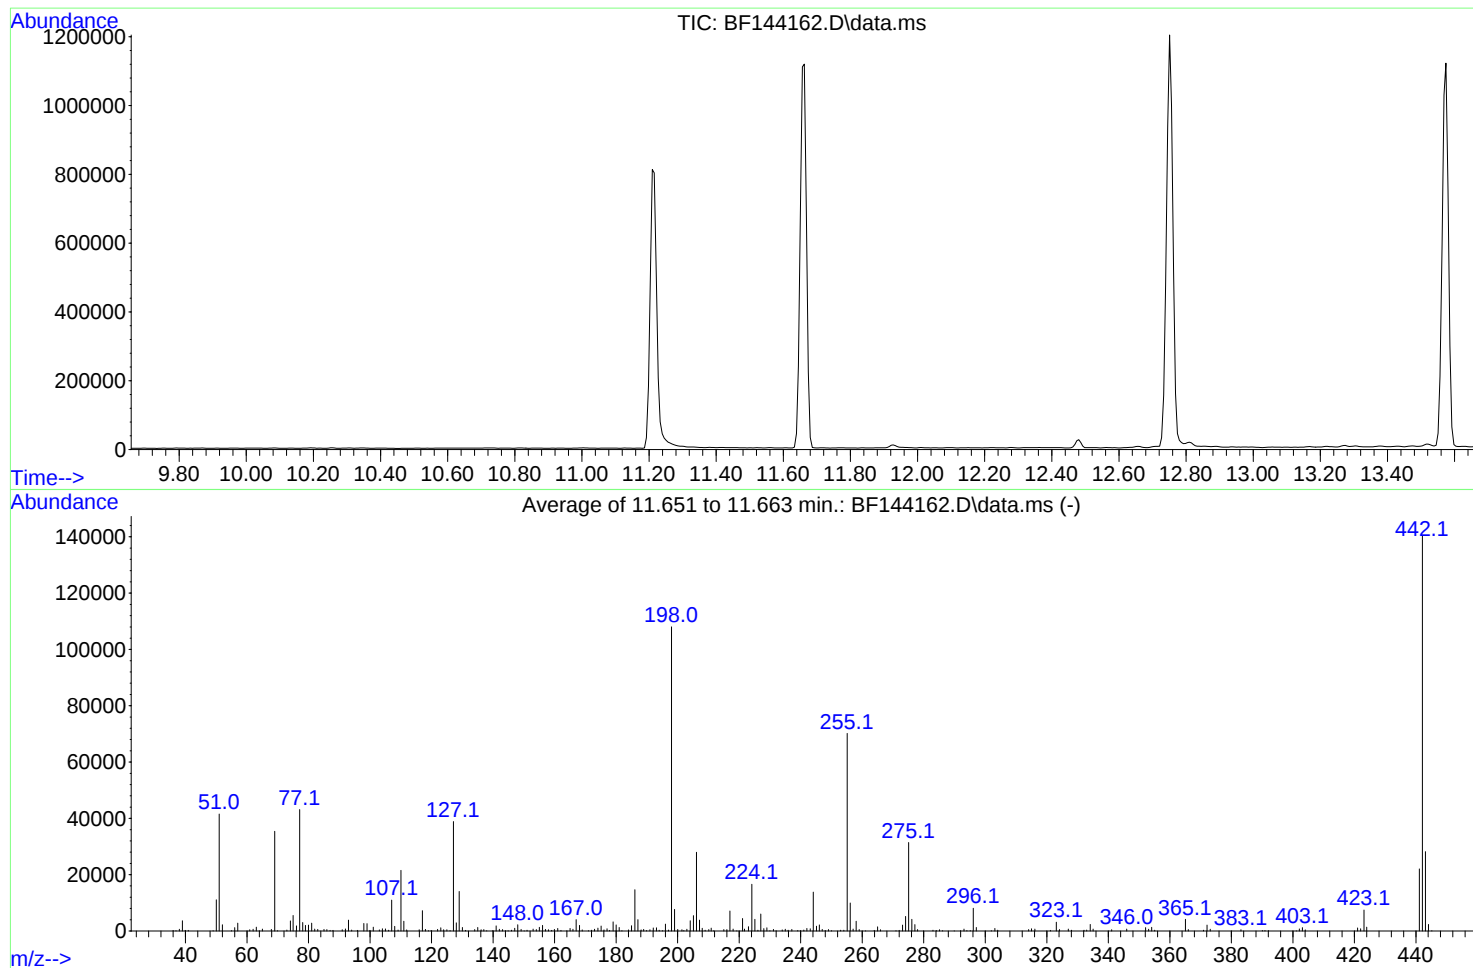

AutoFind: Scans 1608, 1609, 1610; Background Corrected with Scan 1602

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.6	569	PASS
69	69	100	100	100.0	35389	PASS
70	69	0.00	2	0.4	139	PASS
197	198	0.00	2	0.3	330	PASS
198	198	100	100	100.0	108037	PASS
199	198	5	9	7.1	7648	PASS
365	198	1	100	3.8	4130	PASS
441	443	0.01	150	78.3	22078	PASS
442	442	100	100	100.0	140232	PASS
443	442	15	24	20.1	28181	PASS

DDT Breakdown


Date	Instrument Name	DFTPP Data File
10/30/2025	BNA_F	<u>BF144144.D</u>
Compound Name	Response	Retention Time
DDT	310573	13.574
DDD	3768	13.274
DDE	204	12.939
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3972	314545	1.26

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110325\
Data File : BF144162.D
Acq On : 03 Nov 2025 15:42
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 04 10:13:17 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 24 17:30:25 2025
Response via : Initial Calibration

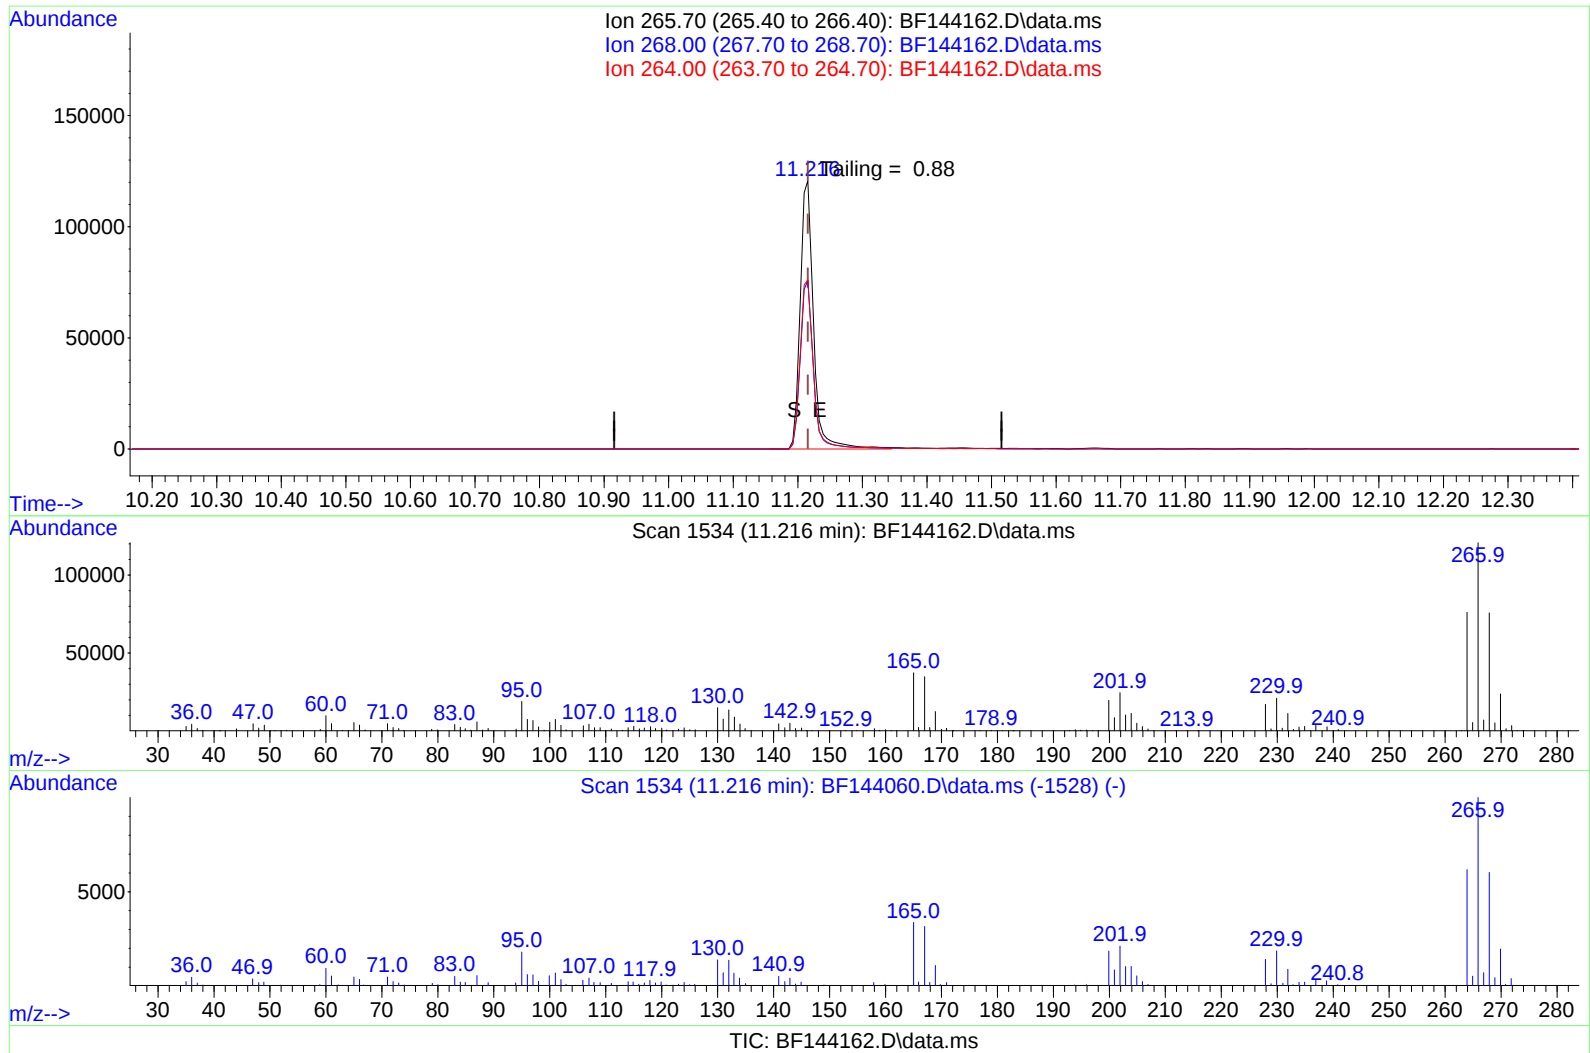

(70) Pentachlorophenol (C)

11.216min (-0.000) 42346.37 ng




response 175188

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	60.30	62.74
264.00	61.70	63.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110325\
Data File : BF144162.D
Acq On : 03 Nov 2025 15:42
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 04 10:13:17 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 24 17:30:25 2025
Response via : Initial Calibration

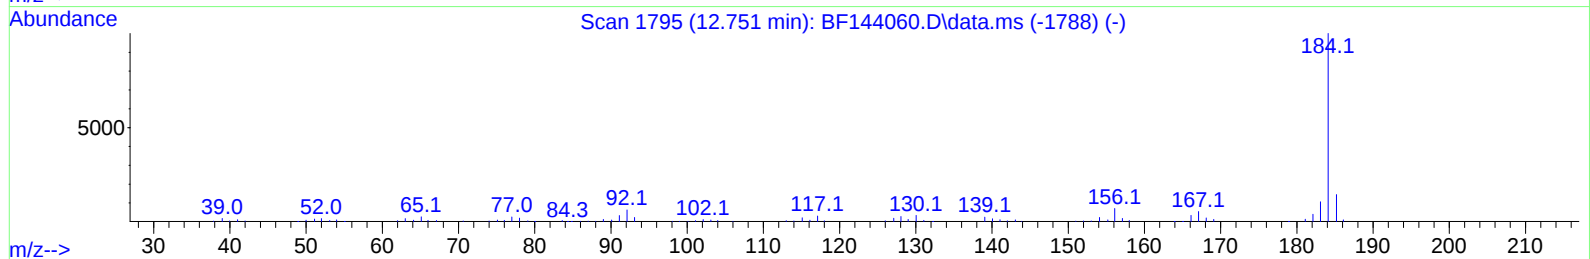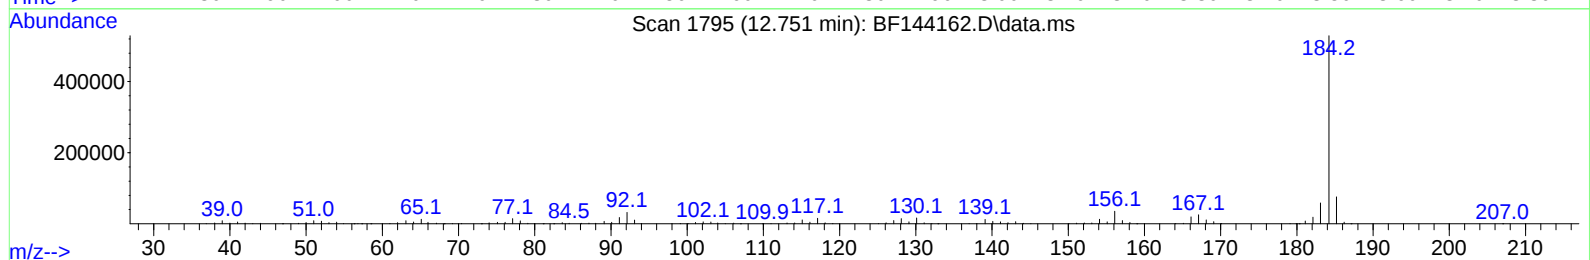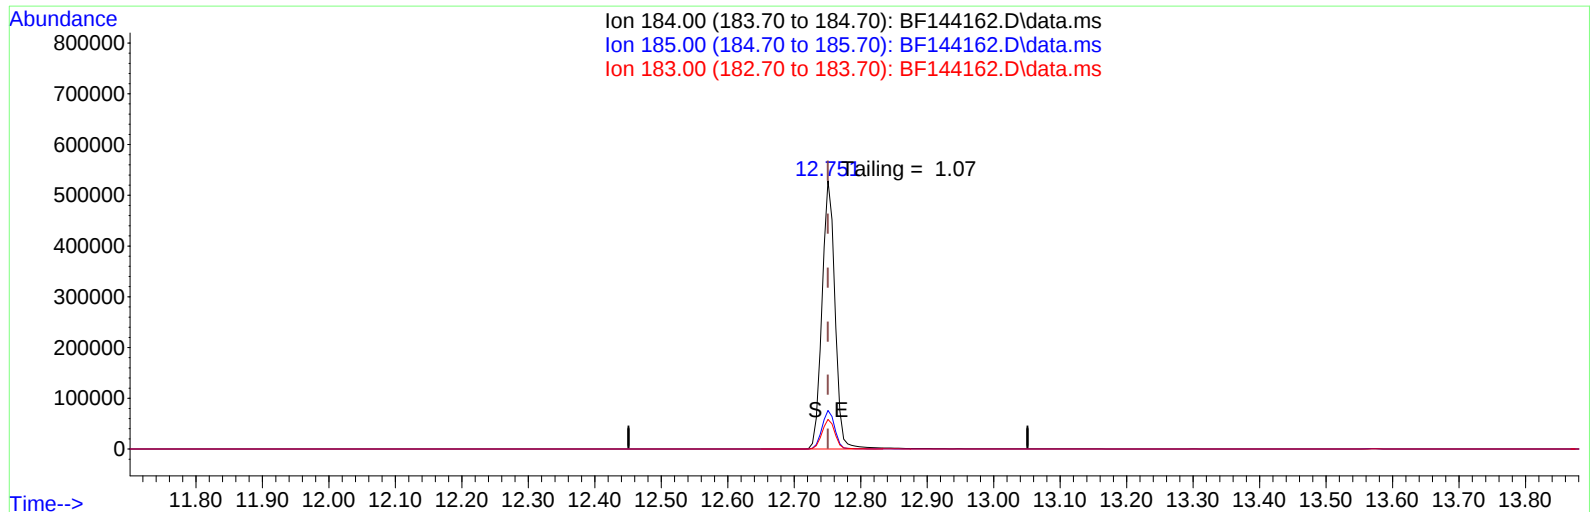

TIC: BF144162.D\data.ms

(77) Benzidine

12.751min (-0.000) 0.00 ng

response 719483

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.36
183.00	10.60	11.06
0.00	0.00	0.00