

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110421\
 Data File : BF126046.D
 Acq On : 4 Nov 2021 15:24
 Operator : JU/CG
 Sample : M4449-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PAINTED-WALLS

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF126046.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.134	3	8	13	rVB	1097360	1400865	21.12%	1.886%
2	3.316	205	209	222	rBV	90642	202454	3.05%	0.273%
3	5.463	568	574	578	rVV	1933598	2310006	34.82%	3.110%
4	5.798	628	631	639	rVB	515057	440289	6.64%	0.593%
5	6.022	658	669	672	rBV	1174766	2056293	31.00%	2.768%
6	6.087	677	680	687	rVB	163619	184624	2.78%	0.249%
7	6.481	739	747	755	rBV	2222126	2393416	36.08%	3.222%
8	6.657	774	777	779	rBV	344841	258334	3.89%	0.348%
9	6.687	779	782	786	rVB	388125	354164	5.34%	0.477%
10	6.775	794	797	806	rBV	206747	194150	2.93%	0.261%
11	6.851	806	810	813	rBV	1109596	871664	13.14%	1.173%
12	7.410	896	905	908	rBV	1915188	1630934	24.59%	2.195%
13	7.557	924	930	934	rVV	322146	499610	7.53%	0.673%
14	7.616	937	940	944	rVV2	173750	181301	2.73%	0.244%
15	7.863	974	982	985	rBV	4653415	6633414	100.00%	8.930%
16	7.886	985	986	991	rVV	146255	160623	2.42%	0.216%
17	8.045	1008	1013	1016	rBV	1971430	1646131	24.82%	2.216%
18	8.133	1024	1028	1030	rBV	1267696	1028905	15.51%	1.385%
19	8.157	1030	1032	1036	rVB2	322438	272197	4.10%	0.366%
20	8.357	1063	1066	1068	rBV	318686	287755	4.34%	0.387%
21	8.381	1068	1070	1073	rVV	381489	334524	5.04%	0.450%
22	8.504	1083	1091	1093	rBV4	73497	160779	2.42%	0.216%
23	8.651	1113	1116	1118	rVV	291627	357000	5.38%	0.481%
24	8.675	1118	1120	1122	rVB	177250	133724	2.02%	0.180%
25	8.845	1146	1149	1153	rBV	789841	614463	9.26%	0.827%
26	8.945	1162	1166	1172	rBV	296109	251719	3.79%	0.339%
27	9.086	1186	1190	1193	rBV	1863199	1499752	22.61%	2.019%
28	9.210	1205	1211	1214	rBV2	3444557	3991382	60.17%	5.373%
29	9.292	1223	1225	1229	rVV3	253535	260720	3.93%	0.351%
30	9.475	1249	1256	1261	rBV	376840	551841	8.32%	0.743%
31	9.545	1262	1268	1270	rBV	438704	486709	7.34%	0.655%
32	9.569	1270	1272	1275	rVB	331826	263920	3.98%	0.355%
33	9.616	1275	1280	1281	rBV2	115997	139022	2.10%	0.187%
34	9.645	1281	1285	1287	rVV	929117	962573	14.51%	1.296%
35	9.663	1287	1288	1291	rVV2	275486	199693	3.01%	0.269%
36	9.692	1291	1293	1298	rVB4	108099	133181	2.01%	0.179%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110421\
 Data File : BF126046.D
 Acq On : 4 Nov 2021 15:24
 Operator : JU/CG
 Sample : M4449-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PAINTED-WALLS

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	9.822	1312	1315	1318	rBV	545282	383147	5.78%	0.516%
38	9.886	1323	1326	1329	rVV	1273692	1026313	15.47%	1.382%
39	9.927	1330	1333	1335	rVV	221647	175115	2.64%	0.236%
40	9.992	1341	1344	1348	rBV	188113	221830	3.34%	0.299%

41	10.092	1357	1361	1363	rBV2	806874	793445	11.96%	1.068%
42	10.127	1363	1367	1369	rBV	374911	291941	4.40%	0.393%
43	10.204	1377	1380	1382	rBV	252365	225558	3.40%	0.304%
44	10.227	1382	1384	1387	rVV	428768	363927	5.49%	0.490%
45	10.292	1391	1395	1397	rVV	470920	538732	8.12%	0.725%

46	10.322	1397	1400	1403	rVV2	1228904	1041663	15.70%	1.402%
47	10.451	1419	1422	1425	rVV3	151261	178018	2.68%	0.240%
48	10.545	1431	1438	1441	rVV	812780	948593	14.30%	1.277%
49	10.592	1443	1446	1449	rVB5	242123	282745	4.26%	0.381%
50	10.627	1449	1452	1455	rBV3	175347	187749	2.83%	0.253%

51	10.669	1455	1459	1463	rVV4	1678372	1653541	24.93%	2.226%
52	10.710	1463	1466	1471	rVB5	176572	238611	3.60%	0.321%
53	10.798	1477	1481	1482	rBV	2723105	2560811	38.60%	3.447%
54	10.874	1491	1494	1495	rBV2	197569	186905	2.82%	0.252%
55	10.939	1503	1505	1508	rBV4	151312	216799	3.27%	0.292%

56	10.986	1510	1513	1517	rVV3	338644	484541	7.30%	0.652%
57	11.022	1517	1519	1522	rVB2	236464	203060	3.06%	0.273%
58	11.116	1532	1535	1537	rBV4	302682	347828	5.24%	0.468%
59	11.174	1542	1545	1549	rVV	625731	652704	9.84%	0.879%
60	11.216	1550	1552	1554	rVV2	258393	313661	4.73%	0.422%

61	11.245	1554	1557	1560	rVV	2998954	2735499	41.24%	3.682%
62	11.274	1560	1562	1568	rVB	1904093	1836506	27.69%	2.472%
63	11.369	1575	1578	1580	rBV	895273	818980	12.35%	1.102%
64	11.392	1580	1582	1585	rVB	1249507	945434	14.25%	1.273%
65	11.422	1585	1587	1589	rBV2	202844	233203	3.52%	0.314%

66	11.551	1605	1609	1613	rVB2	1116282	996976	15.03%	1.342%
67	11.586	1613	1615	1618	rBV3	196532	202257	3.05%	0.272%
68	11.622	1619	1621	1624	rVV	486096	500086	7.54%	0.673%
69	11.669	1627	1629	1632	rVV	2234861	1918341	28.92%	2.582%
70	11.704	1632	1635	1642	rVB2	731209	830038	12.51%	1.117%

71	11.763	1642	1645	1648	rBV2	544749	471866	7.11%	0.635%
72	11.827	1653	1656	1658	rBV2	329074	404225	6.09%	0.544%
73	11.874	1661	1664	1666	rVV	981369	870947	13.13%	1.172%
74	11.898	1666	1668	1671	rVV2	1333566	1277728	19.26%	1.720%
75	11.933	1671	1674	1677	rVB3	304357	311700	4.70%	0.420%

76	11.980	1678	1682	1684	rVV	650875	695915	10.49%	0.937%
----	--------	------	------	------	-----	--------	--------	--------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110421\
 Data File : BF126046.D
 Acq On : 4 Nov 2021 15:24
 Operator : JU/CG
 Sample : M4449-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PAINTED-WALLS

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

77	12.004	1684	1686	1691	rVB2	521430	602394	9.08%	0.811%
78	12.057	1692	1695	1696	rBV2	436639	381581	5.75%	0.514%
79	12.074	1696	1698	1701	rVV2	1618427	1491266	22.48%	2.007%
80	12.104	1701	1703	1706	rVB2	544591	454374	6.85%	0.612%
81	12.169	1711	1714	1716	rBV	562327	474021	7.15%	0.638%
82	12.298	1733	1736	1737	rBV2	226596	192935	2.91%	0.260%
83	12.321	1737	1740	1742	rVB2	422832	401012	6.05%	0.540%
84	12.351	1742	1745	1747	rBV2	389745	366918	5.53%	0.494%
85	12.421	1755	1757	1760	rBV	598156	507312	7.65%	0.683%
86	12.463	1761	1764	1769	rVB2	777693	973306	14.67%	1.310%
87	12.504	1769	1771	1776	rVB	194045	179431	2.70%	0.242%
88	12.580	1782	1784	1786	rBV2	182958	136682	2.06%	0.184%
89	12.833	1825	1827	1830	rVB	416974	341637	5.15%	0.460%
90	12.868	1830	1833	1836	rBV3	145210	141417	2.13%	0.190%
91	12.957	1844	1848	1856	rVB	2545815	2379415	35.87%	3.203%
92	13.192	1885	1888	1891	rBV2	165469	157933	2.38%	0.213%
93	13.857	1999	2001	2009	rVB	176914	267244	4.03%	0.360%
94	14.004	2021	2026	2032	rVB2	970140	1090573	16.44%	1.468%
95	14.868	2170	2173	2176	rBV	284217	251924	3.80%	0.339%
96	15.468	2270	2275	2279	rBV	672183	783739	11.82%	1.055%
97	15.509	2280	2282	2287	rVB	132572	166370	2.51%	0.224%
98	15.951	2353	2357	2362	rVB	144498	204124	3.08%	0.275%
99	16.451	2439	2442	2450	rVB2	133261	233733	3.52%	0.315%
100	17.051	2539	2544	2550	rVB3	92647	191632	2.89%	0.258%


Sum of corrected areas: 74286042

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110421\
Data File : BF126046.D
Acq On : 4 Nov 2021 15:24
Operator : JU/CG
Sample : M4449-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PAINTED-WALLS

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

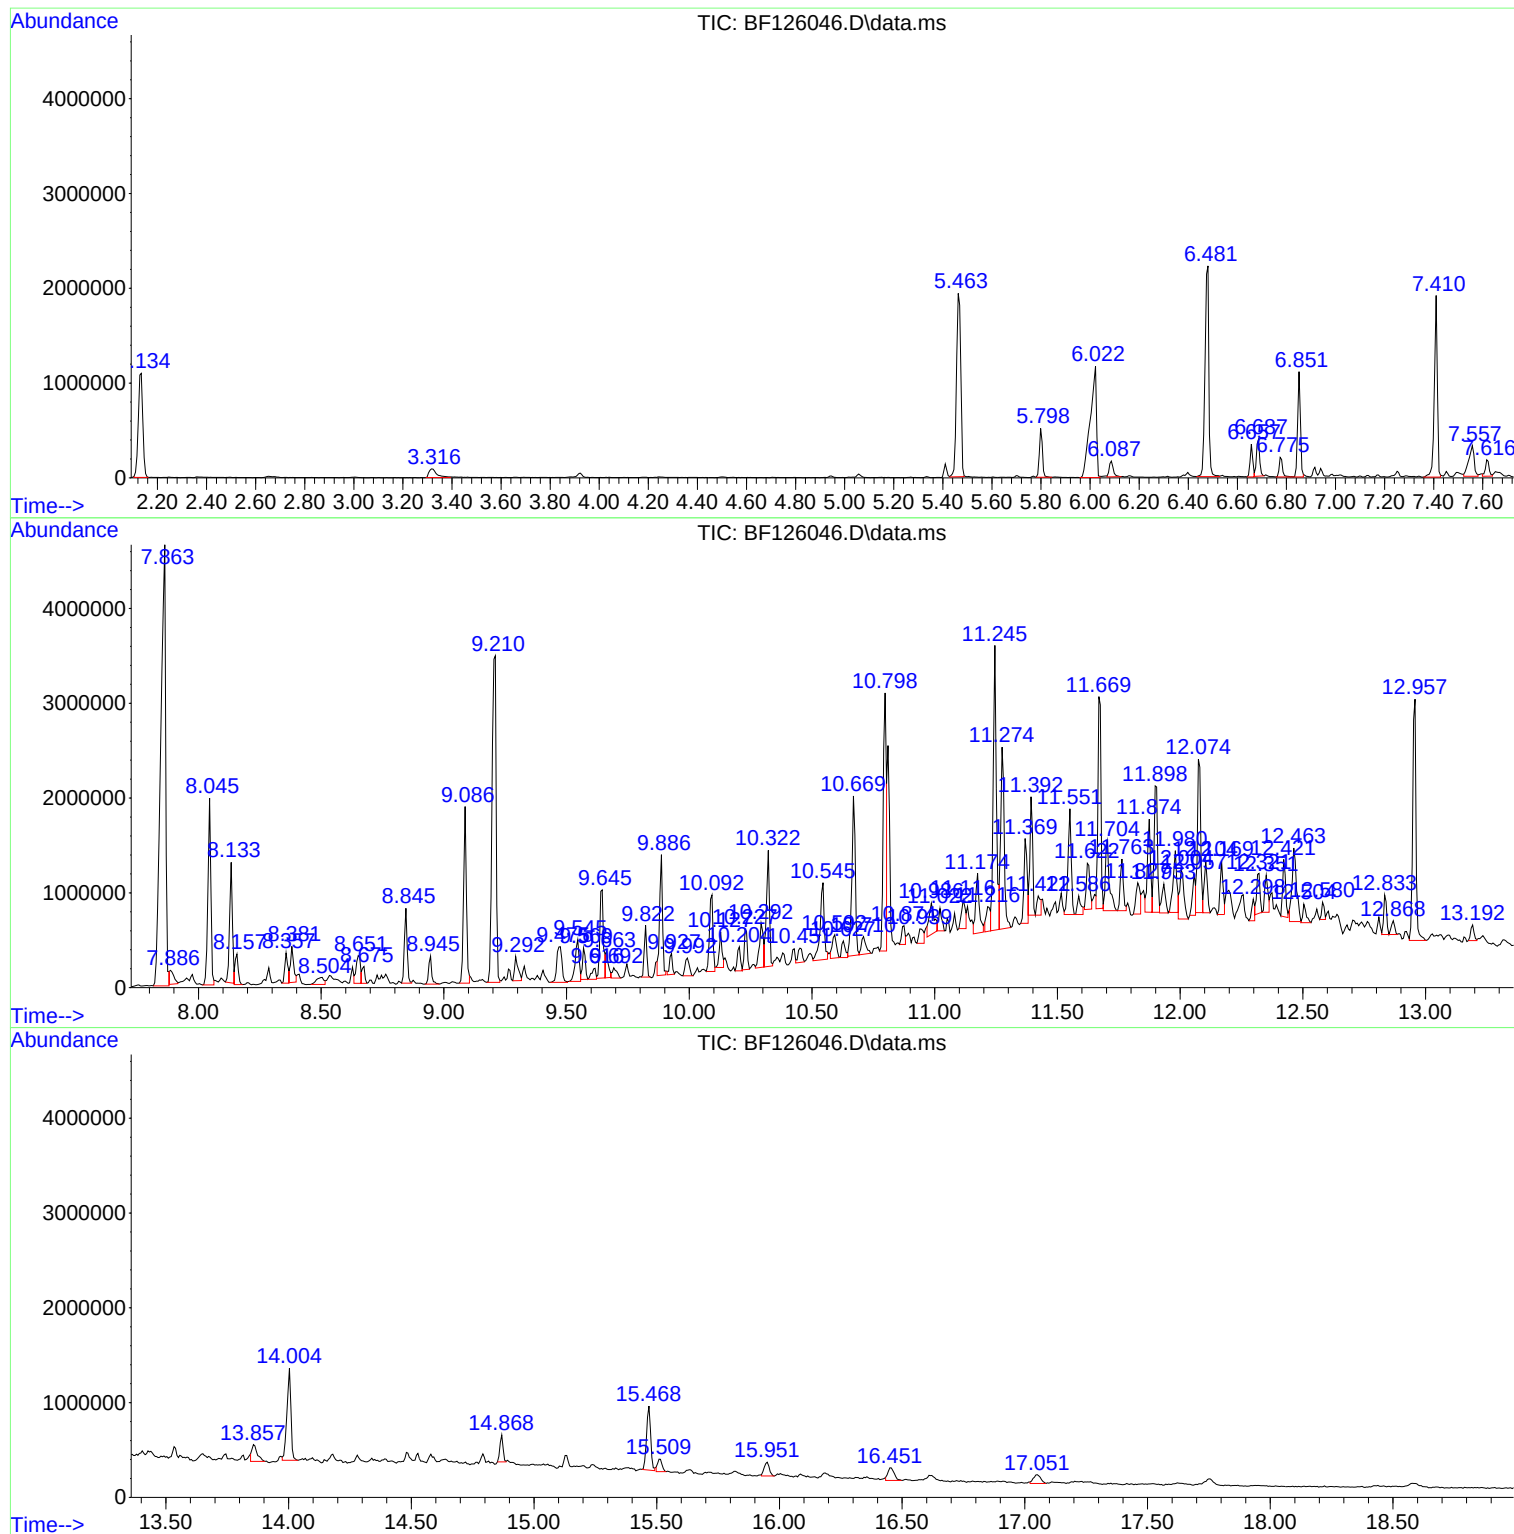

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110421\
Data File : BF126046.D
Acq On : 4 Nov 2021 15:24
Operator : JU/CG
Sample : M4449-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PAINTED-WALLS

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110421\
Data File : BF126046.D
Acq On : 4 Nov 2021 15:24
Operator : JU/CG
Sample : M4449-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PAINTED-WALLS

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------