

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110421\
 Data File : BF126054.D
 Acq On : 4 Nov 2021 19:39
 Operator : JU/CG
 Sample : M4498-04 5X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 WC-2-MD

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF126054.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.910	305	310	314	rVB	11150	15268	1.60%	0.181%
2	5.457	569	573	583	rBV	701652	609263	63.81%	7.233%
3	6.469	742	745	755	rBV	729357	598429	62.67%	7.104%
4	6.851	807	810	814	rBV	972546	846881	88.69%	10.053%
5	7.410	901	905	914	rVB	435022	355407	37.22%	4.219%
6	8.039	1008	1012	1018	rBV	16025	21975	2.30%	0.261%
7	8.133	1024	1028	1032	rBV	1109247	918600	96.20%	10.905%
8	9.210	1207	1211	1223	rBV	673988	587194	61.50%	6.971%
9	9.886	1322	1326	1330	rBV	1106078	901105	94.37%	10.697%
10	10.669	1456	1459	1468	rVB	386416	346314	36.27%	4.111%
11	11.369	1575	1578	1582	rBV	1076071	918823	96.23%	10.907%
12	12.951	1844	1847	1851	rBV	716593	662672	69.40%	7.867%
13	14.010	2023	2027	2031	rBV	1043686	954851	100.00%	11.335%
14	15.474	2271	2276	2280	rBV	557809	687174	71.97%	8.157%




Sum of corrected areas: 8423956

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110421\
Data File : BF126054.D
Acq On : 4 Nov 2021 19:39
Operator : JU/CG
Sample : M4498-04 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC-2-MD

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

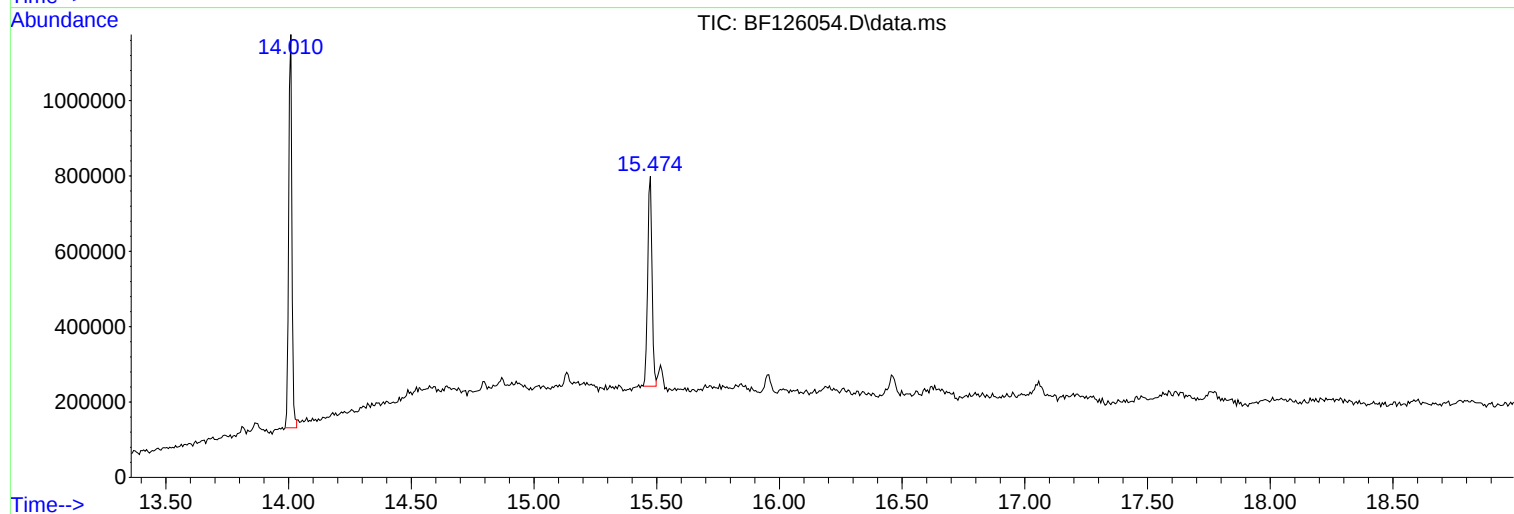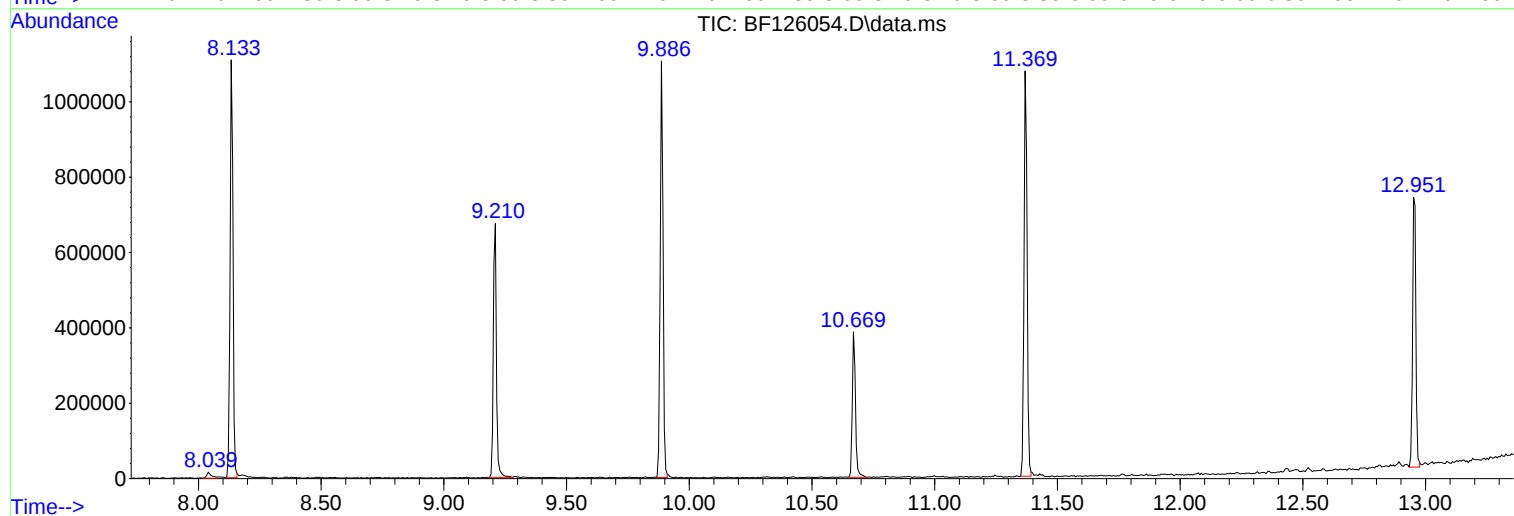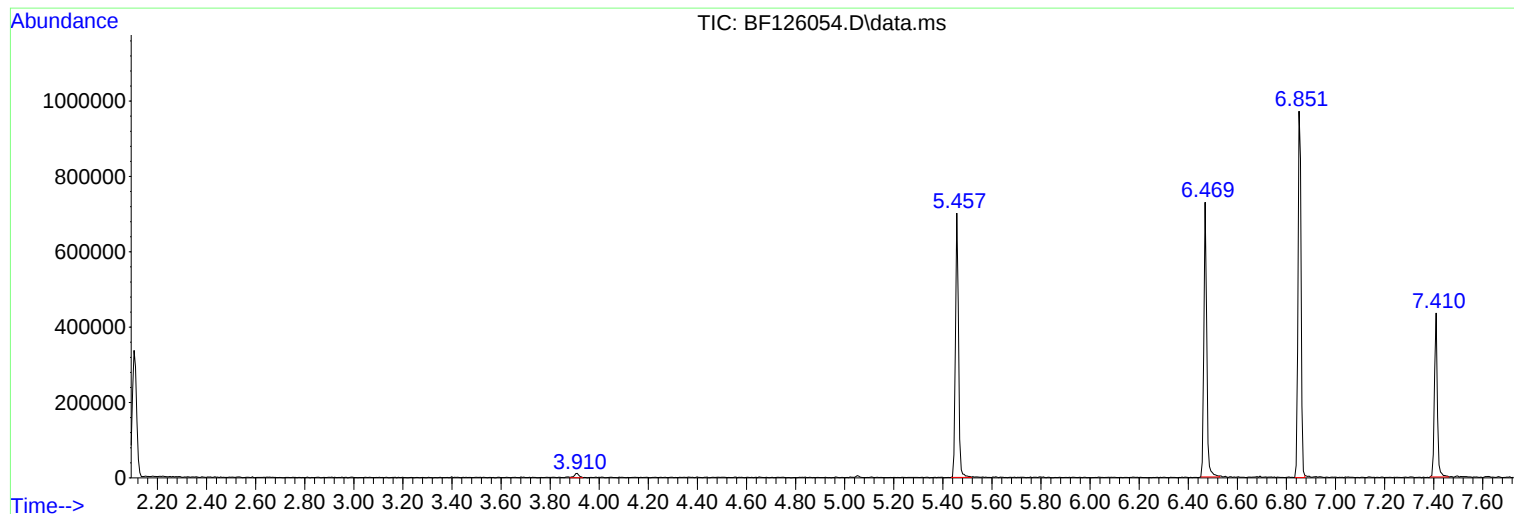

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110421\
Data File : BF126054.D
Acq On : 4 Nov 2021 19:39
Operator : JU/CG
Sample : M4498-04 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC-2-MD

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110421\
Data File : BF126054.D
Acq On : 4 Nov 2021 19:39
Operator : JU/CG
Sample : M4498-04 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC-2-MD

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------