
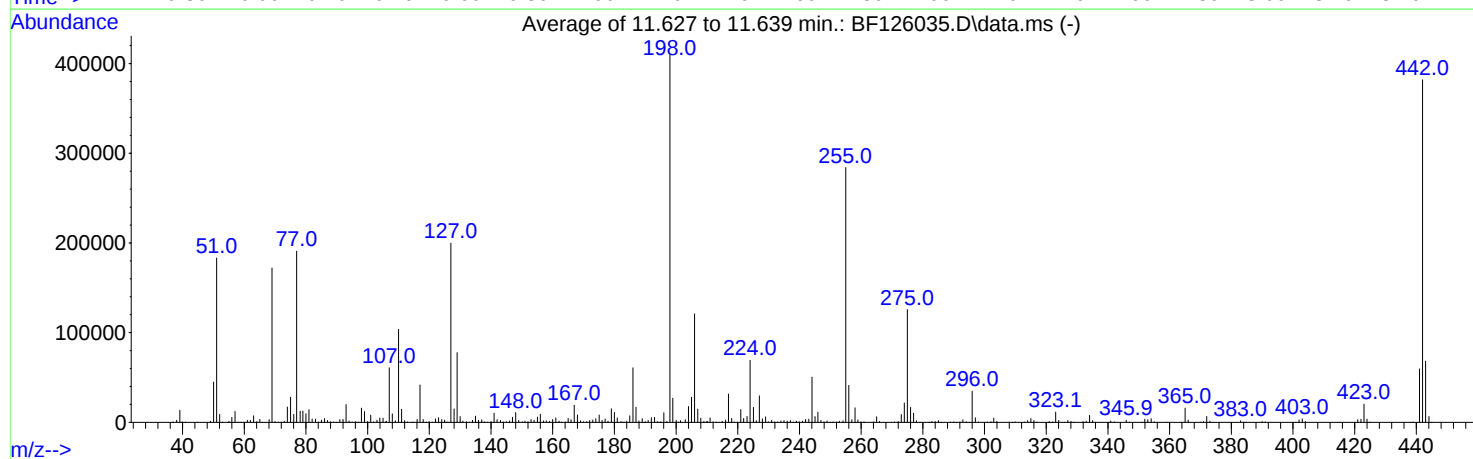


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110421\
 Data File : BF126035.D
 Acq On : 4 Nov 2021 9:20
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 03 17:21:25 2021

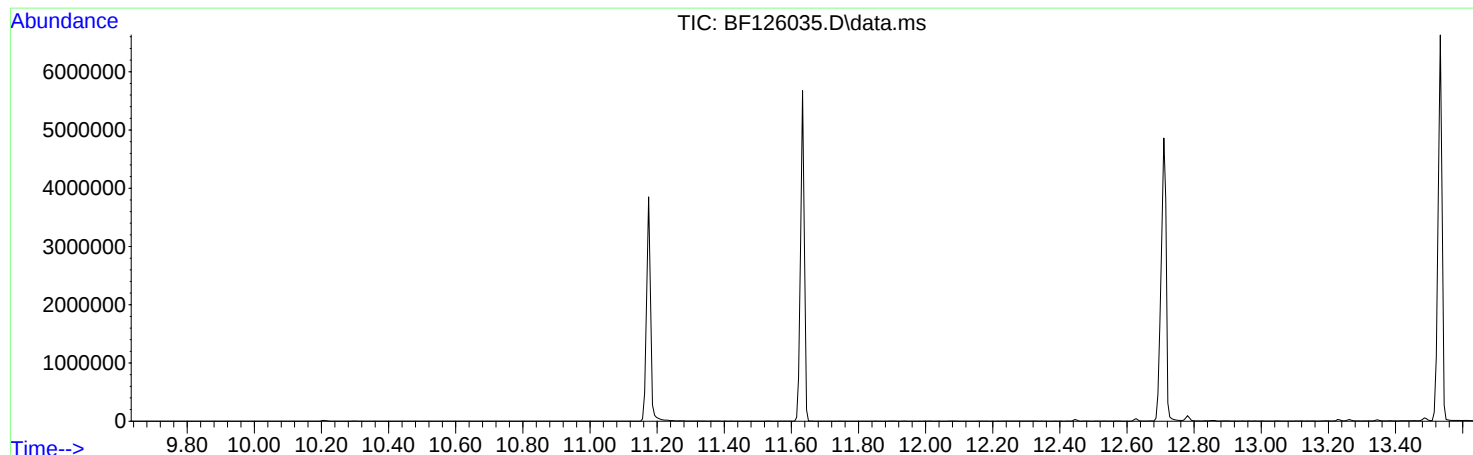




AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.7	183267	PASS
68	69	0.00	2	1.8	3038	PASS
69	198	0.00	100	42.0	172059	PASS
70	69	0.00	2	0.6	967	PASS
127	198	10	80	48.7	199736	PASS
197	198	0.00	2	0.2	1024	PASS
198	198	100	100	100.0	410091	PASS
199	198	5	9	6.6	26899	PASS
275	198	10	60	30.7	125848	PASS
365	198	1	100	3.9	15966	PASS
441	198	0.01	100	14.5	59581	PASS
442	442	50	100	100.0	381824	PASS
443	442	15	24	17.9	68341	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110421\
Data File : BF126035.D
Acq On : 4 Nov 2021 9:20
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 04 15:03:30 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 03 17:21:25 2021
Response via : Initial Calibration

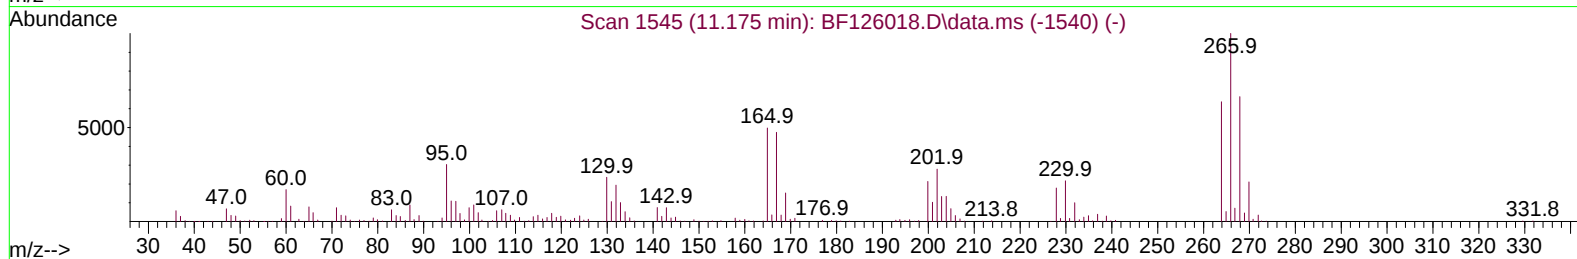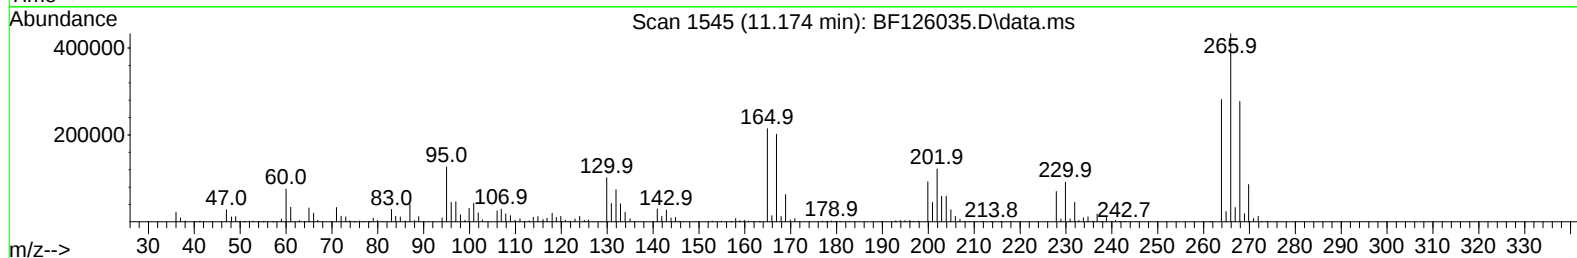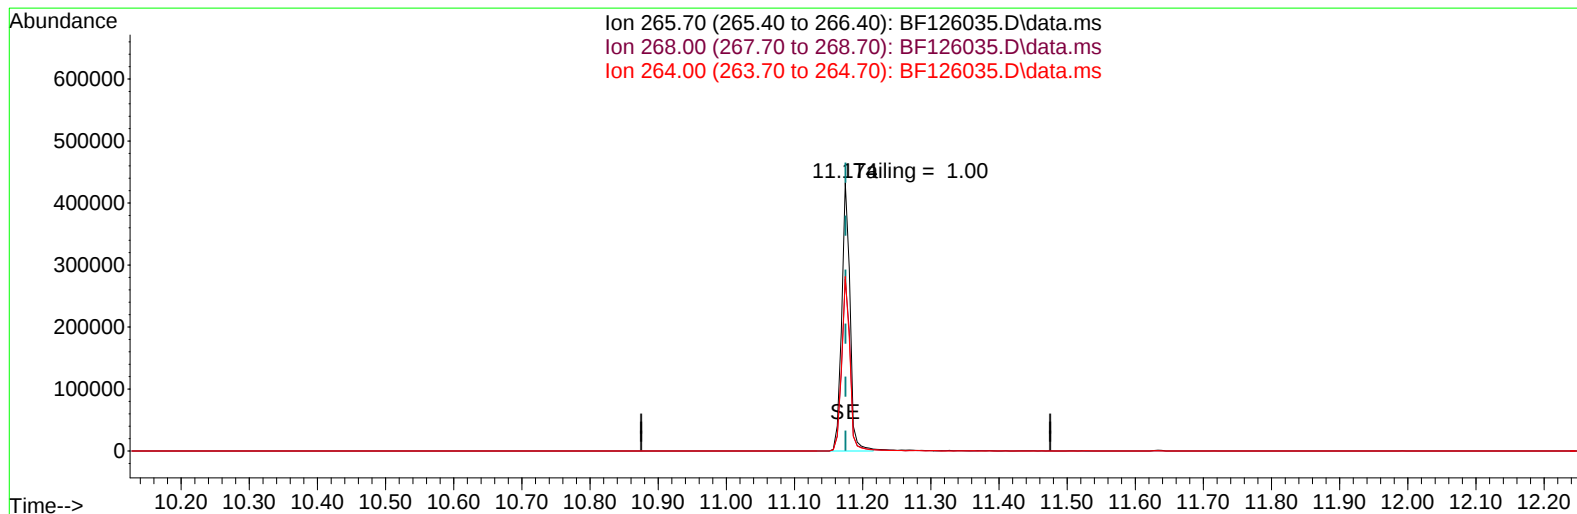

TIC: BF126035.D\data.ms

(70) Pentachlorophenol (C)

11.174min (-0.001) 27253.18 ng




response 370698

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	64.00
264.00	69.90	64.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110421\
Data File : BF126035.D
Acq On : 4 Nov 2021 9:20
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 04 15:03:30 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 03 17:21:25 2021
Response via : Initial Calibration

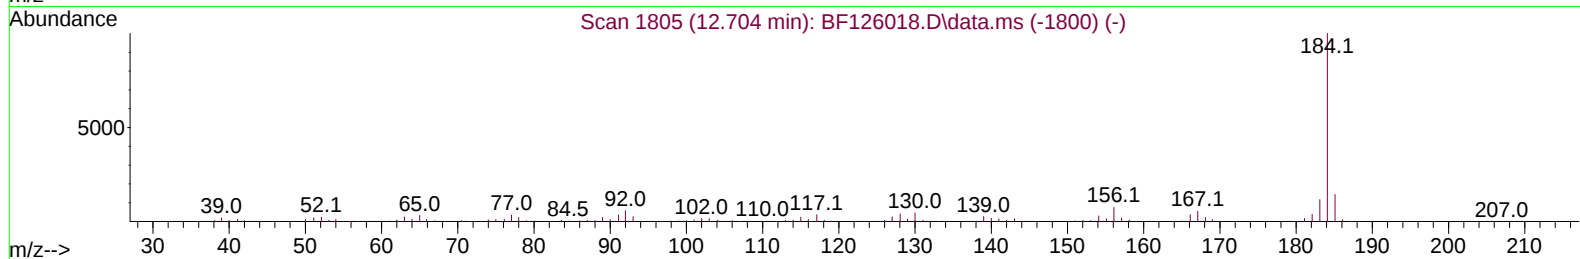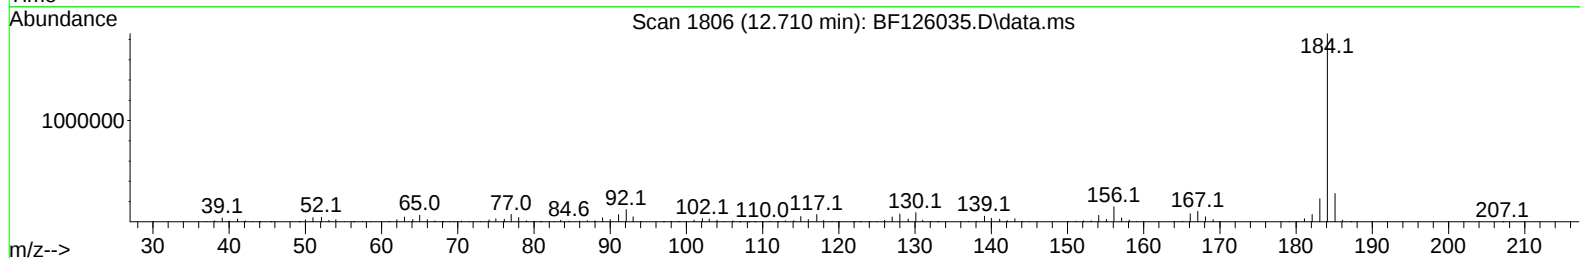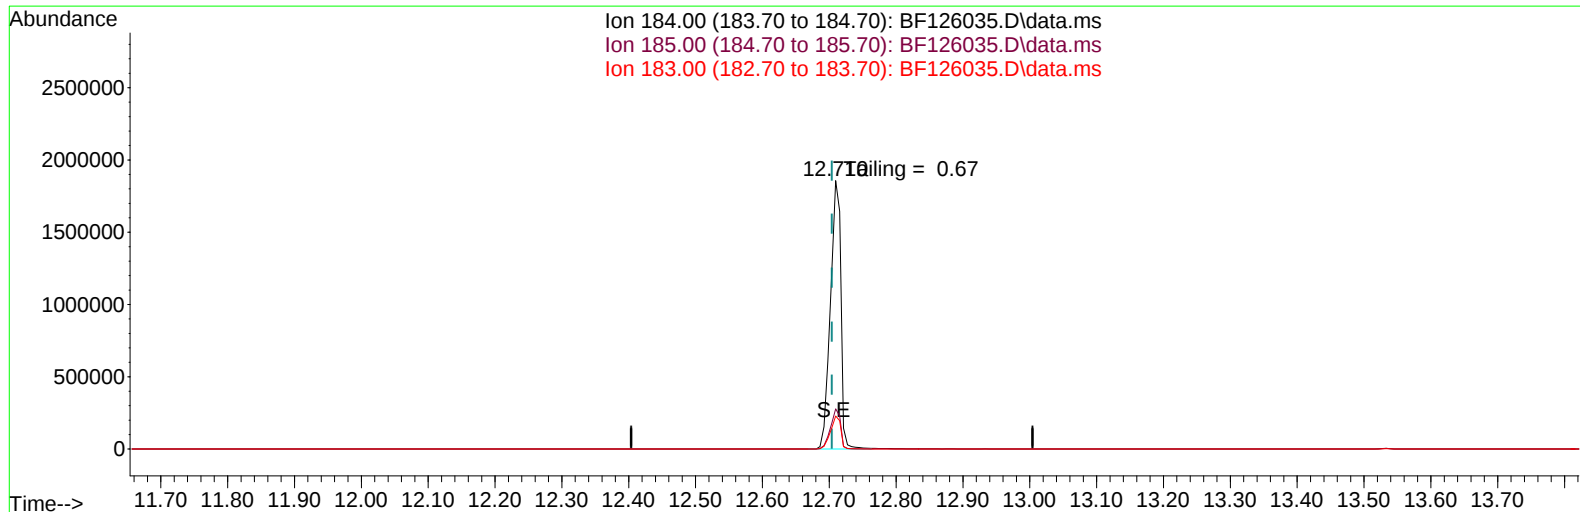

TIC: BF126035.D\data.ms

(77) Benzidine

12.710min (+ 0.006) 0.00 ng

response 2037363

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.98
183.00	10.10	12.28#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/4/2021	BNA_F	<u>BF126035.D</u>
Compound Name	Response	Retention Time
DDT	1043881	13.53
DDD	4959	13.22
DDE	590	12.89
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5549	1049430	0.53

Instrument :
BNA_F
ClientSampleId :
DFTPP