

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF110518\
 Data File : BF110490.D
 Acq On : 6 Nov 2018 3:34
 Operator : JU/SJ
 Sample : J5810-02
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Nov 06 05:30:27 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF102318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 01 16:06:12 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.95	152	95552	20.00	ng	0.00
21) Naphthalene-d8	8.24	136	376554	20.00	ng	0.00
39) Acenaphthene-d10	10.00	164	163246	20.00	ng	0.00
64) Phenanthrene-d10	11.49	188	255388	20.00	ng	0.00
76) Chrysene-d12	14.13	240	174613	20.00	ng	0.00
87) Perylene-d12	15.66	264	130607	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.57	112	267087	45.52	ng	0.00
7) Phenol-d6	6.57	99	219230	29.21	ng	-0.01
23) Nitrobenzene-d5	7.52	82	655079	103.19	ng	0.00
42) 2,4,6-Tribromophenol	10.79	330	131732	81.46	ng	0.00
45) 2-Fluorobiphenyl	9.31	172	1182846	113.78	ng	0.00
79) Terphenyl-d14	13.07	244	826390	98.43	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.52	70	87617	18.197	ng	# 79
25) Isophorone	7.52	82	655124	60.537	ng	# 67
51) 2,6-Dinitrotoluene	10.00	165	20068	7.731	ng	# 22
57) 2,4-Dinitrotoluene	10.00	165	20068	6.087	ng	# 18
67) 4-Bromophenyl-phenylether	10.79	248	8556	3.089	ng	# 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF110518\
Data File : BF110490.D
Acq On : 6 Nov 2018 3:34
Operator : JU/SJ
Sample : J5810-02
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 06 05:30:27 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF102318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 01 16:06:12 2018
Response via : Initial Calibration

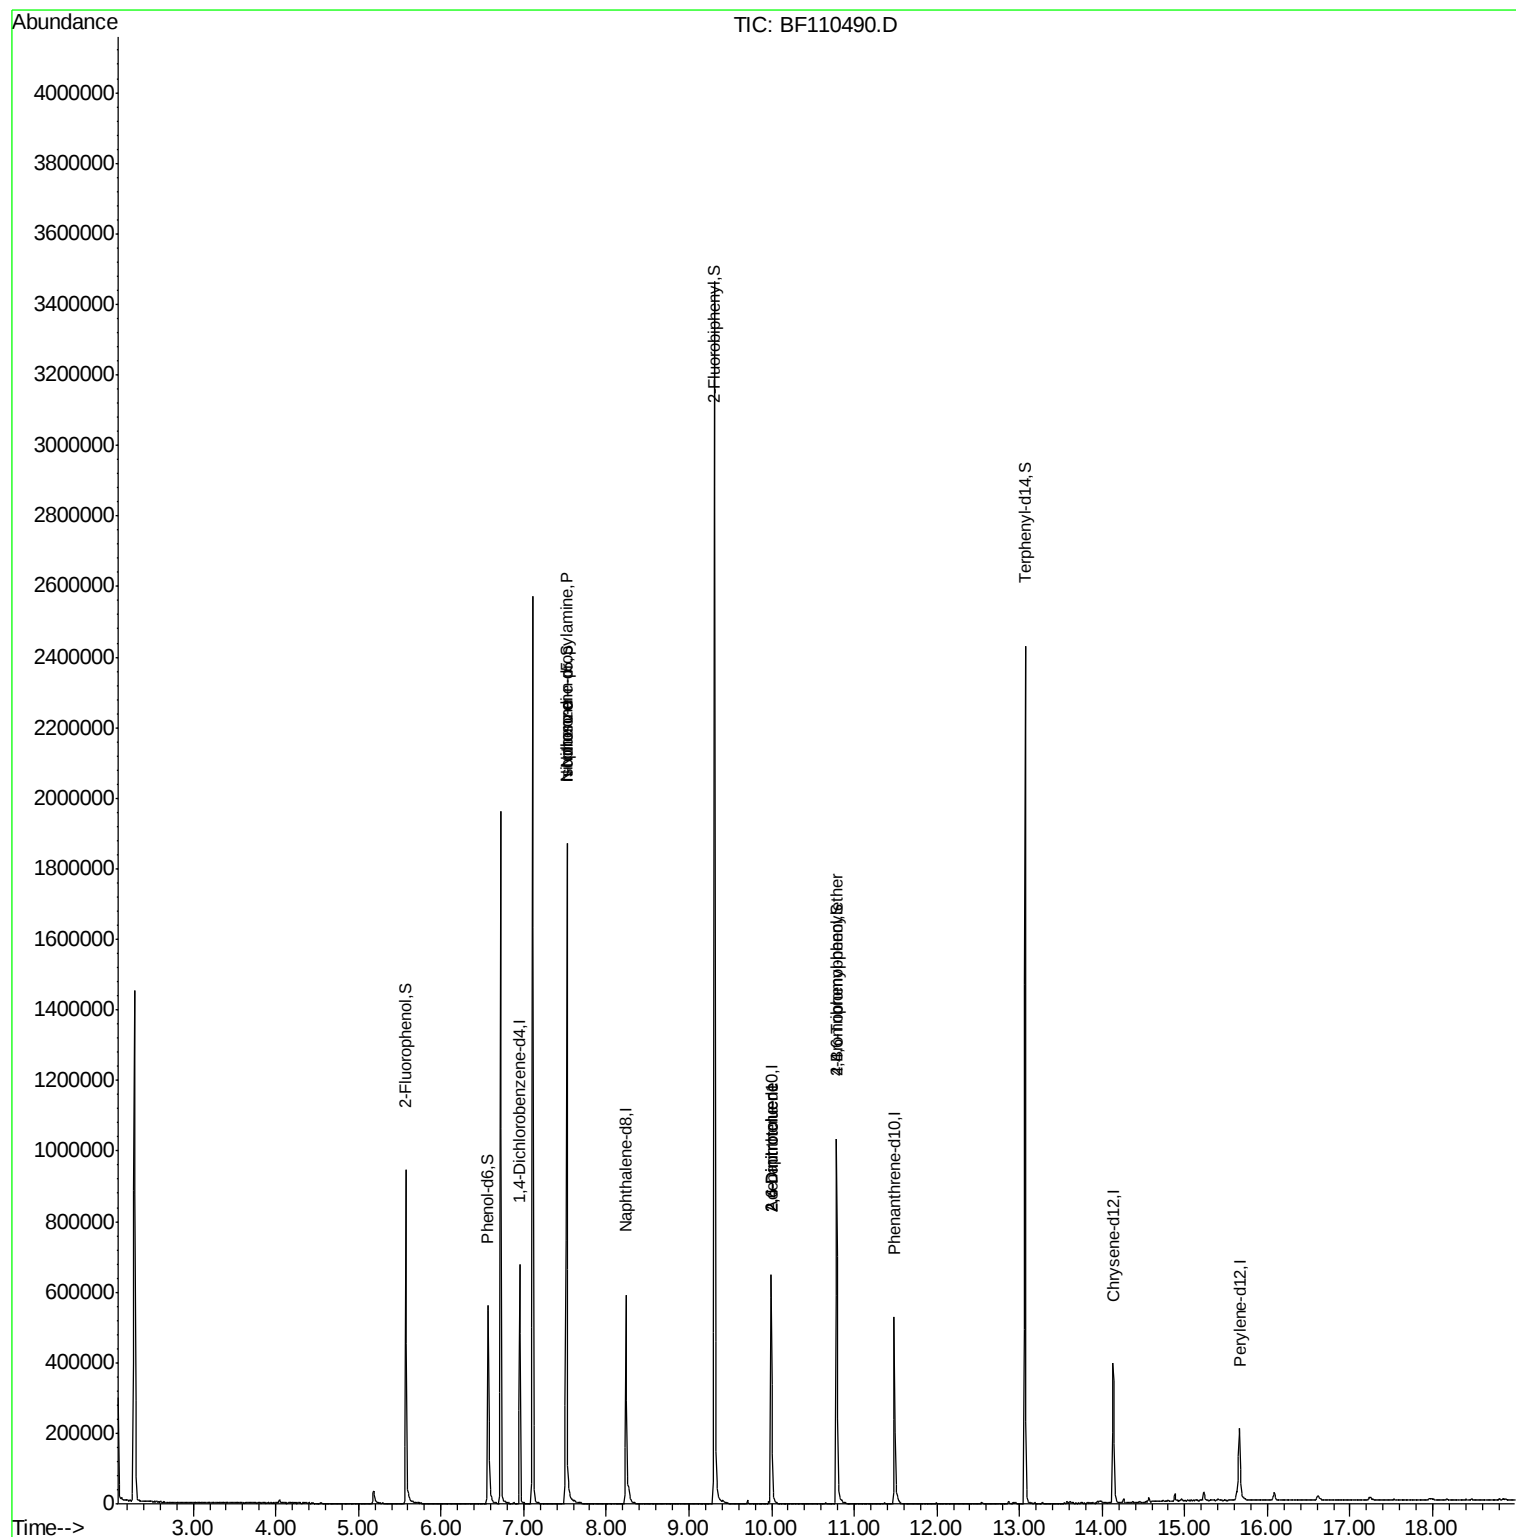




#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.95 min Scan# 827
Delta R.T. -0.01 min
Lab File: BF110490.D
Acq: 6 Nov 2018 3:34

Instrument :
BNA_F
ClientSampleId :
DFTPP

Tgt Ion:152 Resp: 95552
Ion Ratio Lower Upper
152 100
150 156.6 122.7 184.1
115 64.1 49.1 73.7

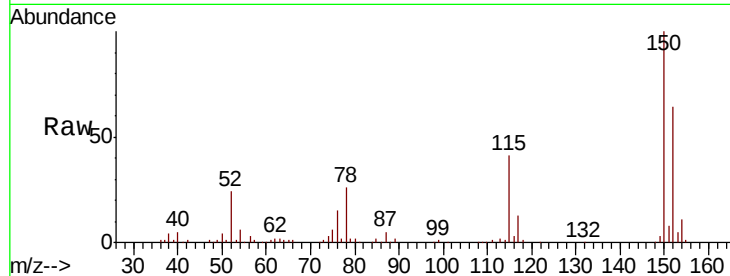


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

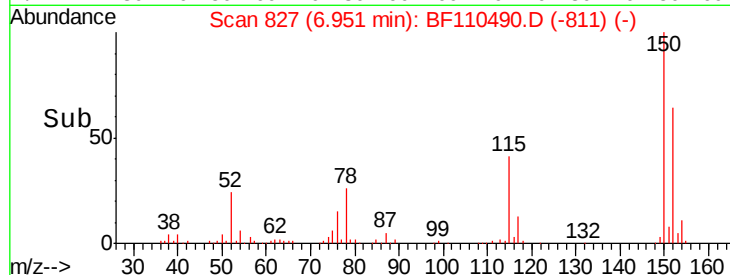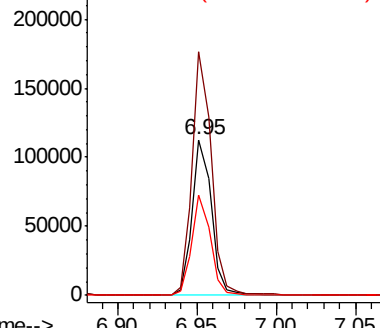



#5

2-Fluorophenol
Concen: 45.518 ng
RT: 5.57 min Scan# 593
Delta R.T. 0.00 min
Lab File: BF110490.D
Acq: 6 Nov 2018 3:34

Tgt Ion:112 Resp: 267087
Ion Ratio Lower Upper
112 100
64 57.6 44.1 66.1
63 30.8 23.7 35.5

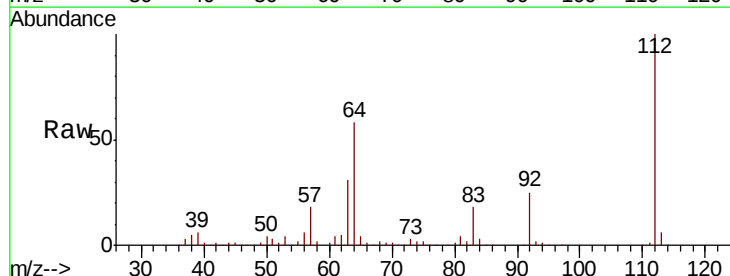

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

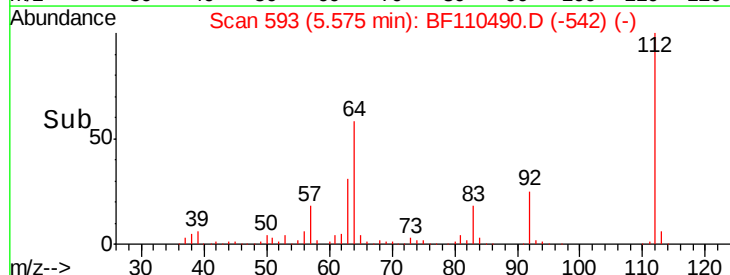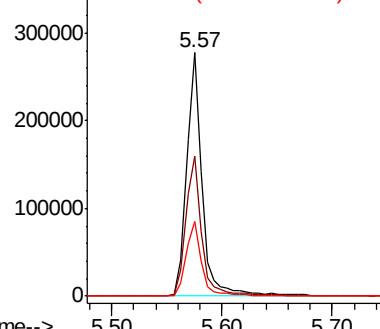



#7

Phenol-d6

Concen: 29.210 ng

RT: 6.57 min Scan# 762

Delta R.T. -0.01 min

Lab File: BF110490.D

Acq: 6 Nov 2018 3:34

Instrument :

BNA_F

ClientSampleId :

DFTPP


Tgt Ion: 99 Resp: 219230

Ion Ratio Lower Upper

99 100

42 19.9 15.8 23.6

71 34.6 28.0 42.0



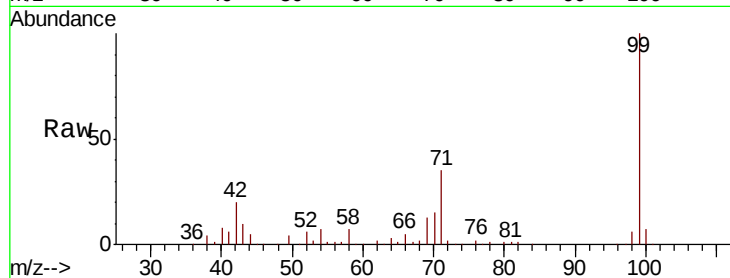


Abundance

Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

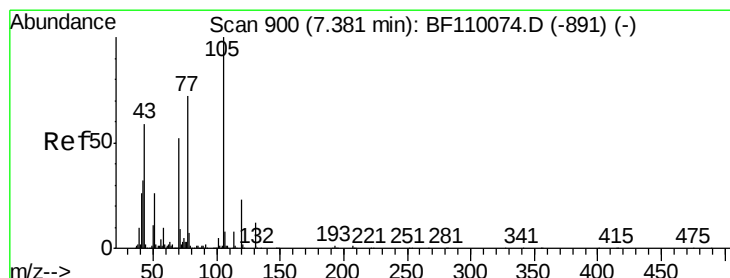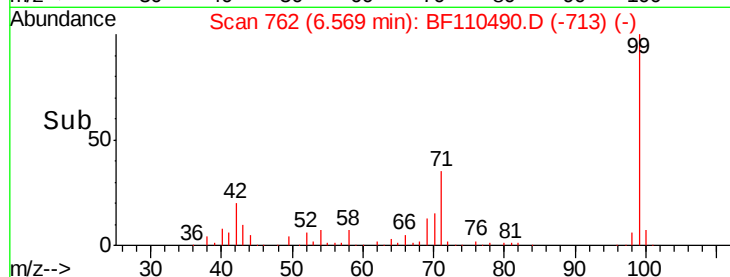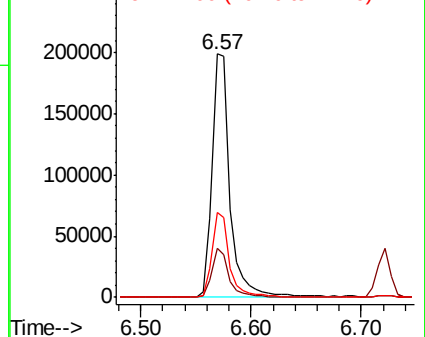

#19

n-Nitroso-di-n-propylamine

Concen: 18.197 ng

RT: 7.52 min Scan# 924

Delta R.T. 0.16 min

Lab File: BF110490.D

Acq: 6 Nov 2018 3:34

Tgt Ion: 70 Resp: 87617


Ion Ratio Lower Upper

70 100

42 49.1 47.4 71.2

101 0.0 7.3 10.9#

130 2.3 16.2 24.2#

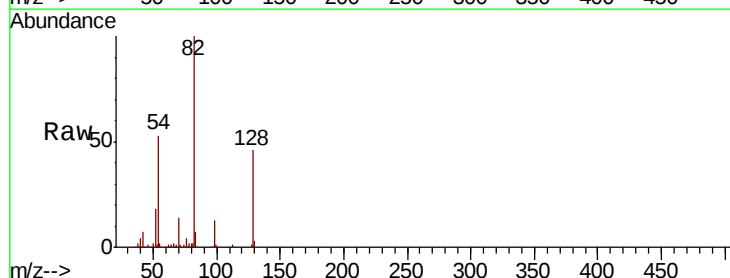



Abundance

Ion 70.00 (69.70 to 70.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 101.00 (100.70 to 101.70): BF1

Ion 130.00 (129.70 to 130.70): BF1

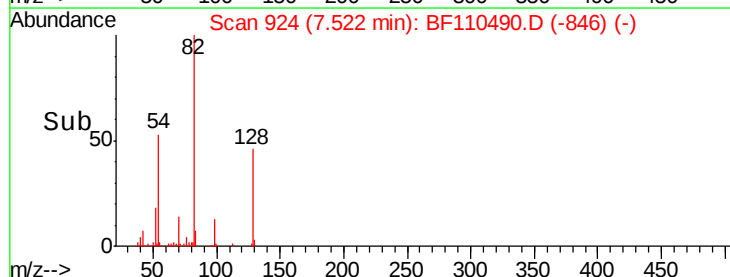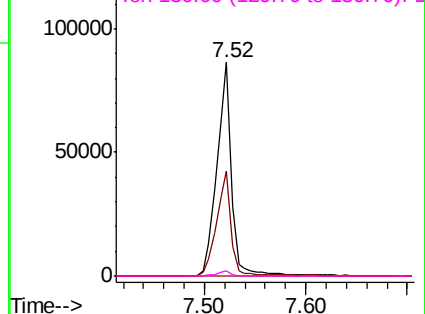







#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.24 min Scan# 1046
Delta R.T. 0.00 min
Lab File: BF110490.D
Acq: 6 Nov 2018 3:34

Instrument :
BNA_F
ClientSampleId :
DFTPP

Tgt Ion: 136 Resp: 376554
Ion Ratio Lower Upper
136 100
137 10.5 8.8 13.2
54 7.7 5.4 8.2
68 4.5 4.2 6.2

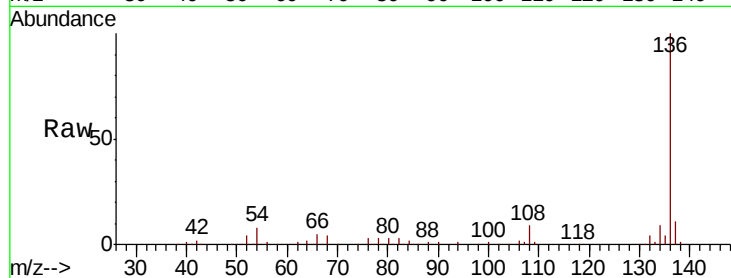


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

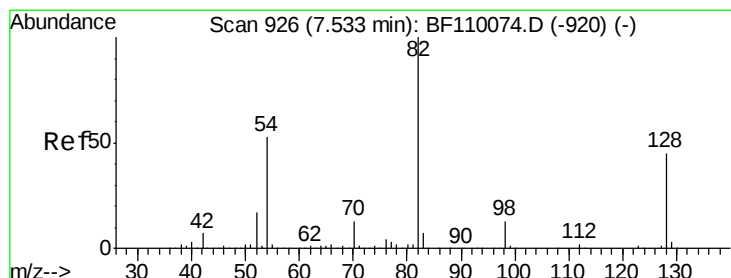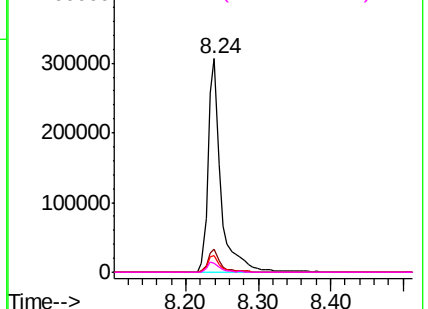
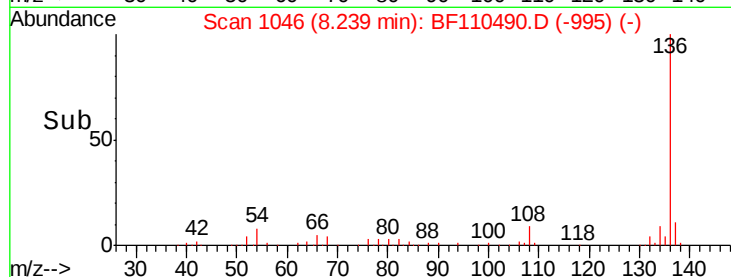



#23
Nitrobenzene-d5
Concen: 103.185 ng
RT: 7.52 min Scan# 924
Delta R.T. 0.00 min
Lab File: BF110490.D
Acq: 6 Nov 2018 3:34

Tgt Ion: 82 Resp: 655079
Ion Ratio Lower Upper
82 100
128 45.5 34.2 51.2
54 52.6 38.6 58.0

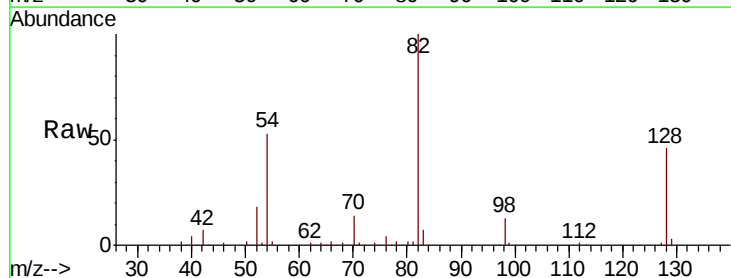

Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF1

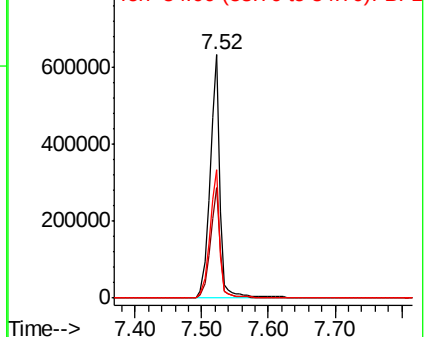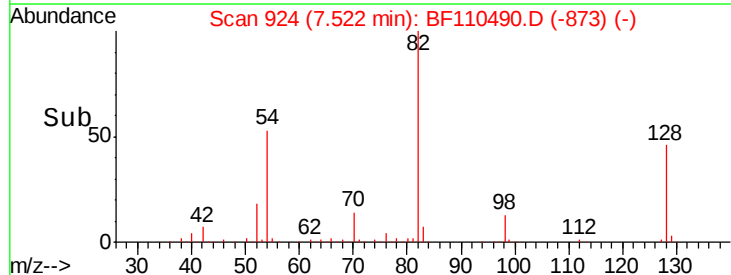

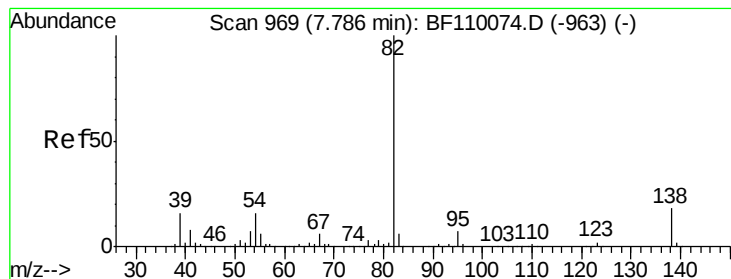

#25

Isophorone

Concen: 60.537 ng

RT: 7.52 min Scan# 924

Delta R.T. -0.25 min

Lab File: BF110490.D

Acq: 6 Nov 2018 3:34

Instrument :

BNA_F

ClientSampleId :

DFTPP


Tgt Ion: 82 Resp: 655124

Ion Ratio Lower Upper

82 100

95 0.0 5.7 8.5#




138 0.0 13.2 19.8#

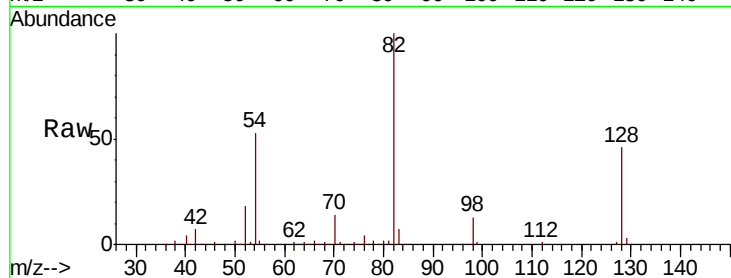

Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 95.00 (94.70 to 95.70): BF1

Ion 138.00 (137.70 to 138.70): BF1

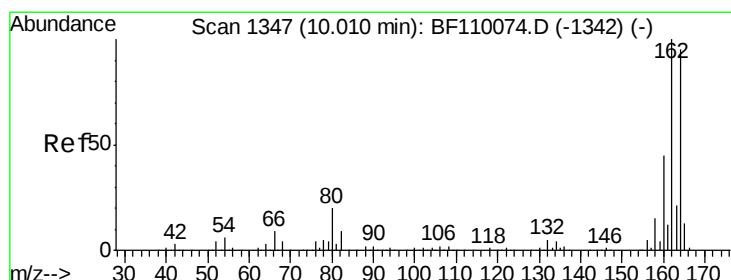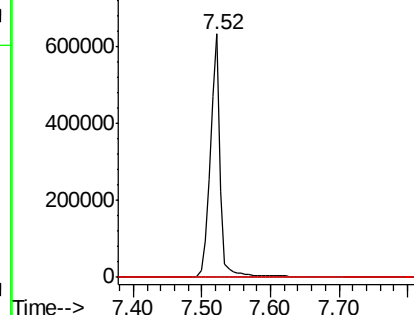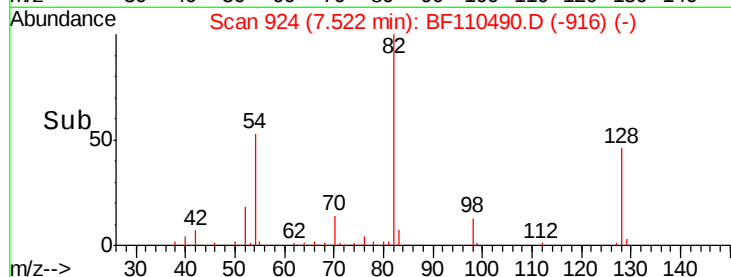

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 10.00 min Scan# 1345

Delta R.T. 0.00 min

Lab File: BF110490.D

Acq: 6 Nov 2018 3:34


Tgt Ion: 164 Resp: 163246

Ion Ratio Lower Upper

164 100

162 103.1 83.0 124.6



160 46.1 37.0 55.6

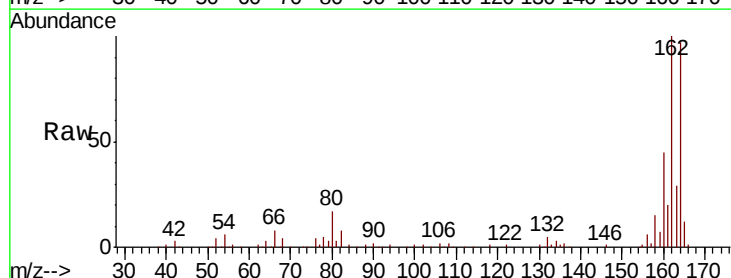


Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

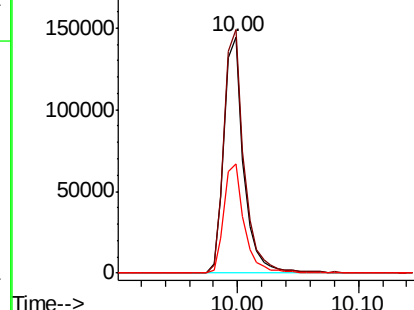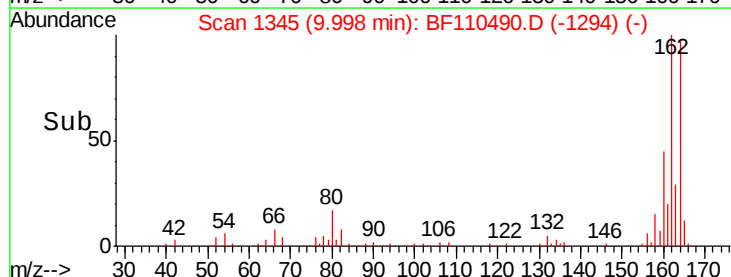


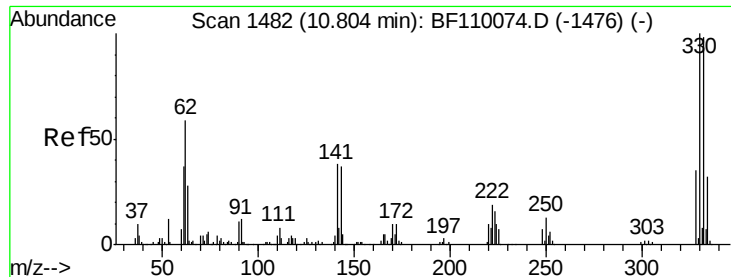




#42
 2,4,6-Tribromophenol
 Concen: 81.464 ng
 RT: 10.79 min Scan# 1479
 Delta R.T. -0.01 min
 Lab File: BF110490.D
 Acq: 6 Nov 2018 3:34

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Tgt Ion:330 Resp: 131732
 Ion Ratio Lower Upper
 330 100
 332 96.5 77.1 115.7
 141 37.2 27.0 40.4

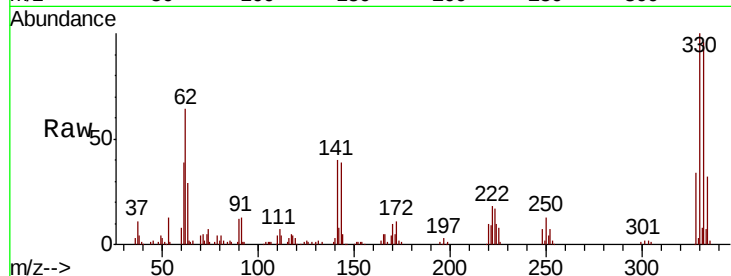


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

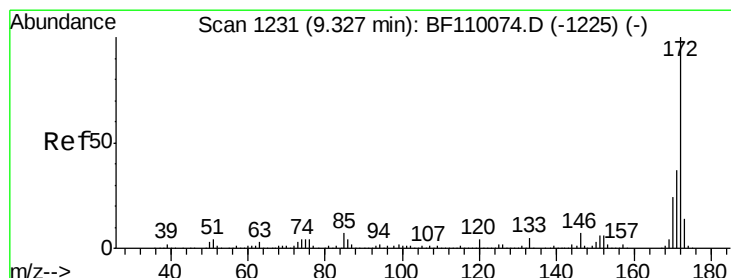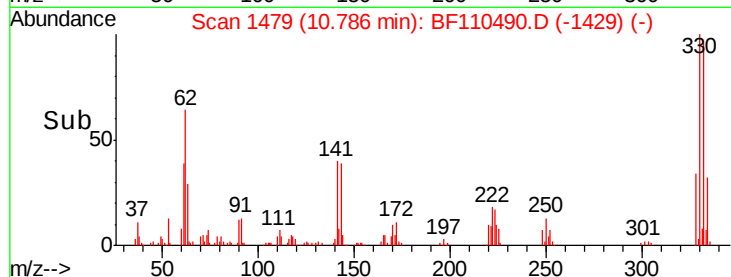
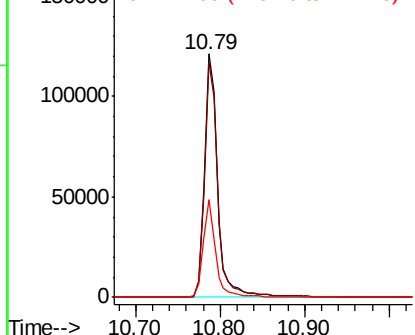


#45
 2-Fluorobiphenyl
 Concen: 113.778 ng
 RT: 9.31 min Scan# 1228
 Delta R.T. -0.01 min
 Lab File: BF110490.D
 Acq: 6 Nov 2018 3:34

Tgt Ion:172 Resp: 1182846
 Ion Ratio Lower Upper
 172 100
 171 36.0 28.6 43.0
 170 23.4 19.7 29.5

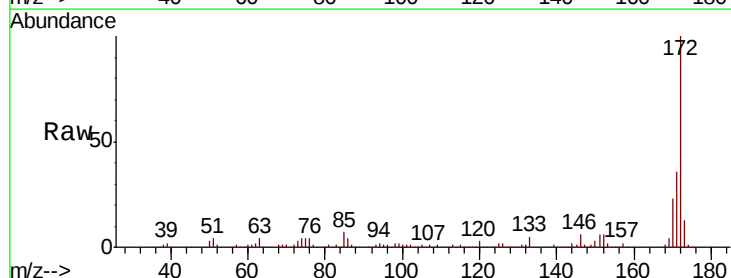

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

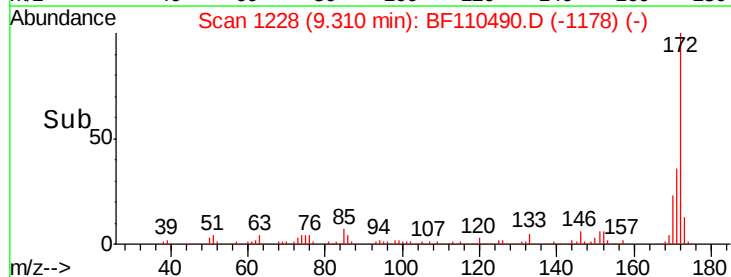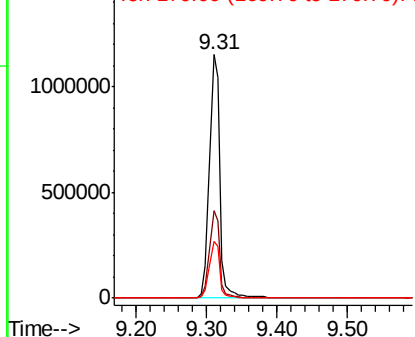



#51

2,6-Dinitrotoluene

Concen: 7.731 ng

RT: 10.00 min Scan# 1345

Delta R.T. 0.22 min

Lab File: BF110490.D

Acq: 6 Nov 2018 3:34

Instrument :

BNA_F

ClientSampleId :

DFTPP


Tgt Ion:165 Resp: 20068

Ion Ratio Lower Upper

165 100

63 2.0 48.9 73.3#




89 0.0 46.6 69.8#

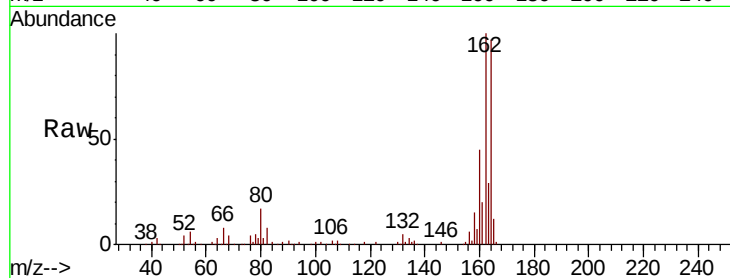

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF1

Ion 89.00 (88.70 to 89.70): BF1

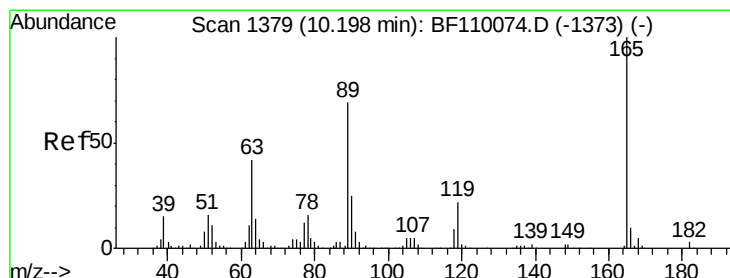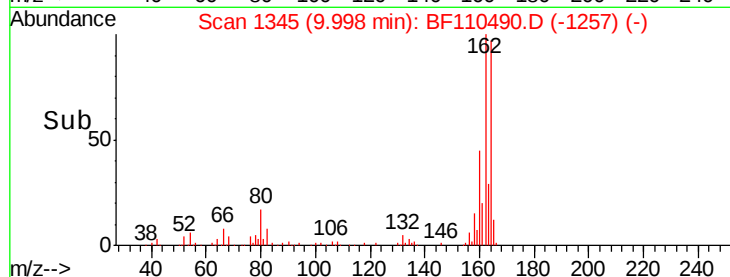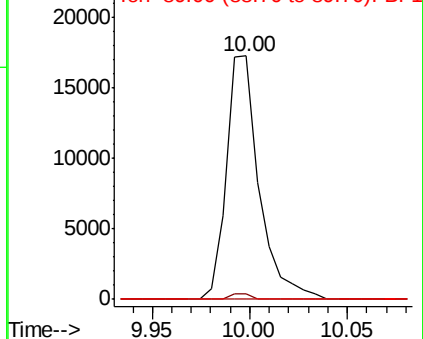

#57

2,4-Dinitrotoluene

Concen: 6.087 ng

RT: 10.00 min Scan# 1345

Delta R.T. -0.19 min

Lab File: BF110490.D

Acq: 6 Nov 2018 3:34

Tgt Ion:165 Resp: 20068


Ion Ratio Lower Upper

165 100

63 2.0 44.8 67.2#

89 0.0 62.2 93.4#

182 0.0 2.1 3.1#


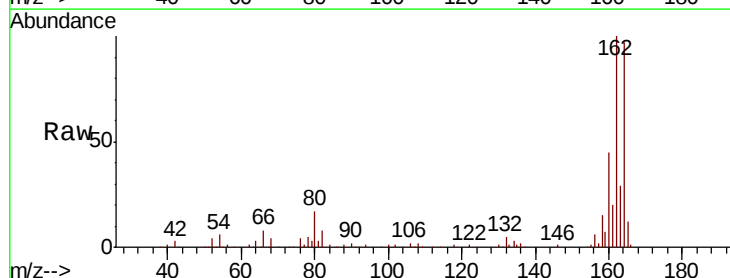



Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF1

Ion 89.00 (88.70 to 89.70): BF1

Ion 182.00 (181.70 to 182.70): E



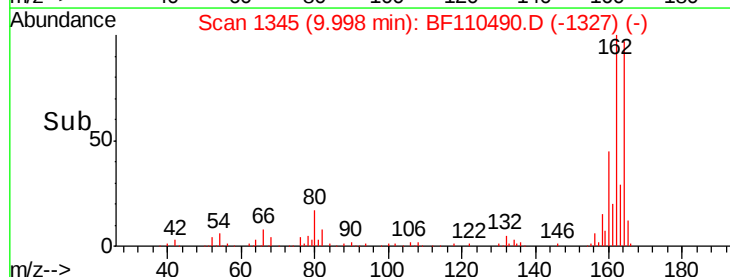
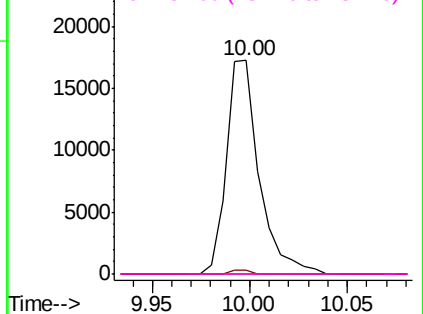


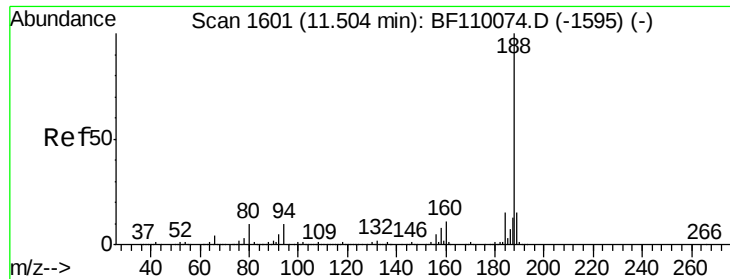

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.49 min Scan# 1598
Delta R.T. -0.01 min
Lab File: BF110490.D
Acq: 6 Nov 2018 3:34




Instrument :
BNA_F
ClientSampleId :
DFTPP


Tgt Ion:188 Resp: 255388
Ion Ratio Lower Upper
188 100
94 9.0 7.2 10.8
80 9.9 7.9 11.9

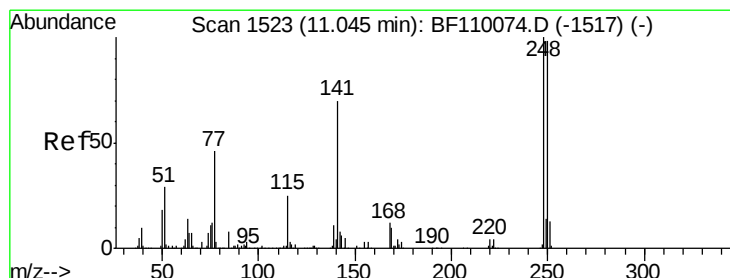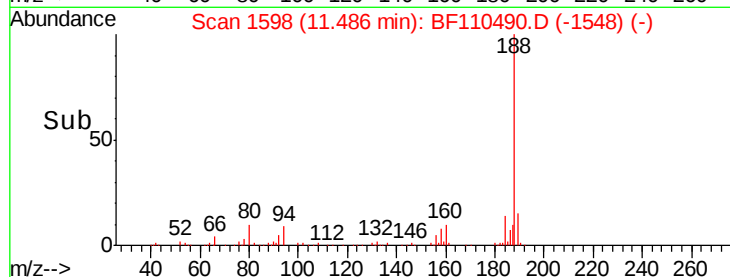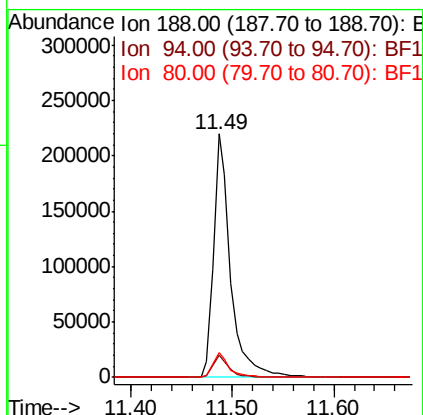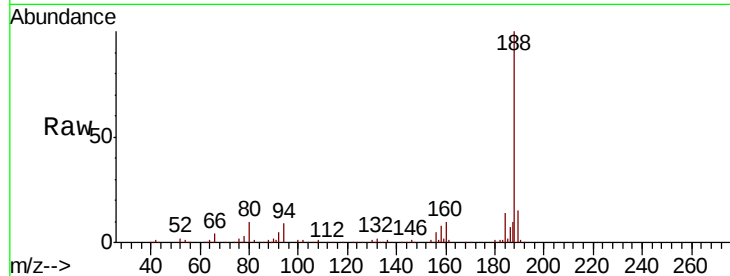

#67
4-Bromophenyl-phenylether
Concen: 3.089 ng
RT: 10.79 min Scan# 1479
Delta R.T. -0.24 min
Lab File: BF110490.D
Acq: 6 Nov 2018 3:34

Tgt Ion:248 Resp: 8556
Ion Ratio Lower Upper
248 100
250 189.0 79.4 119.2#
141 560.6 55.9 83.9#

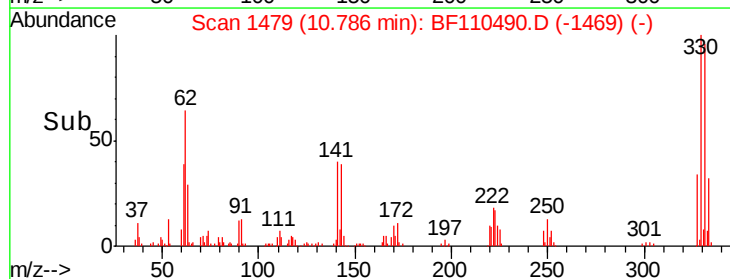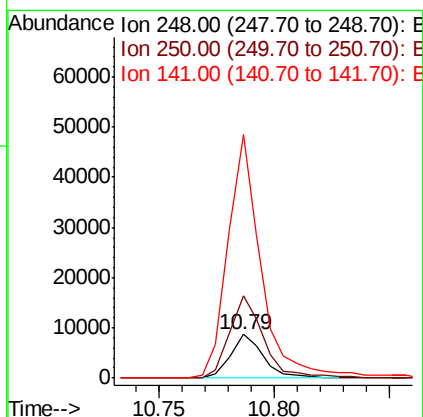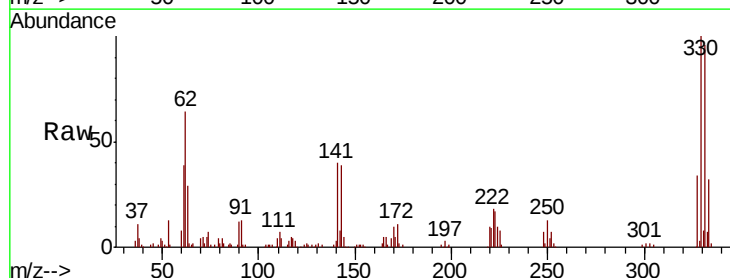


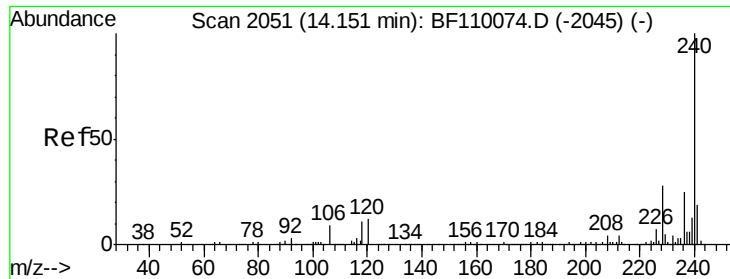

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.13 min Scan# 2048
Delta R.T. -0.01 min
Lab File: BF110490.D
Acq: 6 Nov 2018 3:34

Instrument :
BNA_F
ClientSampleId :
DFTPP

Tgt Ion	Ratio	Lower	Upper
240	100		
120	11.4	8.3	12.5
236	25.0	21.2	31.8



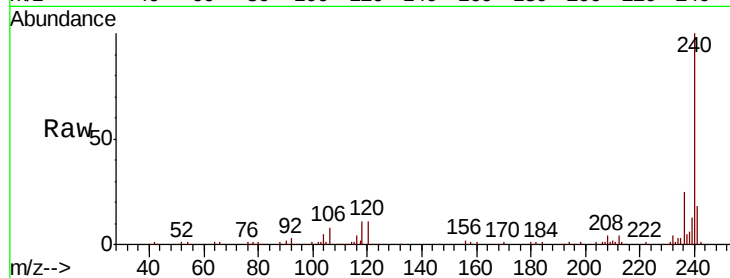


Abundance

Ion 240.00 (239.70 to 240.70): E


Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

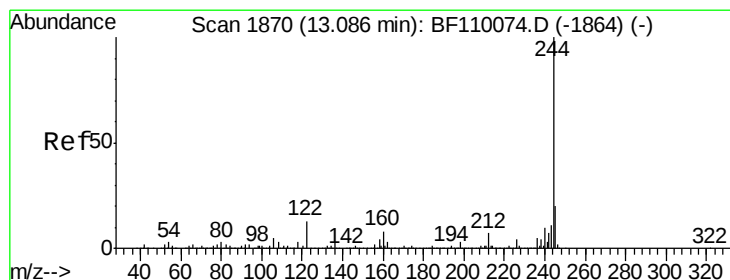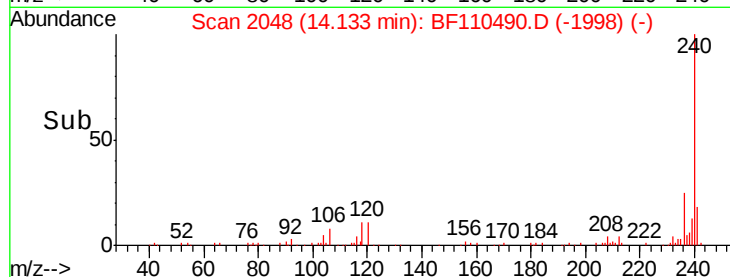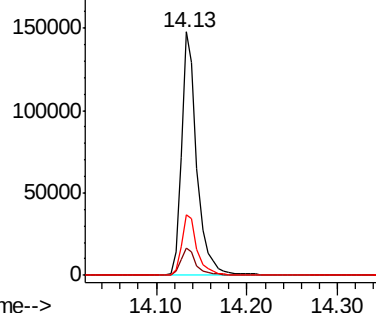

#79
Terphenyl-d14
Concen: 98.426 ng
RT: 13.07 min Scan# 1867
Delta R.T. -0.01 min
Lab File: BF110490.D
Acq: 6 Nov 2018 3:34

Tgt Ion	Ratio	Lower	Upper
244	100		
212	7.1	5.8	8.8
122	12.8	8.7	13.1


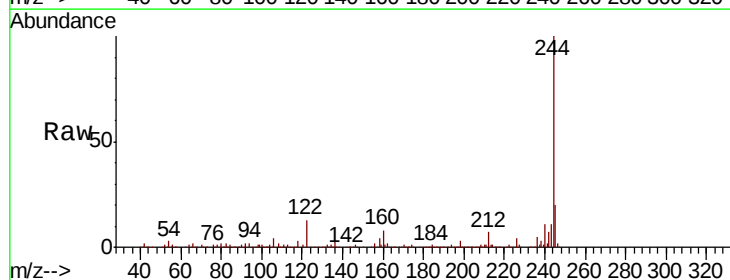



Abundance

Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

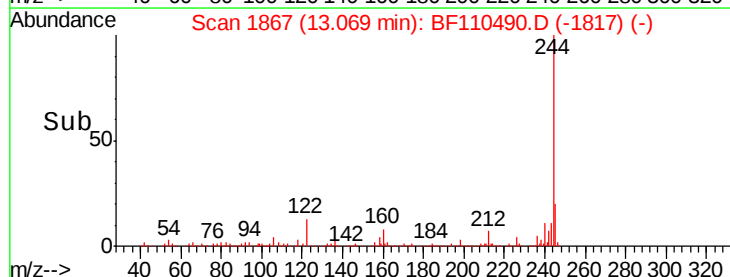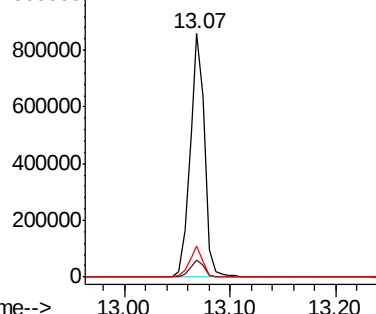

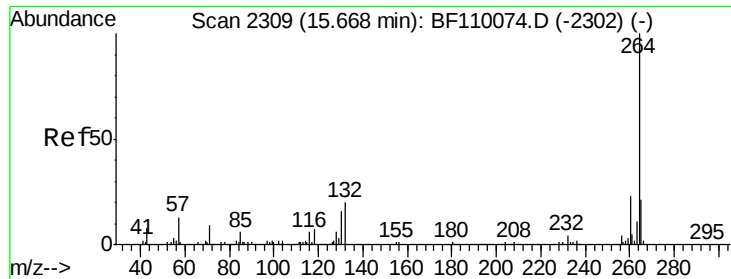

#87
Perylene-d12
Concen: 20.000 ng
RT: 15.66 min Scan# 2308
Delta R.T. 0.01 min
Lab File: BF110490.D
Acq: 6 Nov 2018 3:34

Instrument :
BNA_F
ClientSampleId :
DFTPP

Tgt Ion:264 Resp: 130607
Ion Ratio Lower Upper
264 100
260 23.5 18.7 28.1
265 22.5 16.7 25.1

