
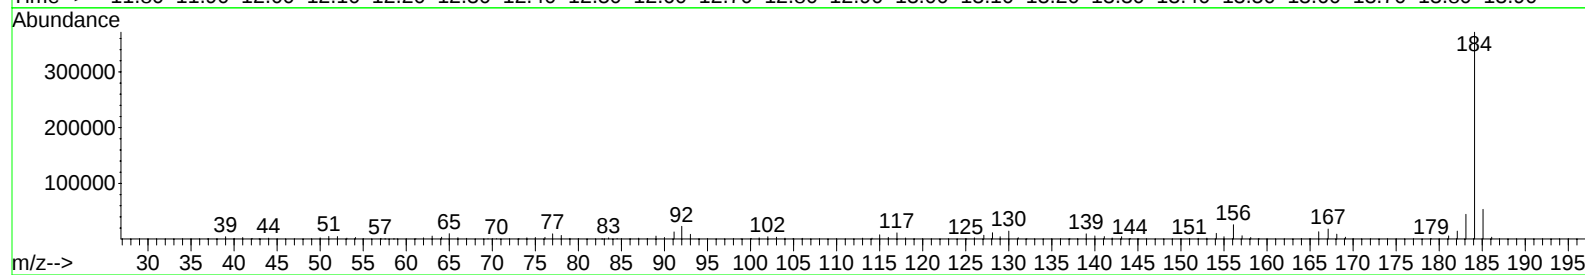



Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF110618\
 Data File : BF110503.D
 Acq On : 6 Nov 2018 9:46
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 06 13:44:25 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF102318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 01 16:06:12 2018
 Response via : Initial Calibration

Ion 184.00 (183.70 to 184.70): BF110503.D
 Ion 185.00 (184.70 to 185.70): BF110503.D
 Ion 183.00 (182.70 to 183.70): BF110503.D

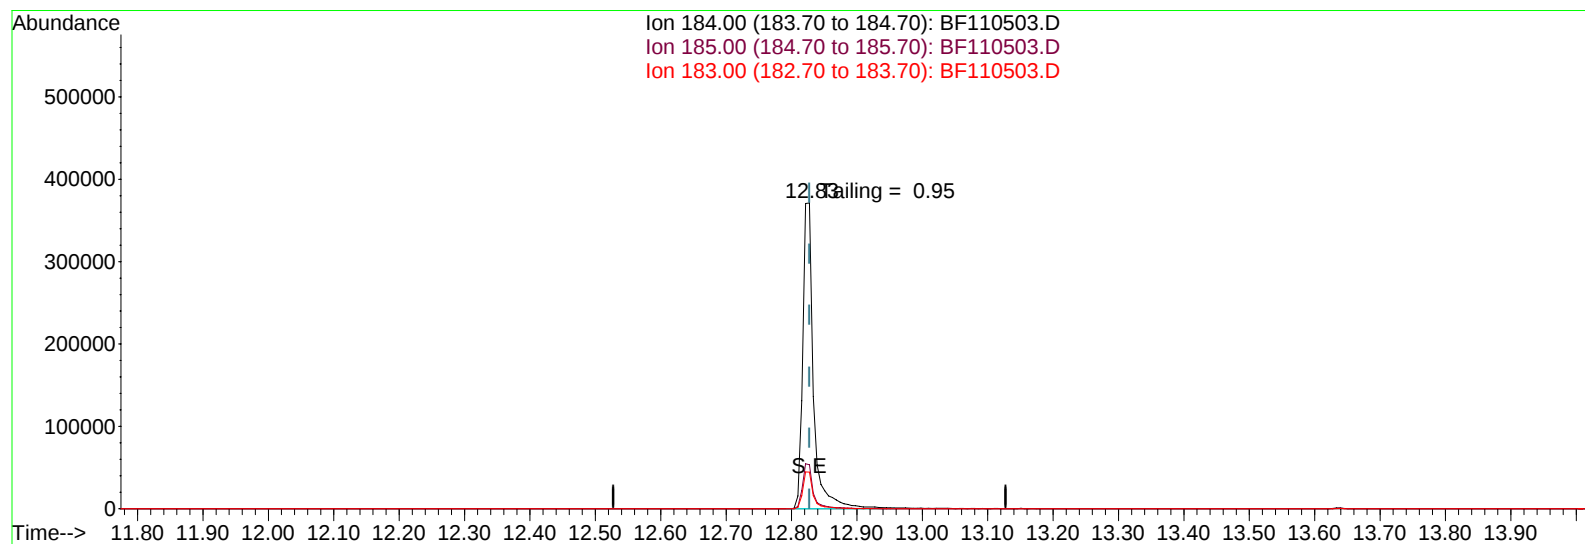

Scan 1828 (12.839 min): BF110074.D (-1822) (-)

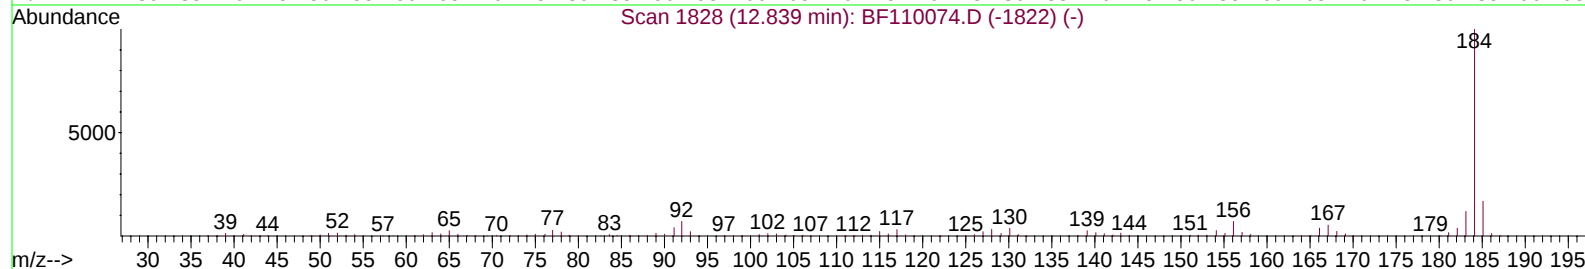

TIC: BF110503.D

(77) Benzidine




12.827min (+0.000) 0.00ng

response 431246

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	14.39
183.00	11.80	11.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF110618\
Data File : BF110503.D
Acq On : 6 Nov 2018 9:46
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 06 13:44:25 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF102318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 01 16:06:12 2018
Response via : Initial Calibration

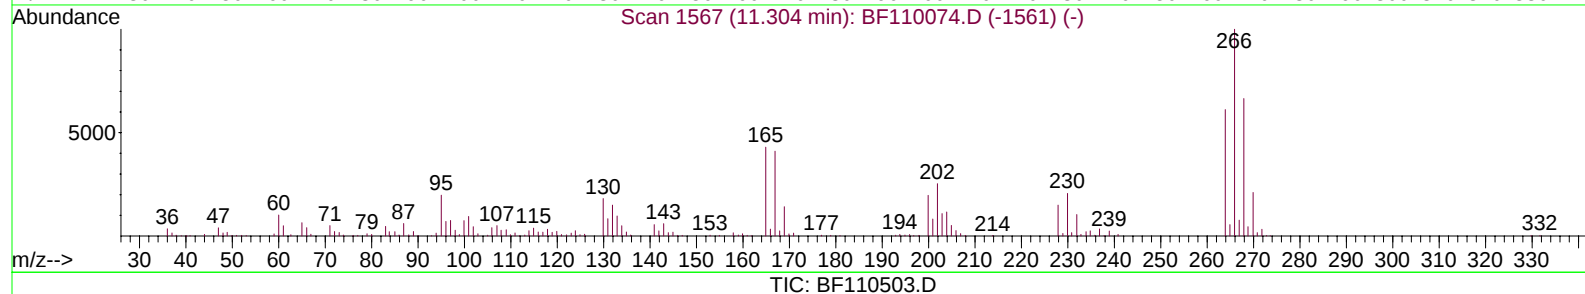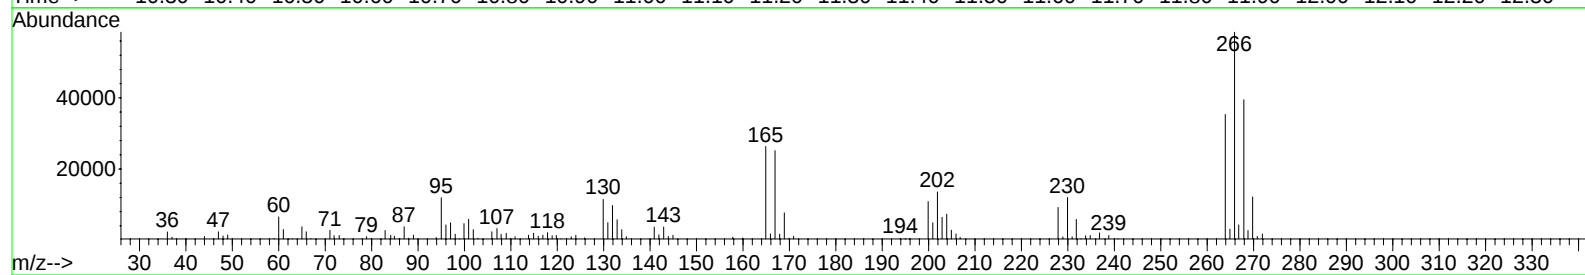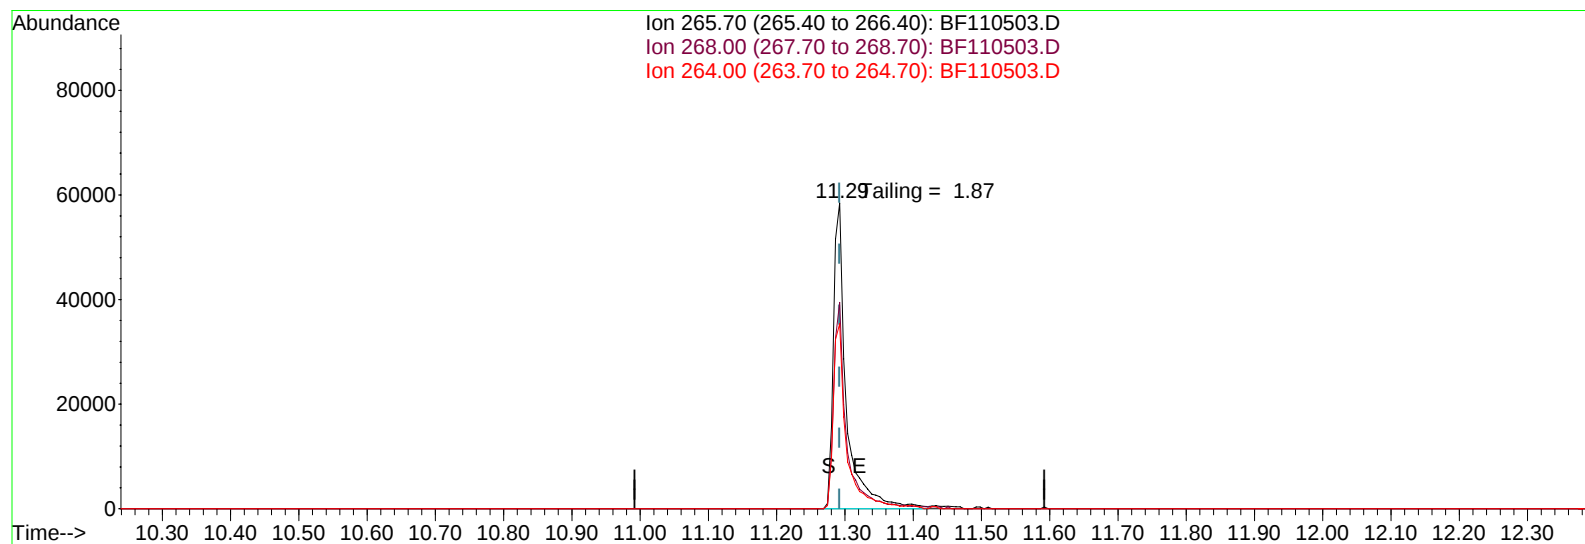

(70) Pentachlorophenol (C)

11.292min (+0.000) 69238.70ng

response 76205

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	67.49
264.00	63.20	60.47
0.00	0.00	0.00