
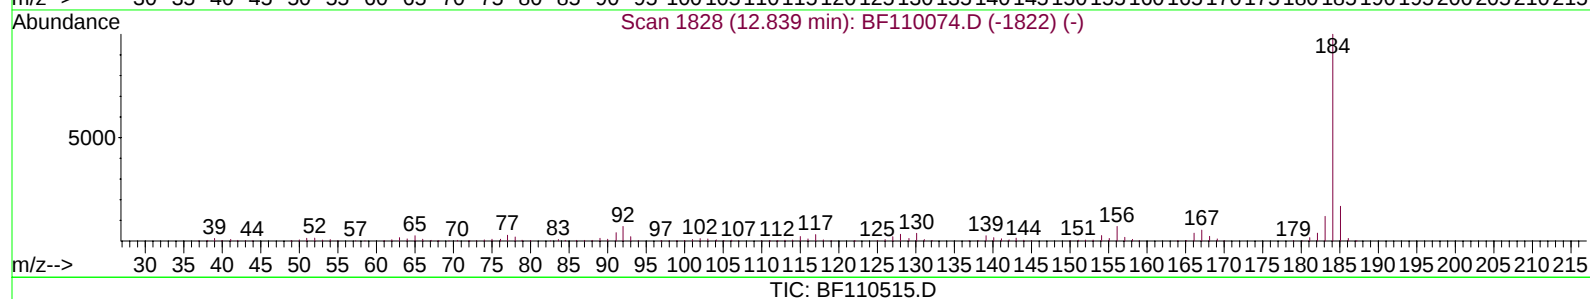
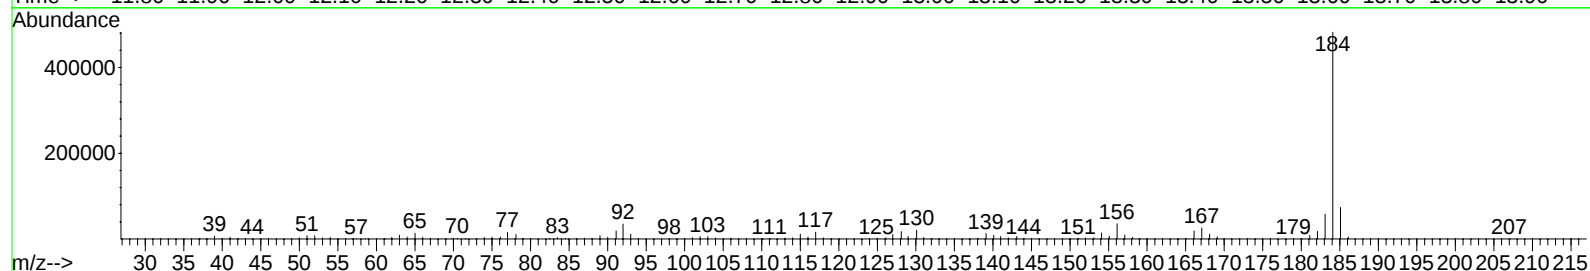


```
Data Path   : Z:\svoasrv\HPCHEM1\BNA F\Data\BF110618\  
Data File   : BF110515.D  
Acq On      : 6 Nov 2018 15:18  
Operator    : JU/SJ  
Sample      : DFTPP  
Misc        :  
ALS Vial    : 1      Sample Multiplier: 1
```

Quant Time: Nov 06 17:47:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF102318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 01 16:06:12 2018
Response via : Initial Calibration

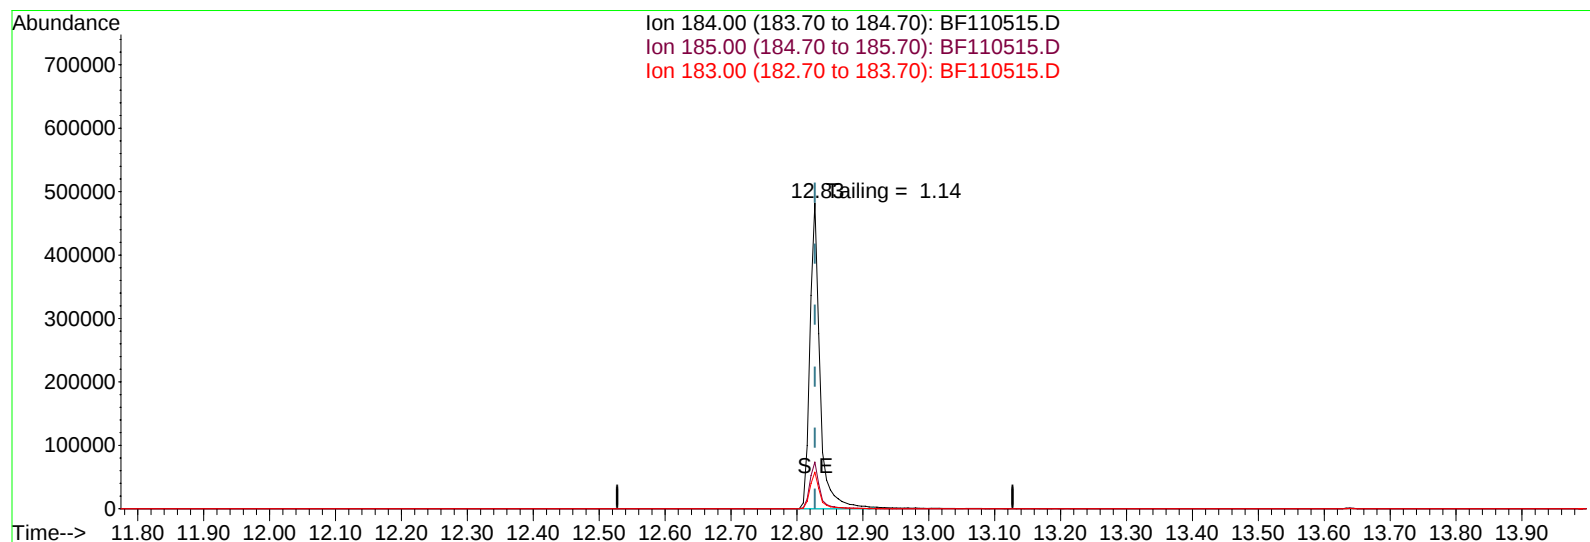

(77) Benzidine




12.827min (-0.000) 0.00ng

response 520193

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	15.30
183.00	11.80	11.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF110618\
Data File : BF110515.D
Acq On : 6 Nov 2018 15:18
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 06 17:47:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF102318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 01 16:06:12 2018
Response via : Initial Calibration

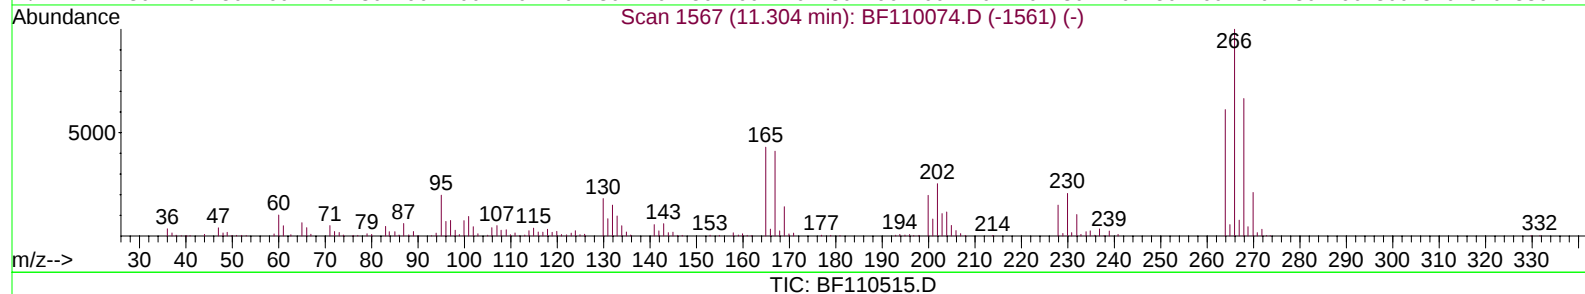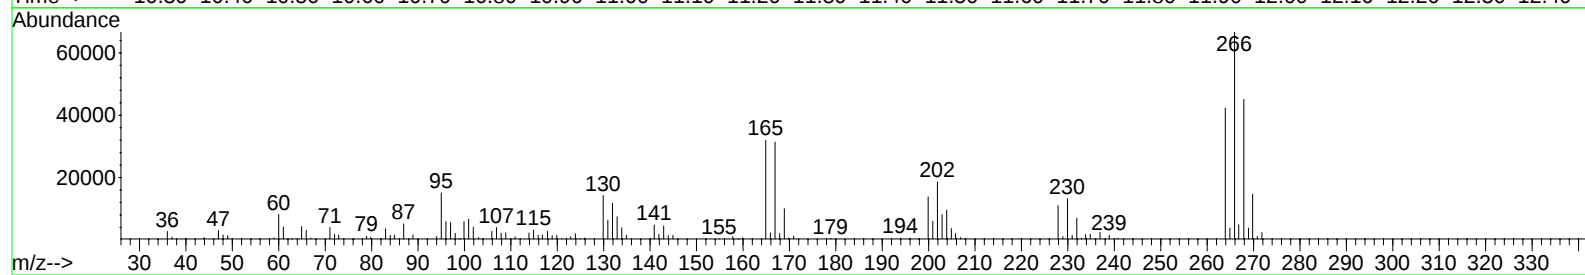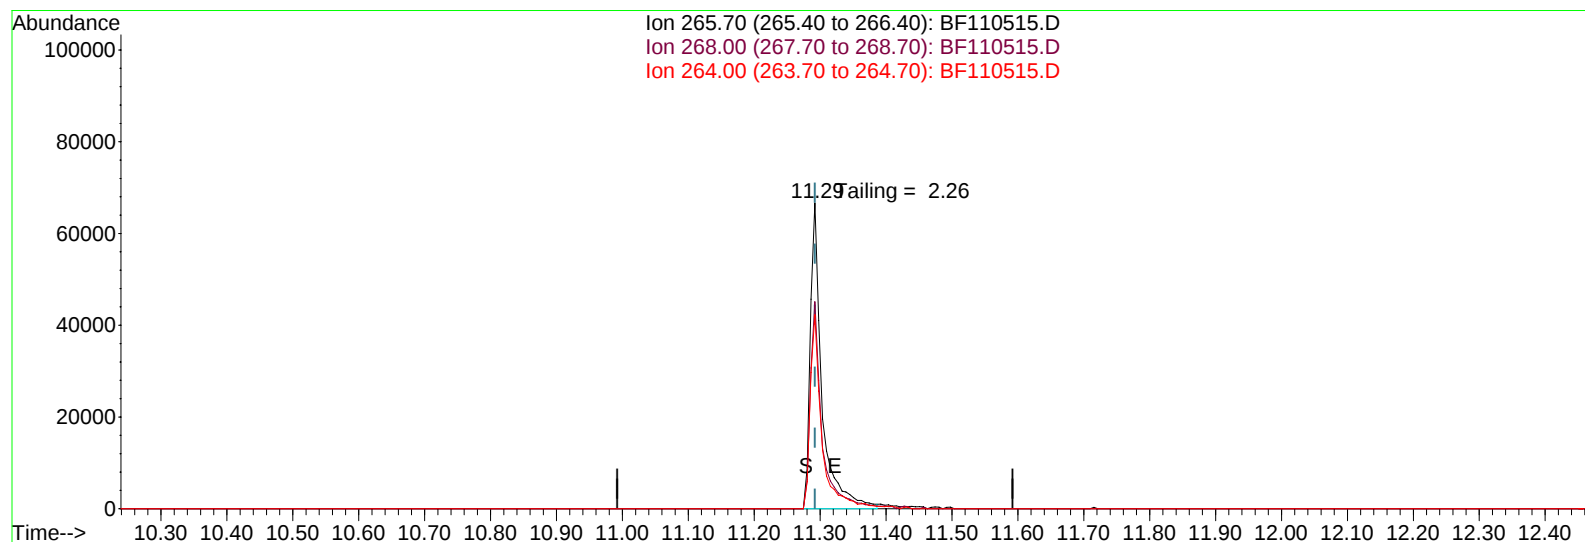

(70) Pentachlorophenol (C)

11.292min (-0.000) 36801.53ng

response 86195

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	67.73
264.00	63.20	63.50
0.00	0.00	0.00