
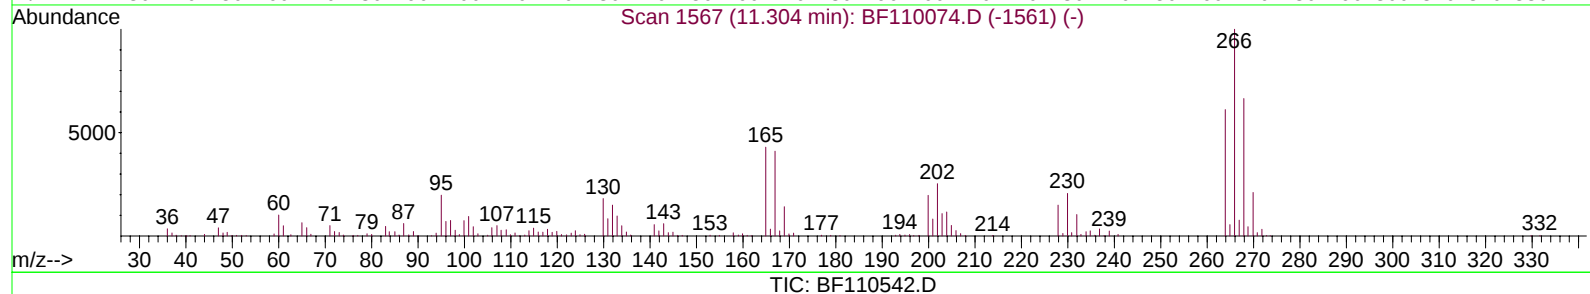
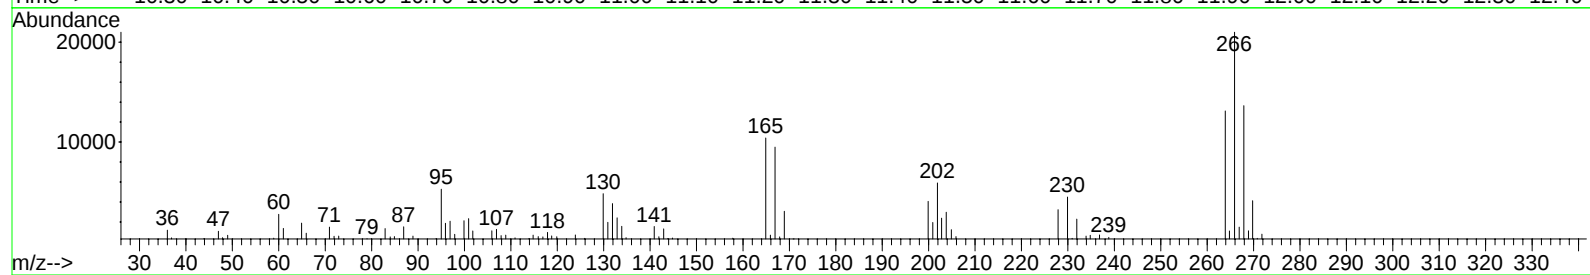


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF110618\
Data File : BF110542.D
Acq On : 7 Nov 2018 4:25
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 07 15:18:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF102318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 01 16:06:12 2018
Response via : Initial Calibration

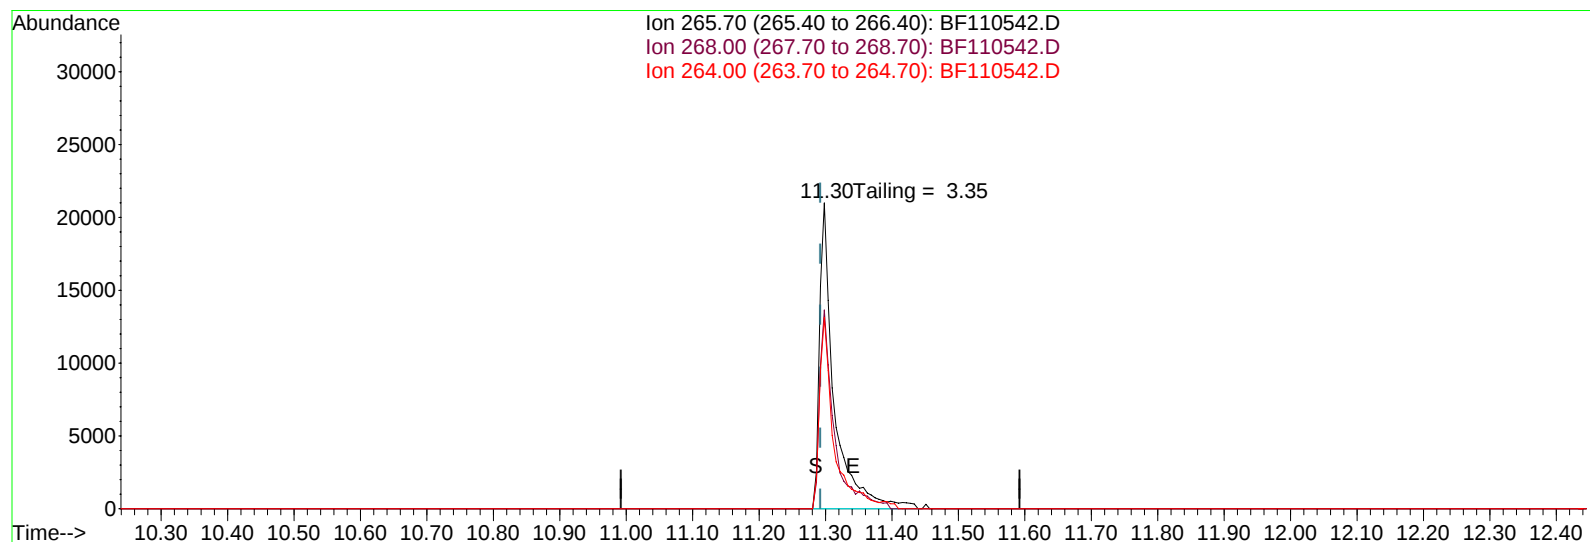

(70) Pentachlorophenol (C)




11.298min (+0.006) 0.00ng

response 32377

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	64.98
264.00	63.20	62.48
0.00	0.00	0.00

```
Data Path   : Z:\svoasrv\HPCHEM1\BNA F\Data\BF110618\  
Data File   : BF110542.D  
Acq On      : 7 Nov 2018    4:25  
Operator    : JU/SJ  
Sample      : DFTPP  
Misc        :  
ALS Vial    : 1      Sample Multiplier: 1
```

Quant Time: Nov 07 15:18:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF102318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 01 16:06:12 2018
Response via : Initial Calibration

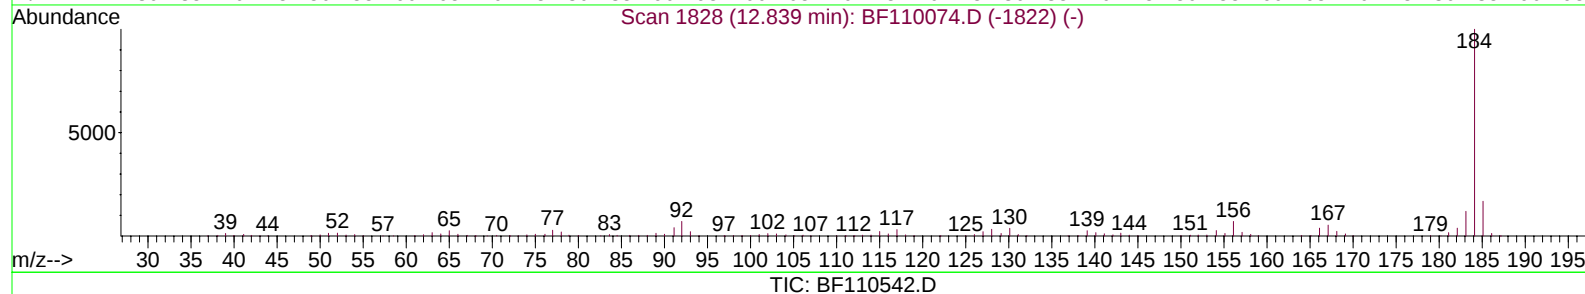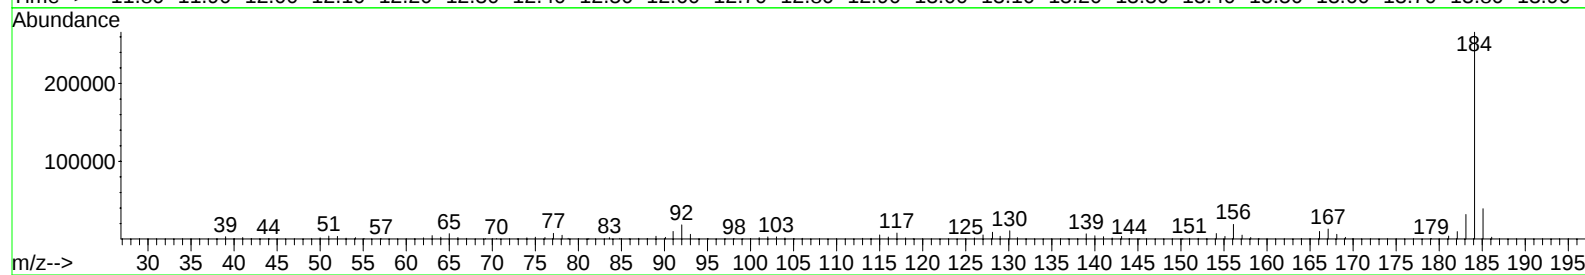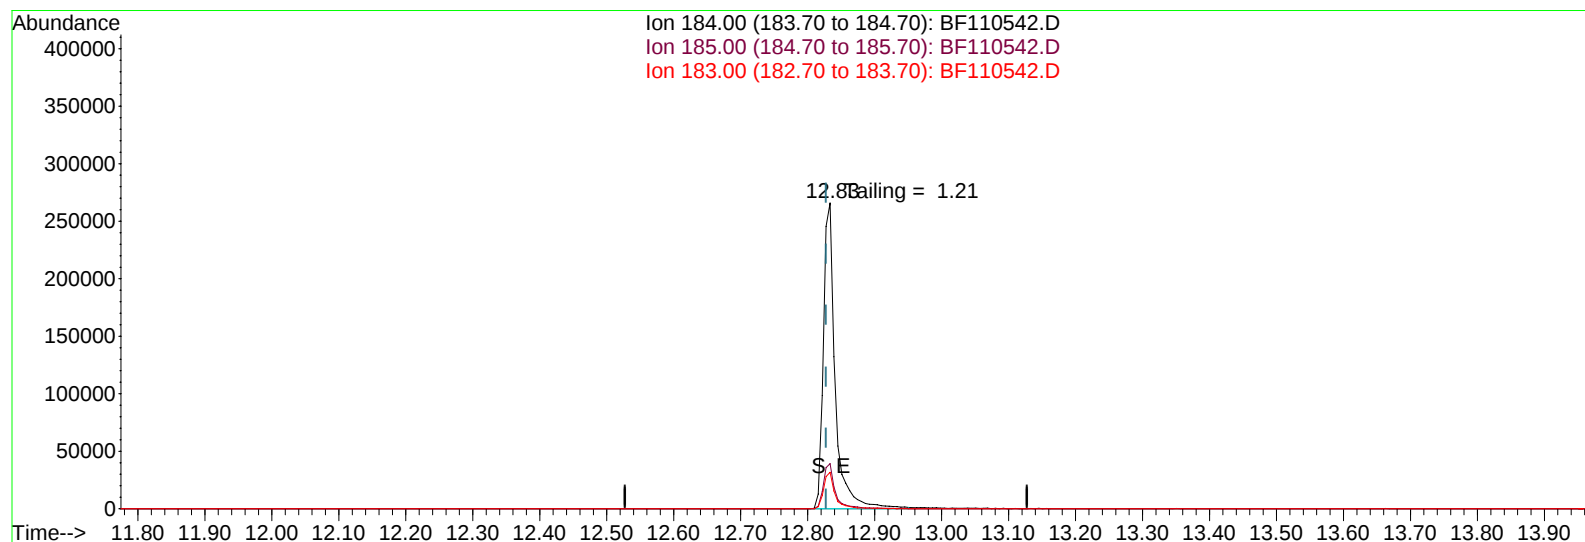

(77) Benzidine

12.833min (+0.006) 0.00ng

```
response 329880
```

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	14.74
183.00	11.80	11.94
0.00	0.00	0.00