


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110618\
 Data File : BF110542.D
 Acq On : 7 Nov 2018 4:25
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF102318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Nov 01 16:06:12 2018

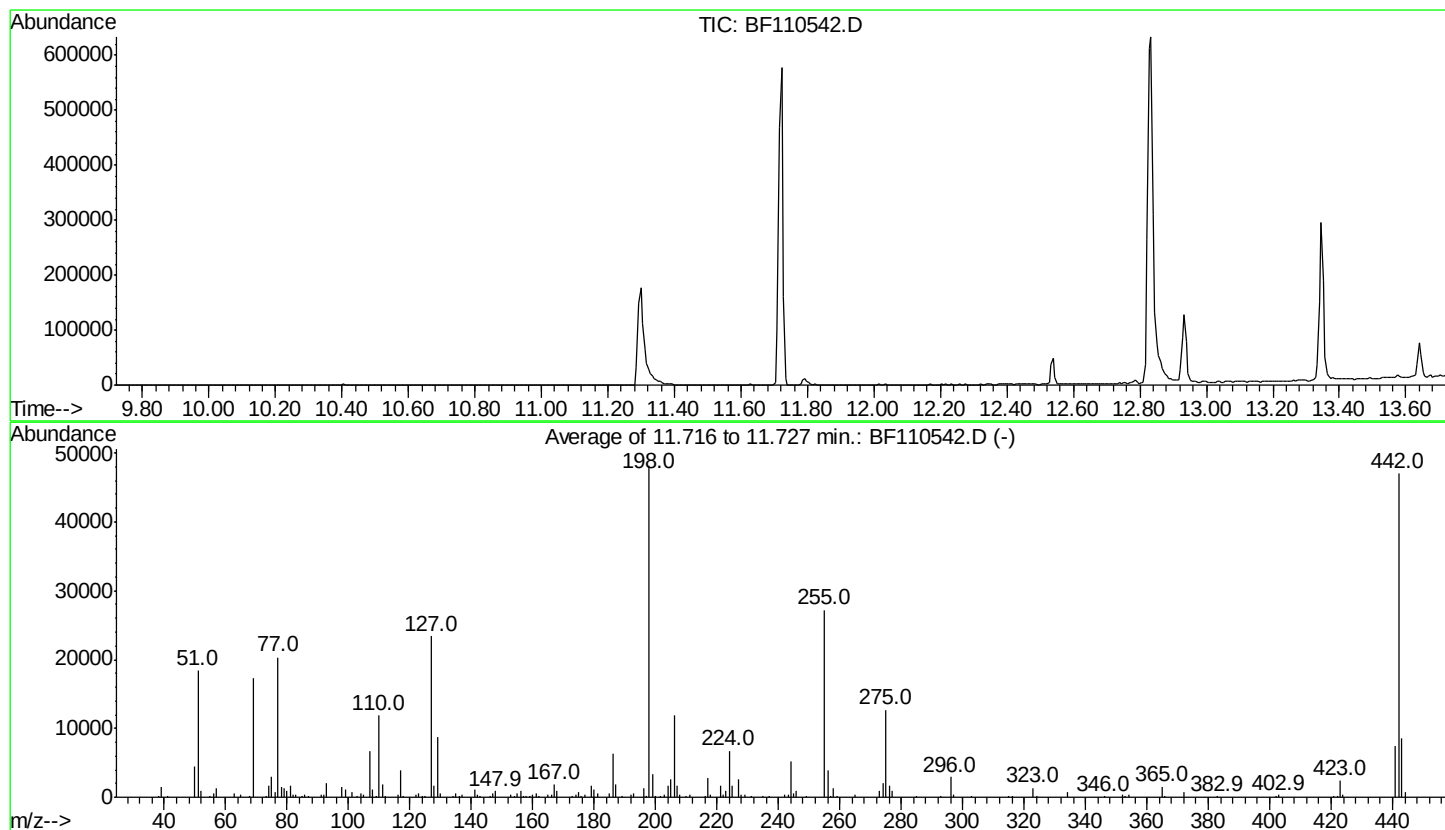

AutoFind: Scans 1637, 1638, 1639; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.2	18393	PASS
68	69	0.00	2	1.5	254	PASS
69	198	0.00	100	35.8	17245	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.5	23356	PASS
197	198	0.00	2	0.4	207	PASS
198	198	100	100	100.0	48181	PASS
199	198	5	9	6.9	3320	PASS
275	198	10	60	26.3	12673	PASS
365	198	1	100	3.2	1540	PASS
441	198	0.01	100	15.3	7364	PASS
442	198	50	100	97.8	47109	PASS
443	442	15	24	18.3	8625	PASS