


Data Path : Z:\SVOASRV\HPCHEM1\BNA\_F\DATA\BF110619\  
 Data File : BF117694.D  
 Acq On : 6 Nov 2019 12:08  
 Operator : JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF110619.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed Nov 06 17:27:10 2019

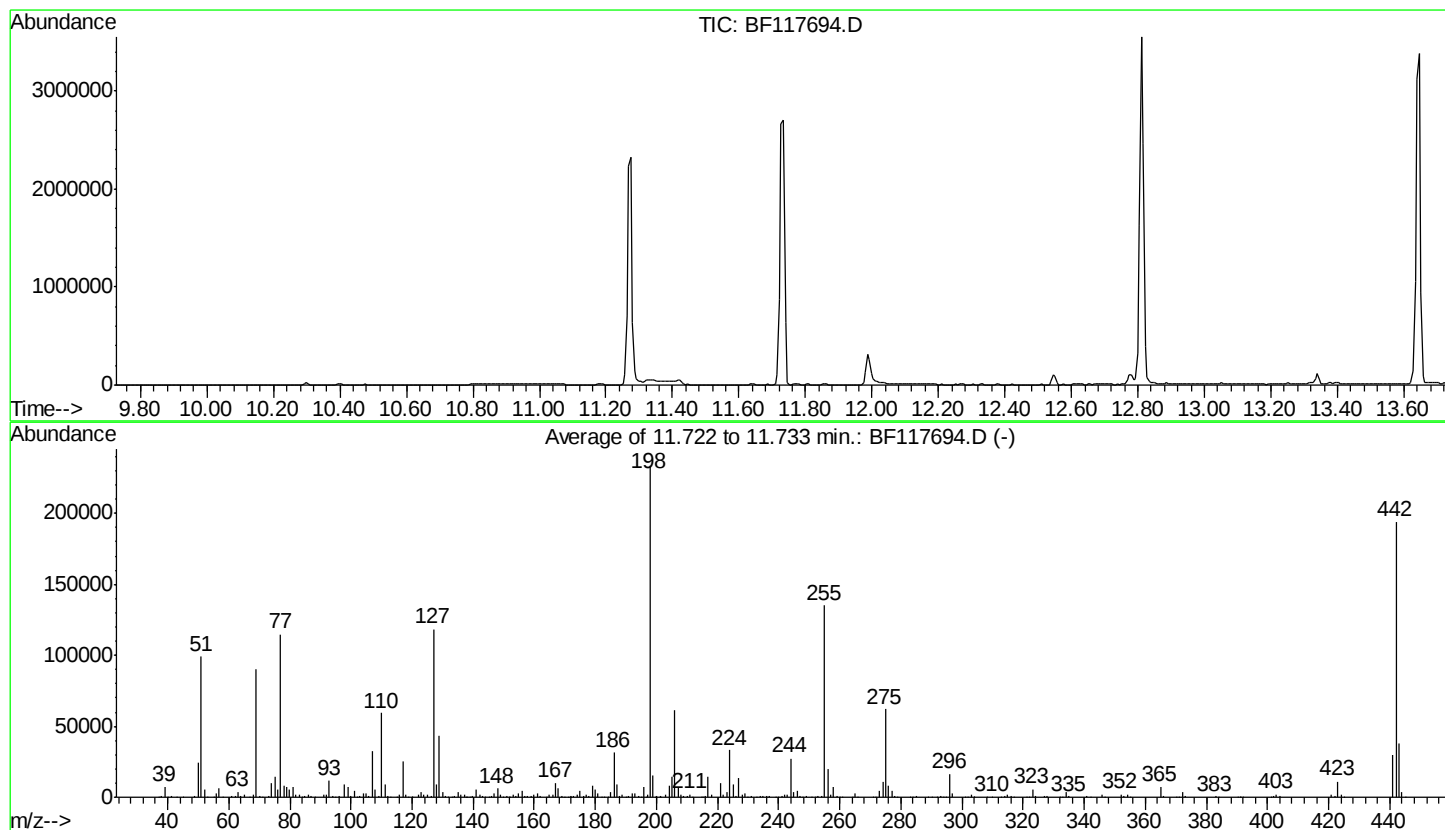

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 42.3         | 98816      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.9          | 1669       | PASS                |
| 69             | 198             | 0.00            | 100             | 38.6         | 90205      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.6          | 529        | PASS                |
| 127            | 198             | 10              | 80              | 50.7         | 118469     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.6          | 1466       | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 233642     | PASS                |
| 199            | 198             | 5               | 9               | 6.7          | 15684      | PASS                |
| 275            | 198             | 10              | 60              | 26.5         | 61890      | PASS                |
| 365            | 198             | 1               | 100             | 3.2          | 7447       | PASS                |
| 441            | 198             | 0.01            | 100             | 12.8         | 30015      | PASS                |
| 442            | 198             | 50              | 100             | 83.2         | 194373     | PASS                |
| 443            | 442             | 15              | 24              | 19.7         | 38240      | PASS                |