
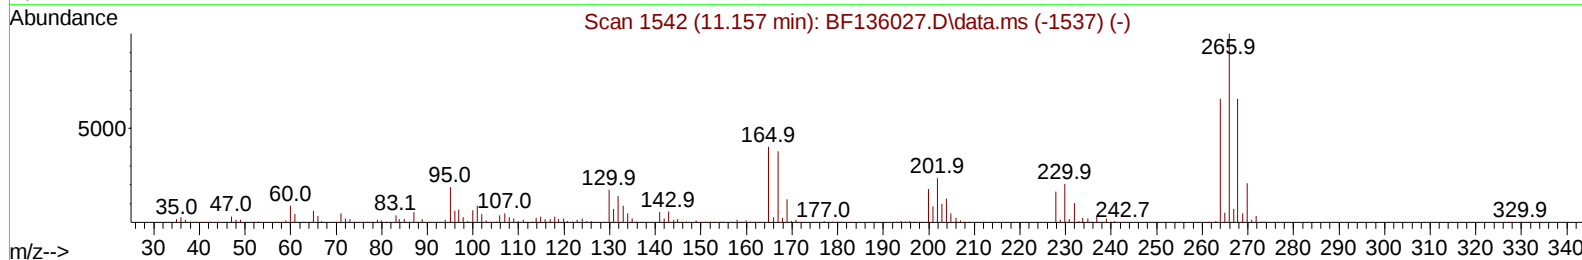
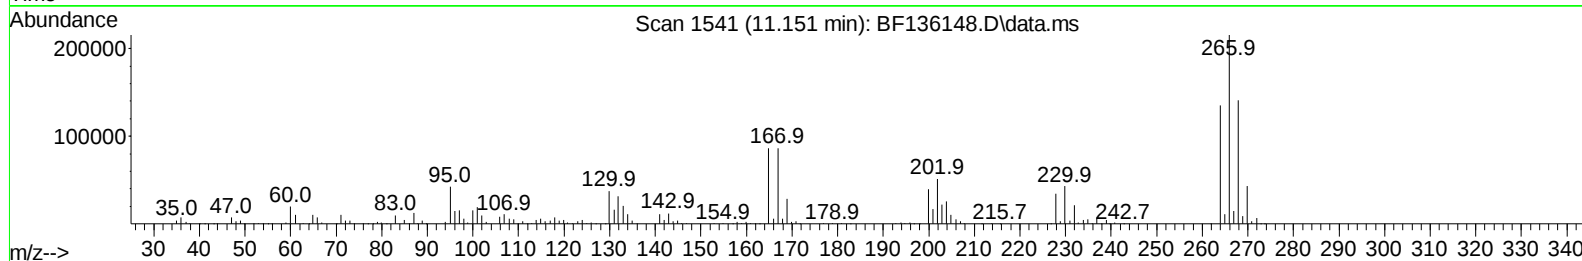


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110623\
Data File : BF136148.D
Acq On : 06 Nov 2023 11:31
Operator : CG\JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 06 18:57:33 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 06 00:53:35 2023
Response via : Initial Calibration

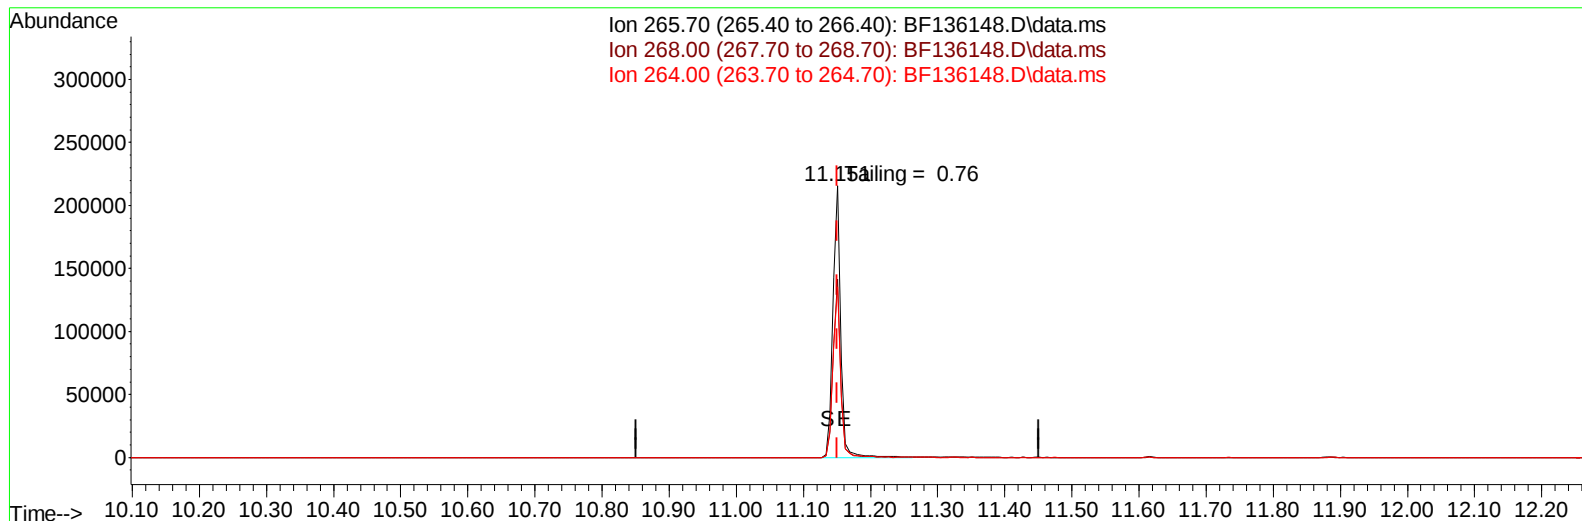

TIC: BF136148.D\data.ms

(70) Pentachlorophenol (C)




11.151min (+ 0.000) 82371.86 ng

response 177706

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	65.58
264.00	65.30	62.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110623\
Data File : BF136148.D
Acq On : 06 Nov 2023 11:31
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 06 18:57:33 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 06 00:53:35 2023
Response via : Initial Calibration

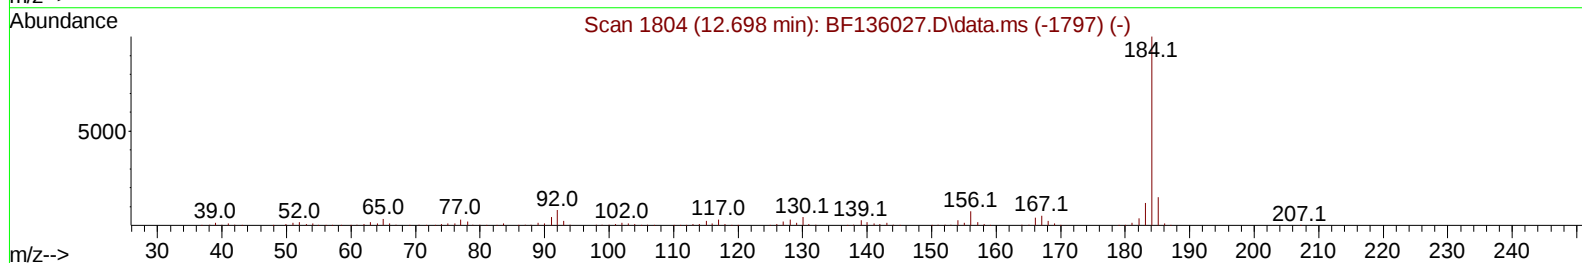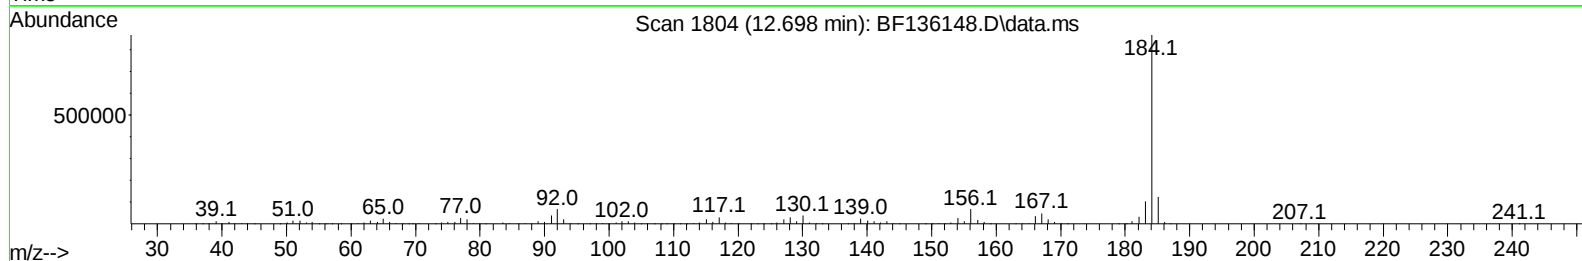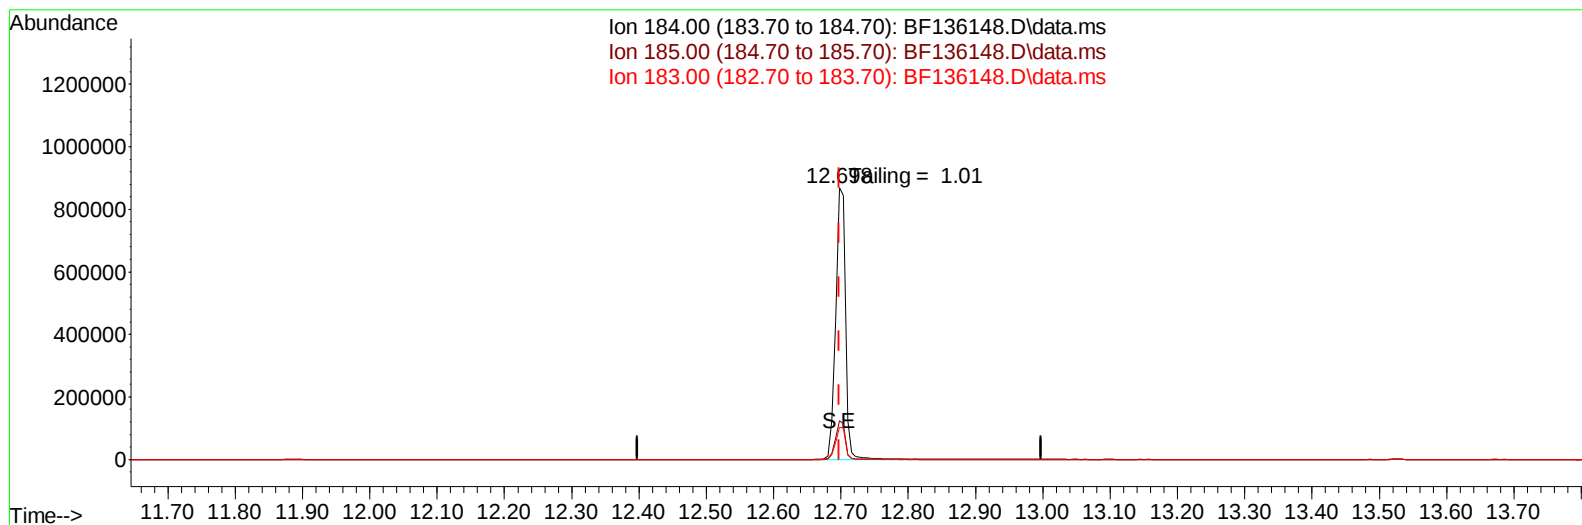

TIC: BF136148.D\data.ms

(77) Benzidine**12.698min (+ 0.000) 636124.38 ng****response 880300**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.28
183.00	11.90	11.92
0.00	0.00	0.00