


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110623\
Data File : BF136148.D
Acq On : 06 Nov 2023 11:31
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Nov 06 00:53:35 2023

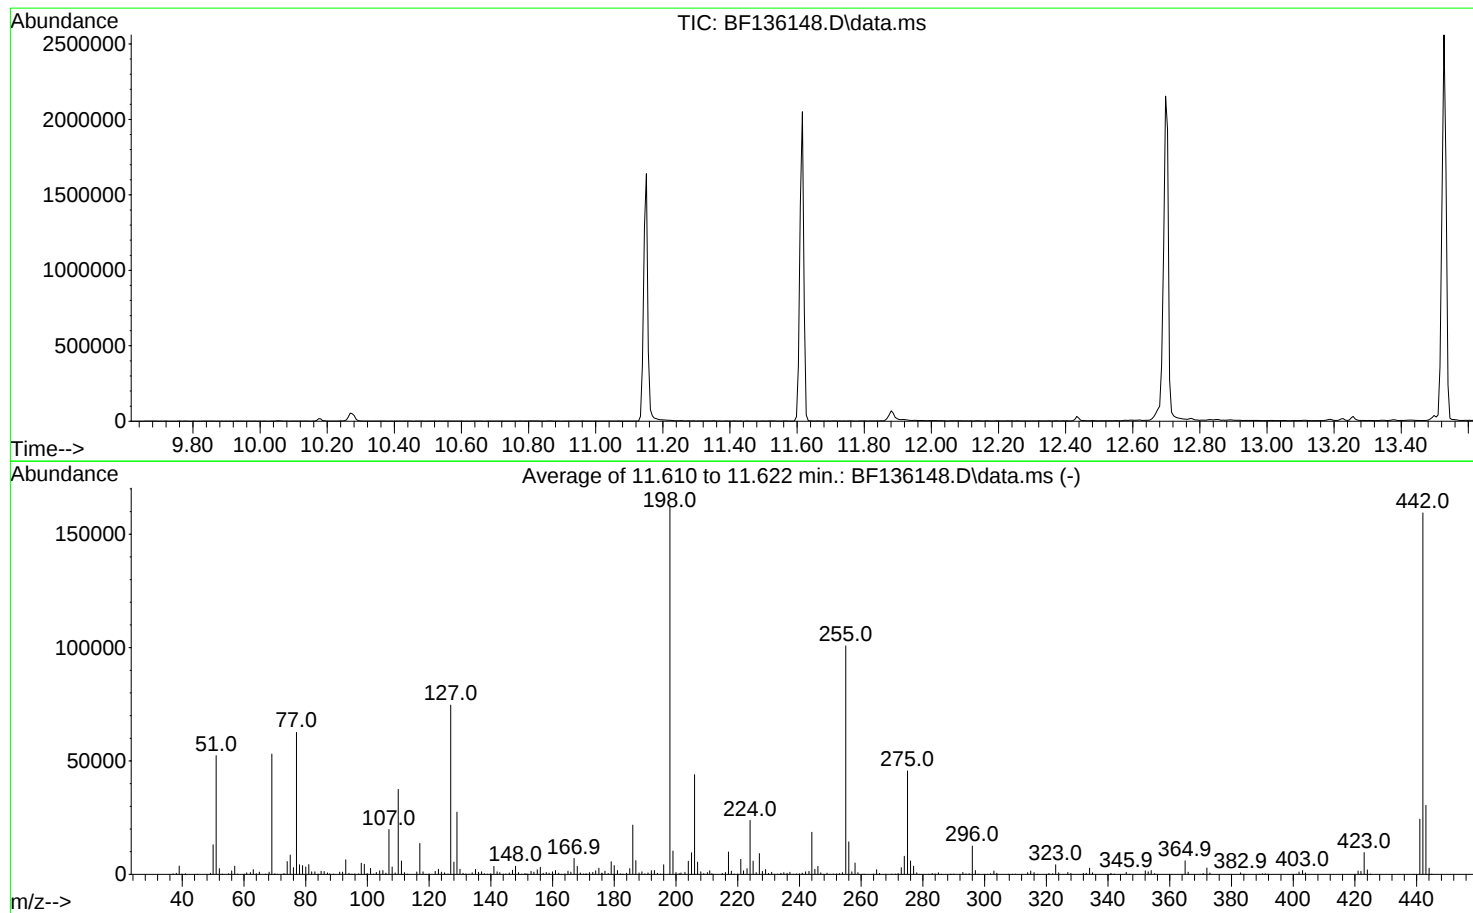




AutoFind: Scans 1619, 1620, 1621; Background Corrected with Scan 1614

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.3	52372	PASS
68	69	0.00	2	1.8	969	PASS
69	198	0.00	100	32.7	53045	PASS
70	69	0.00	2	0.5	274	PASS
127	198	10	80	46.0	74651	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	162232	PASS
199	198	5	9	6.3	10281	PASS
275	198	10	60	28.1	45568	PASS
365	198	1	100	3.7	6022	PASS
441	198	0.01	100	15.0	24356	PASS
442	442	50	100	100.0	159424	PASS
443	442	15	24	19.1	30397	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110623\
Data File : BF136148.D
Acq On : 06 Nov 2023 11:31
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 06 18:57:33 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 06 00:53:35 2023
Response via : Initial Calibration

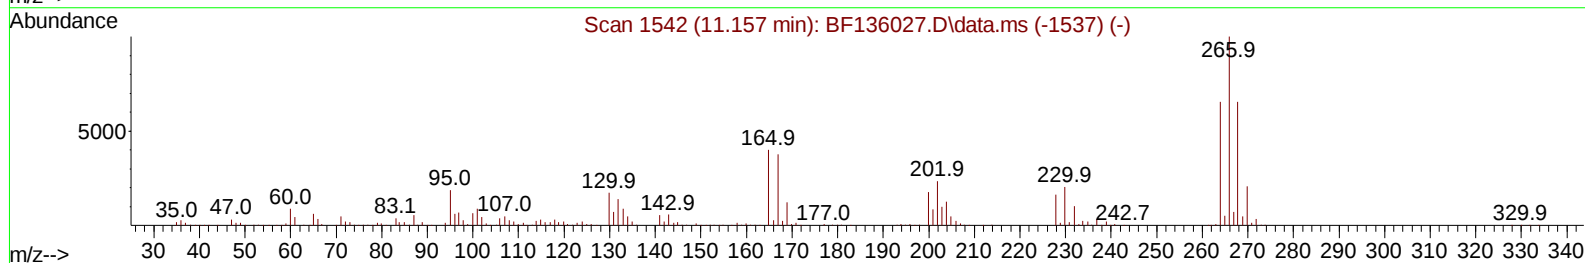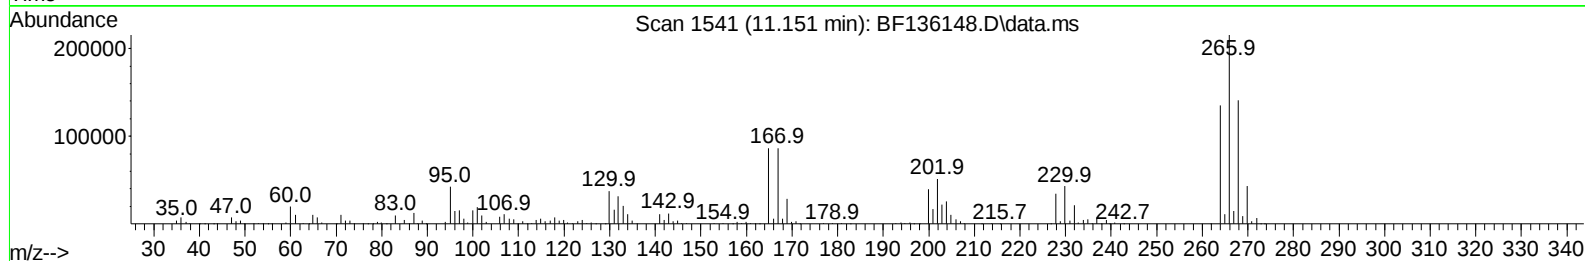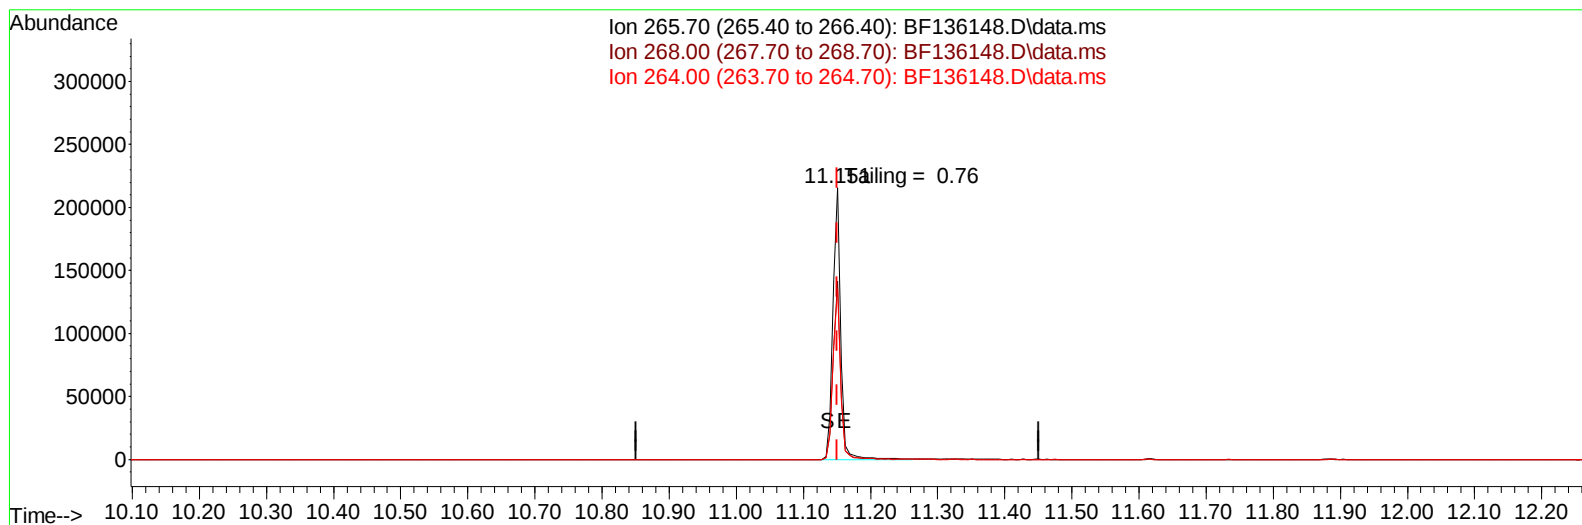

TIC: BF136148.D\data.ms

(70) Pentachlorophenol (C)

11.151min (+ 0.000) 82371.86 ng




response 177706

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	65.58
264.00	65.30	62.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110623\
 Data File : BF136148.D
 Acq On : 06 Nov 2023 11:31
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Nov 06 18:57:33 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 06 00:53:35 2023
 Response via : Initial Calibration

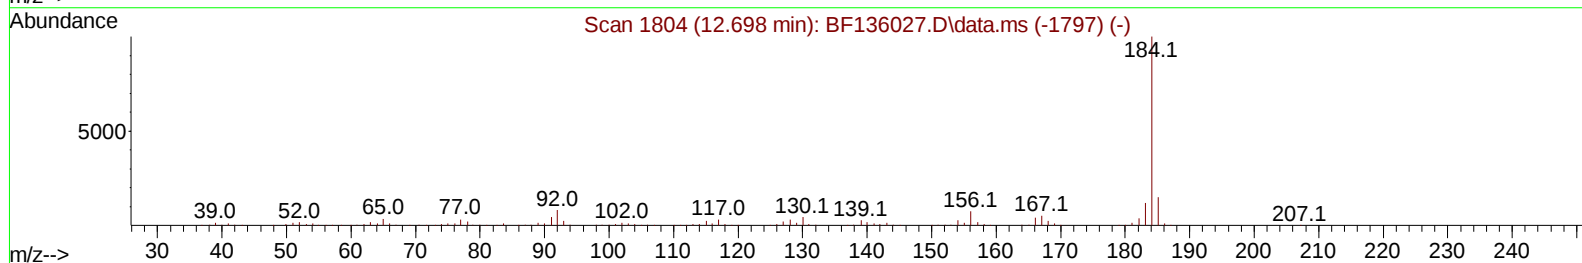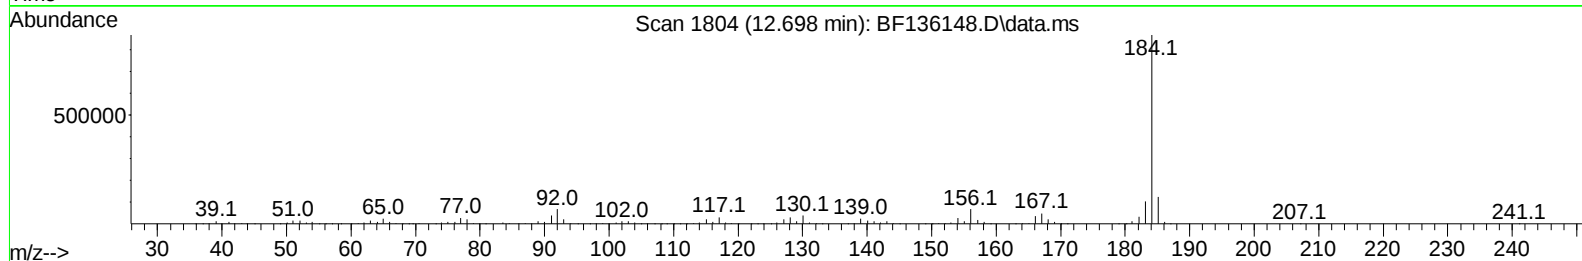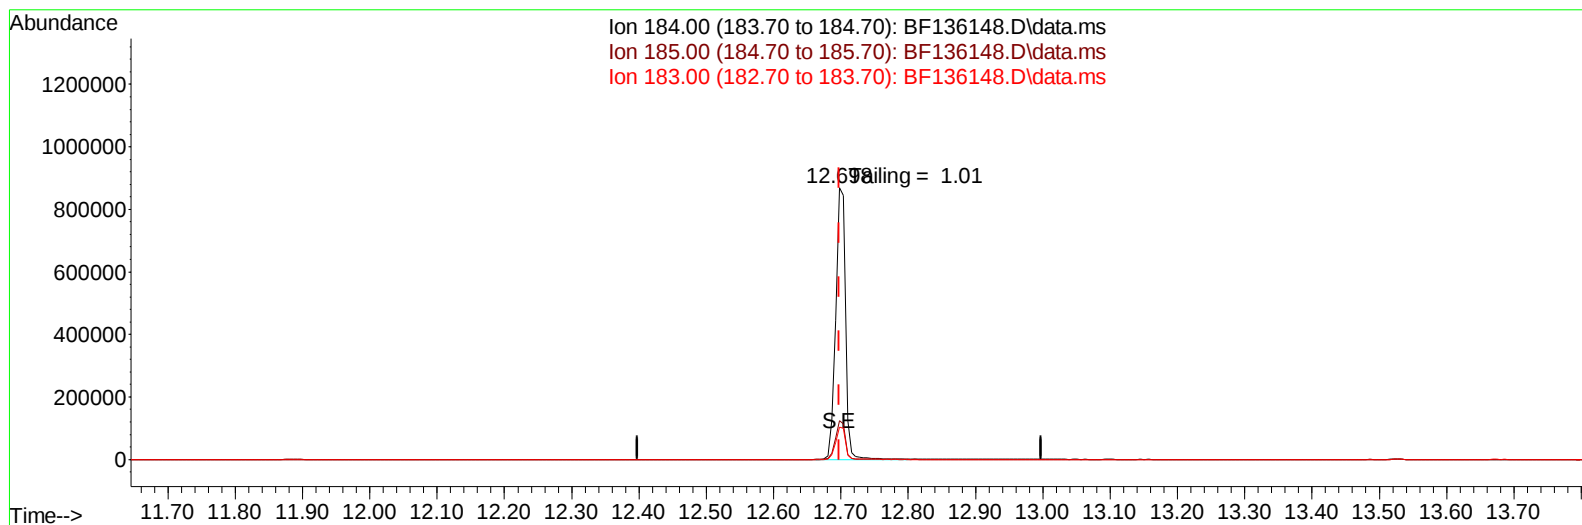

TIC: BF136148.D\data.ms

(77) Benzidine**12.698min (+ 0.000) 636124.38 ng****response 880300**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.28
183.00	11.90	11.92
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/6/2023	BNA_F	<u>BF136148.D</u>
Compound Name	Response	Retention Time
DDT	452190	13.527
DDD	6741	13.257
DDE	468	12.886
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7209	459399	1.57

Instrument :
BNA_F
ClientSampleId :
DFTPP