

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110625\
 Data File : BF144181.D
 Acq On : 06 Nov 2025 11:42
 Operator : RC/JU
 Sample : PB170402BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB170402BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF144181.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.116	492	497	504	rBV	19543	30873	1.10%	0.185%
2	5.498	556	562	582	rBV	1559622	2118469	75.76%	12.678%
3	6.504	726	733	752	rBV	1469383	2131822	76.24%	12.758%
4	6.875	791	796	808	rBV	341156	444288	15.89%	2.659%
5	7.434	885	891	908	rBV	1024776	1387675	49.63%	8.305%
6	8.151	1008	1013	1027	rBV	426500	581628	20.80%	3.481%
7	9.233	1190	1197	1216	rBV	1952011	2696021	96.42%	16.134%
8	9.910	1307	1312	1324	rVB	543354	700089	25.04%	4.190%
9	10.704	1441	1447	1467	rBV	1375550	1829206	65.42%	10.947%
10	11.404	1561	1566	1582	rBV	569935	737568	26.38%	4.414%
11	12.992	1830	1836	1842	rBV	2049143	2796212	100.00%	16.734%
12	14.051	2011	2016	2027	rVB	396835	537537	19.22%	3.217%
13	15.539	2262	2269	2279	rBV	328872	559983	20.03%	3.351%
14	17.233	2546	2557	2573	rVB6	33902	158318	5.66%	0.947%




Sum of corrected areas: 16709689

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110625\
Data File : BF144181.D
Acq On : 06 Nov 2025 11:42
Operator : RC/JU
Sample : PB170402BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB170402BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

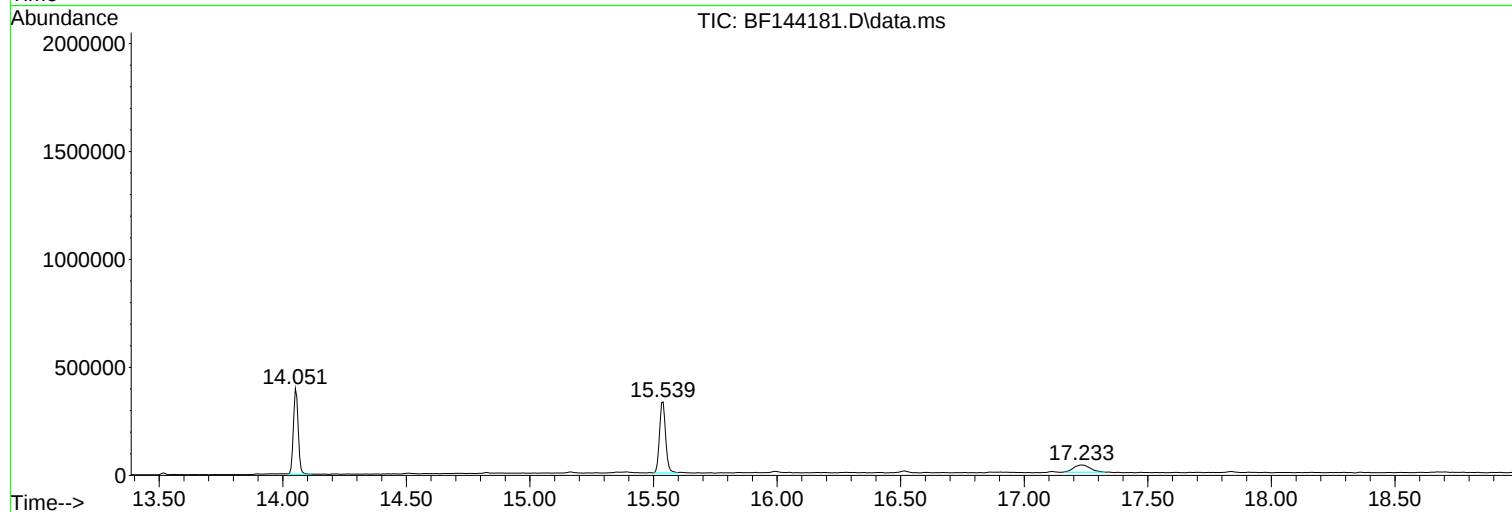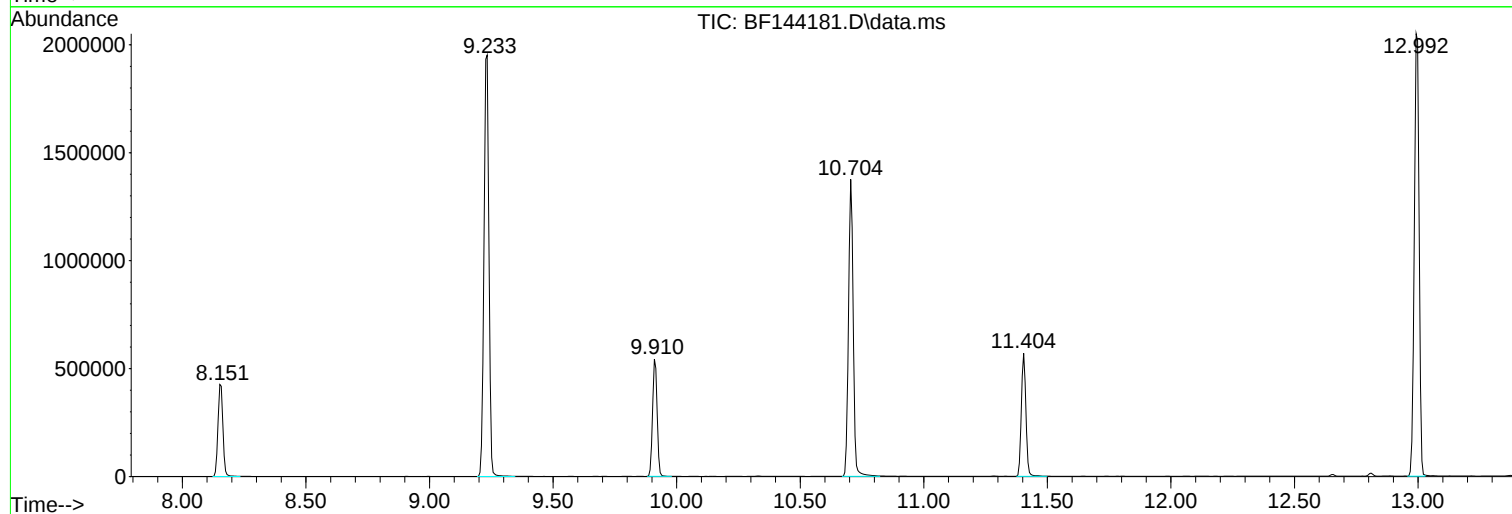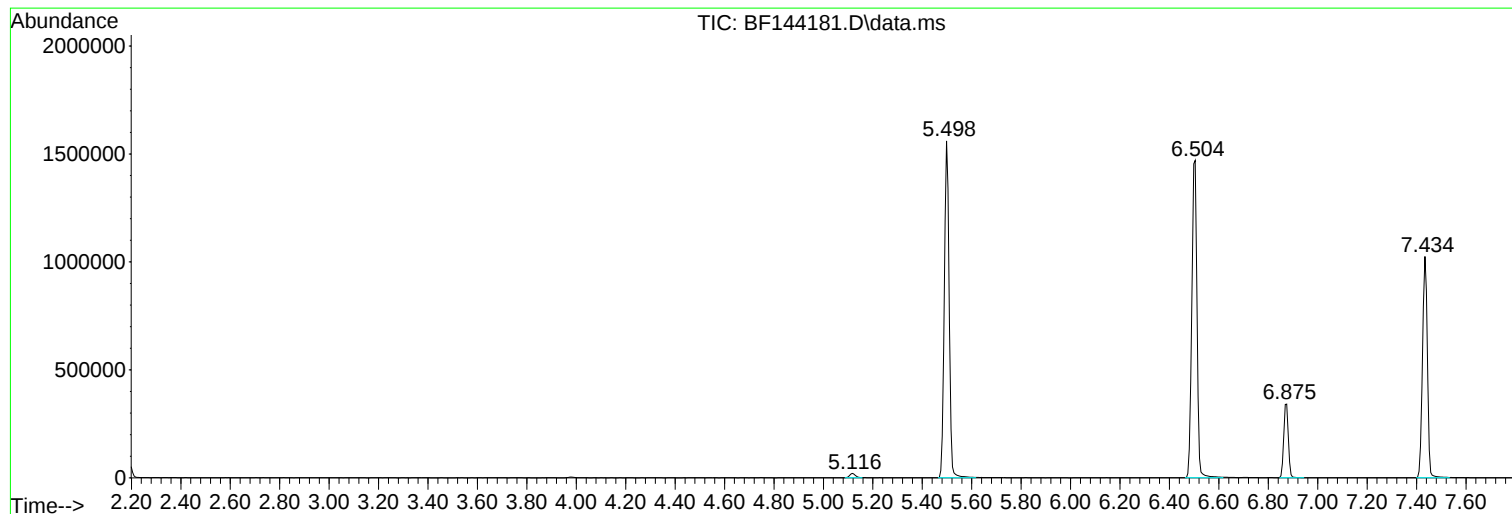

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110625\
Data File : BF144181.D
Acq On : 06 Nov 2025 11:42
Operator : RC/JU
Sample : PB170402BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB170402BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110625\
Data File : BF144181.D
Acq On : 06 Nov 2025 11:42
Operator : RC/JU
Sample : PB170402BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB170402BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------