


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110718\
 Data File : BF110556.D
 Acq On : 7 Nov 2018 14:40
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF102318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Nov 01 16:06:12 2018

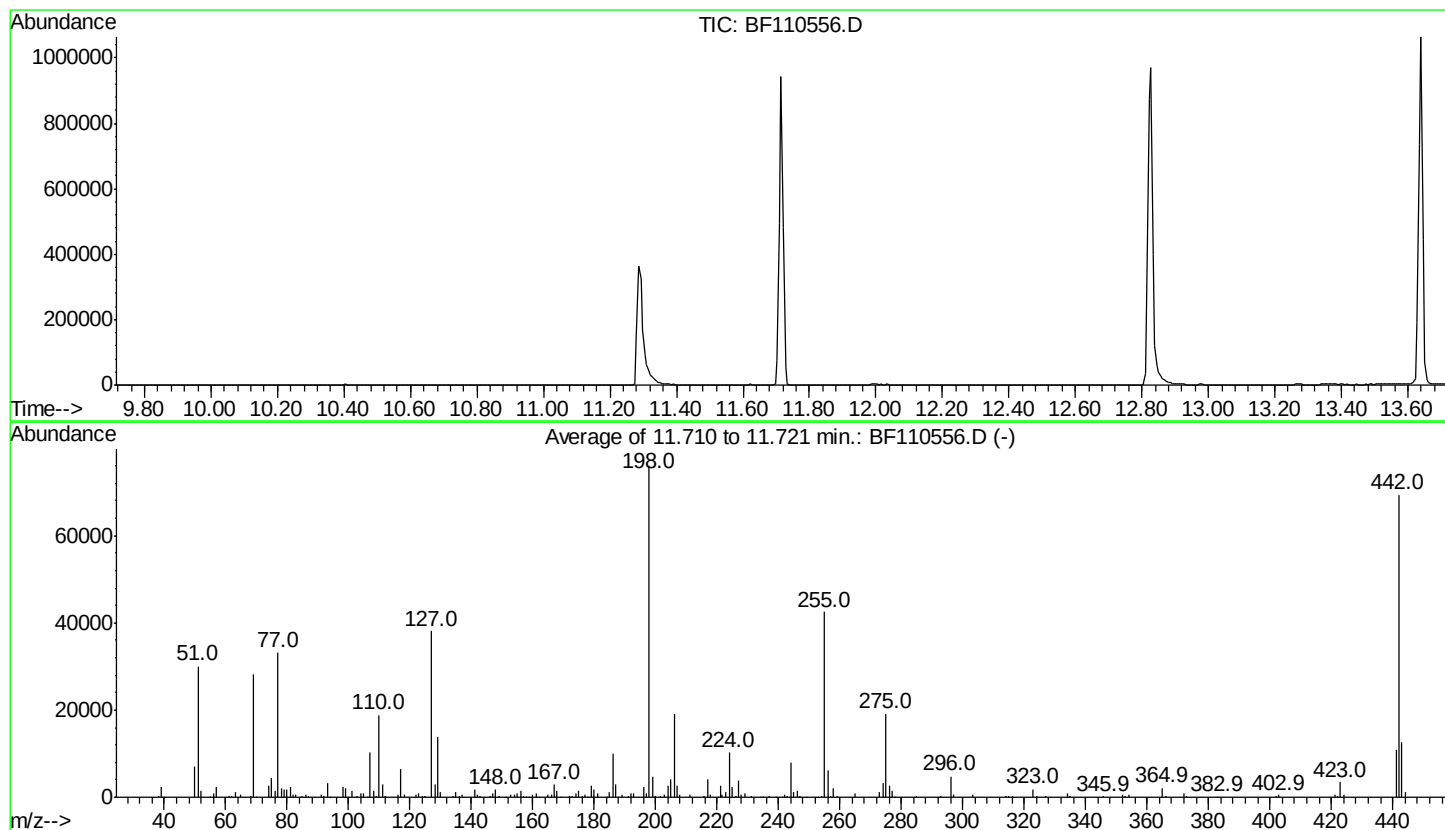

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.5	30063	PASS
68	69	0.00	2	1.4	398	PASS
69	198	0.00	100	37.2	28271	PASS
70	69	0.00	2	0.4	102	PASS
127	198	10	80	50.1	38074	PASS
197	198	0.00	2	1.0	744	PASS
198	198	100	100	100.0	76069	PASS
199	198	5	9	6.3	4811	PASS
275	198	10	60	25.2	19137	PASS
365	198	1	100	2.7	2071	PASS
441	198	0.01	100	14.4	10936	PASS
442	198	50	100	91.1	69328	PASS
443	442	15	24	18.3	12686	PASS