


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110719\
 Data File : BF117704.D
 Acq On : 7 Nov 2019 14:30
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 06 17:27:10 2019

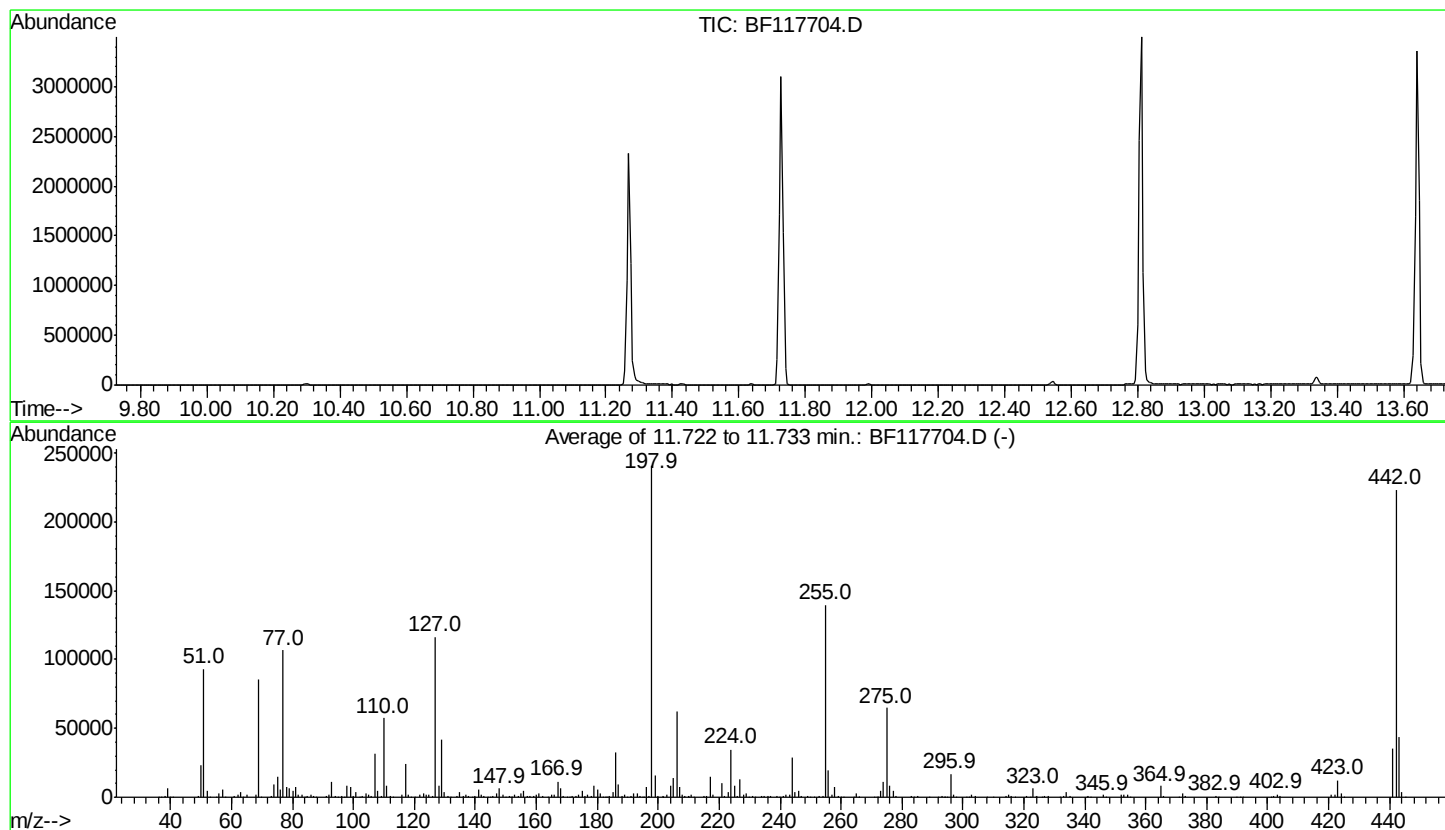

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.7	93221	PASS
68	69	0.00	2	1.8	1547	PASS
69	198	0.00	100	35.5	85600	PASS
70	69	0.00	2	0.4	379	PASS
127	198	10	80	48.4	116653	PASS
197	198	0.00	2	0.5	1153	PASS
198	198	100	100	100.0	240810	PASS
199	198	5	9	6.5	15596	PASS
275	198	10	60	26.9	64816	PASS
365	198	1	100	3.4	8090	PASS
441	198	0.01	100	14.7	35498	PASS
442	198	50	100	92.7	223138	PASS
443	442	15	24	19.5	43461	PASS