
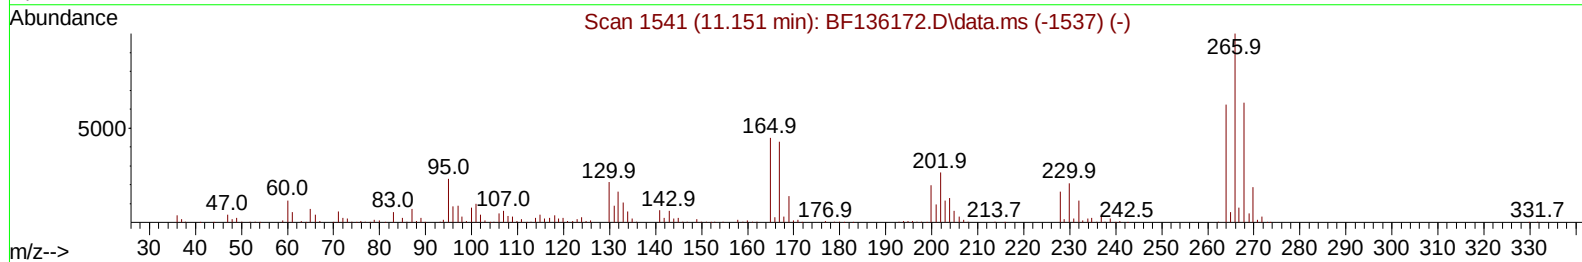
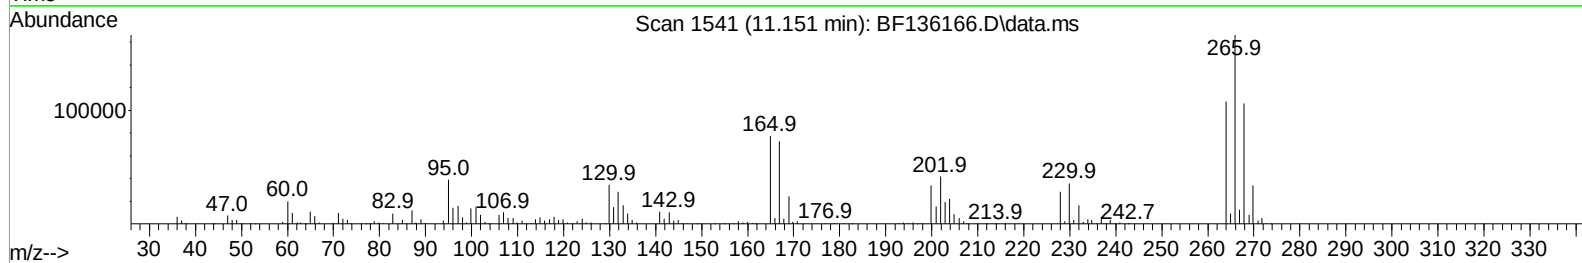


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110723\
Data File : BF136166.D
Acq On : 07 Nov 2023 09:28
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 08 03:03:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 08 02:12:01 2023
Response via : Initial Calibration

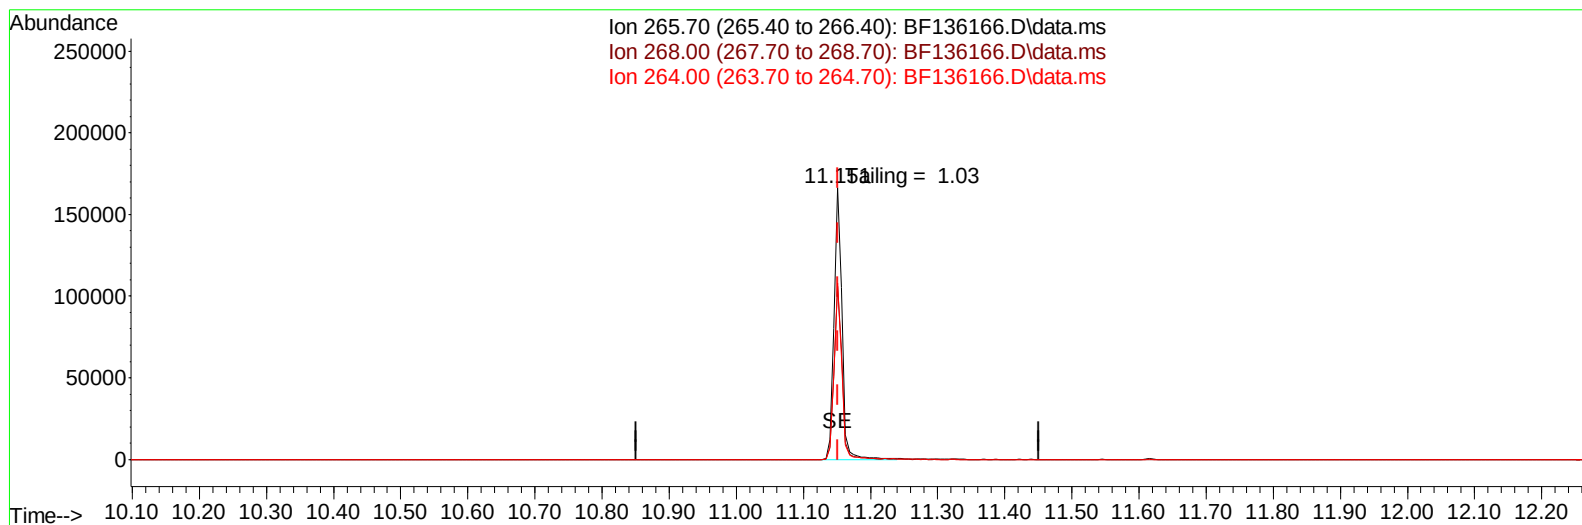

TIC: BF136166.D\data.ms

(70) Pentachlorophenol (C)




11.151min (-0.000) 80784.28 ng

response 141039

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.50	63.86
264.00	62.50	64.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110723\
Data File : BF136166.D
Acq On : 07 Nov 2023 09:28
Operator : CG\JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 08 03:03:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 08 02:12:01 2023
Response via : Initial Calibration

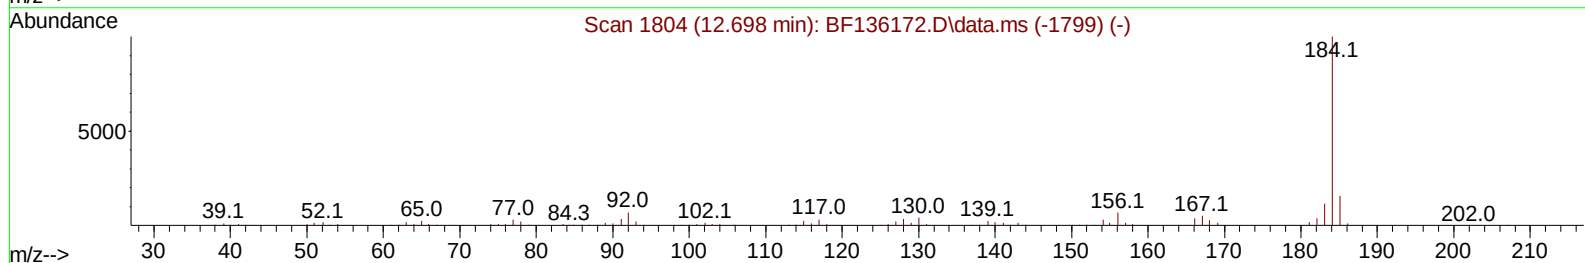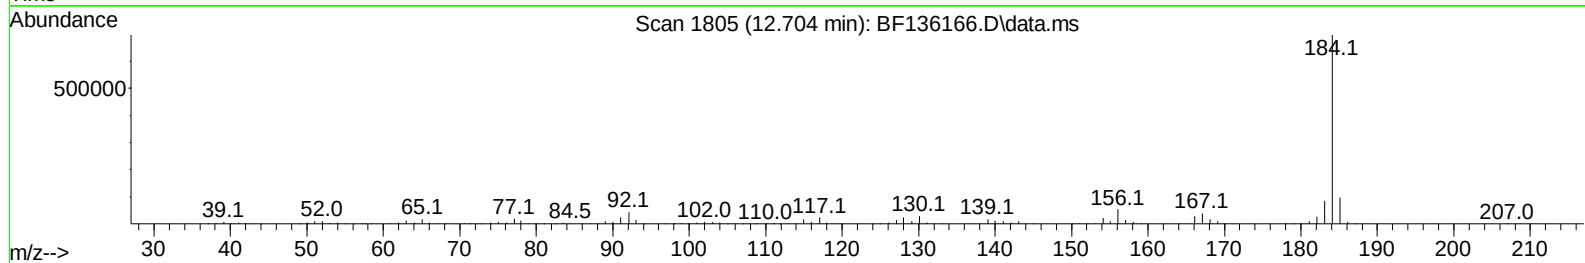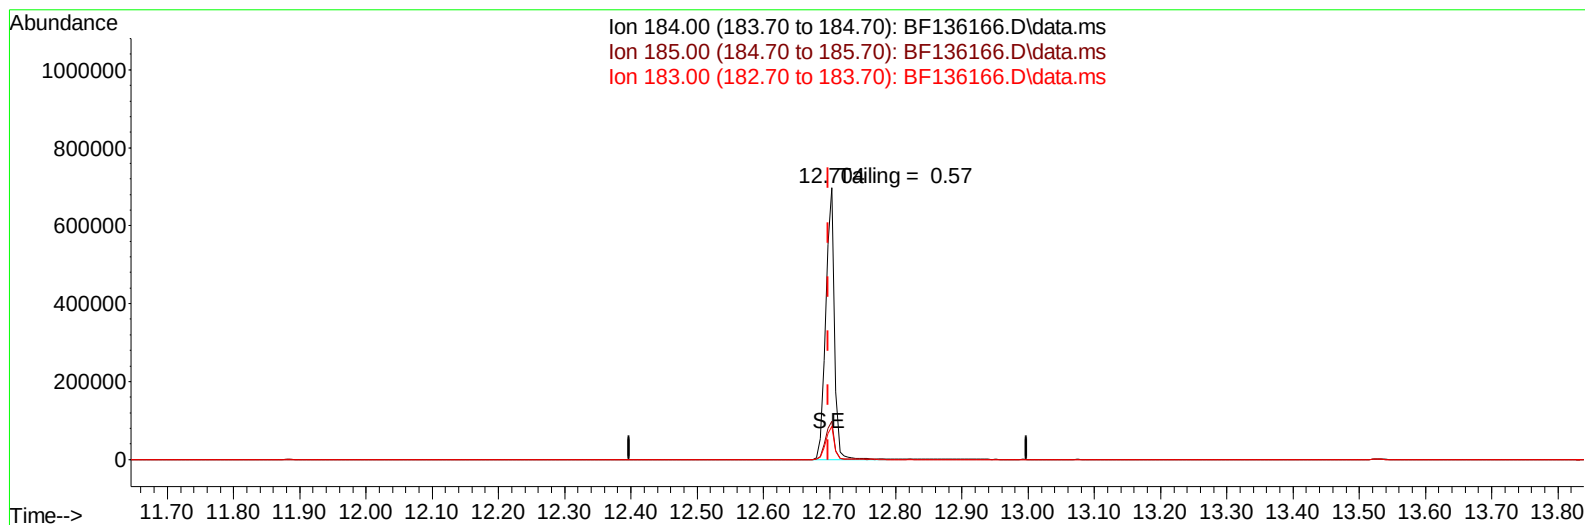

TIC: BF136166.D\data.ms

(77) Benzidine**12.704min (+ 0.006) 599842.57 ng****response 633588**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	14.10
183.00	11.50	12.19
0.00	0.00	0.00