
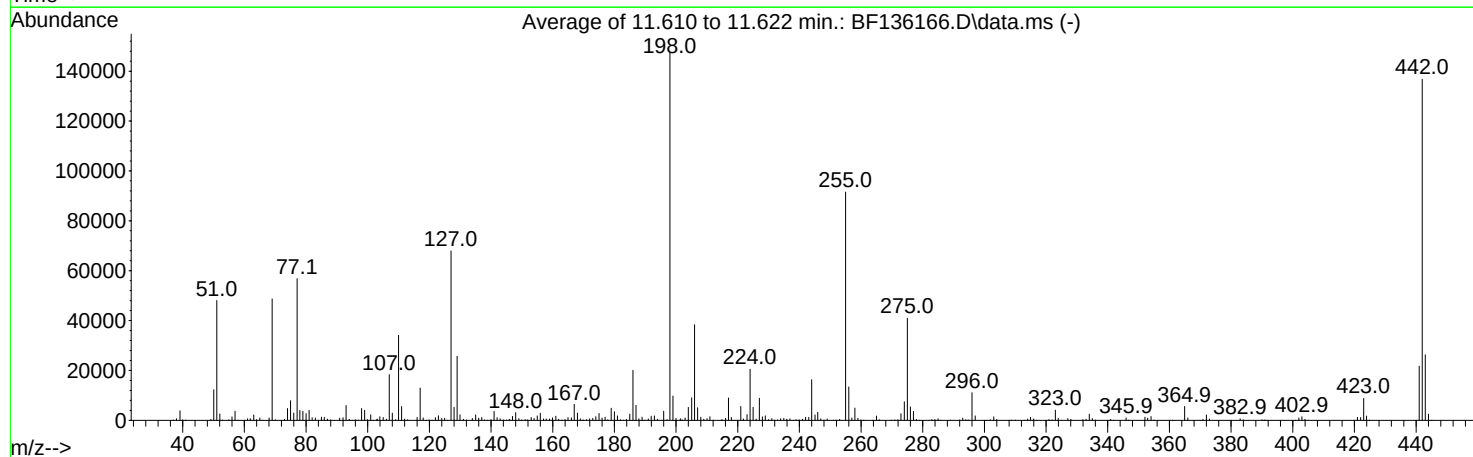


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110723\
Data File : BF136166.D
Acq On : 07 Nov 2023 09:28
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 08 02:12:01 2023

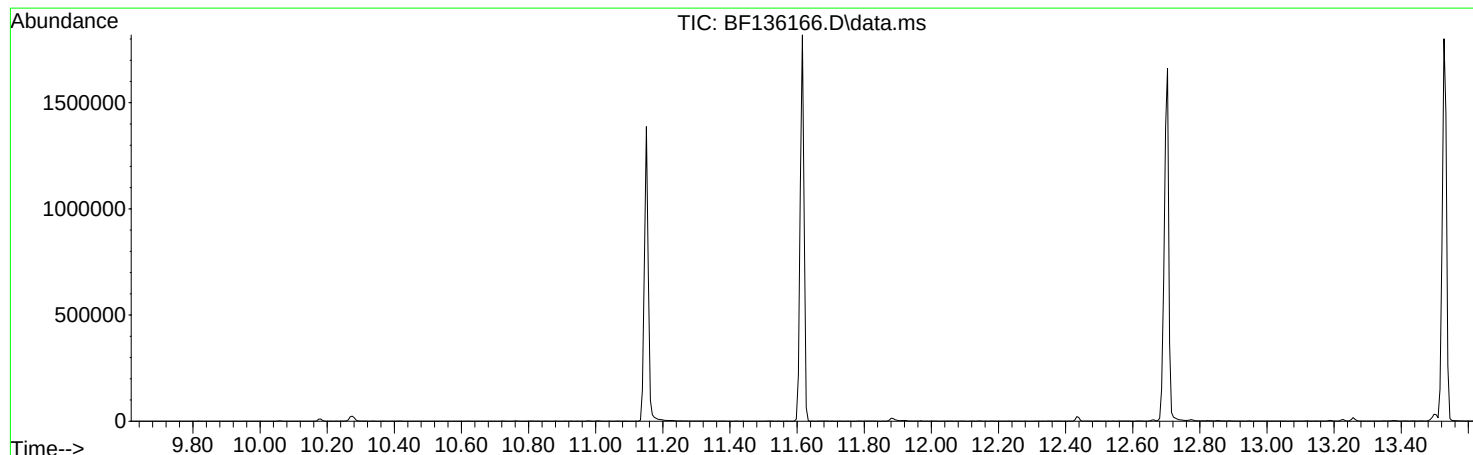




AutoFind: Scans 1619, 1620, 1621; Background Corrected with Scan 1614

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.6	48075	PASS
68	69	0.00	2	2.0	958	PASS
69	198	0.00	100	33.0	48680	PASS
70	69	0.00	2	0.5	233	PASS
127	198	10	80	46.1	67923	PASS
197	198	0.00	2	0.2	307	PASS
198	198	100	100	100.0	147480	PASS
199	198	5	9	6.6	9759	PASS
275	198	10	60	27.7	40912	PASS
365	198	1	100	3.8	5582	PASS
441	198	0.01	100	14.8	21769	PASS
442	442	50	100	100.0	136771	PASS
443	442	15	24	19.2	26305	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110723\
Data File : BF136166.D
Acq On : 07 Nov 2023 09:28
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 08 03:03:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 08 02:12:01 2023
Response via : Initial Calibration

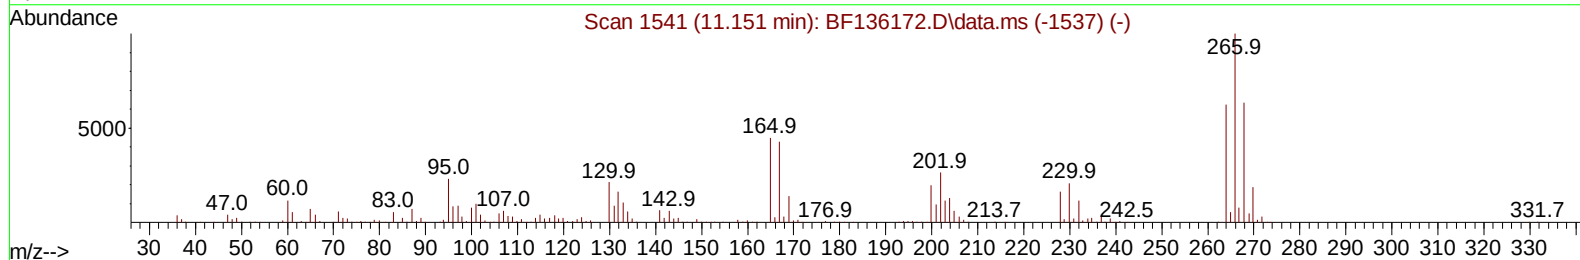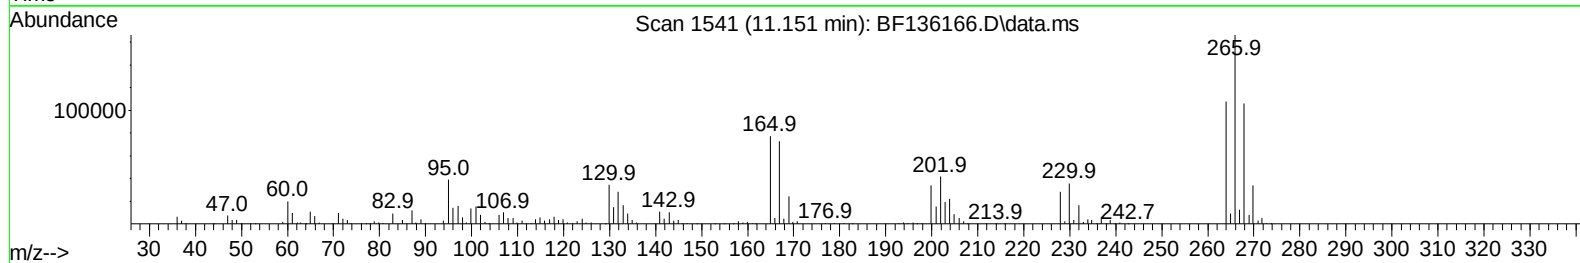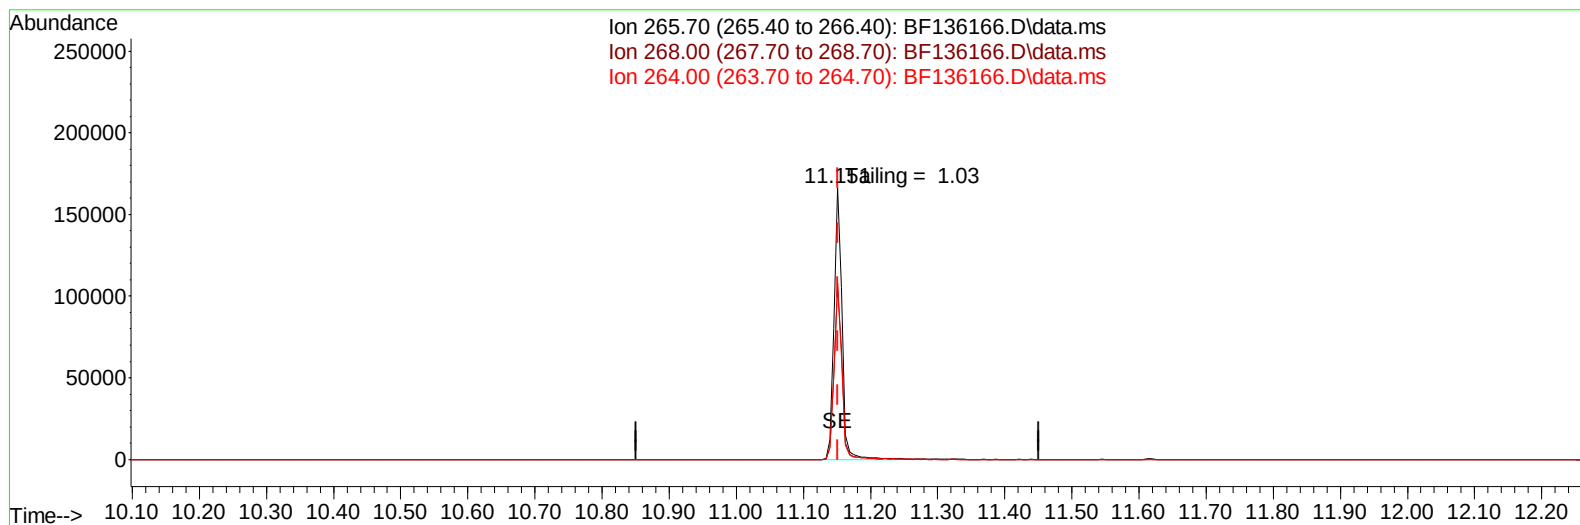

TIC: BF136166.D\data.ms

(70) Pentachlorophenol (C)

11.151min (-0.000) 80784.28 ng




response 141039

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.50	63.86
264.00	62.50	64.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110723\
Data File : BF136166.D
Acq On : 07 Nov 2023 09:28
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 08 03:03:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 08 02:12:01 2023
Response via : Initial Calibration

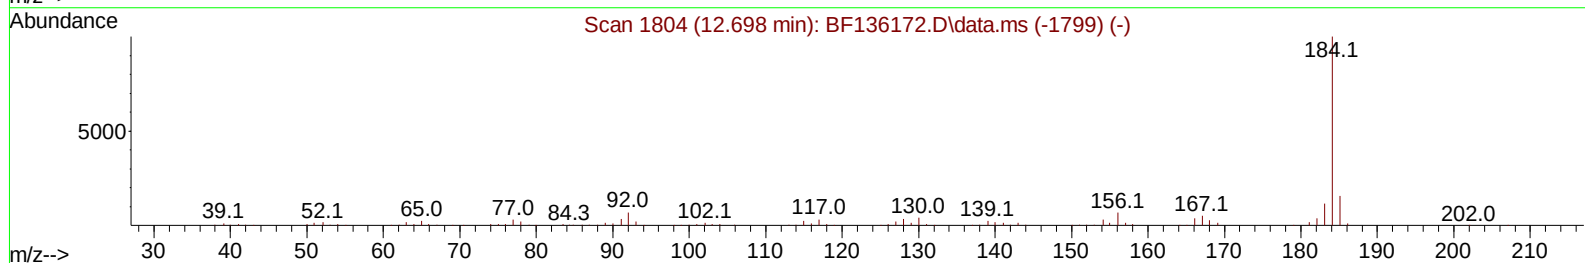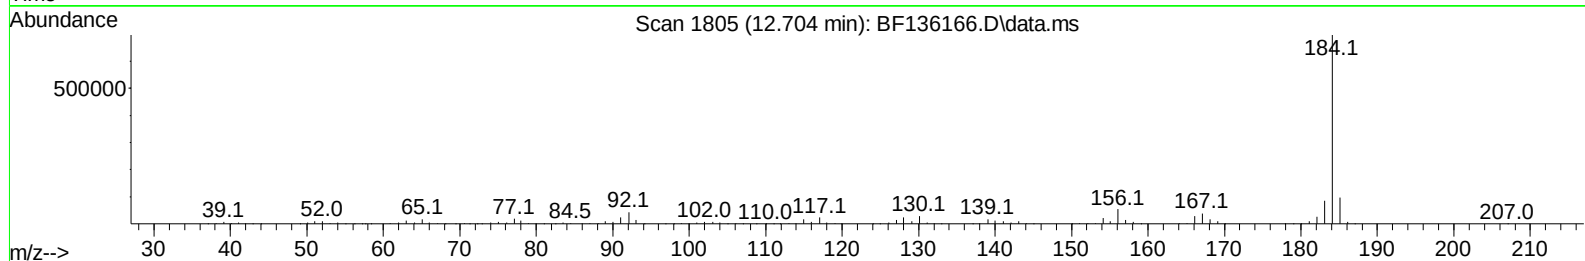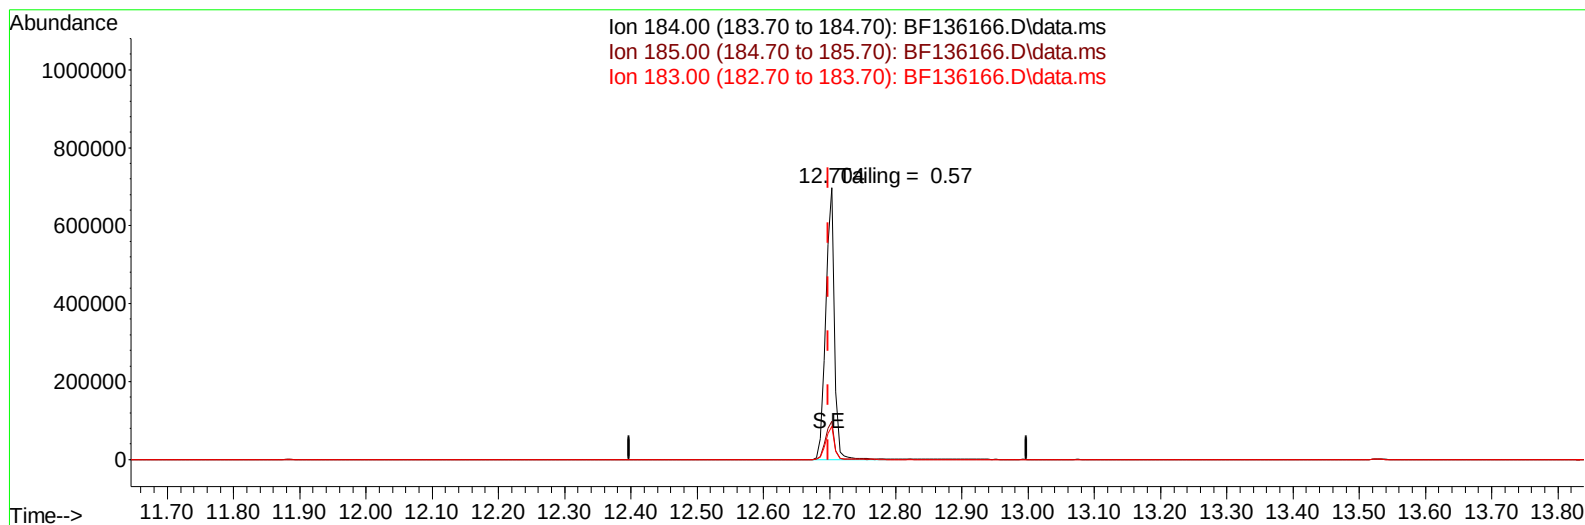

TIC: BF136166.D\data.ms

(77) Benzidine

12.704min (+ 0.006) 599842.57 ng

response 633588

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	14.10
183.00	11.50	12.19
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/7/2023	BNA_F	<u>BF136166.D</u>
Compound Name	Response	Retention Time
DDT	320046	13.527
DDD	4665	13.257
DDE	232	12.886
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4897	324943	1.51

Instrument :
BNA_F
ClientSampleId :
DFTPP