



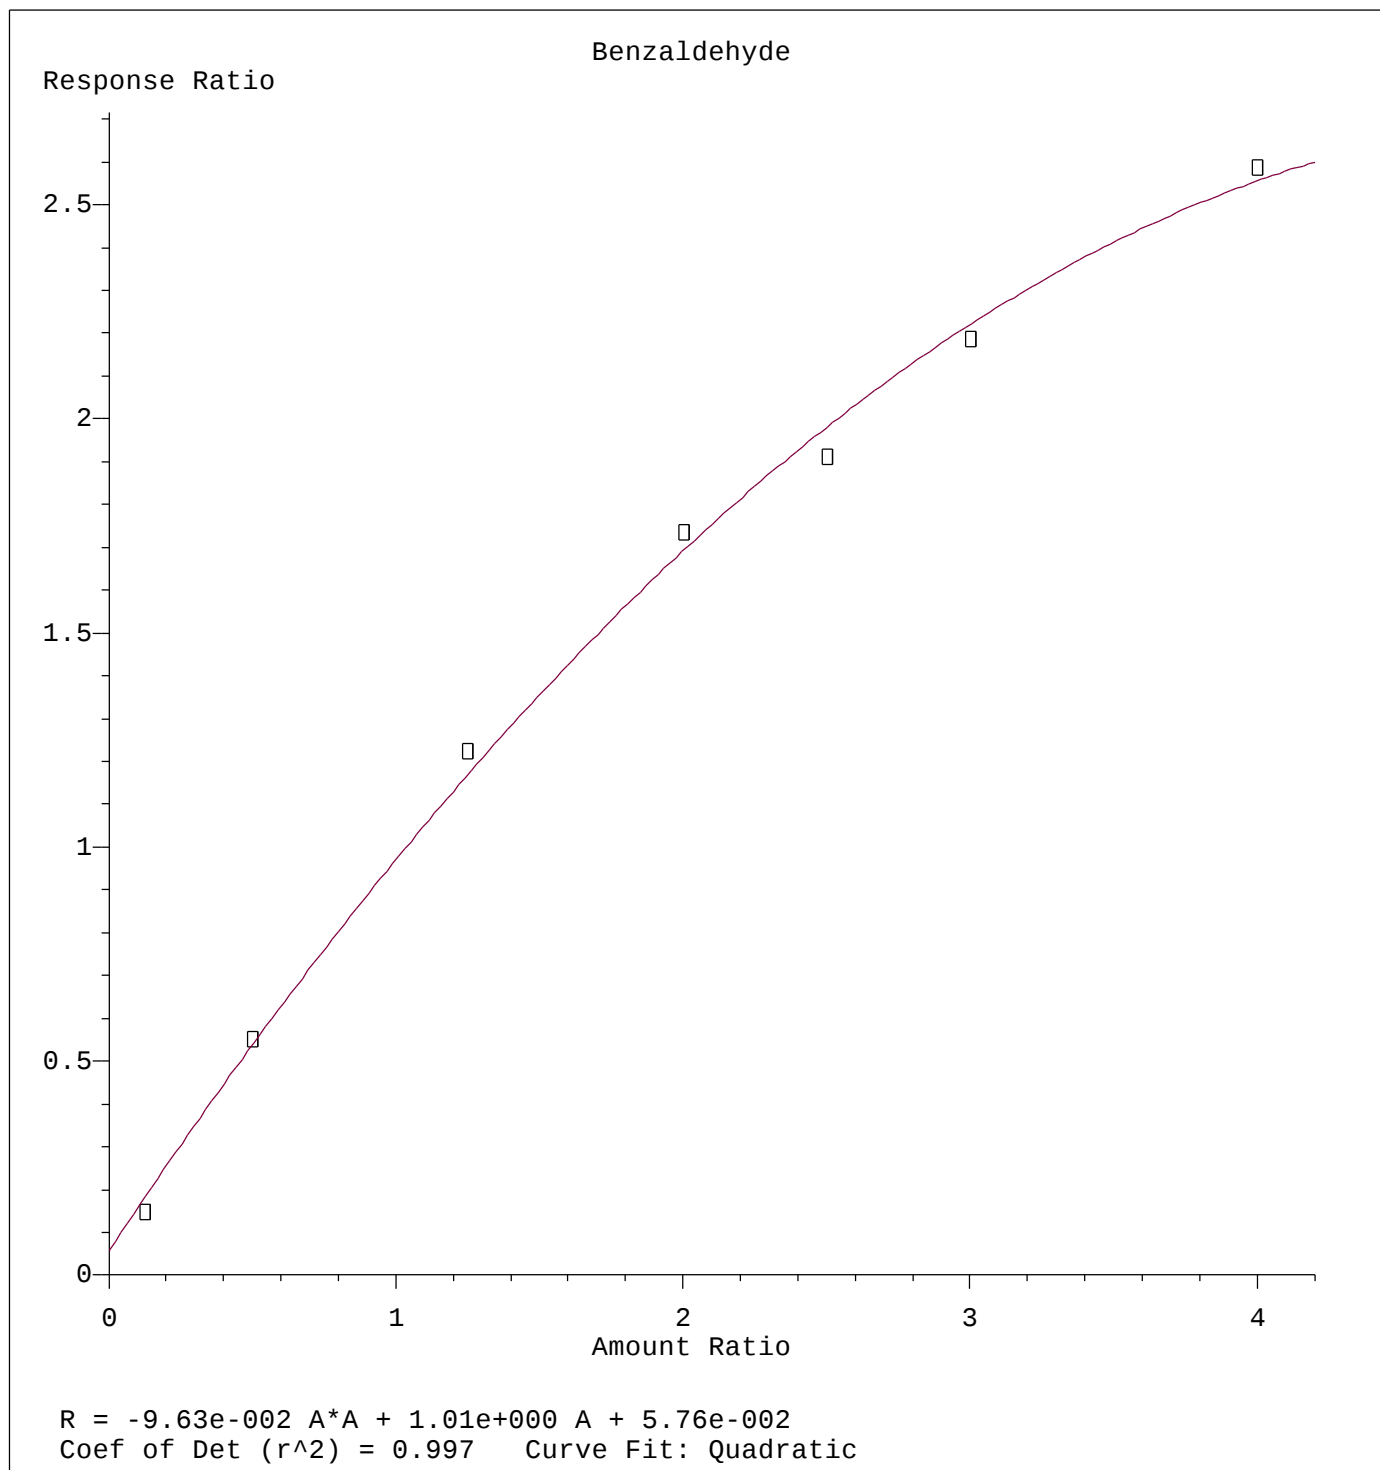

Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110818.M
Calibration Table Last Updated: Fri Nov 09 15:13:13 2018


Hexachlorocyclopentadiene

Response Ratio

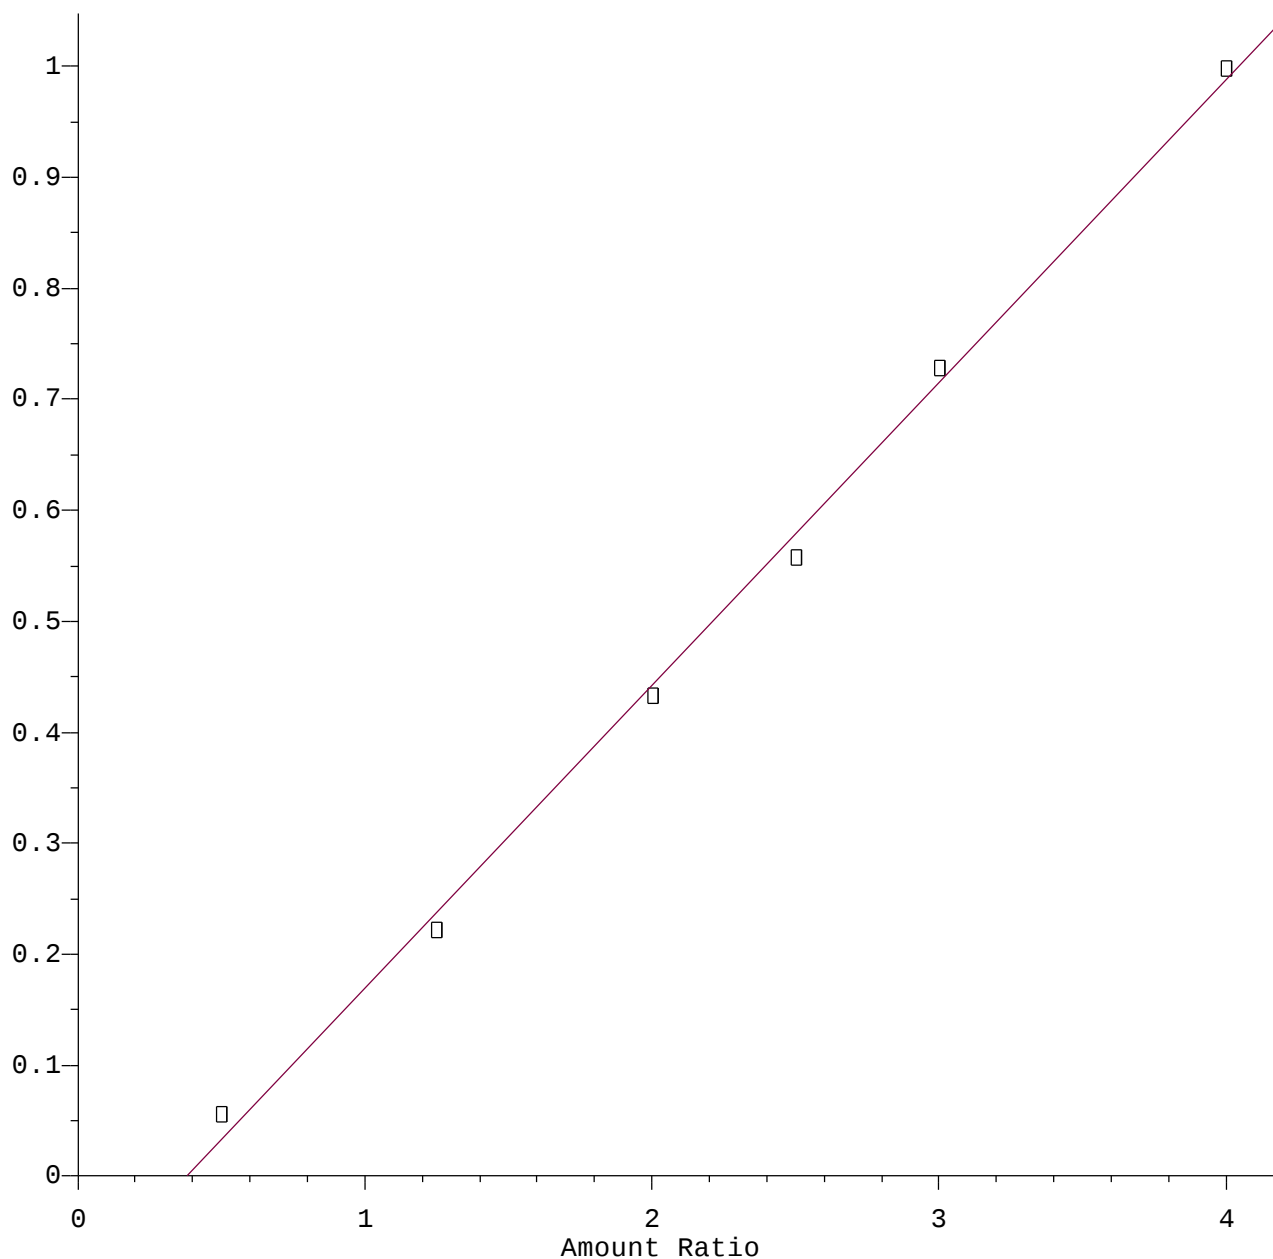

Resp Ratio = $2.73 \times 10^{-1} \times \text{Amt} - 1.04 \times 10^{-1}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110818.M
Calibration Table Last Updated: Fri Nov 09 15:13:13 2018

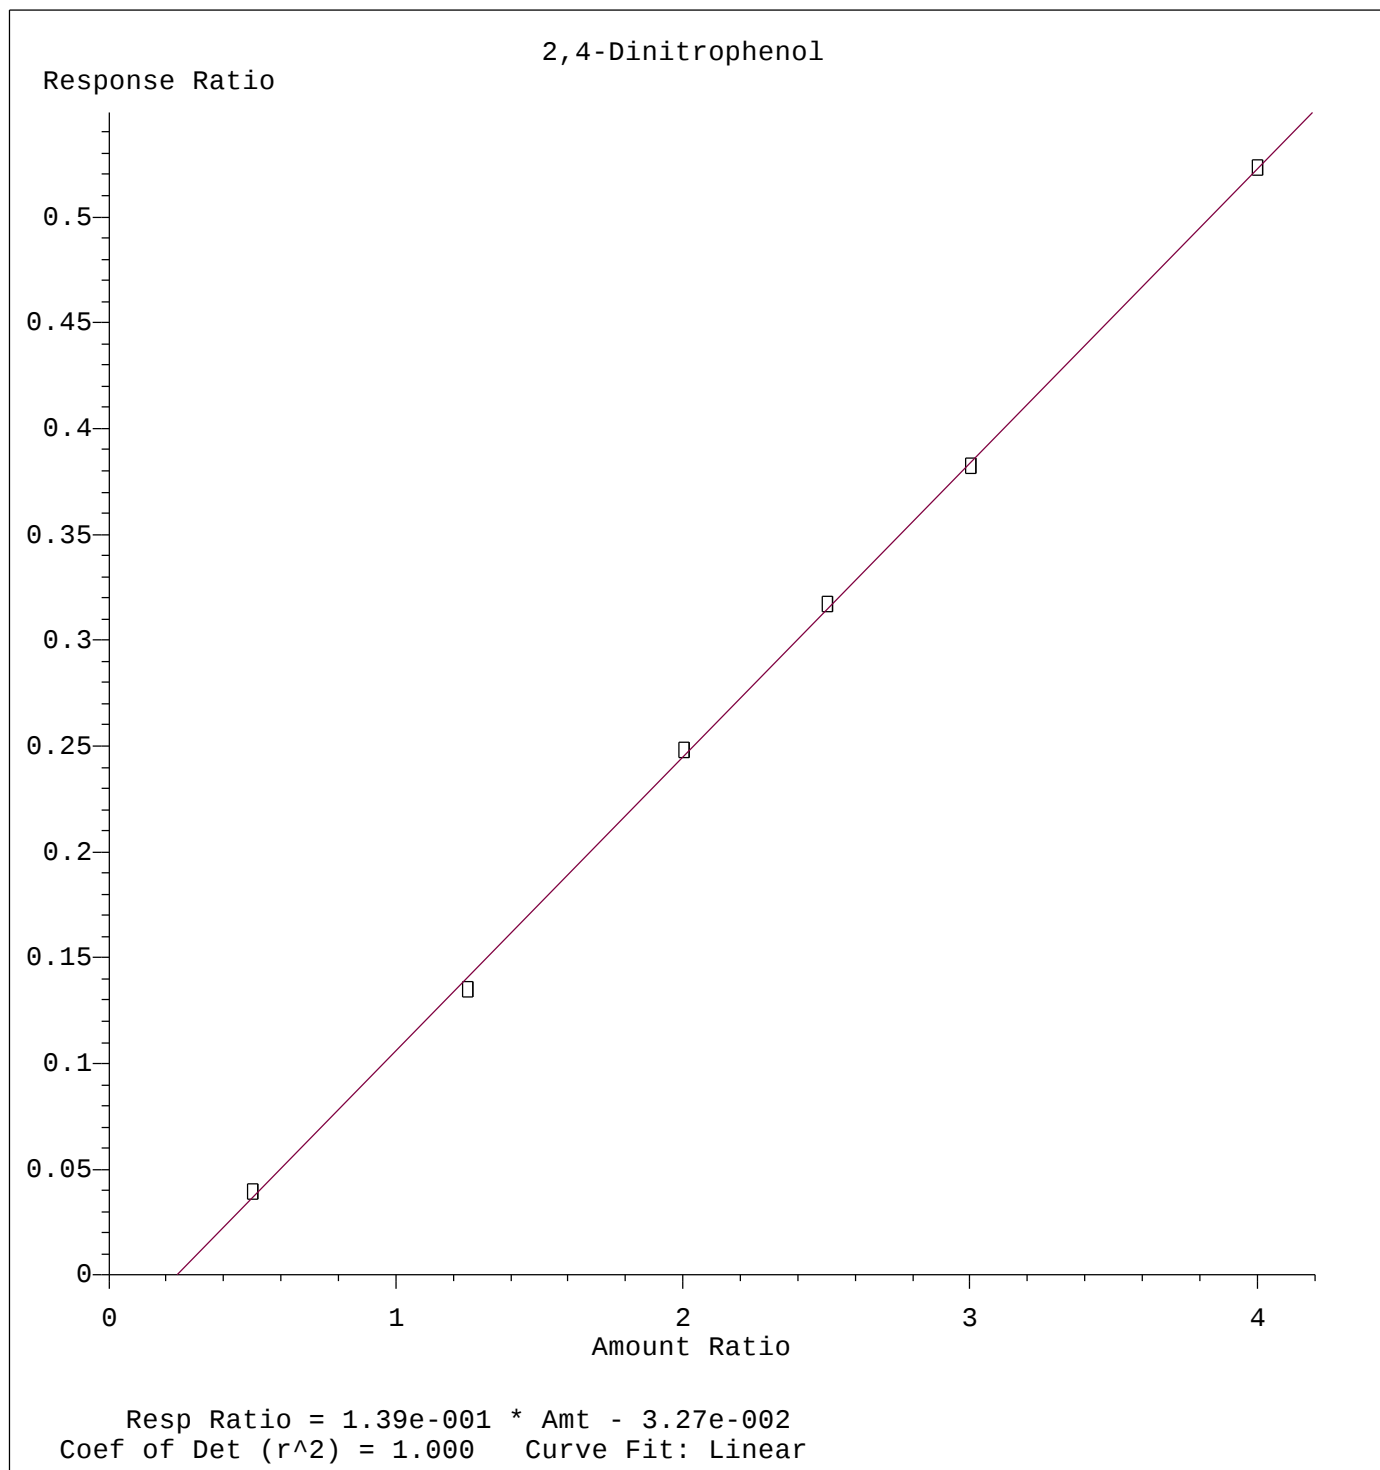

Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110818.M
Calibration Table Last Updated: Fri Nov 09 15:13:13 2018