

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF110818\
 Data File : BF110600.D
 Acq On : 8 Nov 2018 22:15
 Operator : JU/SJ
 Sample : J5858-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-8-S

Quant Time: Nov 09 12:39:39 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF110818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 08 14:14:47 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.95	152	69897	20.00	ng	0.00
21) Naphthalene-d8	8.22	136	283423	20.00	ng	0.00
39) Acenaphthene-d10	9.98	164	136585	20.00	ng	-0.01
64) Phenanthrene-d10	11.48	188	276660	20.00	ng	0.00
76) Chrysene-d12	14.13	240	214167	20.00	ng	-0.01
87) Perylene-d12	15.65	264	144906	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.57	112	629004	146.17	ng	0.00
7) Phenol-d6	6.57	99	807352	146.72	ng	0.00
23) Nitrobenzene-d5	7.51	82	508996	103.42	ng	0.00
42) 2,4,6-Tribromophenol	10.78	330	202093	146.84	ng	0.00
45) 2-Fluorobiphenyl	9.30	172	950222	99.36	ng	0.00
79) Terphenyl-d14	13.06	244	1029243	90.00	ng	0.00
Target Compounds						
10) Phenol	6.58	94	40386	6.329	ng	Qvalue # 72
50) Dimethylphthalate	9.69	163	82906	8.135	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF110818\
Data File : BF110600.D
Acq On : 8 Nov 2018 22:15
Operator : JU/SJ
Sample : J5858-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-8-S

Quant Time: Nov 09 12:39:39 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF110818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 08 14:14:47 2018
Response via : Initial Calibration

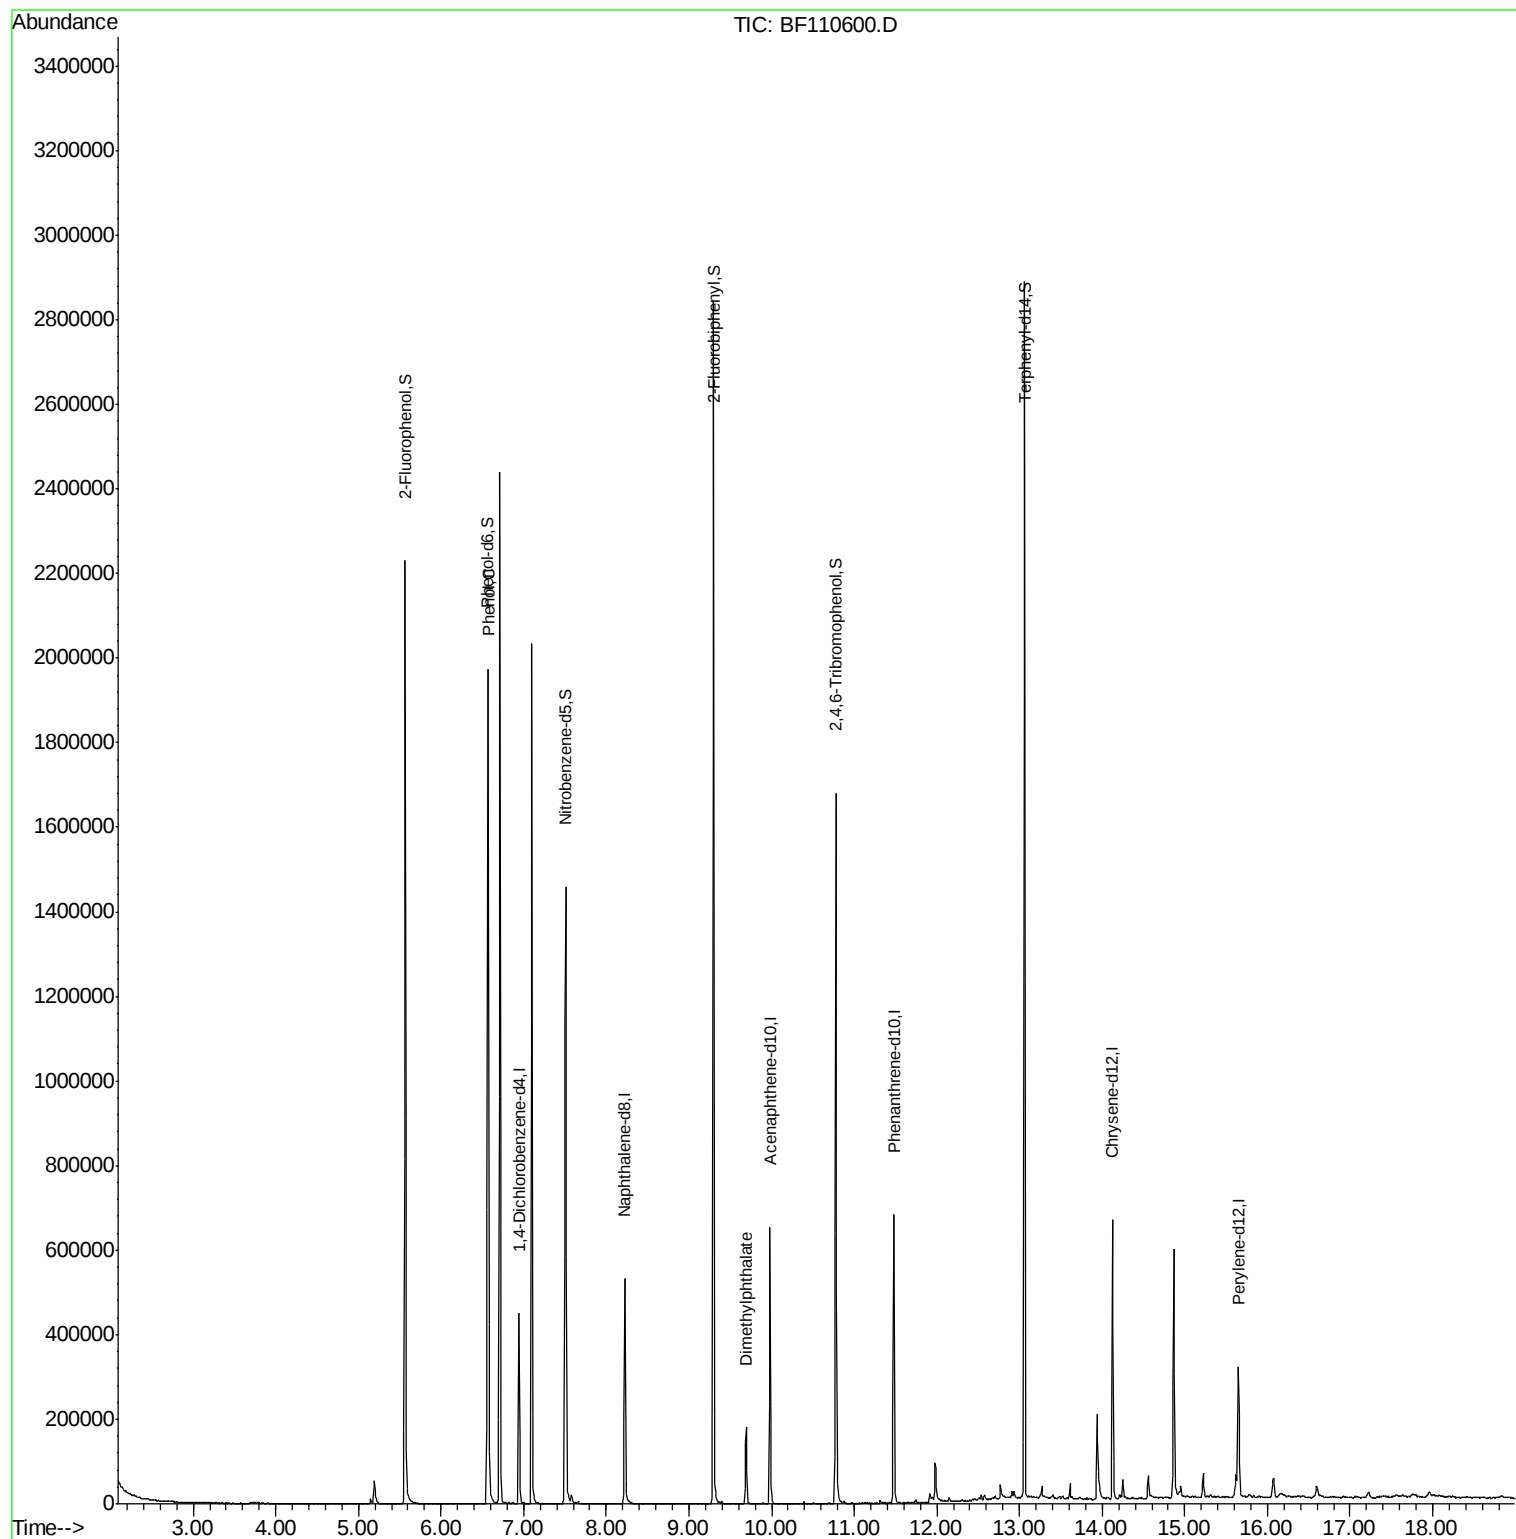


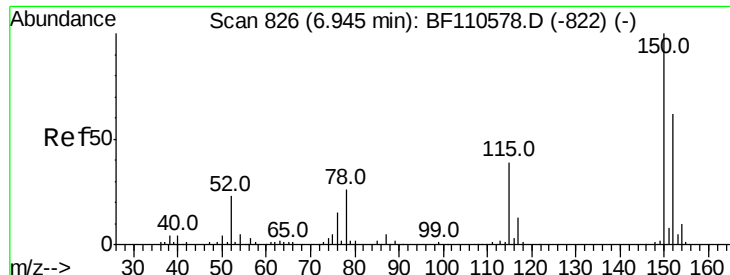




#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.95 min Scan# 826
 Delta R.T. 0.00 min
 Lab File: BF110600.D
 Acq: 8 Nov 2018 22:15

Instrument :
 BNA_F
 ClientSampleId :
 SB-8-S

Tot Ion:152 Resp: 69897
 Ion Ratio Lower Upper
 152 100
 150 156.9 122.7 184.1
 115 59.0 49.1 73.7

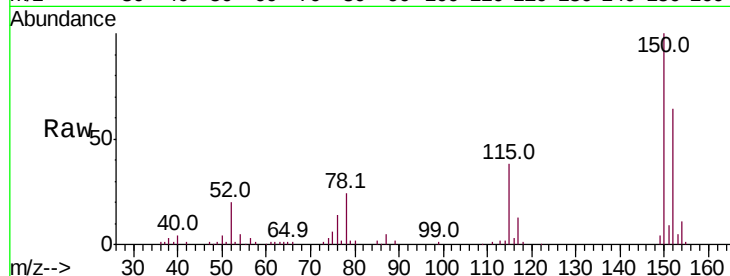


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

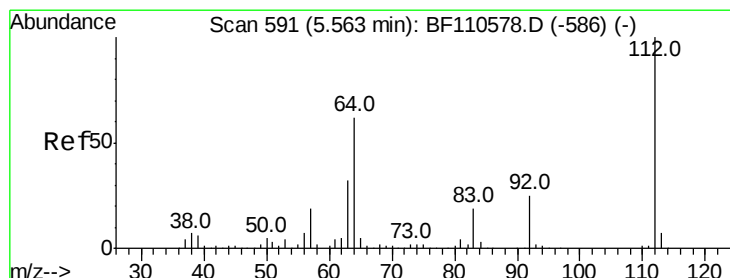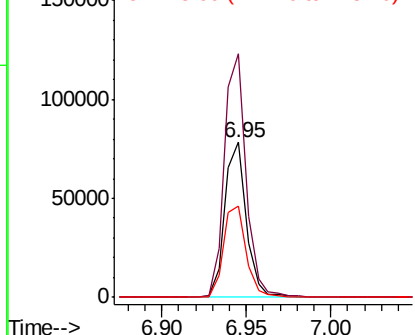
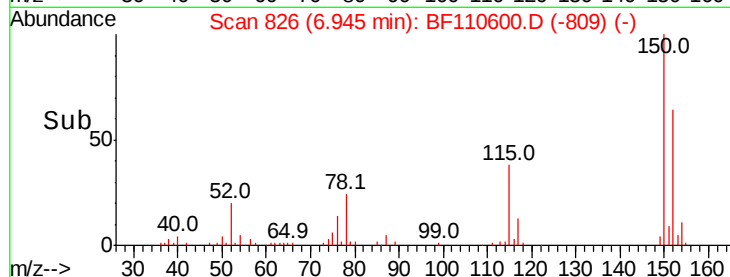


#5
 2-Fluorophenol
 Concen: 146.172 ng
 RT: 5.57 min Scan# 592
 Delta R.T. 0.01 min
 Lab File: BF110600.D
 Acq: 8 Nov 2018 22:15

Tgt Ion:112 Resp: 629004
 Ion Ratio Lower Upper
 112 100
 64 59.6 44.1 66.1
 63 31.6 23.7 35.5

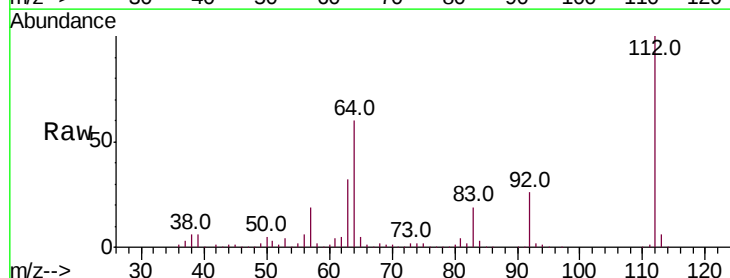

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF1
 Ion 63.00 (62.70 to 63.70): BF1

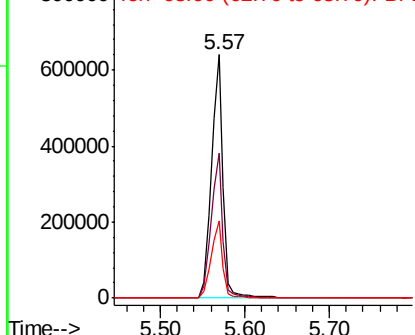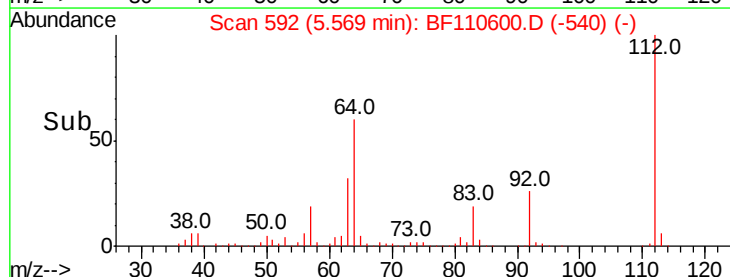



#7

Phenol-d6

Concen: 146.719 ng

RT: 6.57 min Scan# 762

Delta R.T. -0.01 min

Lab File: BF110600.D

Acq: 8 Nov 2018 22:15

Instrument :

BNA_F

ClientSampleId :

SB-8-S


Tot Ion: 99 Resp: 807352

Ion Ratio Lower Upper




99 100

42 20.1 15.8 23.6

71 35.8 28.0 42.0

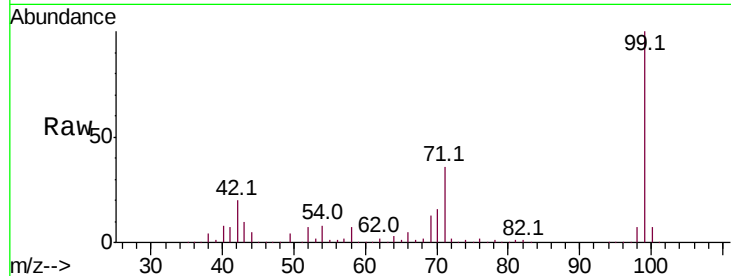

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

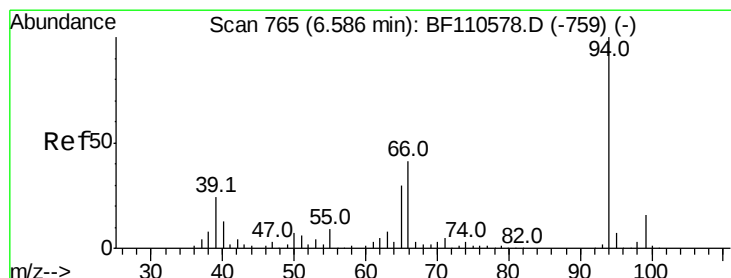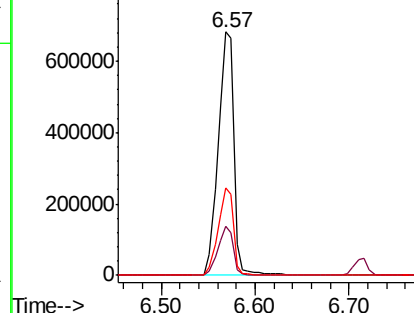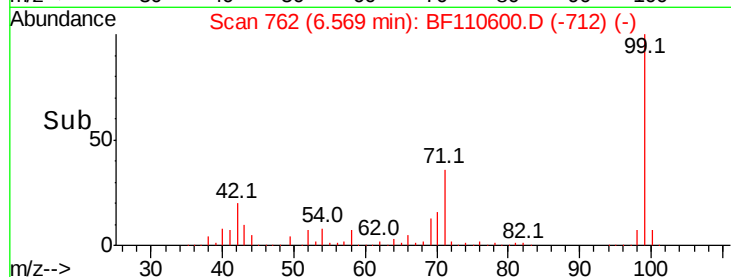

#10

Phenol

Concen: 6.329 ng

RT: 6.58 min Scan# 764

Delta R.T. -0.01 min

Lab File: BF110600.D

Acq: 8 Nov 2018 22:15


Tgt Ion: 94 Resp: 40386

Ion Ratio Lower Upper



94 100


65 32.7 25.3 65.3

66 46.0 54.5 94.5#

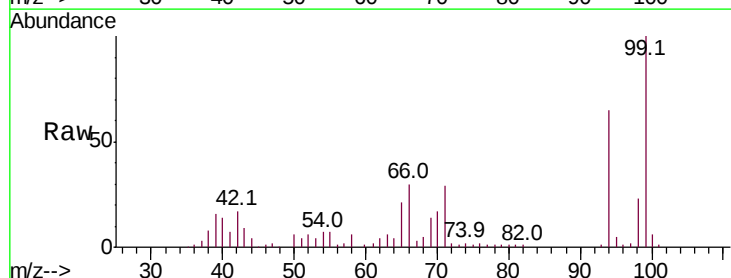

Abundance Ion 94.00 (93.70 to 94.70): BF1
Ion 65.00 (64.70 to 65.70): BF1
Ion 66.00 (65.70 to 66.70): BF1

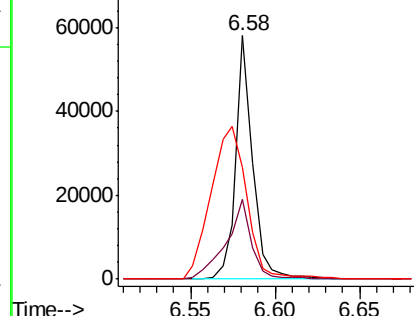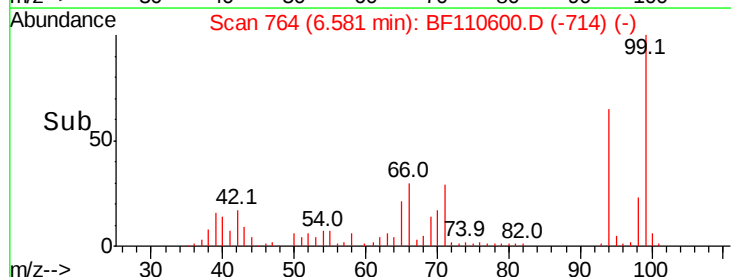

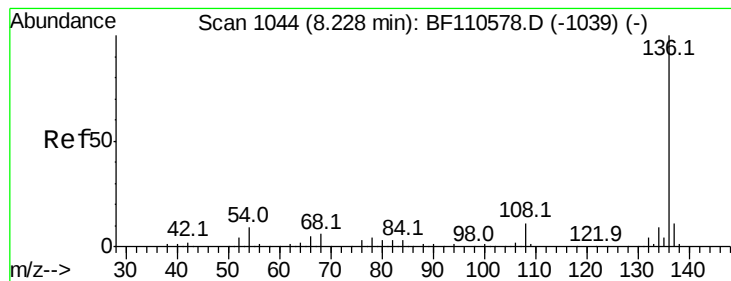

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.22 min Scan# 1043

Delta R.T. -0.01 min

Lab File: BF110600.D

Acq: 8 Nov 2018 22:15

Instrument :

BNA_F

ClientSampleId :

SB-8-S

Tot Ion:136 Resp: 283423



Ion Ratio Lower Upper

136 100

137 11.2 8.8 13.2

54 8.4 5.4 8.2#

68 5.5 4.2 6.2

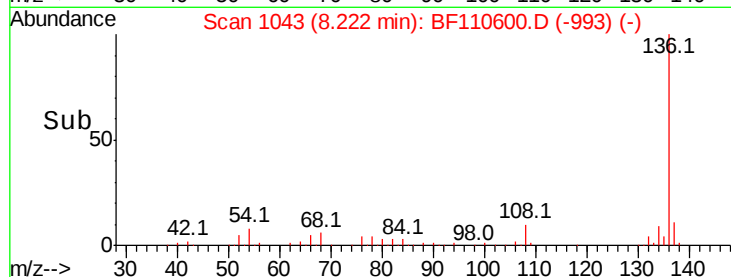
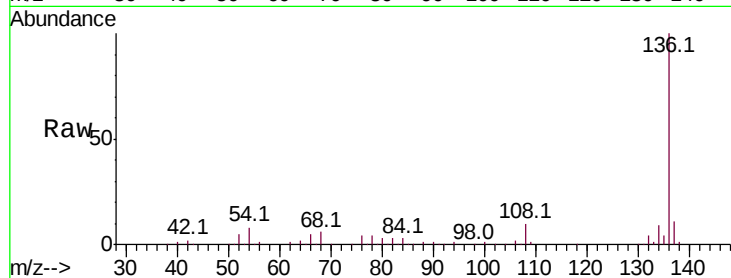


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

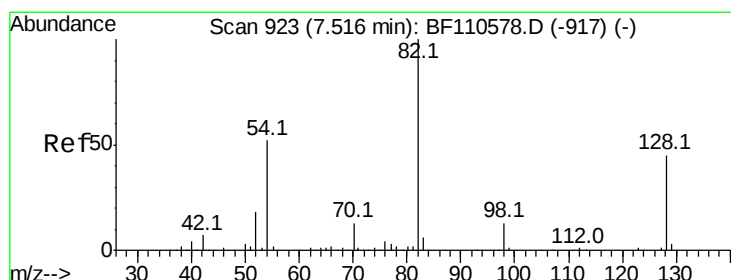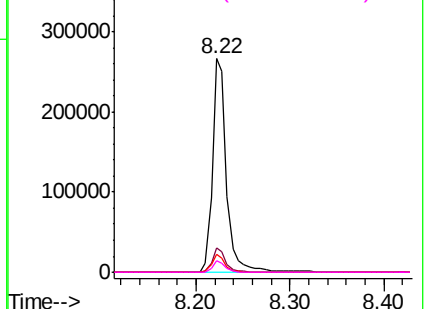

#23

Nitrobenzene-d5

Concen: 103.424 ng

RT: 7.51 min Scan# 922

Delta R.T. -0.01 min

Lab File: BF110600.D

Acq: 8 Nov 2018 22:15



Tgt Ion: 82 Resp: 508996

Ion Ratio Lower Upper

82 100

128 45.1 34.2 51.2


54 52.1 38.6 58.0

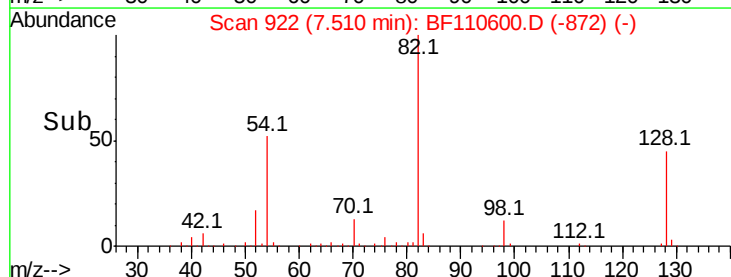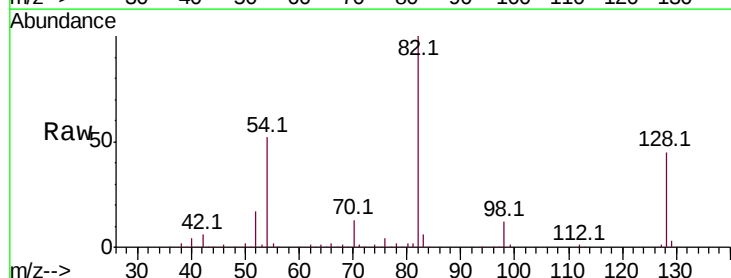


Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF1

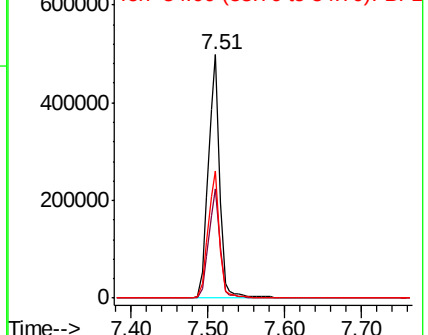


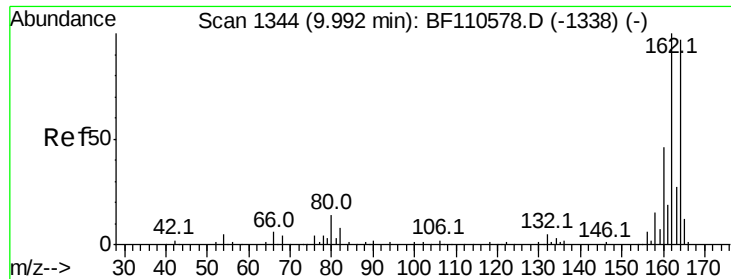



#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.98 min Scan# 1342
Delta R.T. -0.01 min
Lab File: BF110600.D
Acq: 8 Nov 2018 22:15

Instrument :
BNA_F
ClientSampleId :
SB-8-S

Tot Ion:164 Resp: 136585
Ion Ratio Lower Upper
164 100
162 104.3 83.0 124.6
160 46.4 37.0 55.6

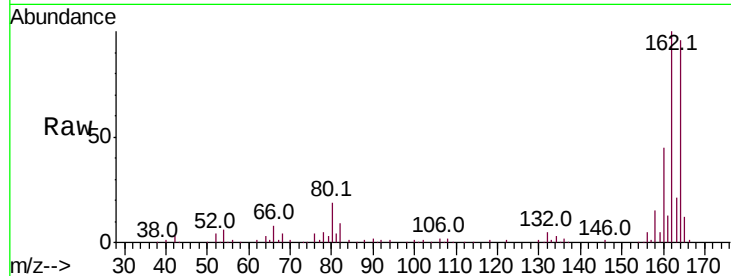


Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

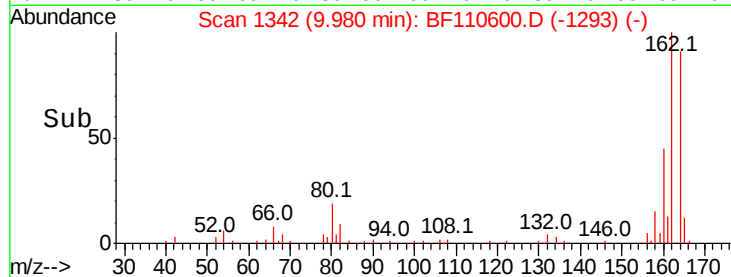
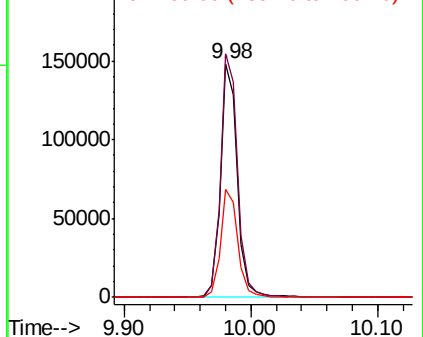



#42
2,4,6-Tribromophenol
Concen: 146.842 ng
RT: 10.78 min Scan# 1478
Delta R.T. -0.01 min
Lab File: BF110600.D
Acq: 8 Nov 2018 22:15

Tgt Ion:330 Resp: 202093
Ion Ratio Lower Upper
330 100
332 97.1 77.1 115.7
141 37.7 27.0 40.4

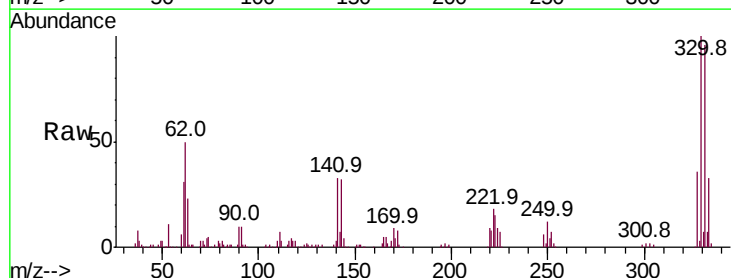

Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

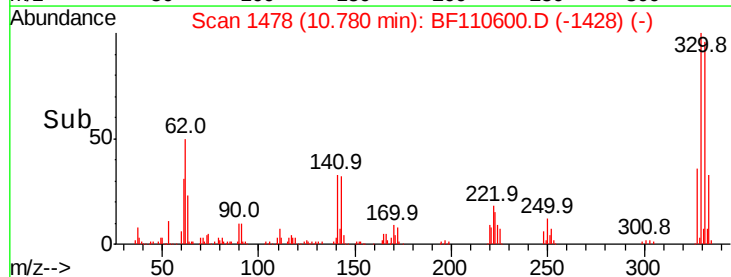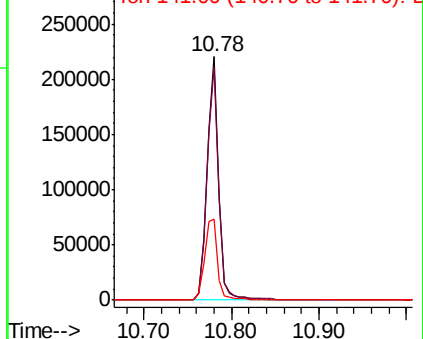


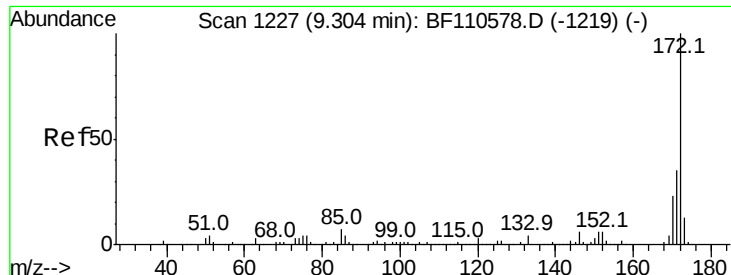




#45
 2-Fluorobiphenyl
 Concen: 99.359 ng
 RT: 9.30 min Scan# 1226
 Delta R.T. -0.01 min
 Lab File: BF110600.D
 Acq: 8 Nov 2018 22:15

Instrument :
 BNA_F
 ClientSampleId :
 SB-8-S

Tot Ion:172 Resp: 950222
 Ion Ratio Lower Upper
 172 100
 171 35.4 28.6 43.0
 170 23.6 19.7 29.5

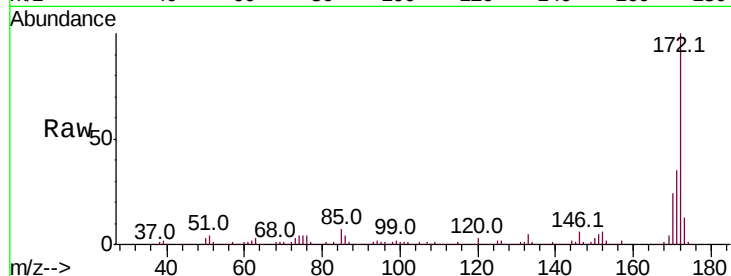


Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

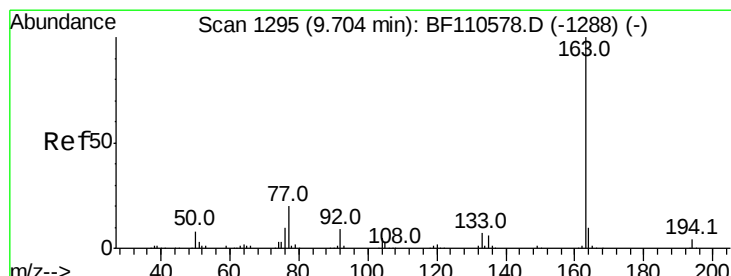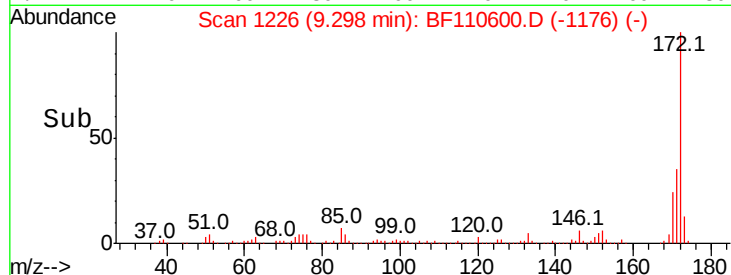
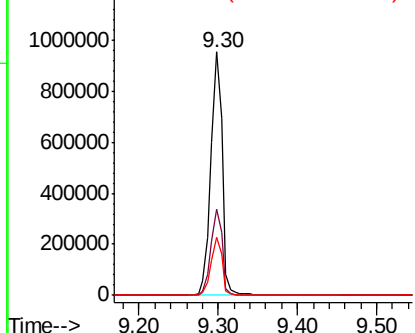



#50
 Dimethylphthalate
 Concen: 8.135 ng
 RT: 9.69 min Scan# 1293
 Delta R.T. -0.01 min
 Lab File: BF110600.D
 Acq: 8 Nov 2018 22:15

Tgt Ion:163 Resp: 82906
 Ion Ratio Lower Upper
 163 100
 194 3.8 3.2 4.8
 164 9.4 8.1 12.1

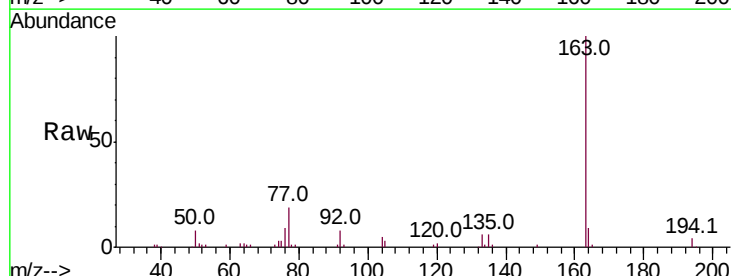

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

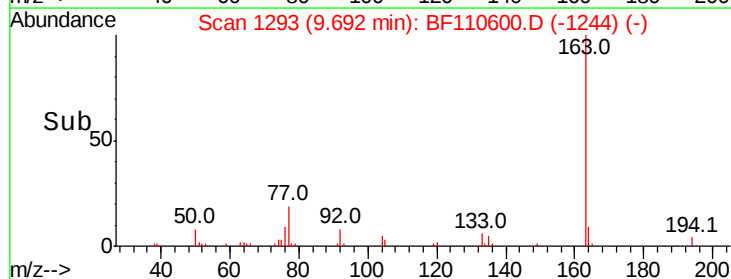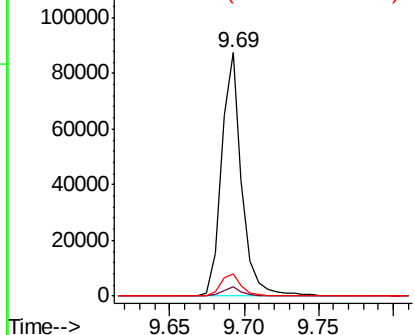

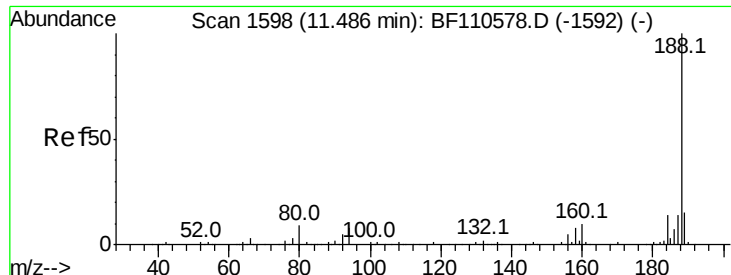

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.48 min Scan# 1597

Delta R.T. -0.01 min

Lab File: BF110600.D

Acq: 8 Nov 2018 22:15

Instrument :

BNA_F

ClientSampleId :

SB-8-S


Tot Ion:188 Resp: 276660

Ion Ratio Lower Upper

188 100

94 8.1 7.2 10.8




80 8.7 7.9 11.9

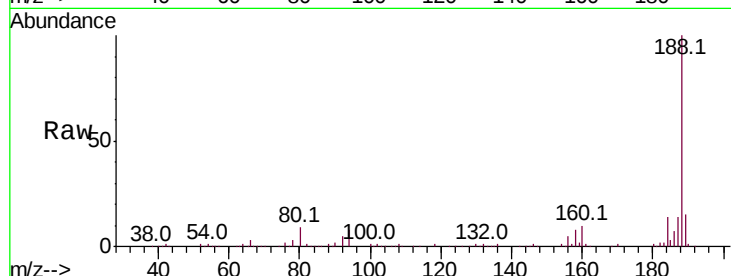

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

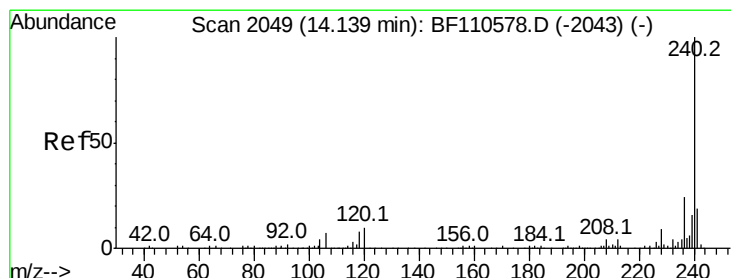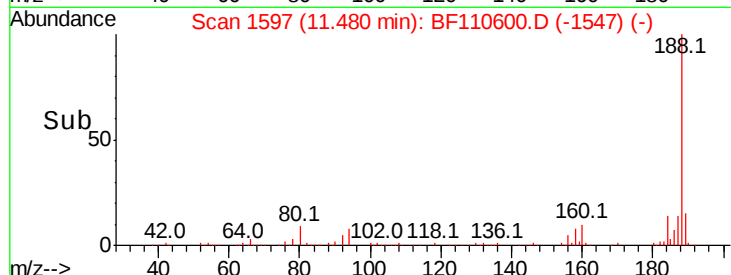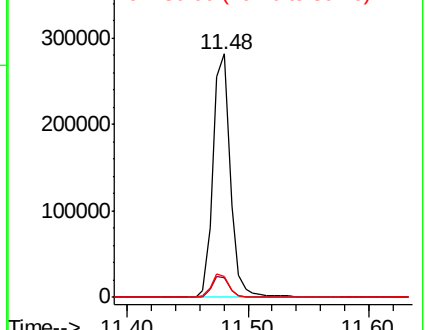

#76

Chrysene-d12

Concen: 20.000 ng

RT: 14.13 min Scan# 2047

Delta R.T. -0.01 min

Lab File: BF110600.D

Acq: 8 Nov 2018 22:15


Tgt Ion:240 Resp: 214167

Ion Ratio Lower Upper

240 100

120 11.6 8.3 12.5



236 25.8 21.2 31.8

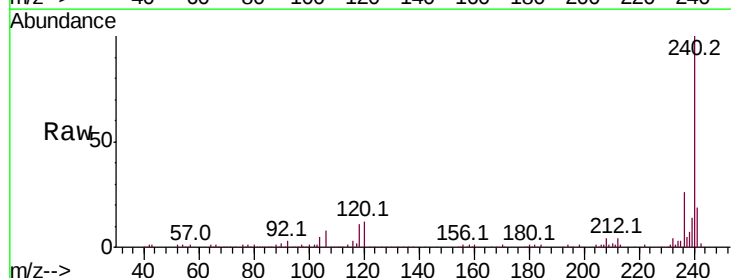


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E



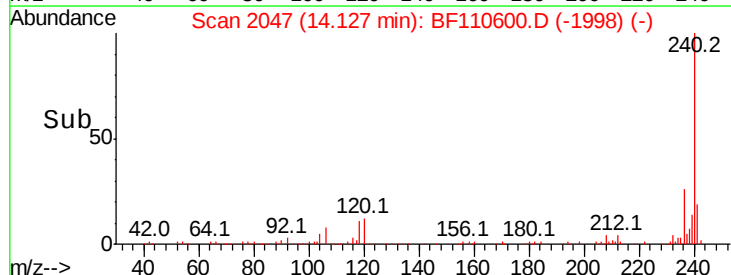
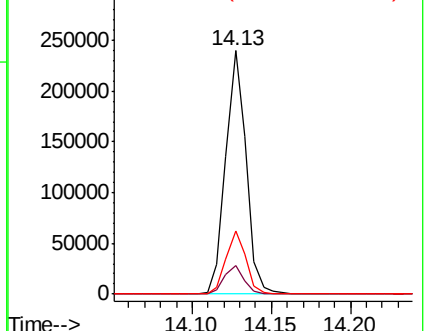


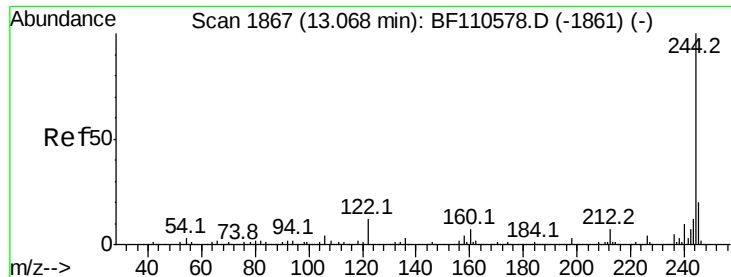

#79
 Terphenyl-d14
 Concen: 90.001 ng
 RT: 13.06 min Scan# 1866
 Delta R.T. -0.01 min
 Lab File: BF110600.D
 Acq: 8 Nov 2018 22:15

Instrument :
 BNA_F
 ClientSampleId :
 SB-8-S

Tot Ion:244 Resp: 1029243
 Ion Ratio Lower Upper
 244 100
 212 7.2 5.8 8.8
 122 12.9 8.7 13.1

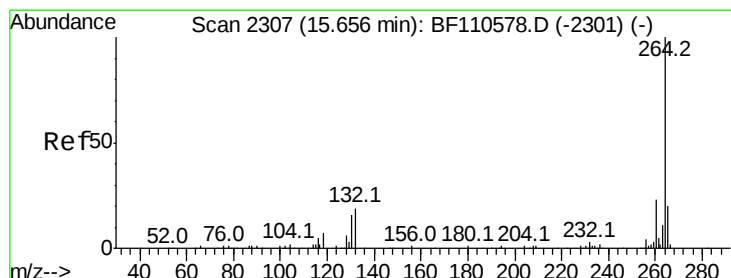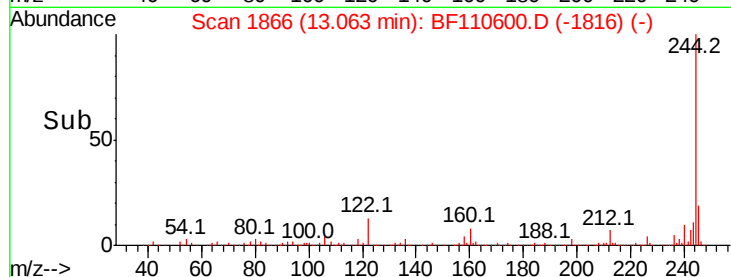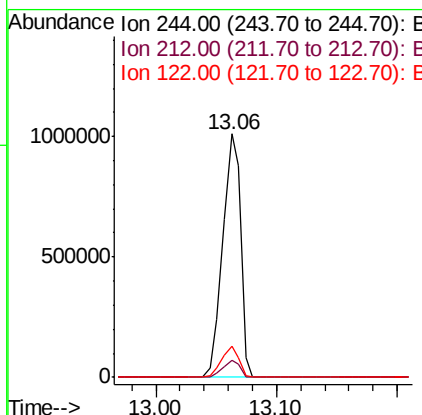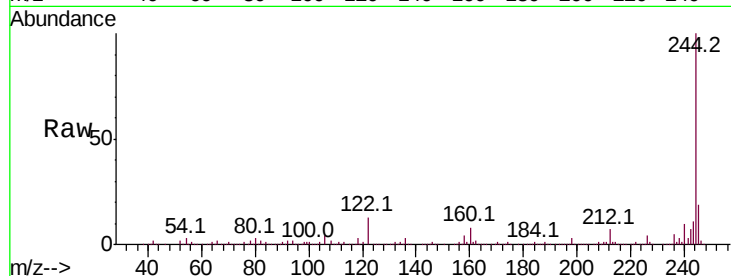

#87
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.65 min Scan# 2306
 Delta R.T. -0.01 min
 Lab File: BF110600.D
 Acq: 8 Nov 2018 22:15

Tgt Ion:264 Resp: 144906
 Ion Ratio Lower Upper
 264 100
 260 22.7 18.7 28.1
 265 20.6 16.7 25.1

