

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF110818\
 Data File : BF110605.D
 Acq On : 9 Nov 2018 00:29
 Operator : JU/SJ
 Sample : J5857-02 2X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PS-CON-2

Quant Time: Nov 09 13:27:45 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF110818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 08 14:14:47 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.95	152	88718	20.00	ng	0.00
21) Naphthalene-d8	8.23	136	364557	20.00	ng	0.00
39) Acenaphthene-d10	9.99	164	157532	20.00	ng	0.00
64) Phenanthrene-d10	11.48	188	250671	20.00	ng	0.00
76) Chrysene-d12	14.13	240	208046	20.00	ng	-0.01
87) Perylene-d12	15.65	264	168887	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.56	112	311908	57.11	ng	0.00
7) Phenol-d6	6.56	99	440422	63.06	ng	-0.01
23) Nitrobenzene-d5	7.50	82	282857	44.68	ng	-0.01
42) 2,4,6-Tribromophenol	10.77	330	71127	44.81	ng	-0.01
45) 2-Fluorobiphenyl	9.30	172	540383	48.99	ng	0.00
79) Terphenyl-d14	13.06	244	415870	37.44	ng	-0.01


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF110818\
Data File : BF110605.D
Acq On : 9 Nov 2018 00:29
Operator : JU/SJ
Sample : J5857-02 2X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PS-CON-2

Quant Time: Nov 09 13:27:45 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF110818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 08 14:14:47 2018
Response via : Initial Calibration

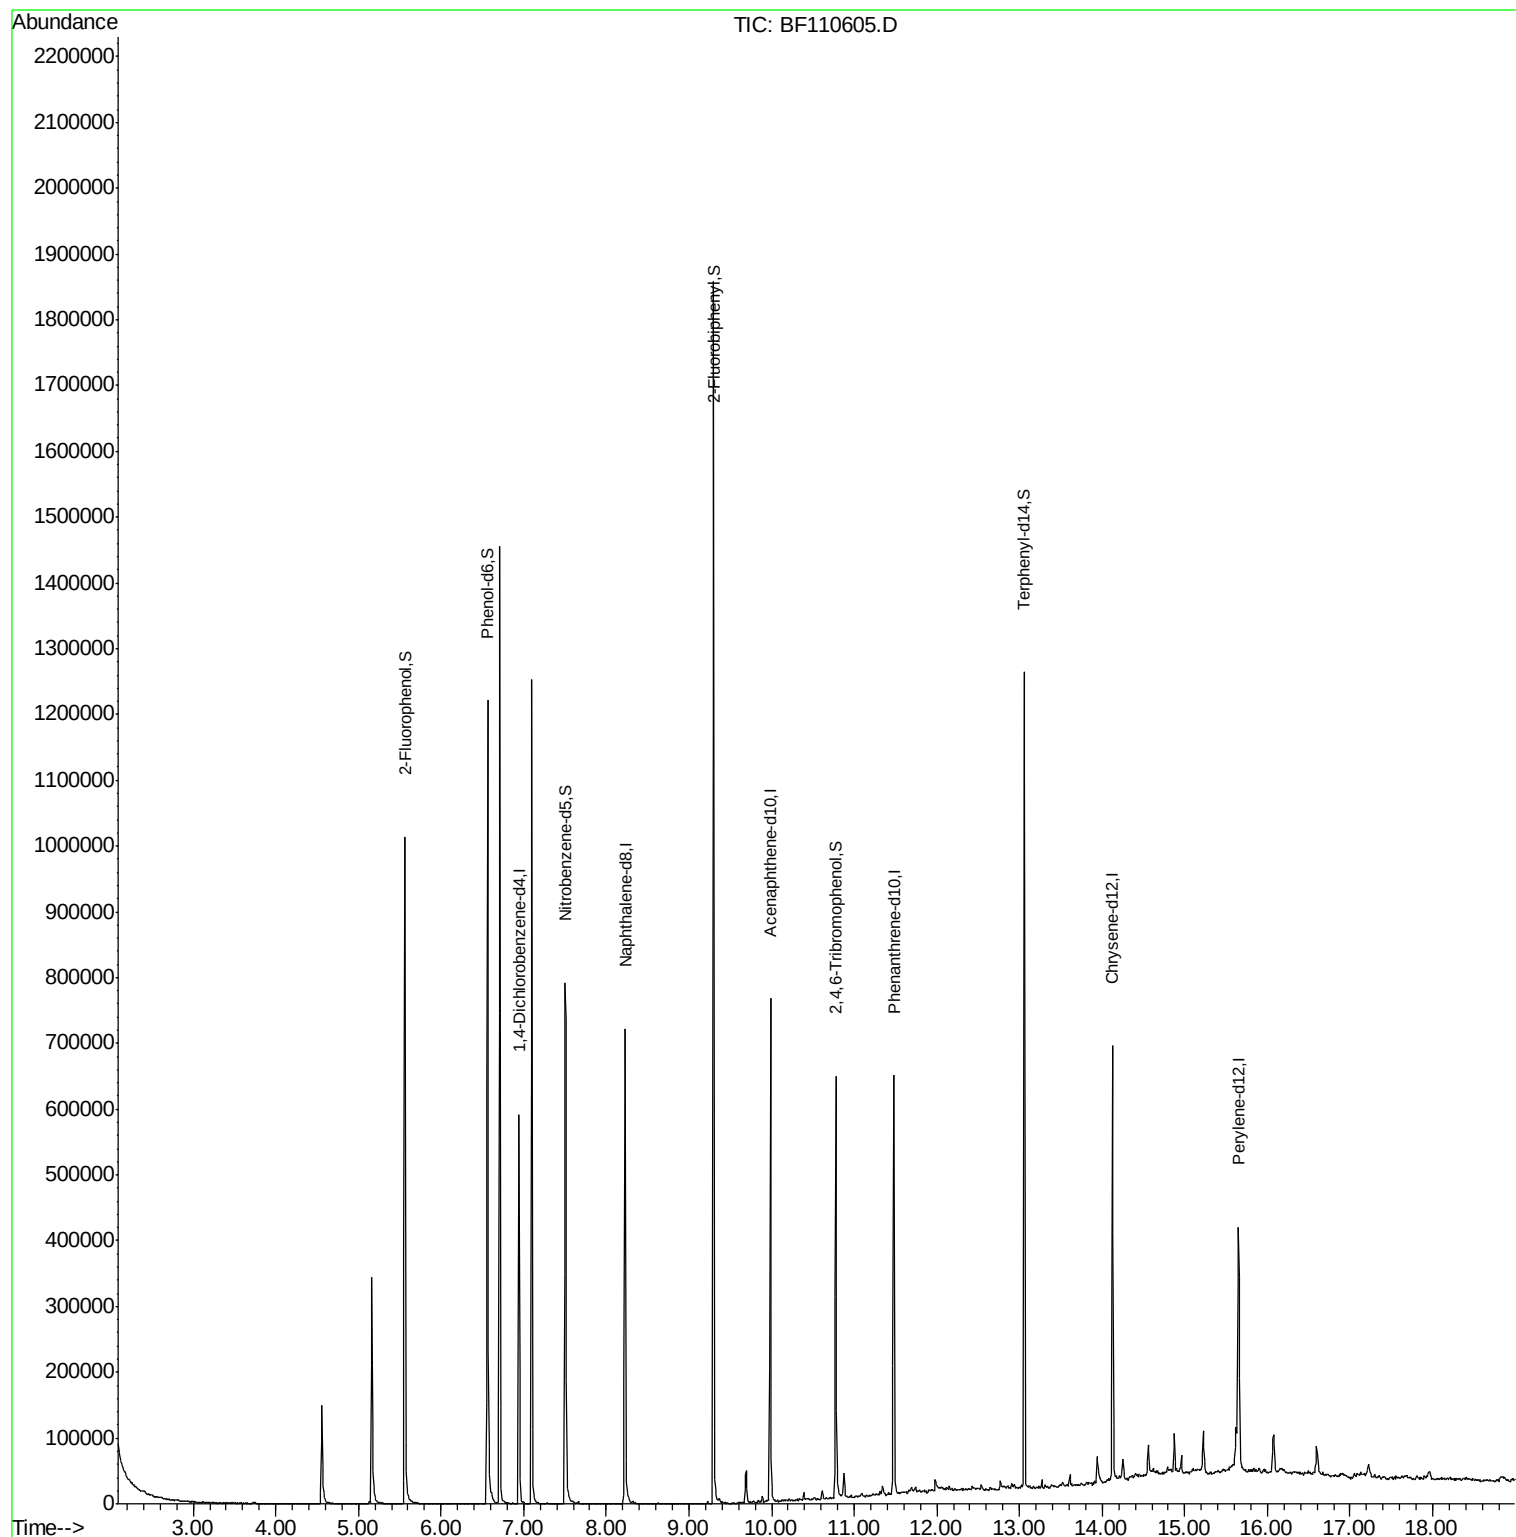

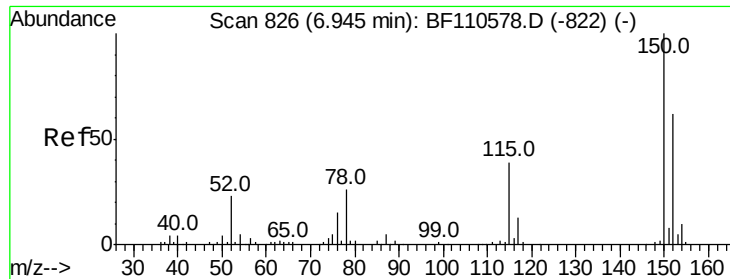


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.95 min Scan# 826
Delta R.T. 0.00 min
Lab File: BF110605.D
Acq: 9 Nov 2018 00:29

Instrument :
BNA_F
ClientSampleId :
PS-CON-2

Tot Ion:152 Resp: 88718
Ion Ratio Lower Upper
152 100
150 156.6 122.7 184.1
115 60.5 49.1 73.7

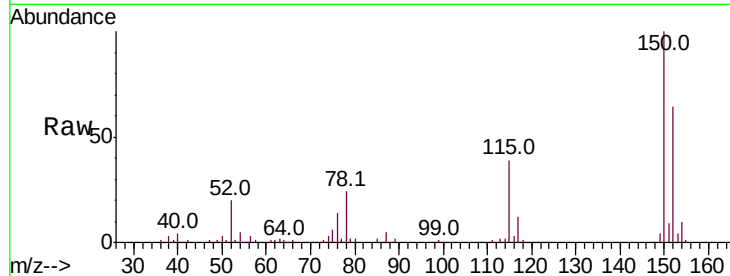


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

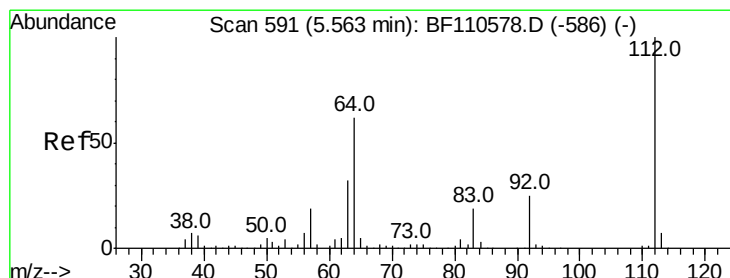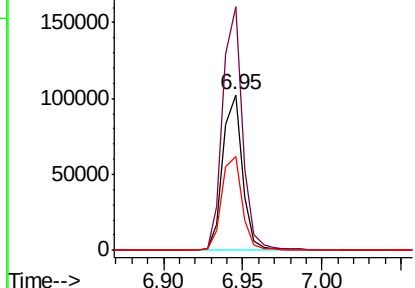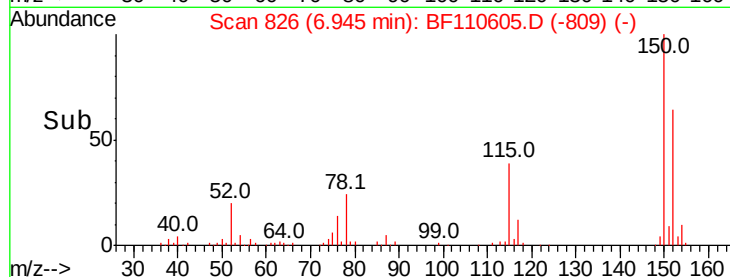



#5


2-Fluorophenol
Concen: 57.106 ng
RT: 5.56 min Scan# 591
Delta R.T. 0.00 min
Lab File: BF110605.D
Acq: 9 Nov 2018 00:29

Tgt Ion:112 Resp: 311908
Ion Ratio Lower Upper
112 100
64 57.2 44.1 66.1
63 30.2 23.7 35.5

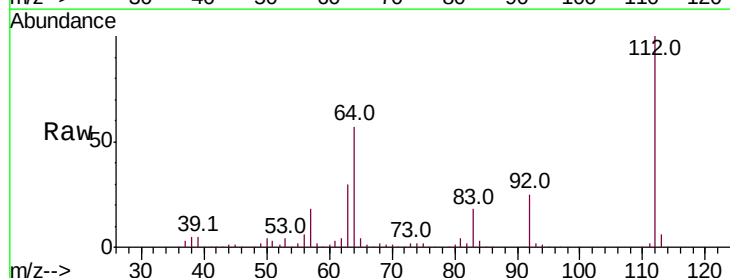

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

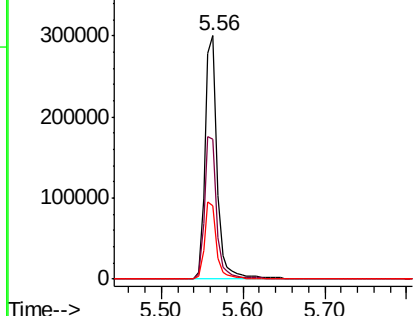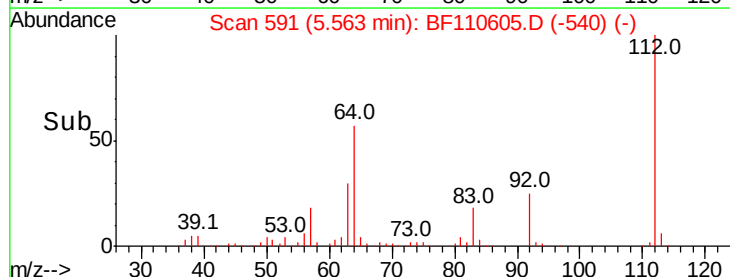

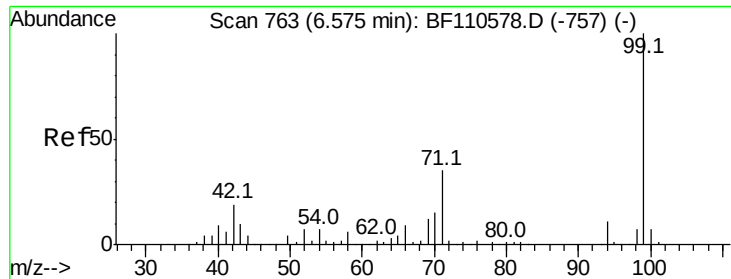

#7

Phenol-d6

Concen: 63.058 ng

RT: 6.56 min Scan# 761

Delta R.T. -0.01 min

Lab File: BF110605.D

Acq: 9 Nov 2018 00:29

Instrument :

BNA_F

ClientSampled :

PS-CON-2


Tot Ion: 99 Resp: 440422

Ion Ratio Lower Upper

99 100

42 20.1 15.8 23.6




71 35.2 28.0 42.0



Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

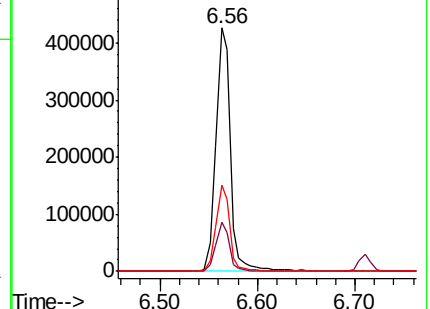

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.23 min Scan# 1044

Delta R.T. 0.00 min

Lab File: BF110605.D

Acq: 9 Nov 2018 00:29

Tgt Ion: 136 Resp: 364557


Ion Ratio Lower Upper

136 100

137 10.4 8.8 13.2

54 7.2 5.4 8.2

68 4.6 4.2 6.2






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

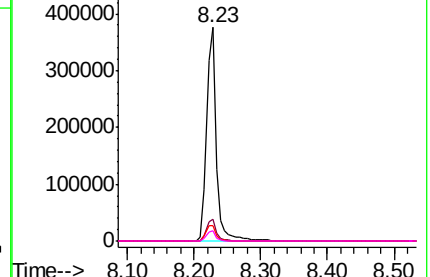


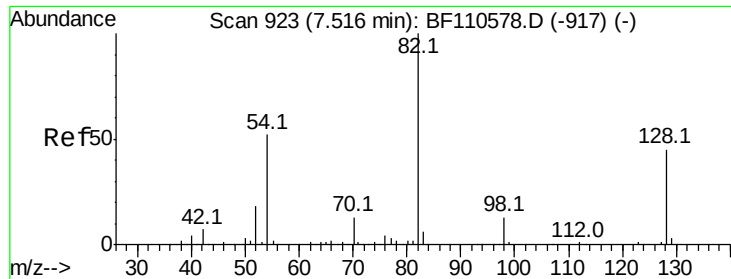




#23
 Nitrobenzene-d5
 Concen: 44.683 ng
 RT: 7.50 min Scan# 921
 Delta R.T. -0.01 min
 Lab File: BF110605.D
 Acq: 9 Nov 2018 00:29

Instrument :
 BNA_F
 ClientSampled :
 PS-CON-2

Tot Ion	82	Resp	282857
Ion Ratio	Lower	Upper	
82	100		
128	43.0	34.2	51.2
54	53.5	38.6	58.0

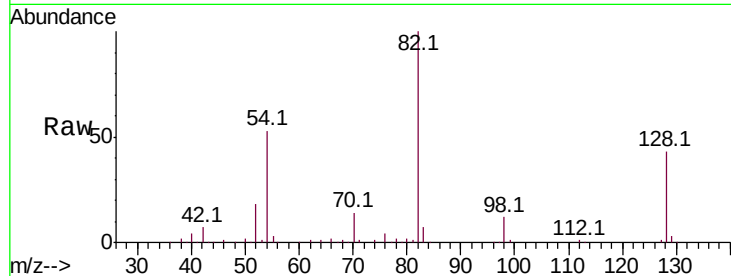


Abundance Ion 82.00 (81.70 to 82.70): BF1
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF1


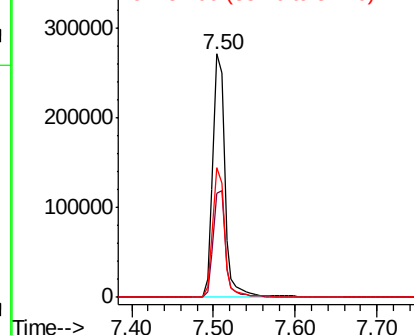



#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.99 min Scan# 1343
 Delta R.T. -0.01 min
 Lab File: BF110605.D
 Acq: 9 Nov 2018 00:29

Tgt Ion	164	Resp	157532
Ion Ratio	Lower	Upper	
164	100		
162	105.4	83.0	124.6
160	47.3	37.0	55.6



Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

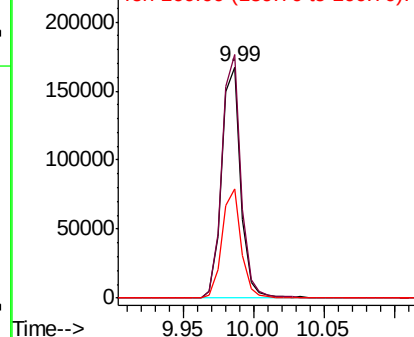







#42
 2,4,6-Tribromophenol
 Concen: 44.809 ng
 RT: 10.77 min Scan# 1477
 Delta R.T. -0.01 min
 Lab File: BF110605.D
 Acq: 9 Nov 2018 00:29

Instrument :
 BNA_F
 ClientSampleId :
 PS-CON-2

Tot Ion:330 Resp: 71127
 Ion Ratio Lower Upper
 330 100
 332 97.5 77.1 115.7
 141 38.8 27.0 40.4

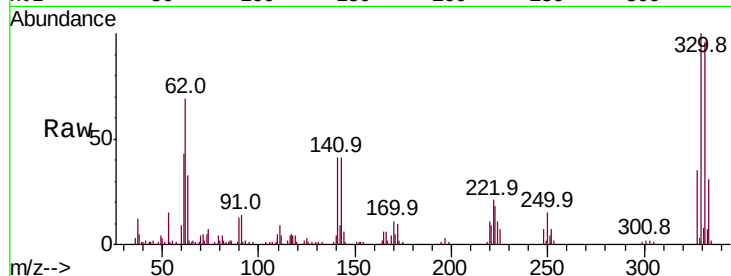


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

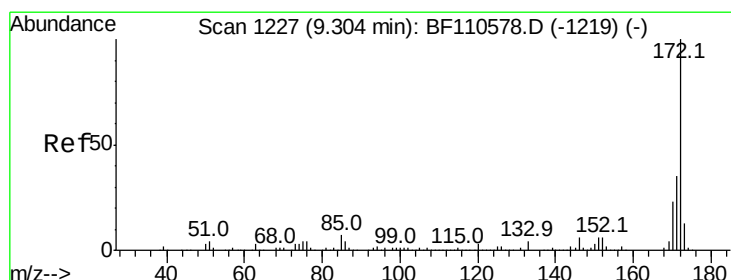
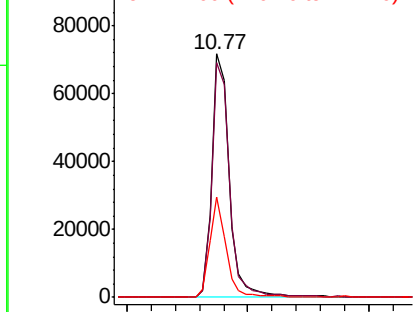



#45
 2-Fluorobiphenyl
 Concen: 48.991 ng
 RT: 9.30 min Scan# 1226
 Delta R.T. -0.01 min
 Lab File: BF110605.D
 Acq: 9 Nov 2018 00:29

Tgt Ion:172 Resp: 540383
 Ion Ratio Lower Upper
 172 100
 171 35.5 28.6 43.0
 170 23.3 19.7 29.5



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E




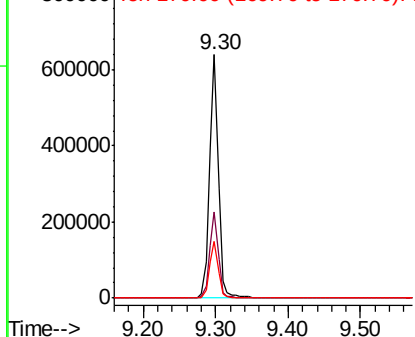


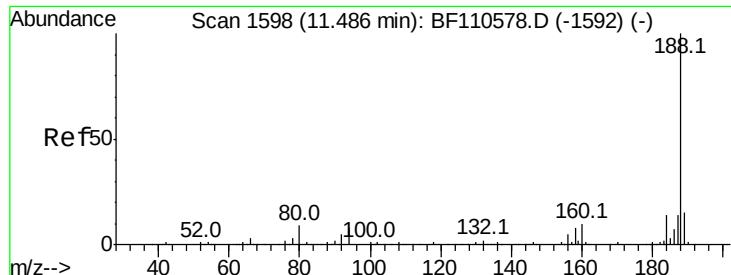

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.48 min Scan# 1597
Delta R.T. -0.01 min
Lab File: BF110605.D
Acq: 9 Nov 2018 00:29




Instrument :
BNA_F
ClientSampleId :
PS-CON-2


Tot Ion:188 Resp: 250671
Ion Ratio Lower Upper
188 100
94 8.2 7.2 10.8
80 8.1 7.9 11.9

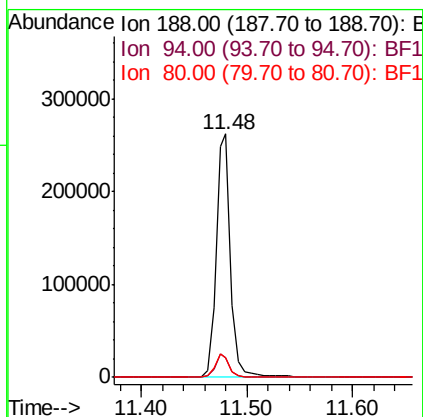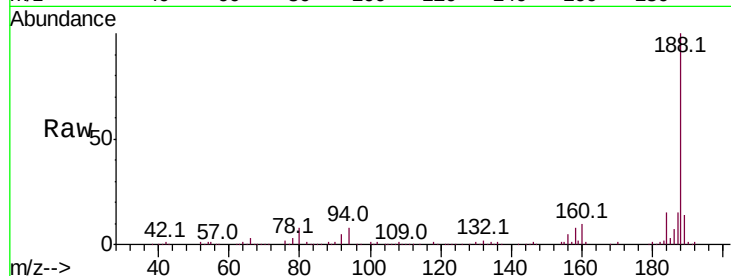

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.13 min Scan# 2047
Delta R.T. -0.01 min
Lab File: BF110605.D
Acq: 9 Nov 2018 00:29

Tgt Ion:240 Resp: 208046
Ion Ratio Lower Upper
240 100
120 11.0 8.3 12.5
236 25.6 21.2 31.8

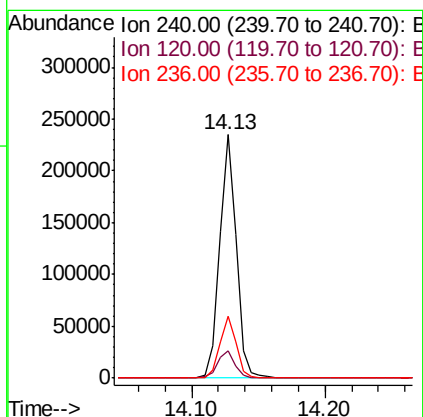

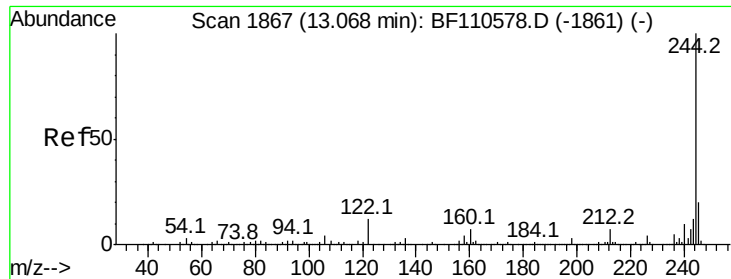

#79

Terphenyl-d14

Concen: 37.435 ng

RT: 13.06 min Scan# 1865

Delta R.T. -0.01 min

Lab File: BF110605.D

Acq: 9 Nov 2018 00:29

Instrument :

BNA_F

ClientSampleId :

PS-CON-2



Tot Ion:244 Resp: 415870

Ion Ratio Lower Upper

244 100

212 6.9 5.8 8.8



122 12.6 8.7 13.1



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

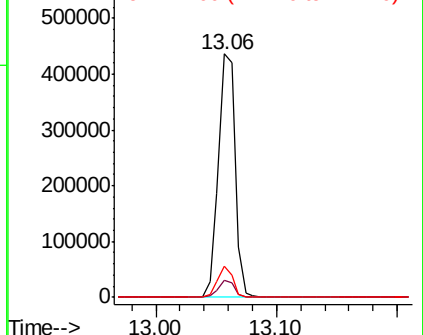

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.65 min Scan# 2306

Delta R.T. -0.01 min

Lab File: BF110605.D

Acq: 9 Nov 2018 00:29



Tgt Ion:264 Resp: 168887

Ion Ratio Lower Upper

264 100

260 23.6 18.7 28.1

265 20.5 16.7 25.1



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

