


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110818\
 Data File : BF110574.D
 Acq On : 8 Nov 2018 10:22
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Nov 08 14:14:47 2018

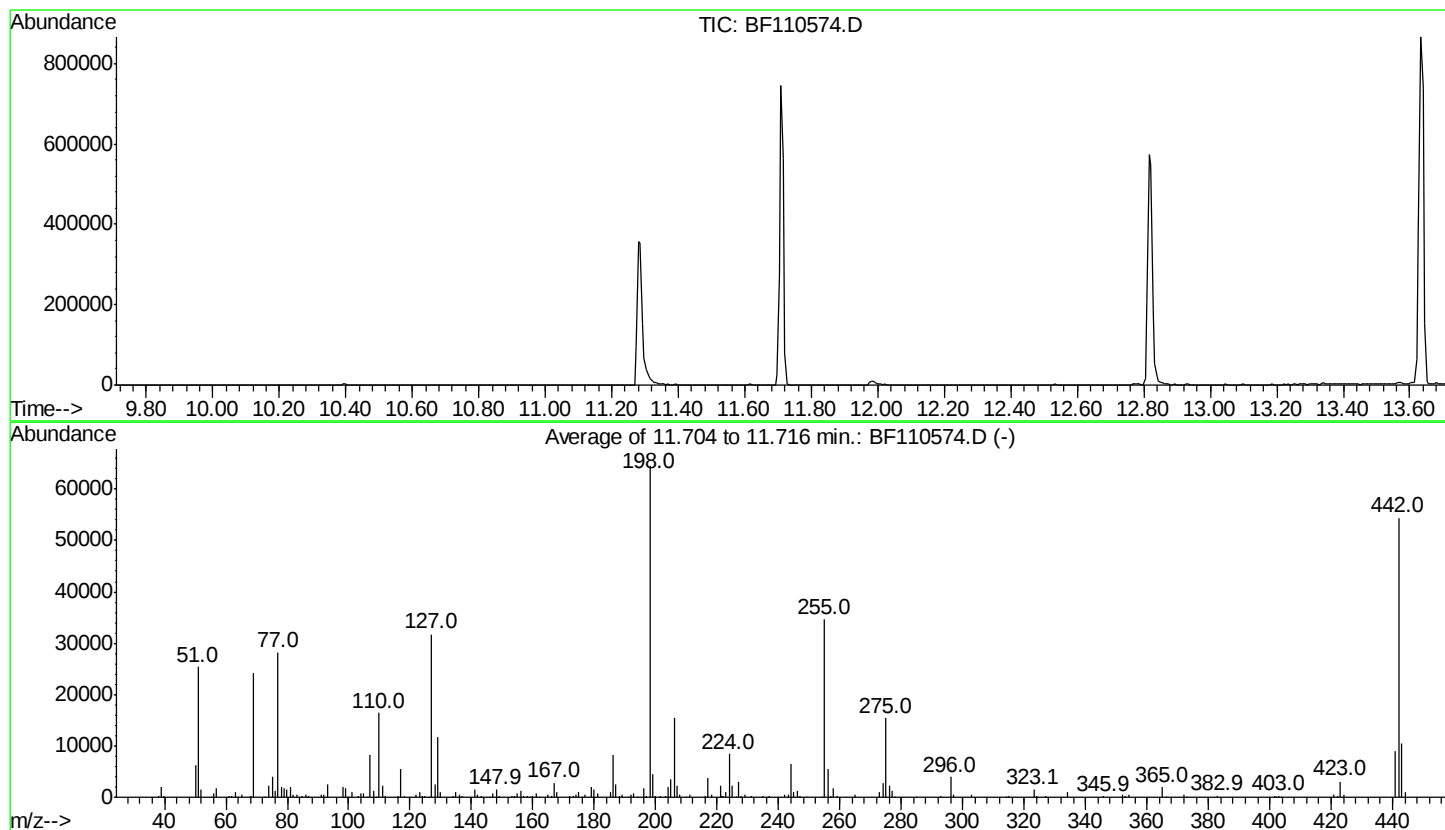

AutoFind: Scans 1635, 1636, 1637; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.3	25373	PASS
68	69	0.00	2	1.4	330	PASS
69	198	0.00	100	37.6	24258	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.1	31714	PASS
197	198	0.00	2	0.2	157	PASS
198	198	100	100	100.0	64560	PASS
199	198	5	9	6.8	4389	PASS
275	198	10	60	23.9	15407	PASS
365	198	1	100	3.0	1959	PASS
441	198	0.01	100	13.7	8862	PASS
442	198	50	100	84.2	54366	PASS
443	442	15	24	19.3	10492	PASS