


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110818\
 Data File : BF110583.D
 Acq On : 8 Nov 2018 14:33
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Nov 08 14:14:47 2018

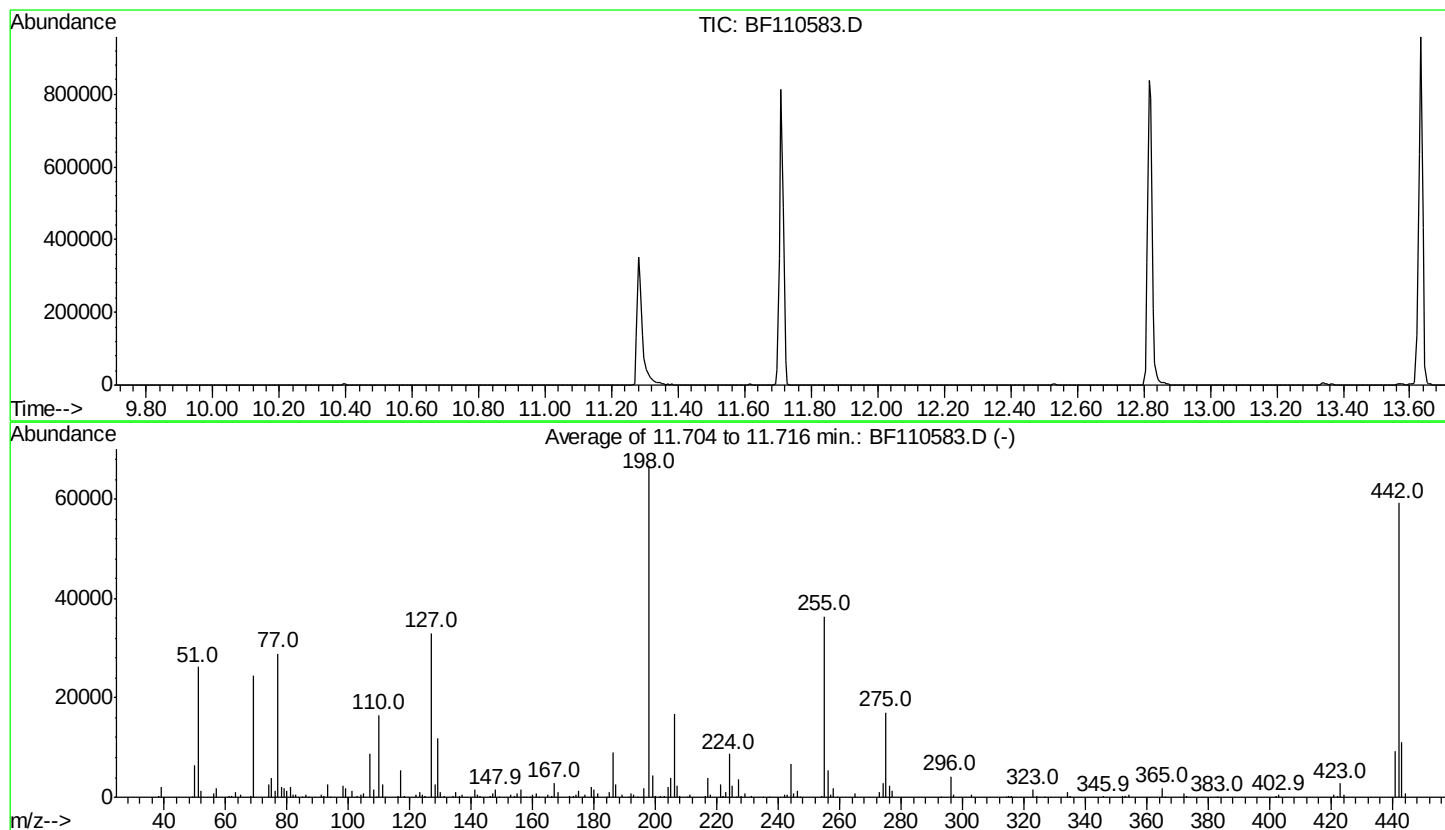

AutoFind: Scans 1635, 1636, 1637; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.4	26274	PASS
68	69	0.00	2	1.2	288	PASS
69	198	0.00	100	36.5	24383	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.5	33018	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	66757	PASS
199	198	5	9	6.6	4414	PASS
275	198	10	60	25.6	17084	PASS
365	198	1	100	2.8	1896	PASS
441	198	0.01	100	14.0	9356	PASS
442	198	50	100	88.7	59197	PASS
443	442	15	24	18.7	11057	PASS