


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF110819\
 Data File : BF117728.D
 Acq On : 8 Nov 2019 12:46
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 06 17:27:10 2019

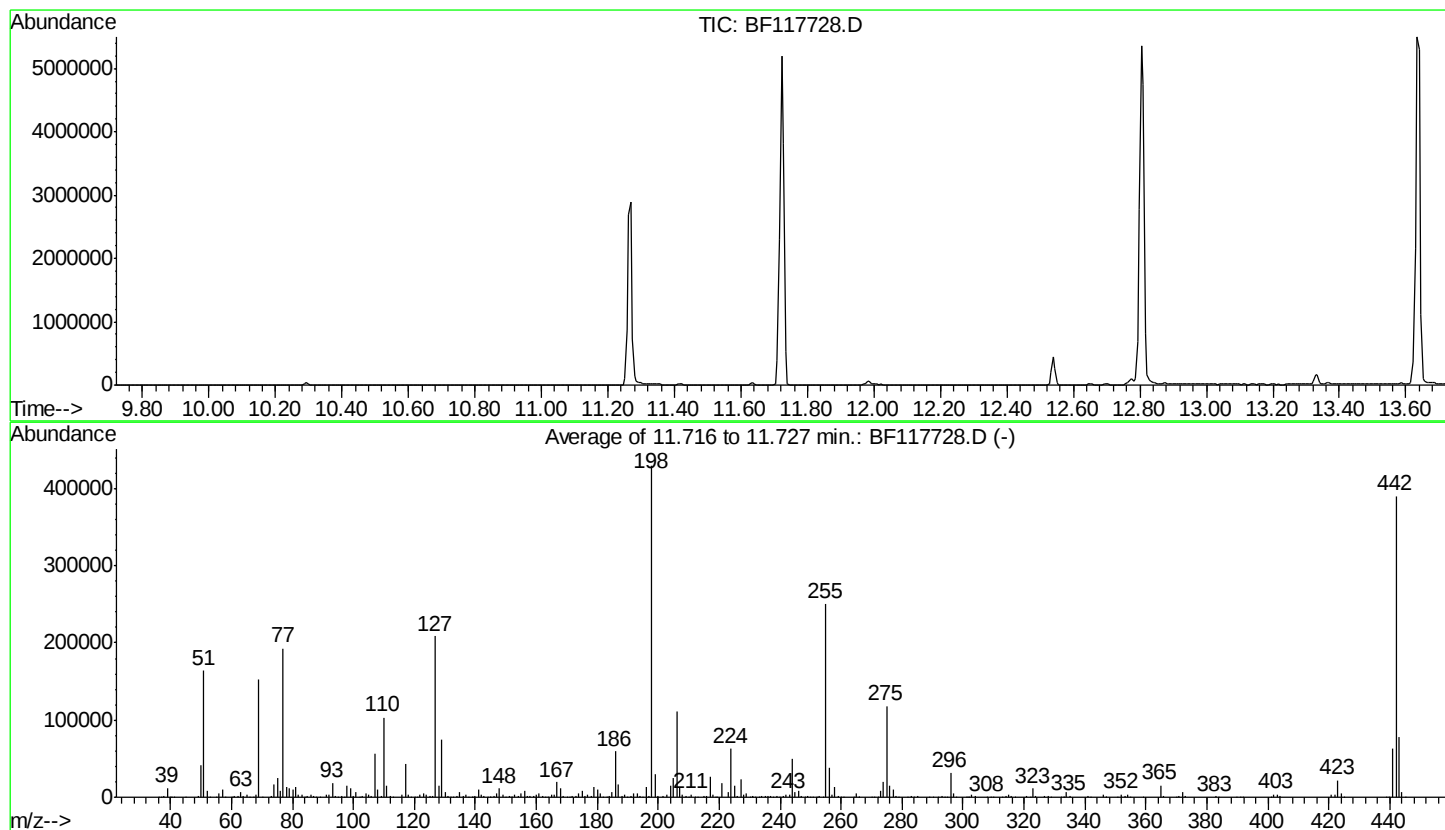

AutoFind: Scans 1637, 1638, 1639; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.1	163909	PASS
68	69	0.00	2	1.7	2581	PASS
69	198	0.00	100	35.5	152584	PASS
70	69	0.00	2	0.5	754	PASS
127	198	10	80	48.5	208554	PASS
197	198	0.00	2	0.3	1428	PASS
198	198	100	100	100.0	429781	PASS
199	198	5	9	6.8	29157	PASS
275	198	10	60	27.6	118501	PASS
365	198	1	100	3.6	15511	PASS
441	198	0.01	100	14.6	62813	PASS
442	198	50	100	90.9	390533	PASS
443	442	15	24	19.8	77392	PASS