
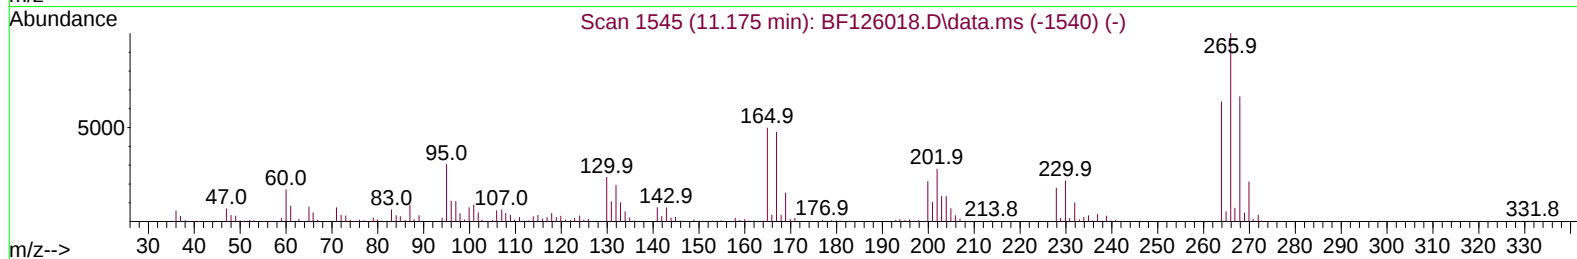
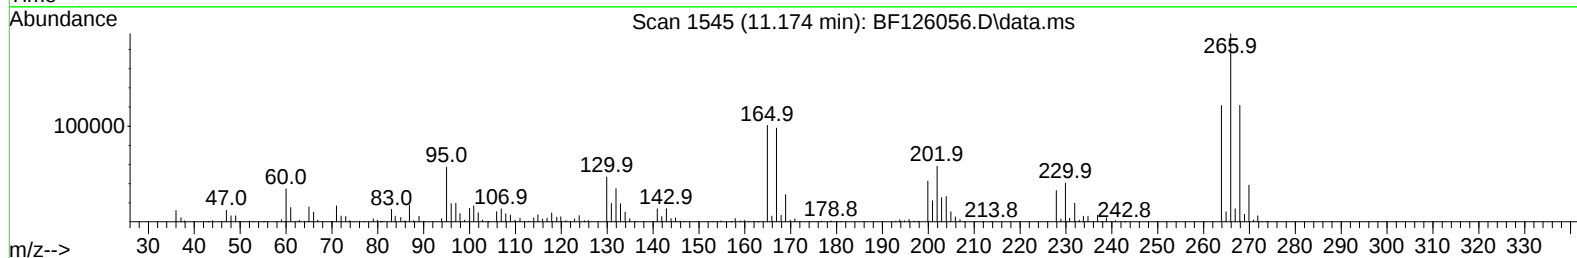


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110821\
Data File : BF126056.D
Acq On : 8 Nov 2021 9:57
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 08 11:30:14 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 03 17:21:25 2021
Response via : Initial Calibration

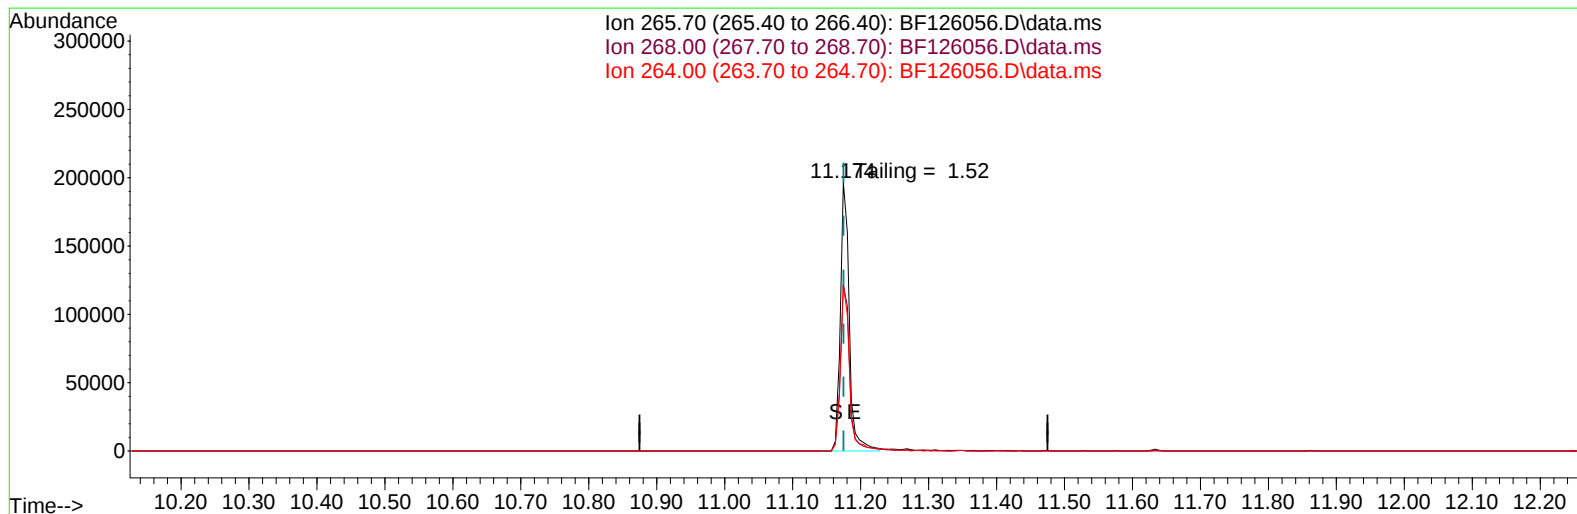

TIC: BF126056.D\data.ms

(70) Pentachlorophenol (C)




11.174min (-0.001) 20431.08 ng

response 181508

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	61.92
264.00	69.90	61.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110821\
Data File : BF126056.D
Acq On : 8 Nov 2021 9:57
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 08 11:30:14 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 03 17:21:25 2021
Response via : Initial Calibration

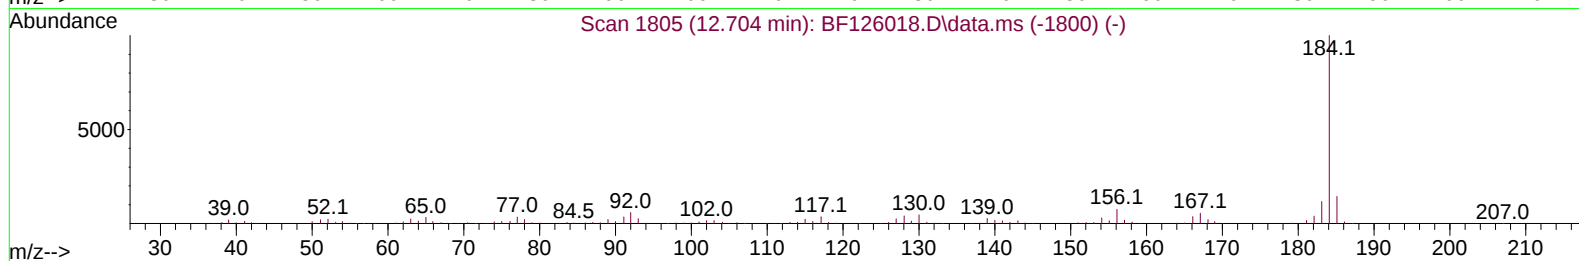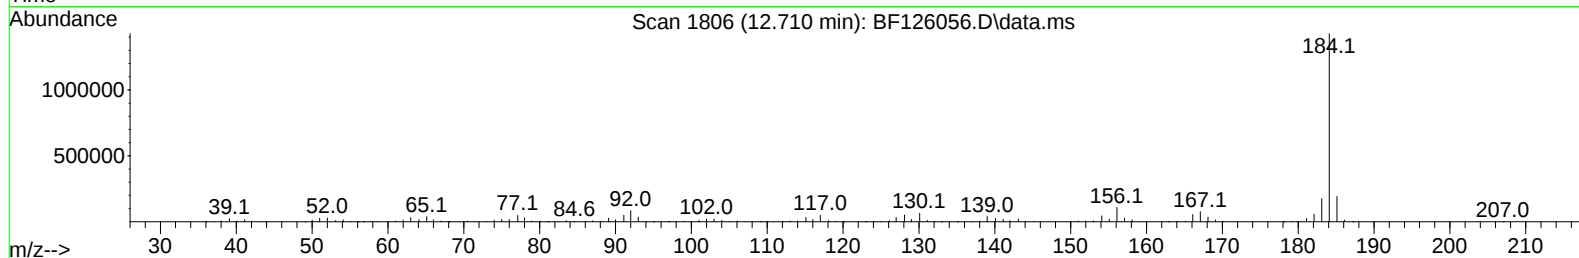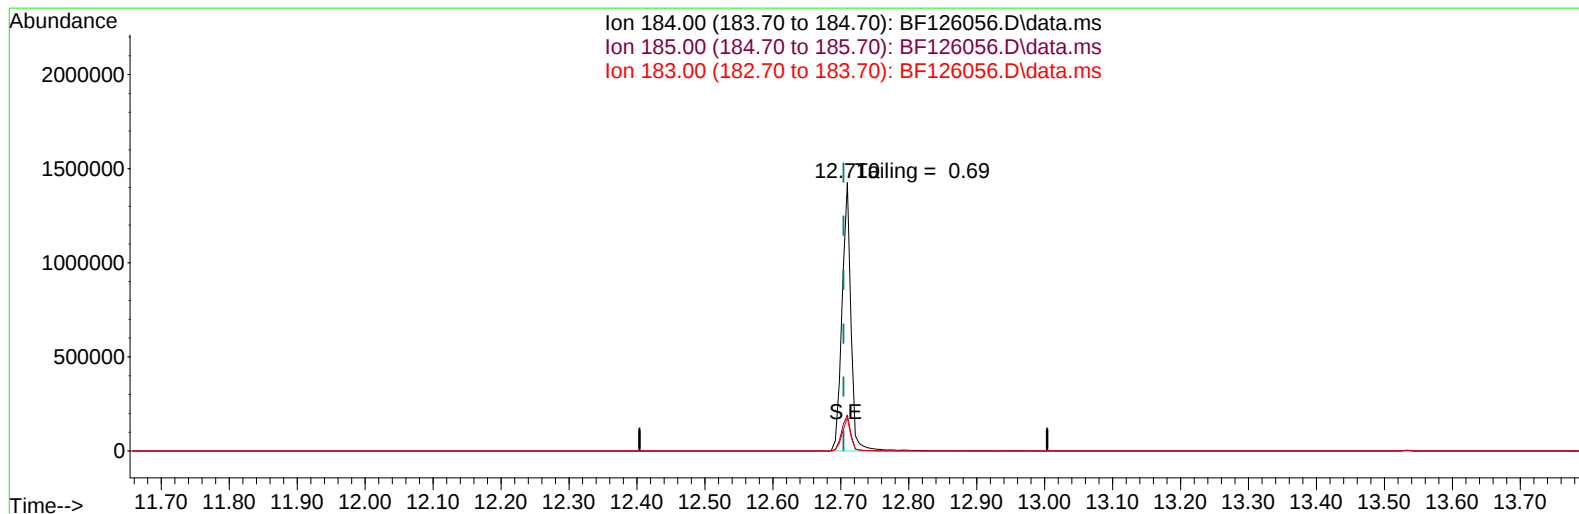

TIC: BF126056.D\data.ms

(77) Benzidine

12.710min (+ 0.006) 0.00 ng

response 1294101

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	13.45
183.00	10.10	12.37#
0.00	0.00	0.00