


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110821\
 Data File : BF126056.D
 Acq On : 8 Nov 2021 9:57
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 03 17:21:25 2021

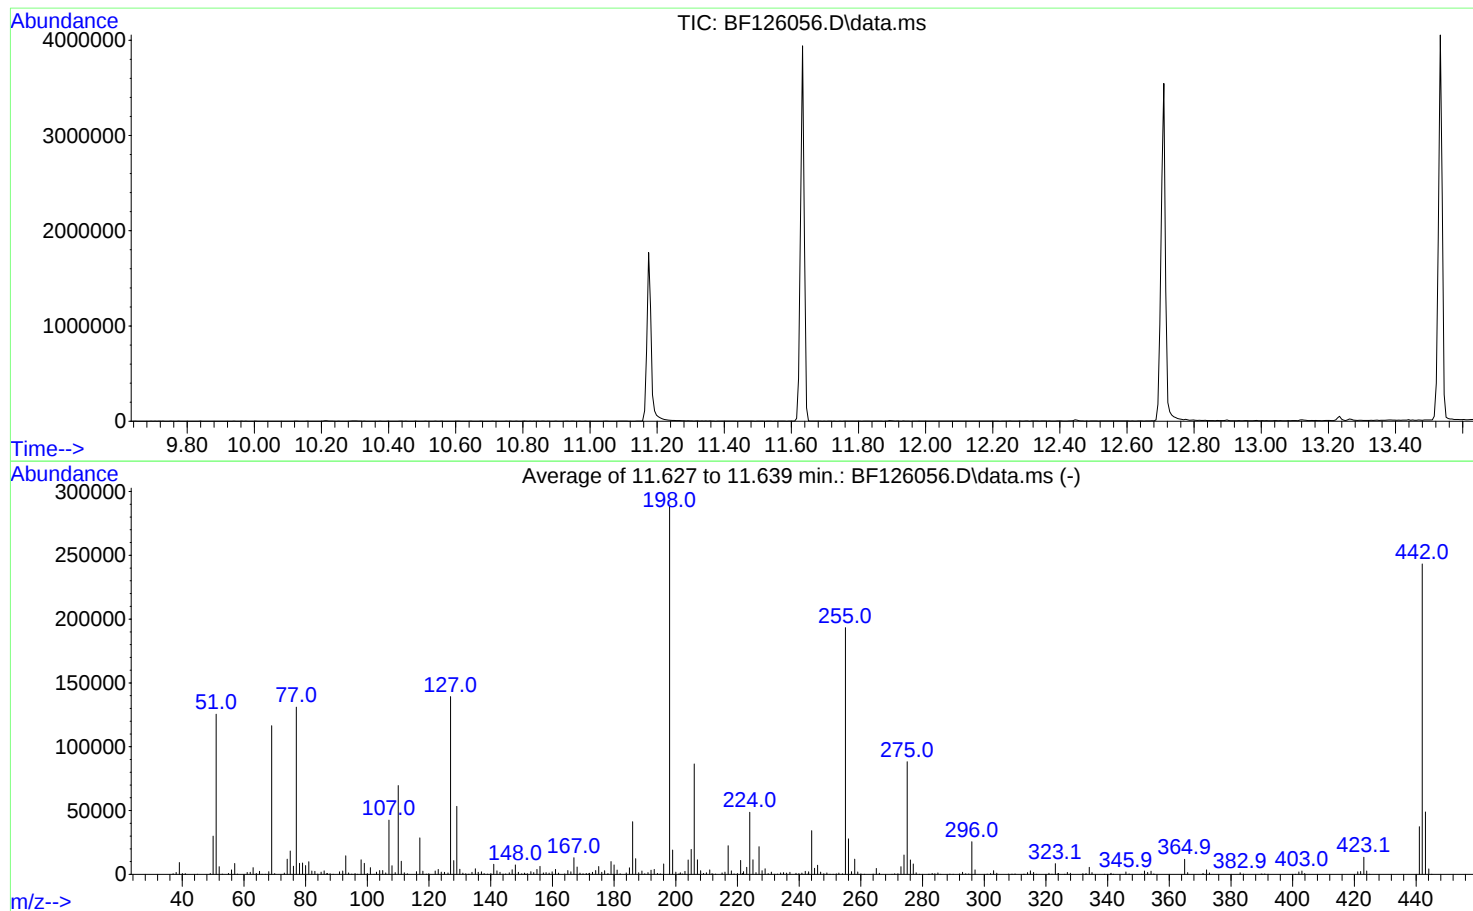




AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.5	125496	PASS
68	69	0.00	2	1.8	2082	PASS
69	198	0.00	100	40.4	116528	PASS
70	69	0.00	2	0.6	647	PASS
127	198	10	80	48.3	139253	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	288235	PASS
199	198	5	9	6.6	19085	PASS
275	198	10	60	30.6	88291	PASS
365	198	1	100	4.1	11842	PASS
441	198	0.01	100	13.0	37368	PASS
442	442	50	100	100.0	243203	PASS
443	442	15	24	20.1	48893	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110821\
 Data File : BF126056.D
 Acq On : 8 Nov 2021 9:57
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Nov 08 11:30:14 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 03 17:21:25 2021
 Response via : Initial Calibration

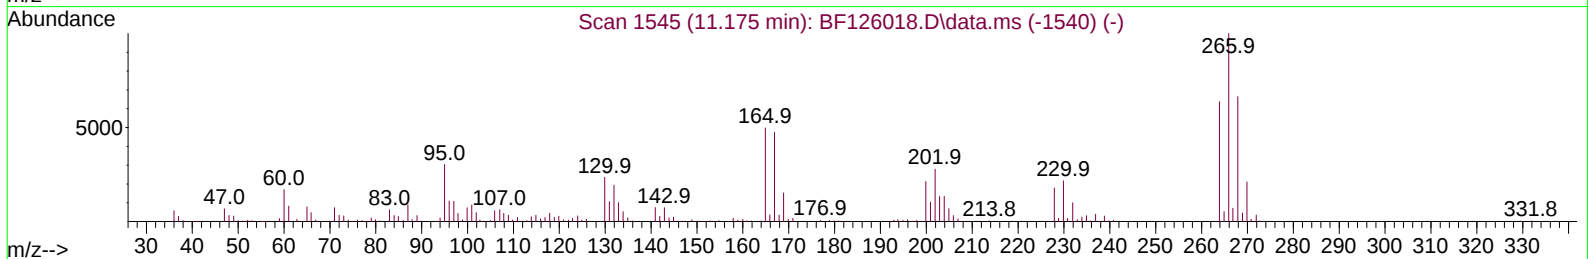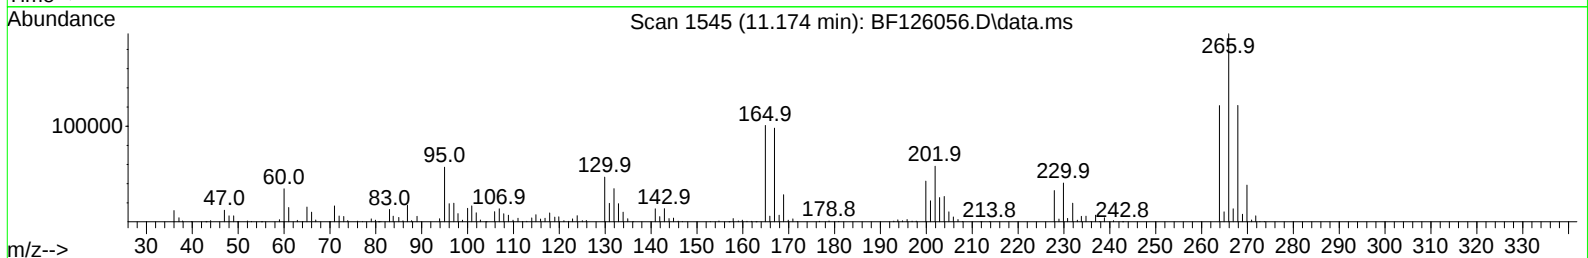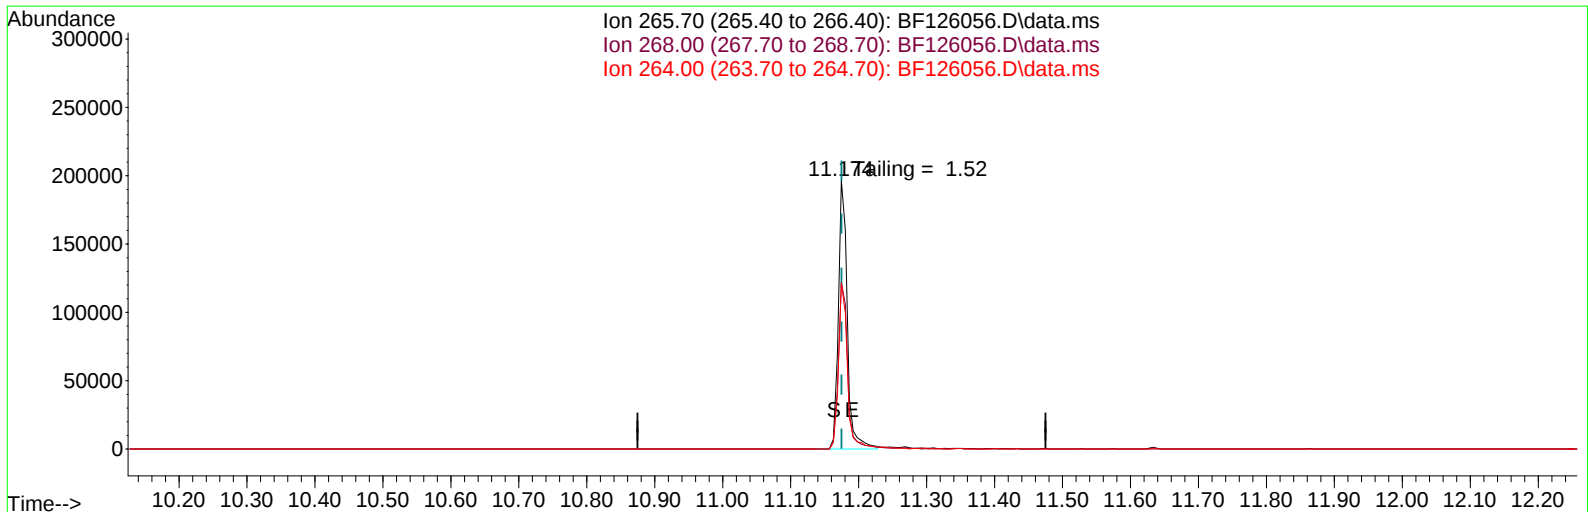

TIC: BF126056.D\data.ms

(70) Pentachlorophenol (C)

11.174min (-0.001) 20431.08 ng




response 181508

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	61.92
264.00	69.90	61.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110821\
Data File : BF126056.D
Acq On : 8 Nov 2021 9:57
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 08 11:30:14 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 03 17:21:25 2021
Response via : Initial Calibration

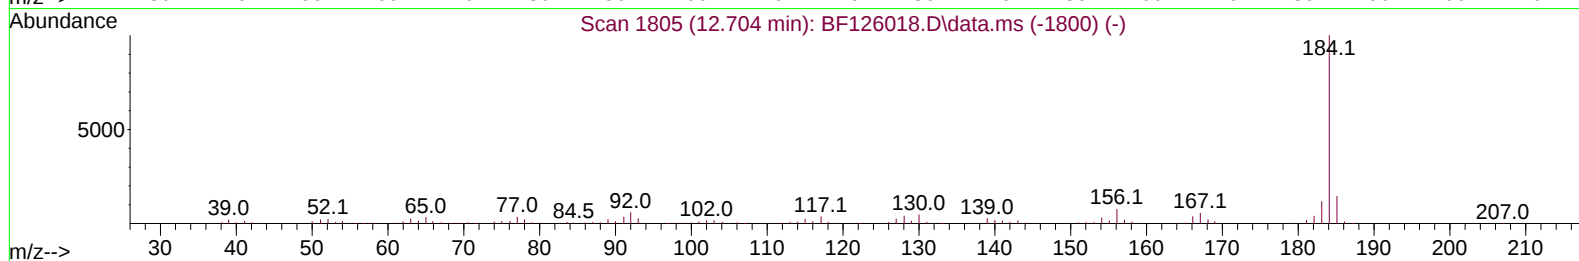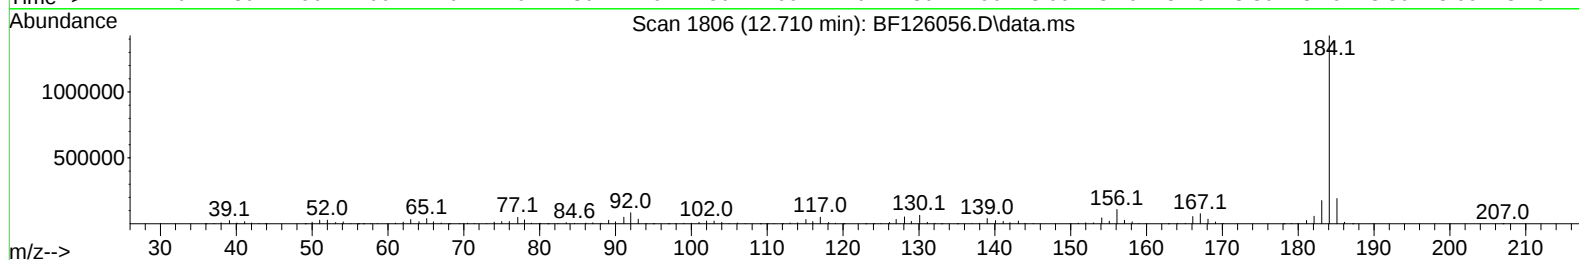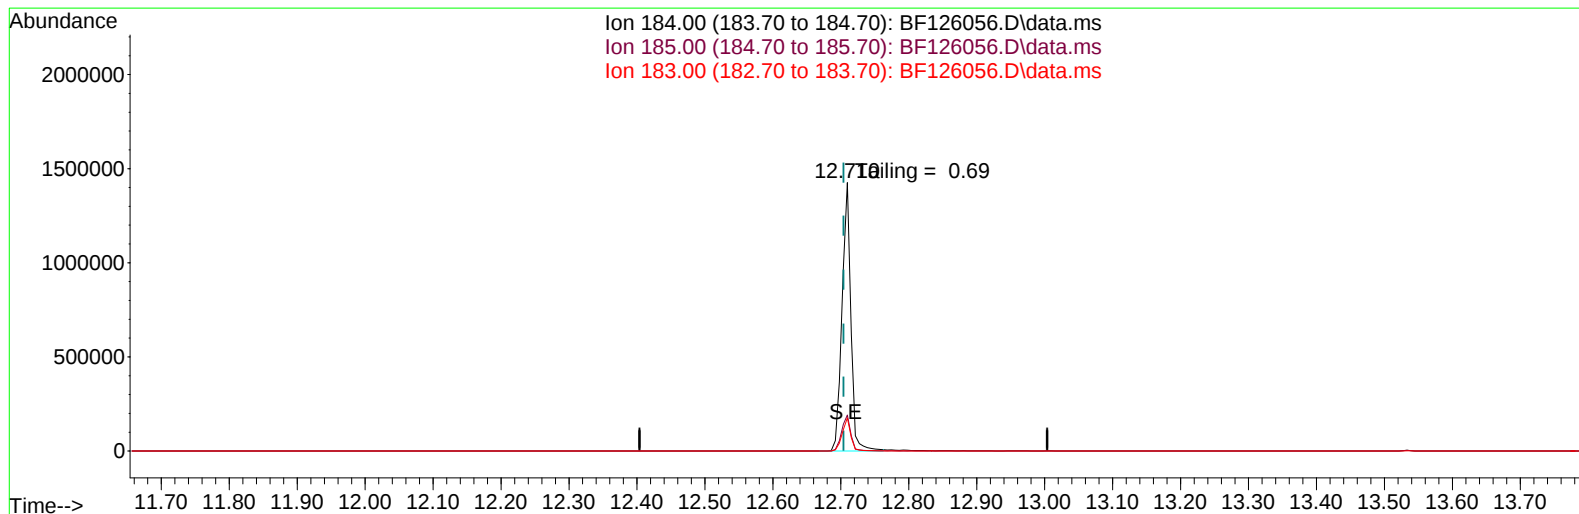

TIC: BF126056.D\data.ms

(77) Benzidine

12.710min (+ 0.006) 0.00 ng

response 1294101

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	13.45
183.00	10.10	12.37#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/8/2021	BNA_F	<u>BF126056.D</u>
Compound Name	Response	Retention Time
DDT	579059	13.53
DDD	7139	13.23
DDE	1033	12.89
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8172	587231	1.39

Instrument :
BNA_F
ClientSampleId :
DFTPP