

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF110918\
 Data File : BF110635.D
 Acq On : 9 Nov 2018 18:53
 Operator : JU/SJ
 Sample : J5864-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Nov 11 03:23:26 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF110818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 09 15:13:13 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.95	152	72122	20.00	ng	0.00
21) Naphthalene-d8	8.23	136	294075	20.00	ng	0.00
39) Acenaphthene-d10	9.99	164	143874	20.00	ng	0.00
64) Phenanthrene-d10	11.48	188	289690	20.00	ng	0.00
76) Chrysene-d12	14.13	240	226422	20.00	ng	-0.01
87) Perylene-d12	15.66	264	140064	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.56	112	431636	97.21	ng	0.00
7) Phenol-d6	6.57	99	551623	97.15	ng	0.00
23) Nitrobenzene-d5	7.51	82	344824	67.53	ng	0.00
42) 2,4,6-Tribromophenol	10.78	330	120480	83.11	ng	0.00
45) 2-Fluorobiphenyl	9.30	172	660460	65.56	ng	0.00
79) Terphenyl-d14	13.06	244	727054	60.14	ng	0.00
Target Compounds						
9) Benzaldehyde	6.57	77	987	Below Cal	Qvalue	# 1
10) Phenol	6.58	94	34025	5.168 ng	#	67
19) n-Nitroso-di-n-propylamine	7.51	70	44842	12.372 ng	#	81
25) Isophorone	7.51	82	344822	41.200 ng	#	67
50) Dimethylphthalate	9.69	163	31040	2.891 ng		97
51) 2,6-Dinitrotoluene	9.99	165	18218	7.714 ng	#	23
57) 2,4-Dinitrotoluene	9.99	165	18218	5.933 ng	#	19
67) 4-Bromophenyl-phenylether	10.78	248	7425	2.319 ng	#	1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF110918\
Data File : BF110635.D
Acq On : 9 Nov 2018 18:53
Operator : JU/SJ
Sample : J5864-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Nov 11 03:23:26 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF110818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 09 15:13:13 2018
Response via : Initial Calibration

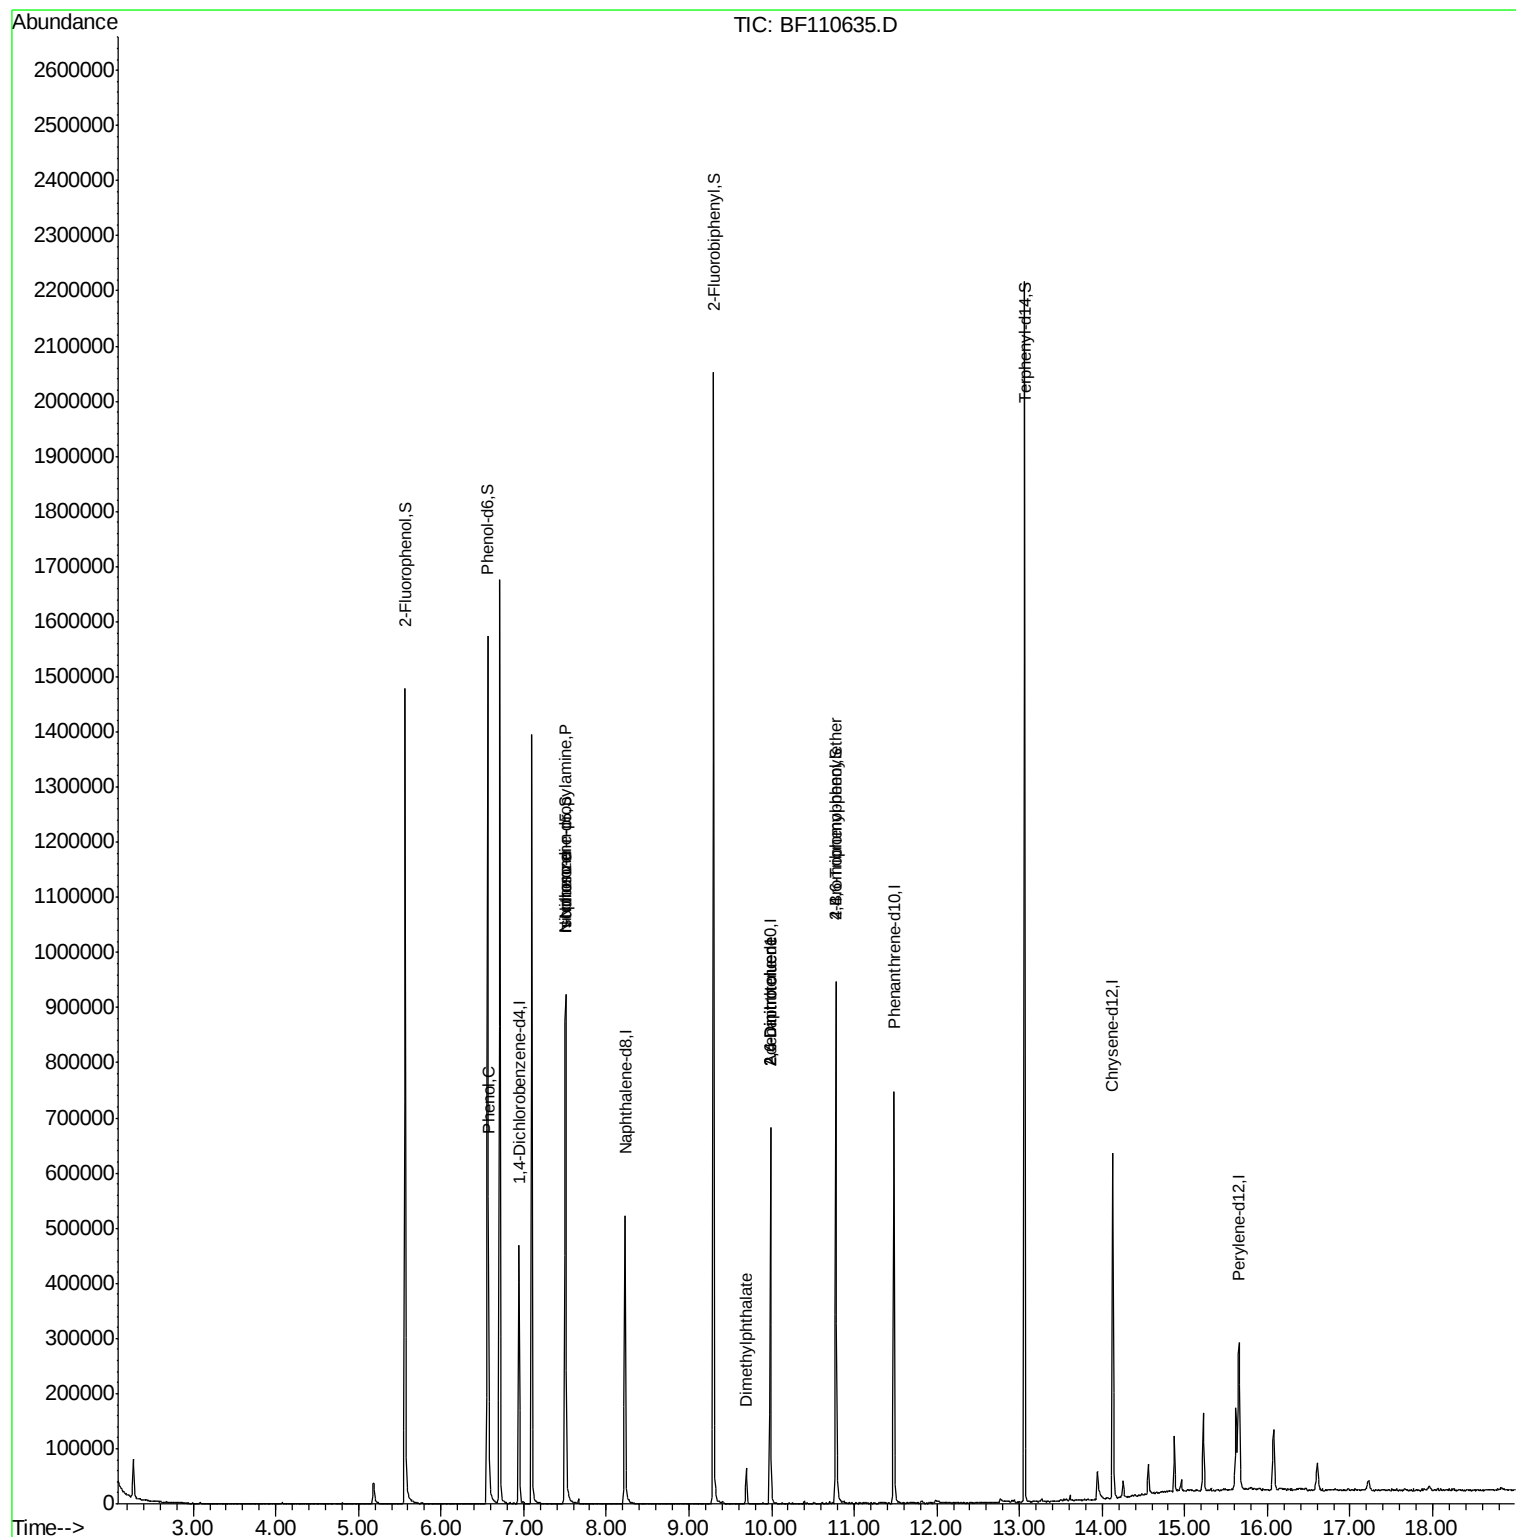




#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.95 min Scan# 826
Delta R.T. 0.00 min
Lab File: BF110635.D
Acq: 9 Nov 2018 18:53

Instrument :
BNA_F
ClientSampleId :

Tot Ion:152 Resp: 72122
Ion Ratio Lower Upper
152 100
150 151.8 122.7 184.1
115 60.6 49.1 73.7

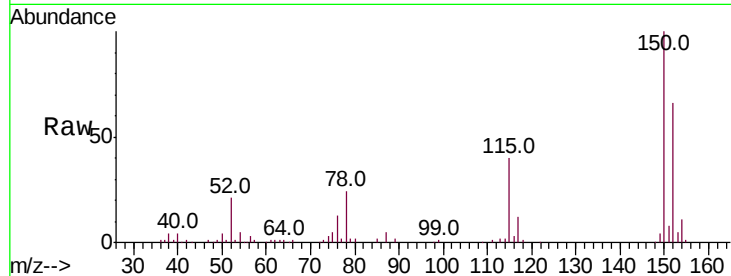


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

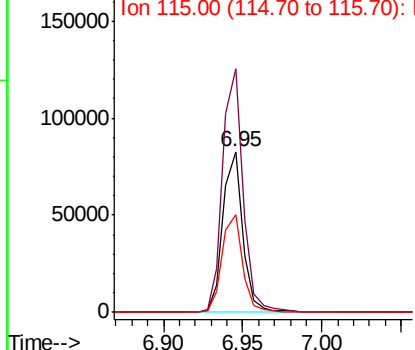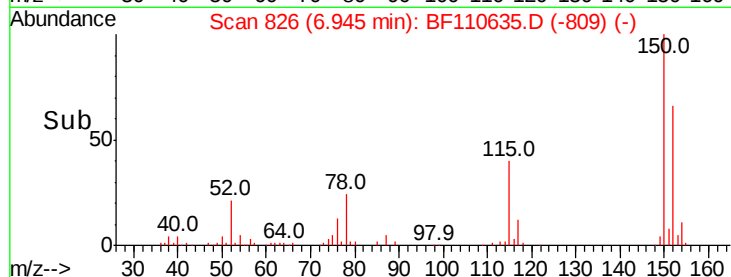



#5


2-Fluorophenol
Concen: 97.212 ng
RT: 5.56 min Scan# 591
Delta R.T. 0.00 min
Lab File: BF110635.D
Acq: 9 Nov 2018 18:53

Tgt Ion:112 Resp: 431636
Ion Ratio Lower Upper
112 100
64 61.2 44.1 66.1
63 32.3 23.7 35.5

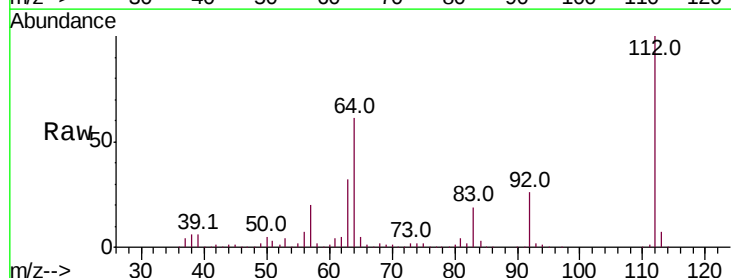

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

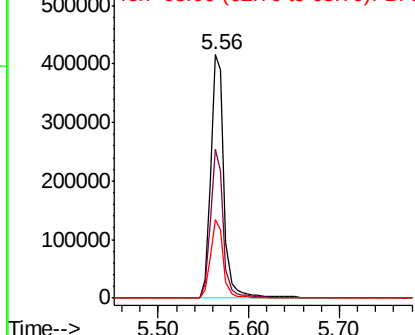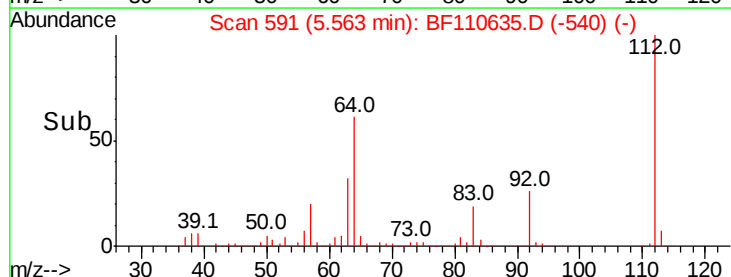

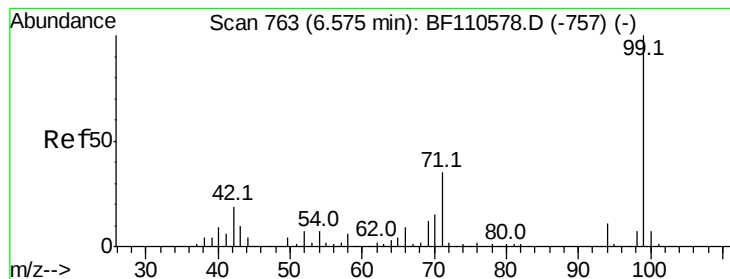

#7

Phenol-d6

Concen: 97.153 ng

RT: 6.57 min Scan# 762

Delta R.T. -0.01 min

Lab File: BF110635.D

Acq: 9 Nov 2018 18:53

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 99 Resp: 551623

Ion Ratio Lower Upper

99 100

42 18.7 15.8 23.6




71 34.4 28.0 42.0

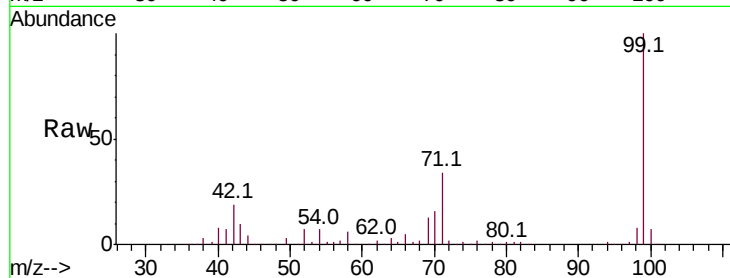

Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

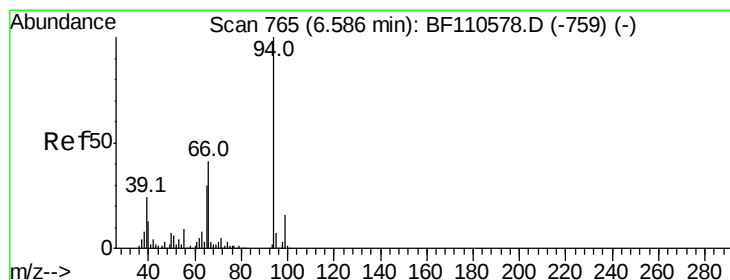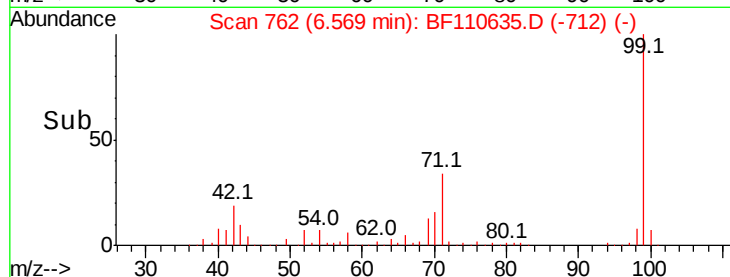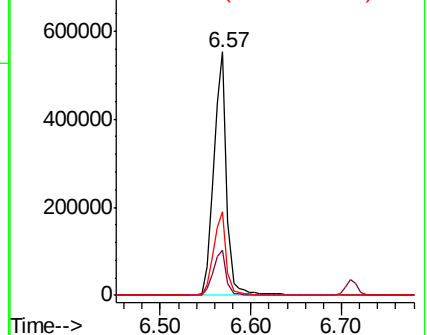

#10

Phenol

Concen: 5.168 ng

RT: 6.58 min Scan# 764

Delta R.T. -0.01 min

Lab File: BF110635.D

Acq: 9 Nov 2018 18:53


Tgt Ion: 94 Resp: 34025

Ion Ratio Lower Upper

94 100

65 28.8 25.3 65.3



66 42.1 54.5 94.5#

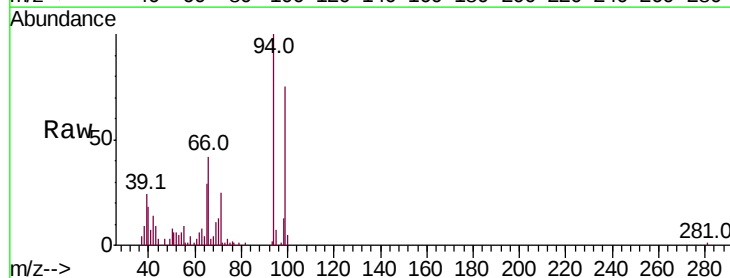


Abundance Ion 94.00 (93.70 to 94.70): BF1

Ion 65.00 (64.70 to 65.70): BF1

Ion 66.00 (65.70 to 66.70): BF1

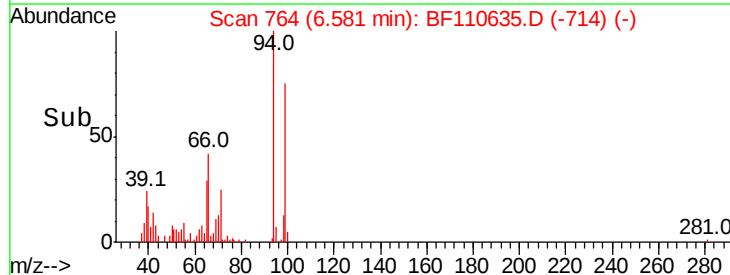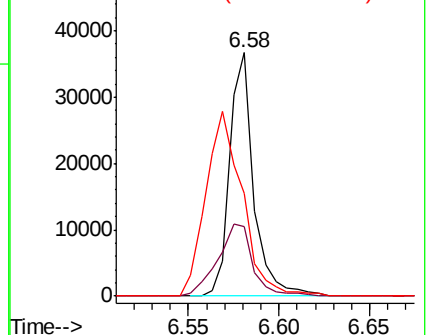

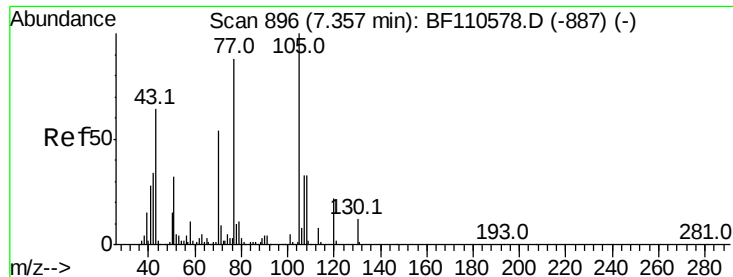

#19

n-Nitroso-di-n-propylamine

Concen: 12.372 ng

RT: 7.51 min Scan# 922

Delta R.T. 0.15 min

Lab File: BF110635.D

Acq: 9 Nov 2018 18:53

Instrument :

BNA_F

ClientSampleId :

Tot Ion: 70 Resp: 44842





Ion Ratio Lower Upper

70 100

42 50.7 47.4 71.2

101 0.0 7.3 10.9#

130 2.0 16.2 24.2#

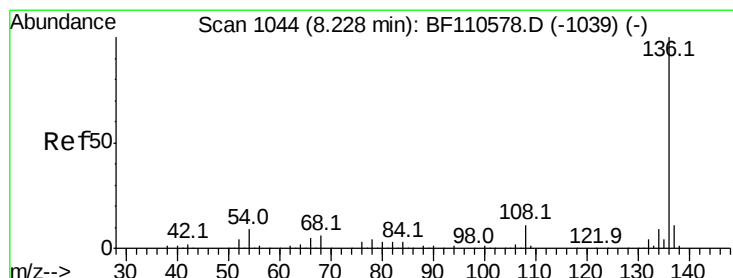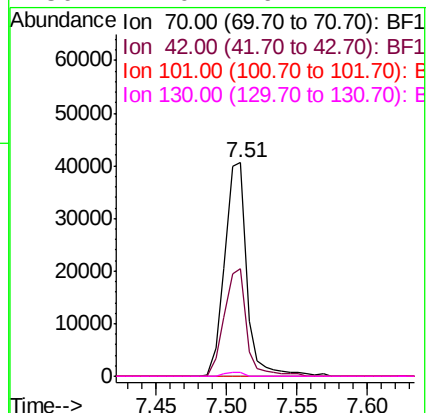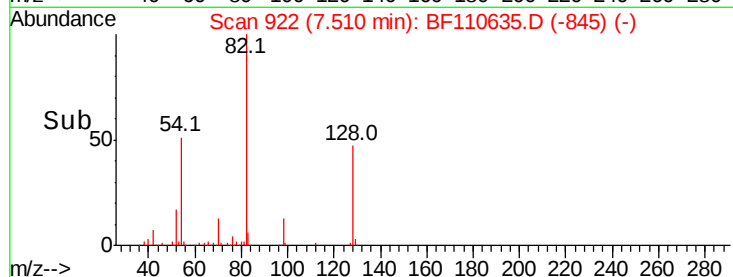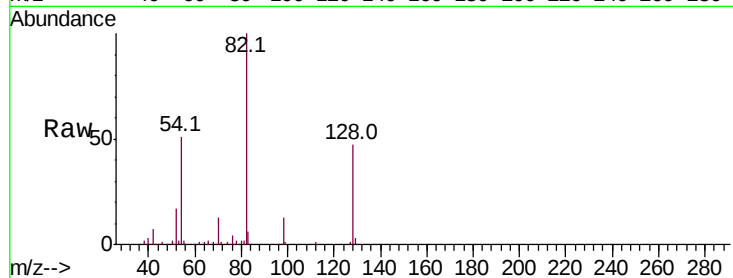

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.23 min Scan# 1044

Delta R.T. 0.00 min

Lab File: BF110635.D

Acq: 9 Nov 2018 18:53

Tgt Ion: 136 Resp: 294075




Ion Ratio Lower Upper


136 100

137 10.6 8.8 13.2

54 7.2 5.4 8.2

68 4.3 4.2 6.2

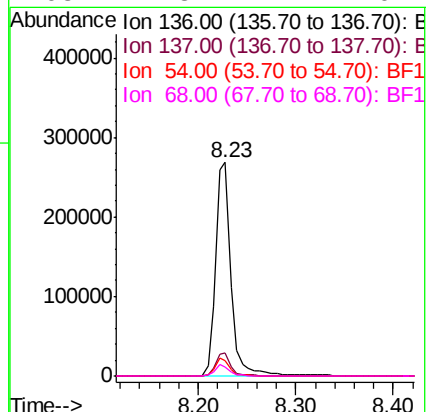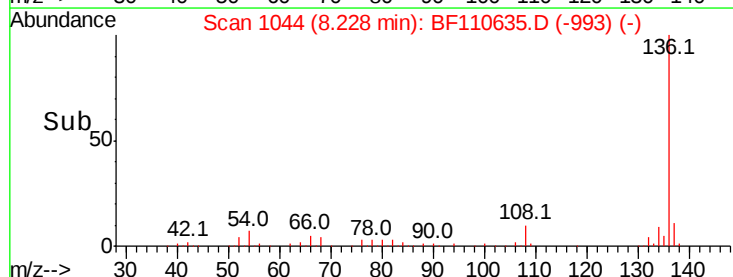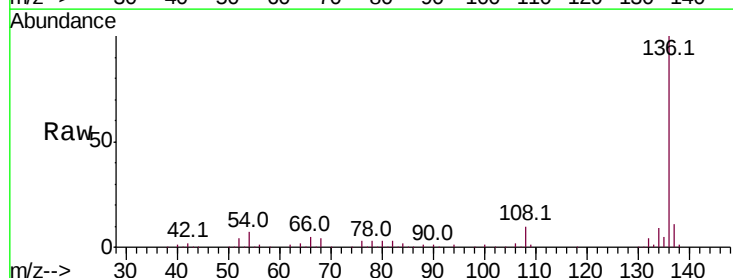


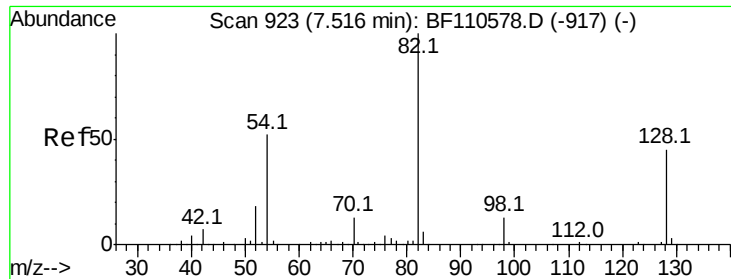




#23
 Nitrobenzene-d5
 Concen: 67.528 ng
 RT: 7.51 min Scan# 922
 Delta R.T. -0.01 min
 Lab File: BF110635.D
 Acq: 9 Nov 2018 18:53

Instrument :
 BNA_F
 ClientSampled :

Tot Ion	82	Resp	344824
Ion Ratio	Lower	Upper	
82	100		
128	47.2	34.2	51.2
54	50.8	38.6	58.0

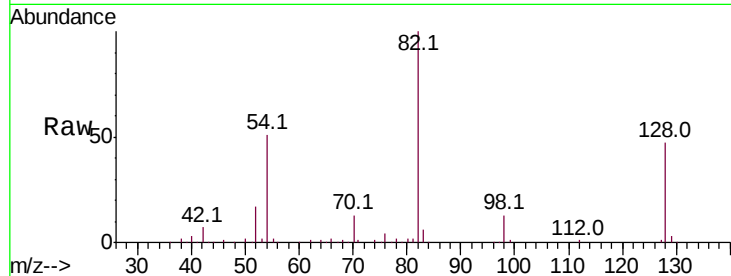


Abundance Ion 82.00 (81.70 to 82.70): BF1
 Ion 128.00 (127.70 to 128.70): BF1
 Ion 54.00 (53.70 to 54.70): BF1

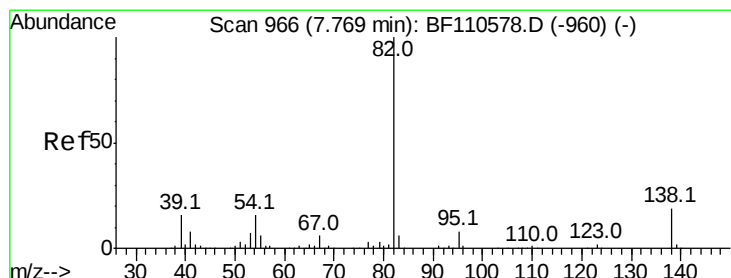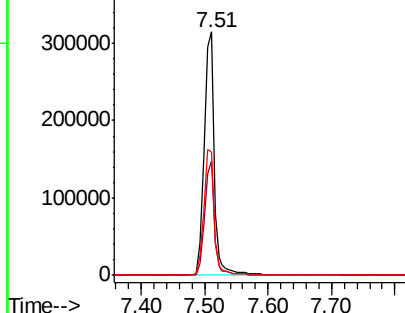
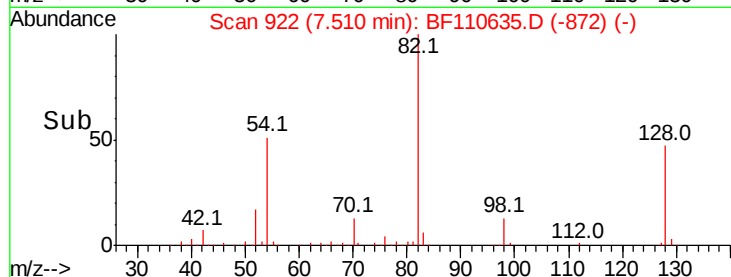



#25
 Isophorone
 Concen: 41.200 ng
 RT: 7.51 min Scan# 922
 Delta R.T. -0.26 min
 Lab File: BF110635.D
 Acq: 9 Nov 2018 18:53

Tgt Ion	82	Resp	344822
Ion Ratio	Lower	Upper	
82	100		
95	0.0	5.7	8.5#
138	0.0	13.2	19.8#

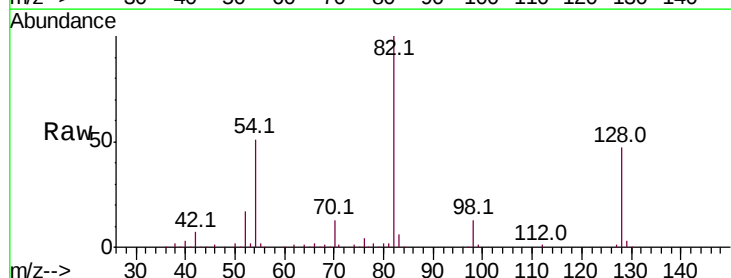

Abundance Ion 82.00 (81.70 to 82.70): BF1
 Ion 95.00 (94.70 to 95.70): BF1
 Ion 138.00 (137.70 to 138.70): BF1

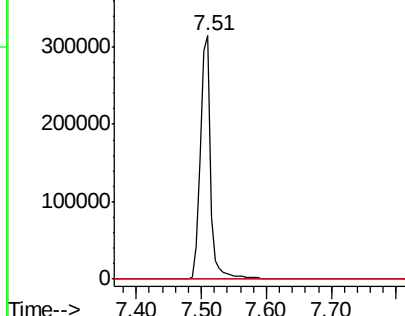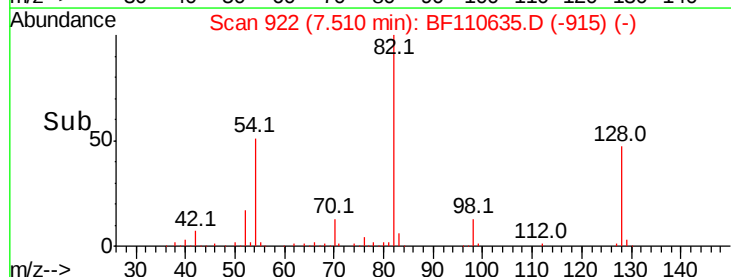


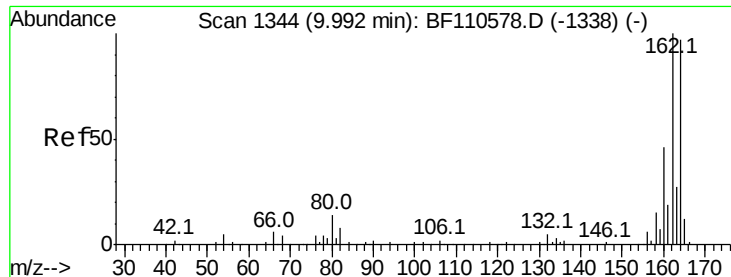




#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.99 min Scan# 1343
Delta R.T. -0.01 min
Lab File: BF110635.D
Acq: 9 Nov 2018 18:53

Instrument :
BNA_F
ClientSampleId :

Tot Ion:164 Resp: 143874
Ion Ratio Lower Upper
164 100
162 102.3 83.0 124.6
160 45.2 37.0 55.6

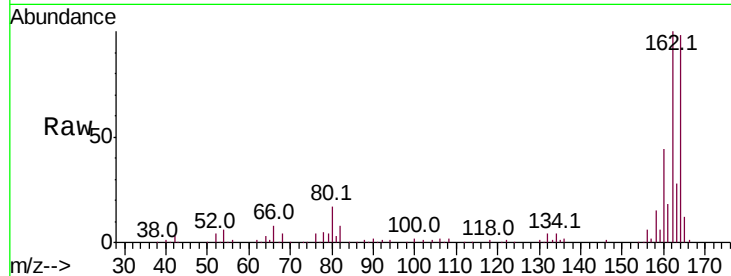


Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

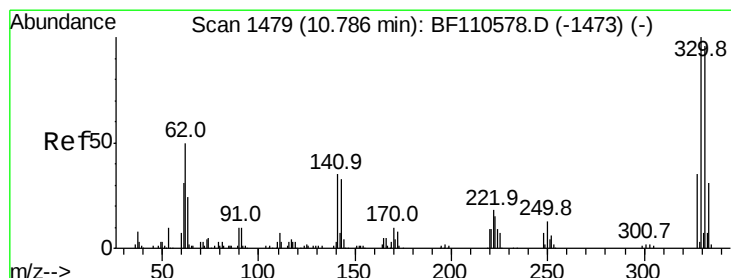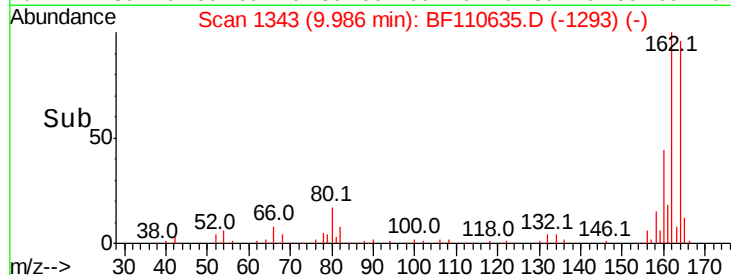
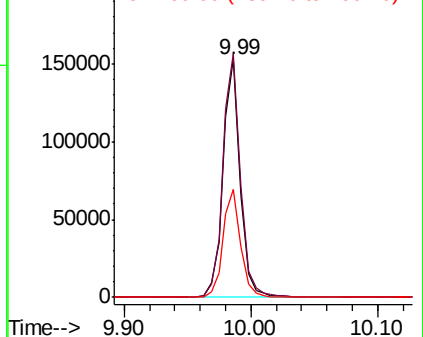



#42
2,4,6-Tribromophenol
Concen: 83.106 ng
RT: 10.78 min Scan# 1478
Delta R.T. -0.01 min
Lab File: BF110635.D
Acq: 9 Nov 2018 18:53

Tgt Ion:330 Resp: 120480
Ion Ratio Lower Upper
330 100
332 96.8 77.1 115.7
141 37.5 27.0 40.4

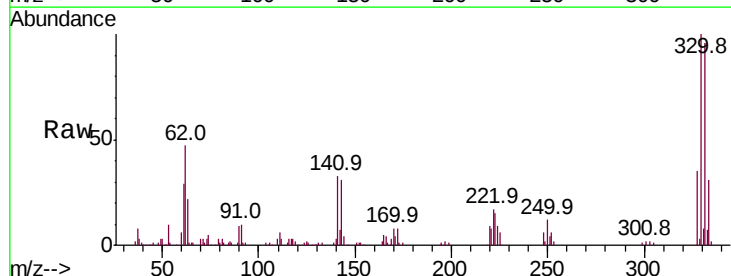

Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

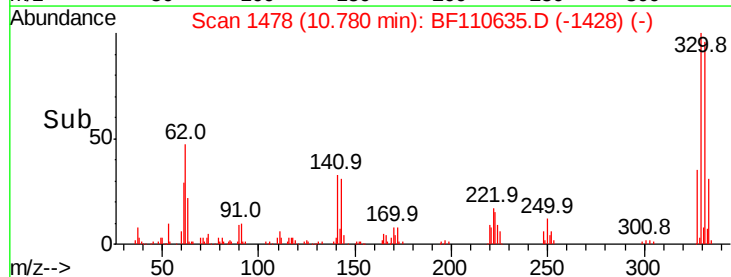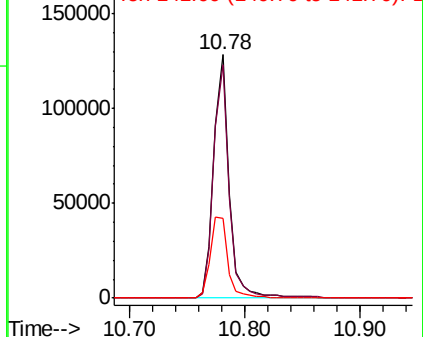


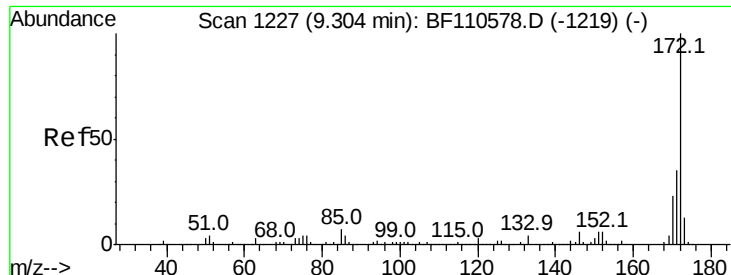




#45
2-Fluorobiphenyl
Concen: 65.561 ng
RT: 9.30 min Scan# 1226
Delta R.T. -0.01 min
Lab File: BF110635.D
Acq: 9 Nov 2018 18:53

Instrument :
BNA_F
ClientSampleId :

Tot Ion:172 Resp: 660460
Ion Ratio Lower Upper
172 100
171 35.6 28.6 43.0
170 23.3 19.7 29.5

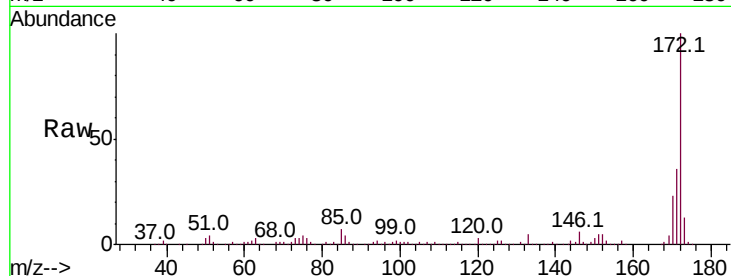


Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

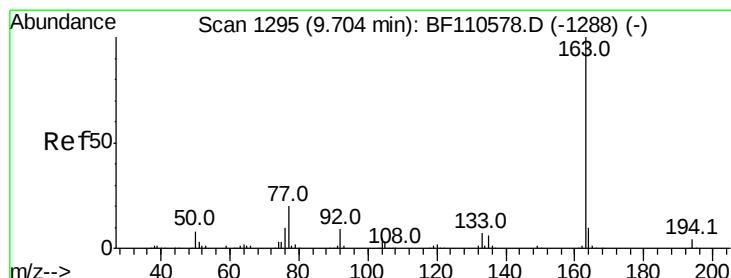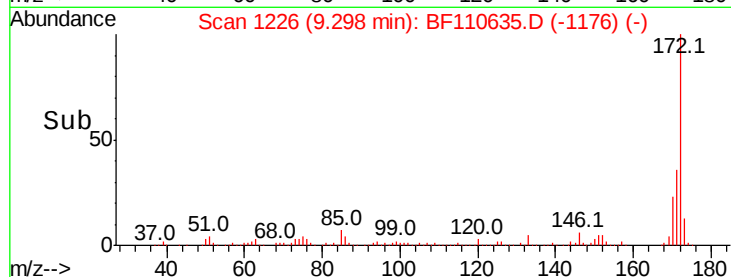
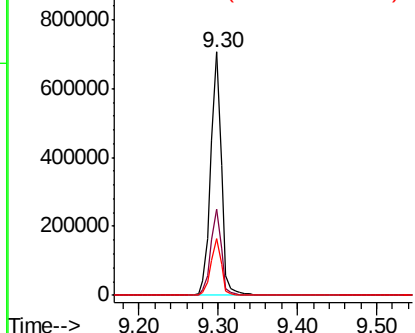



#50
Dimethylphthalate
Concen: 2.891 ng
RT: 9.69 min Scan# 1293
Delta R.T. -0.01 min
Lab File: BF110635.D
Acq: 9 Nov 2018 18:53

Tgt Ion:163 Resp: 31040
Ion Ratio Lower Upper
163 100
194 3.3 3.2 4.8
164 8.9 8.1 12.1

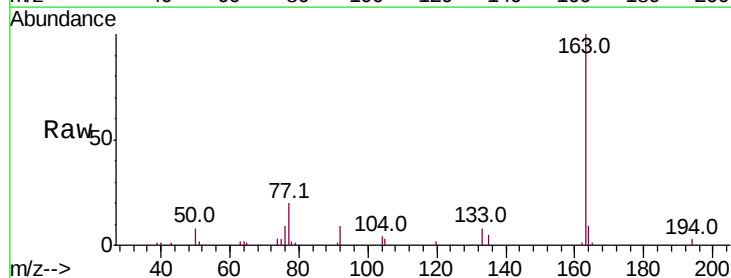

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

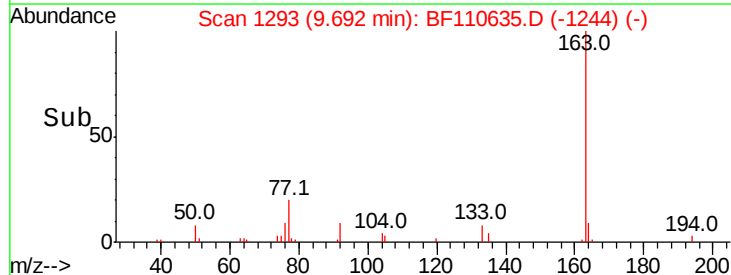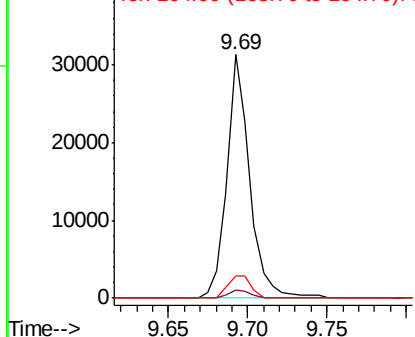


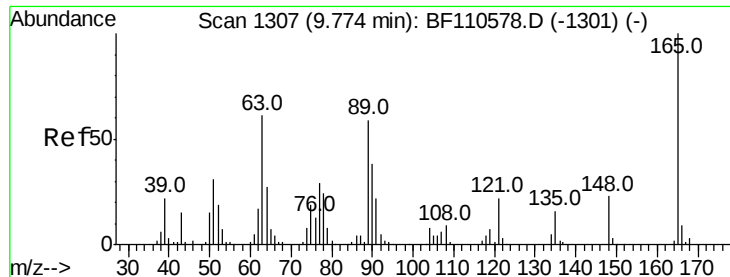




#51
 2,6-Dinitrotoluene
 Concen: 7.714 ng
 RT: 9.99 min Scan# 1343
 Delta R.T. 0.21 min
 Lab File: BF110635.D
 Acq: 9 Nov 2018 18:53

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
165	100		
63	1.7	48.9	73.3#
89	1.7	46.6	69.8#

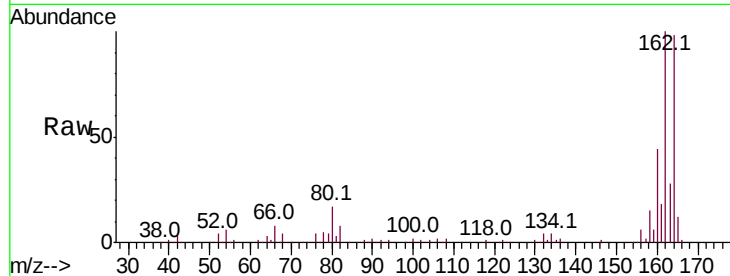




Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BF1
 Ion 89.00 (88.70 to 89.70): BF1

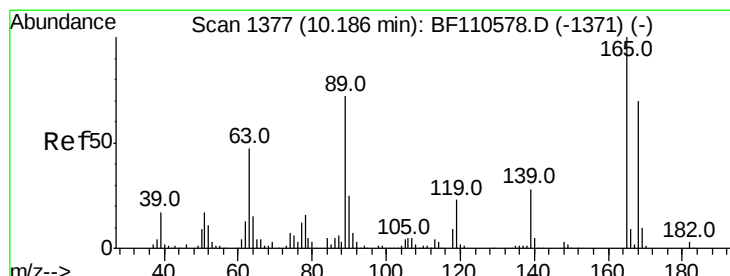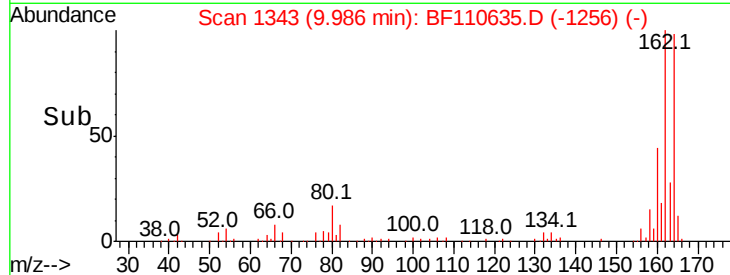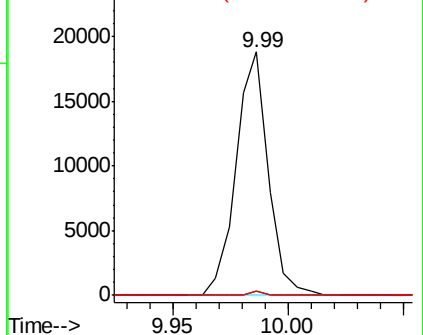


#57
 2,4-Dinitrotoluene
 Concen: 5.933 ng
 RT: 9.99 min Scan# 1343
 Delta R.T. -0.20 min
 Lab File: BF110635.D
 Acq: 9 Nov 2018 18:53

Tgt Ion	Ratio	Lower	Upper
165	100		
63	1.7	44.8	67.2#
89	1.7	62.2	93.4#
182	0.0	2.1	3.1#

Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BF1
 Ion 89.00 (88.70 to 89.70): BF1
 Ion 182.00 (181.70 to 182.70): E


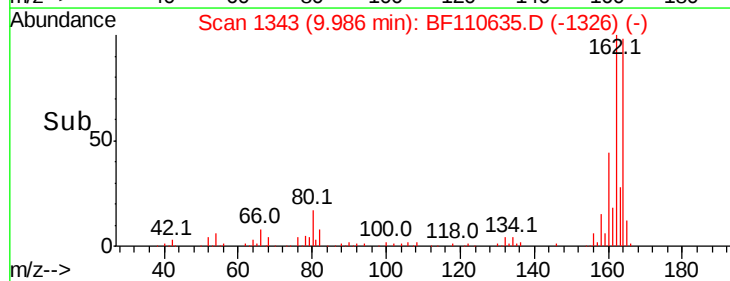
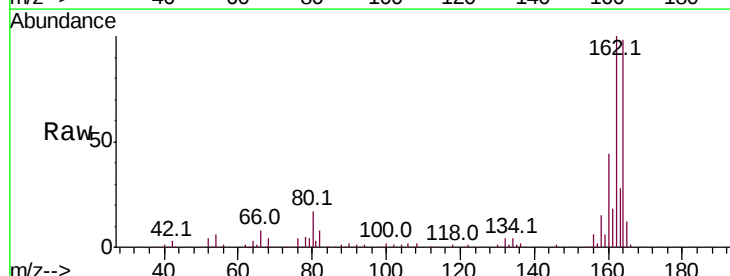
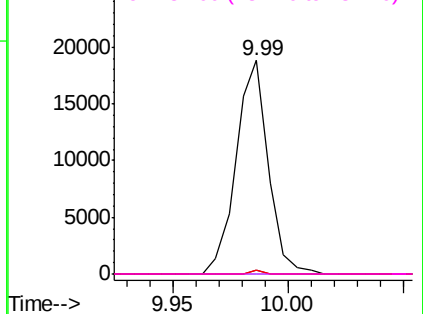


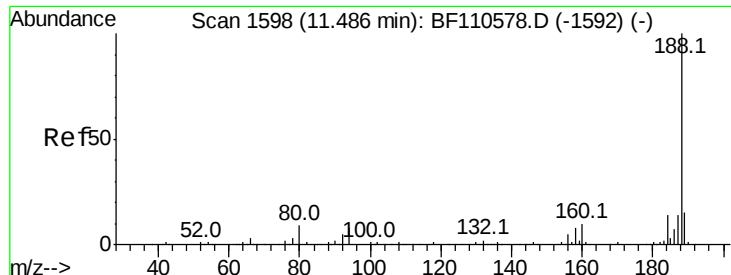

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.48 min Scan# 1597
Delta R.T. -0.01 min
Lab File: BF110635.D
Acq: 9 Nov 2018 18:53




Instrument :
BNA_F
ClientSampleId :


Tot Ion:188 Resp: 289690
Ion Ratio Lower Upper
188 100
94 8.2 7.2 10.8
80 9.2 7.9 11.9

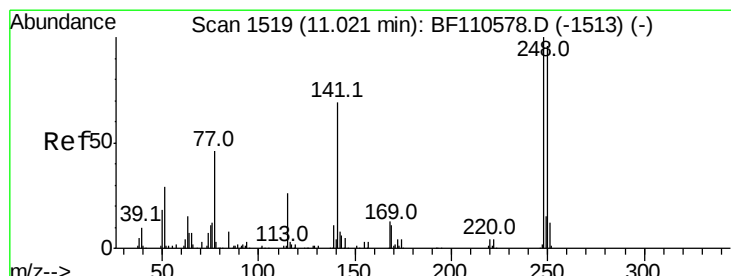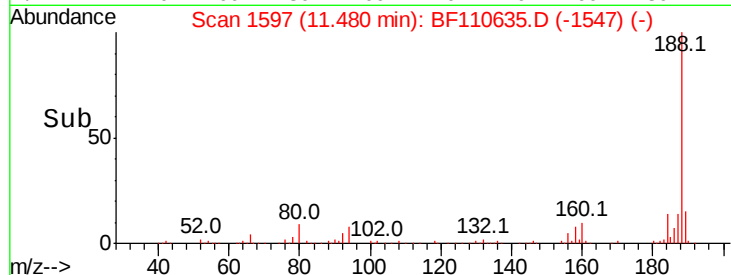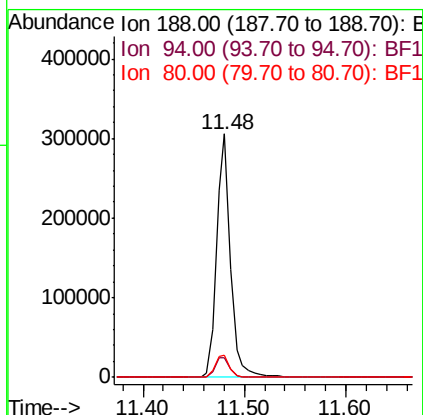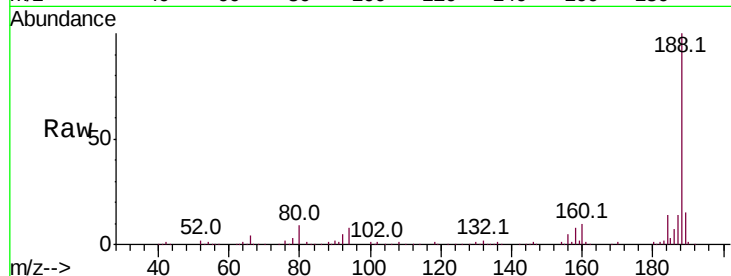

#67
4-Bromophenyl-phenylether
Concen: 2.319 ng
RT: 10.78 min Scan# 1478
Delta R.T. -0.24 min
Lab File: BF110635.D
Acq: 9 Nov 2018 18:53

Tgt Ion:248 Resp: 7425
Ion Ratio Lower Upper
248 100
250 187.4 79.4 119.2#
141 502.1 55.9 83.9#

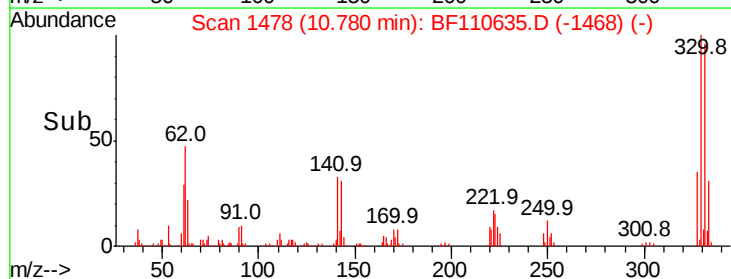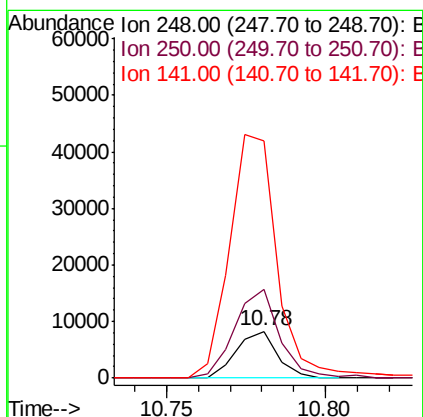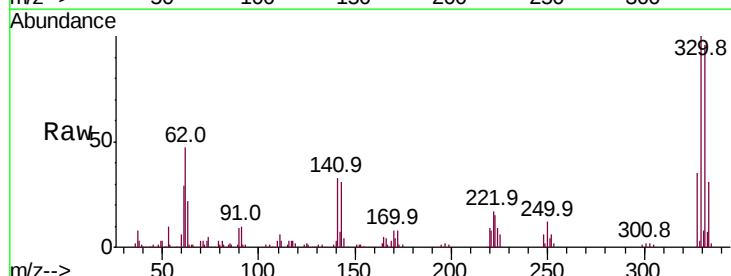


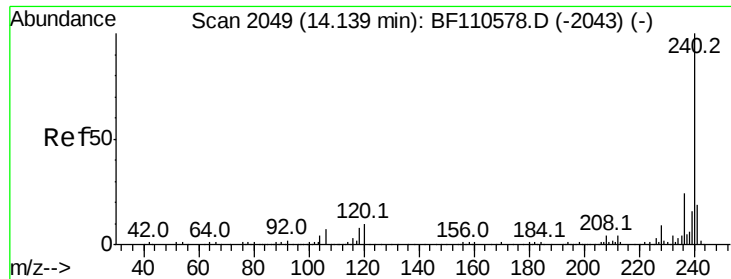




#76
 Chrysene-d12
 Concen: 20.000 ng
 RT: 14.13 min Scan# 2047
 Delta R.T. -0.01 min
 Lab File: BF110635.D
 Acq: 9 Nov 2018 18:53

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:240 Resp: 226422
 Ion Ratio Lower Upper
 240 100
 120 12.3 8.3 12.5
 236 25.4 21.2 31.8

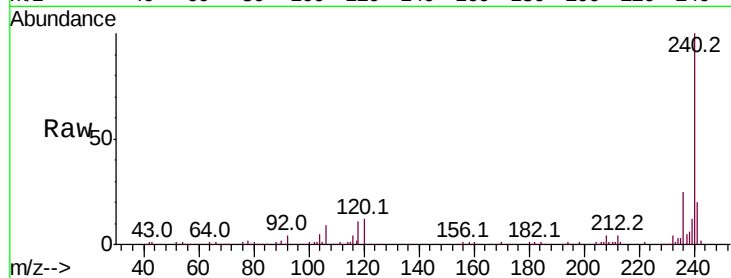


Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E

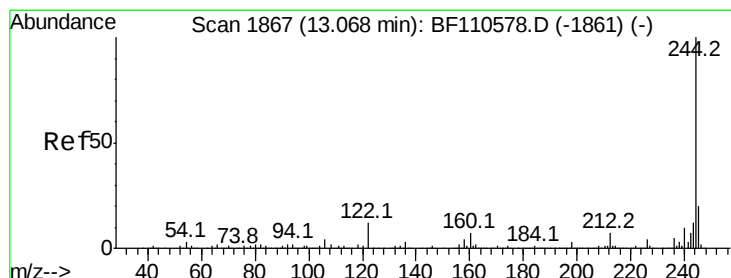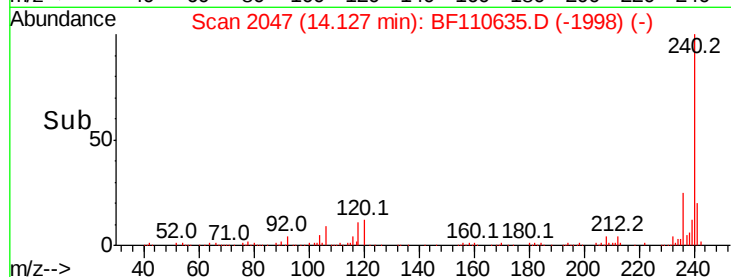
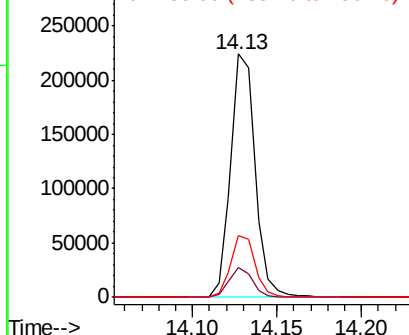



#79
 Terphenyl-d14
 Concen: 60.136 ng
 RT: 13.06 min Scan# 1866
 Delta R.T. -0.01 min
 Lab File: BF110635.D
 Acq: 9 Nov 2018 18:53

Tgt Ion:244 Resp: 727054
 Ion Ratio Lower Upper
 244 100
 212 6.8 5.8 8.8
 122 12.3 8.7 13.1

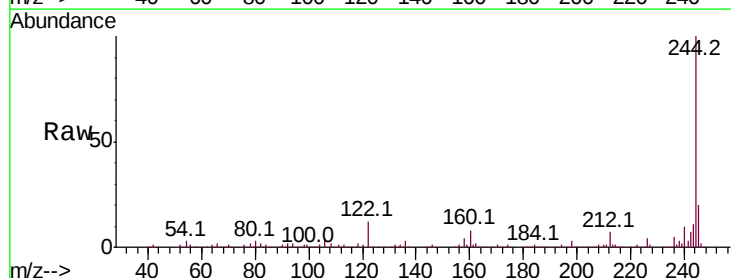

Abundance Ion 244.00 (243.70 to 244.70): E
 Ion 212.00 (211.70 to 212.70): E
 Ion 122.00 (121.70 to 122.70): E

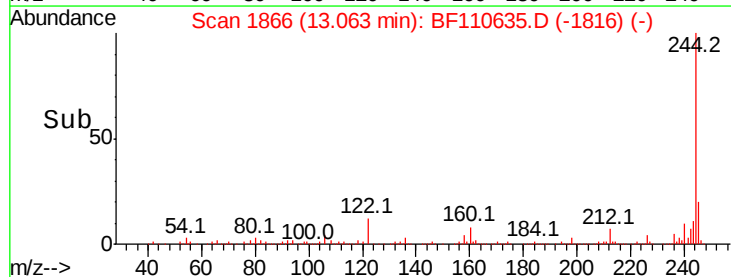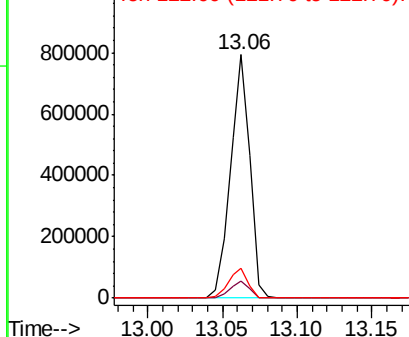


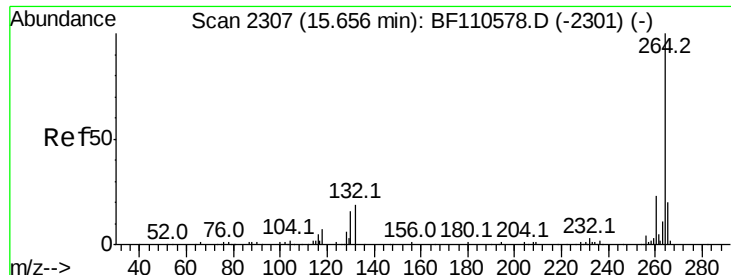

#87
 Pervlene-d12
 Concen: 20.000 ng
 RT: 15.66 min Scan# 2307
 Delta R.T. 0.00 min
 Lab File: BF110635.D
 Acq: 9 Nov 2018 18:53

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:264 Resp: 140064
 Ion Ratio Lower Upper
 264 100
 260 22.8 18.7 28.1
 265 22.0 16.7 25.1

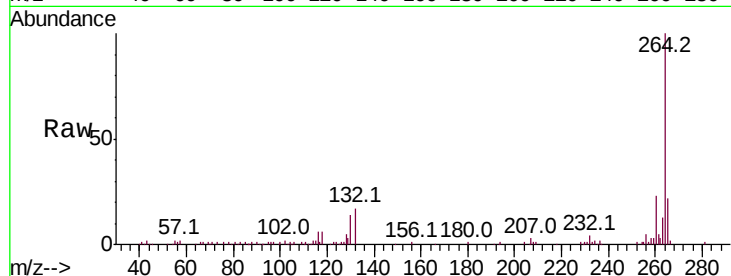

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

