

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF110918\
 Data File : BF110634.D
 Acq On : 9 Nov 2018 18:25
 Operator : JU/SJ
 Sample : J5860-10
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 EP2-EB-01-1118

Quant Time: Nov 11 03:37:11 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF110818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 09 15:13:13 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.95	152	84697	20.00	ng	0.00
21) Naphthalene-d8	8.23	136	351122	20.00	ng	0.00
39) Acenaphthene-d10	9.99	164	170376	20.00	ng	0.00
64) Phenanthrene-d10	11.48	188	340784	20.00	ng	0.00
76) Chrysene-d12	14.13	240	269380	20.00	ng	-0.01
87) Perylene-d12	15.66	264	168827	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.56	112	277513	53.22	ng	0.00
7) Phenol-d6	6.56	99	205838	30.87	ng	-0.01
23) Nitrobenzene-d5	7.51	82	526705	86.39	ng	0.00
42) 2,4,6-Tribromophenol	10.78	330	182950	106.57	ng	0.00
45) 2-Fluorobiphenyl	9.30	172	957809	80.29	ng	0.00
79) Terphenyl-d14	13.07	244	1106709	76.94	ng	0.00


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF110918\
Data File : BF110634.D
Acq On : 9 Nov 2018 18:25
Operator : JU/SJ
Sample : J5860-10
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
EP2-EB-01-1118

Quant Time: Nov 11 03:37:11 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF110818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 09 15:13:13 2018
Response via : Initial Calibration

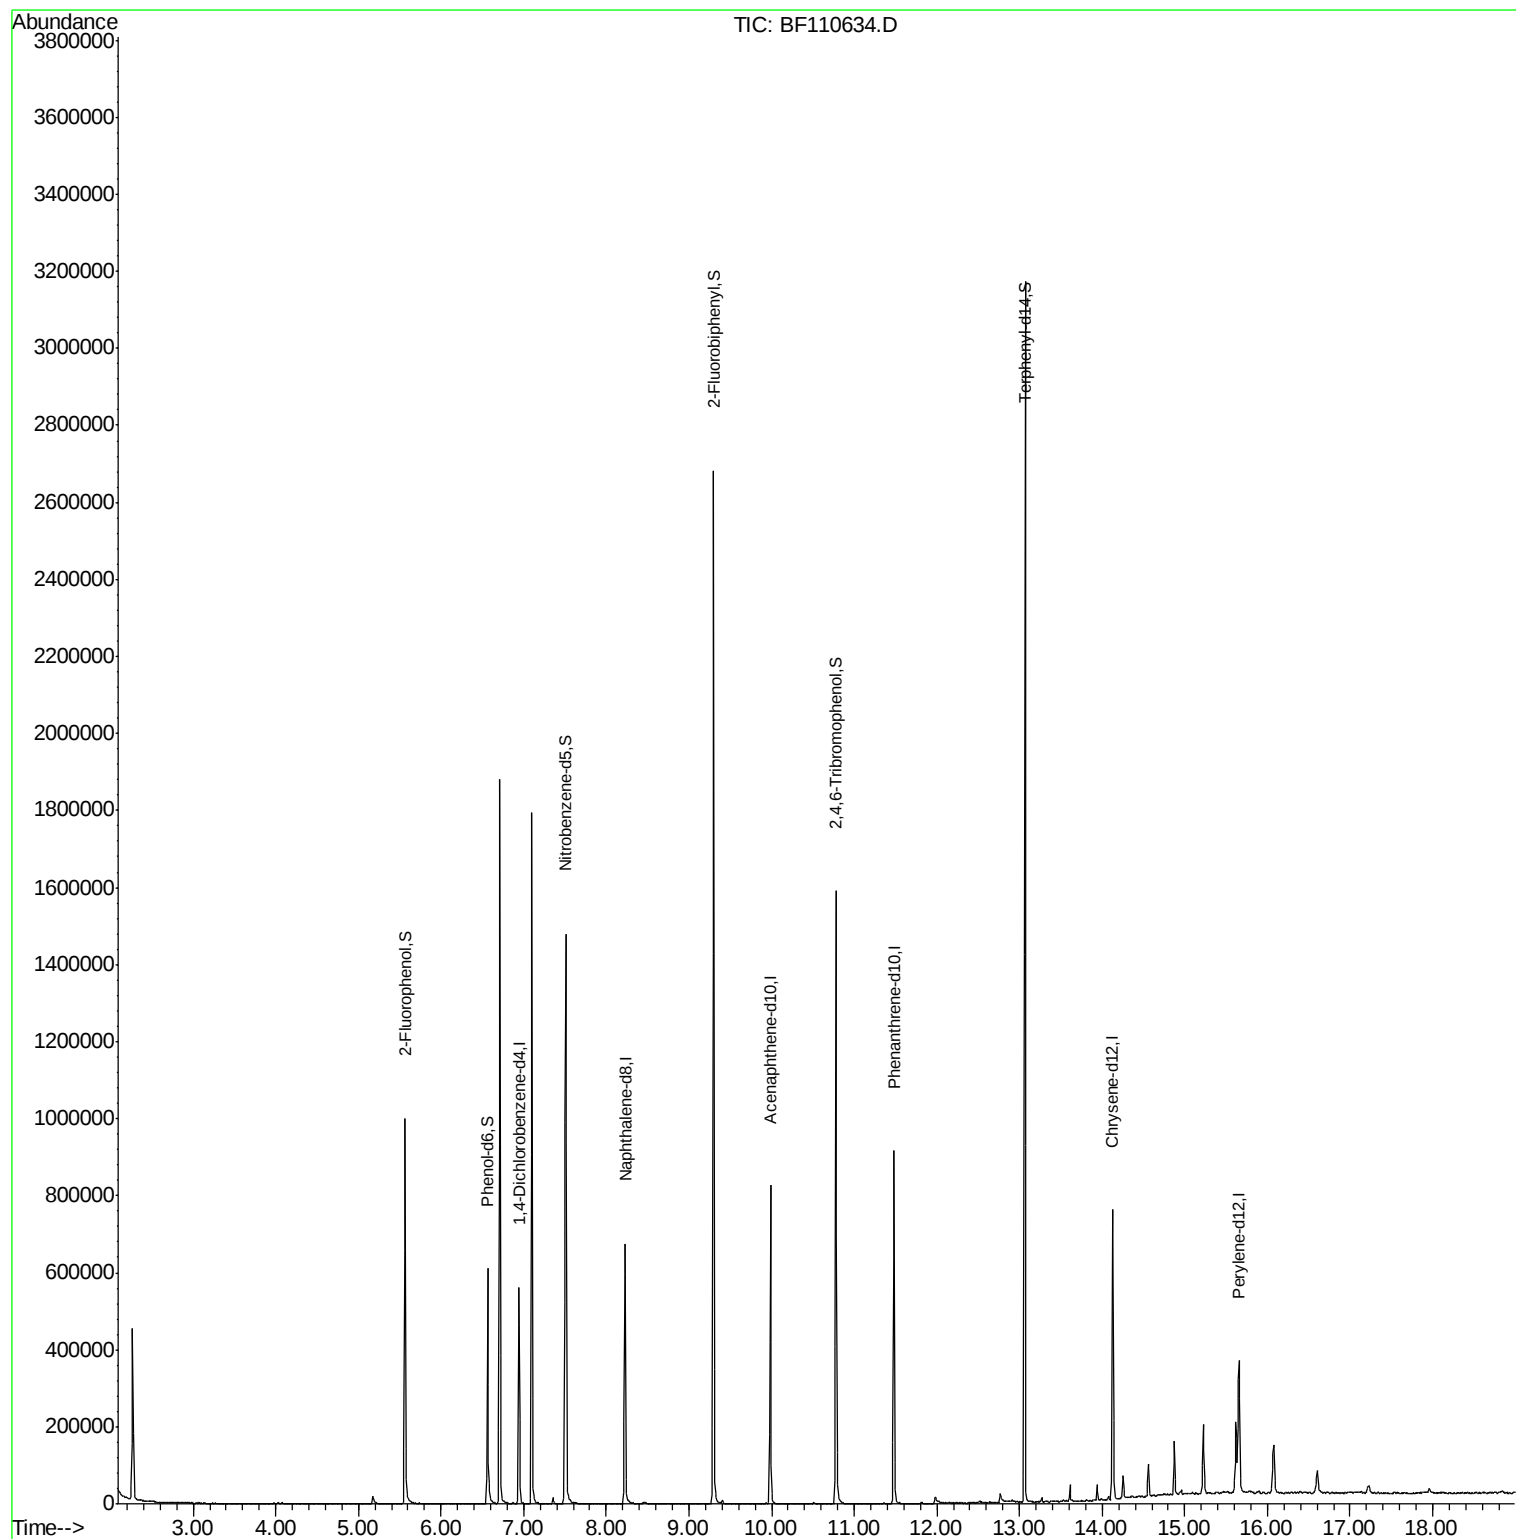




#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.95 min Scan# 826
Delta R.T. 0.00 min
Lab File: BF110634.D
Acq: 9 Nov 2018 18:25

Instrument :
BNA_F
ClientSampleId :
EP2-EB-01-1118

Tot Ion:152 Resp: 84697
Ion Ratio Lower Upper
152 100
150 159.1 122.7 184.1
115 61.6 49.1 73.7

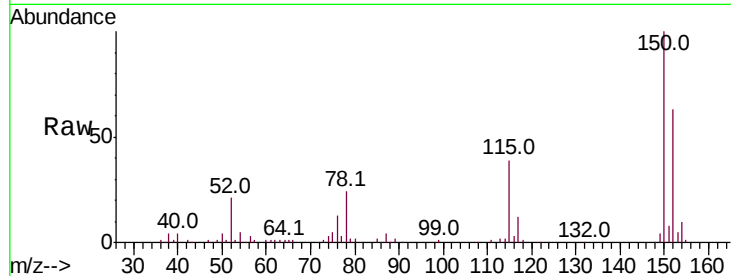


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

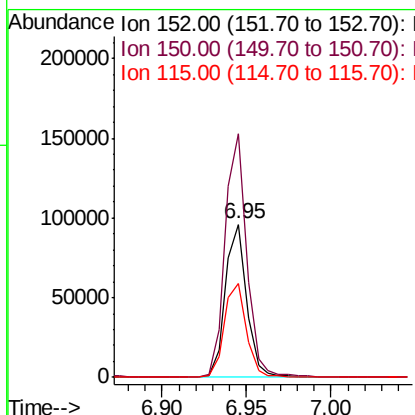



#5

2-Fluorophenol
Concen: 53.221 ng
RT: 5.56 min Scan# 591
Delta R.T. 0.00 min
Lab File: BF110634.D
Acq: 9 Nov 2018 18:25

Tgt Ion:112 Resp: 277513
Ion Ratio Lower Upper
112 100
64 60.5 44.1 66.1
63 31.4 23.7 35.5



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

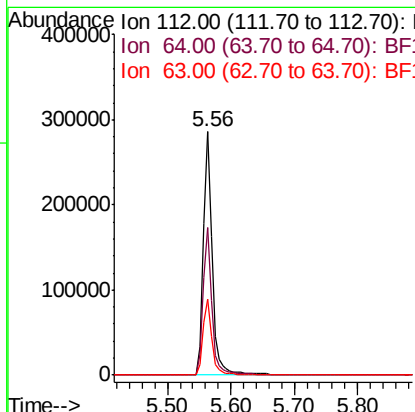



#7

Phenol-d6

Concen: 30.870 ng

RT: 6.56 min Scan# 761

Delta R.T. -0.01 min

Lab File: BF110634.D

Acq: 9 Nov 2018 18:25

Instrument :

BNA_F

ClientSampleId :

EP2-EB-01-1118


Tot Ion: 99 Resp: 205838

Ion Ratio Lower Upper




99 100

42 19.0 15.8 23.6

71 33.7 28.0 42.0



Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

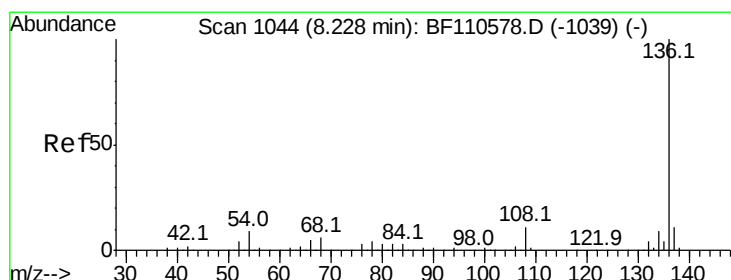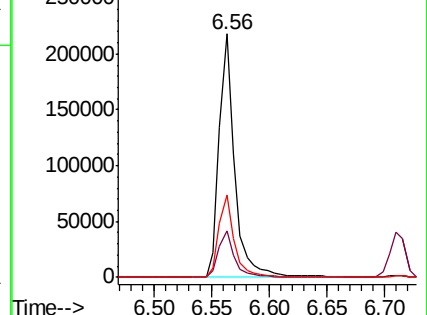

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.23 min Scan# 1044

Delta R.T. 0.00 min

Lab File: BF110634.D

Acq: 9 Nov 2018 18:25

Tgt Ion: 136 Resp: 351122


Ion Ratio Lower Upper

136 100



137 10.5 8.8 13.2

54 7.4 5.4 8.2

68 5.0 4.2 6.2



Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1



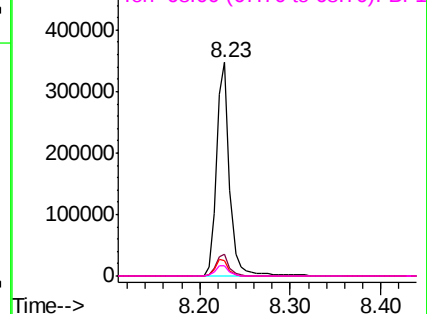





#23
 Nitrobenzene-d5
 Concen: 86.388 ng
 RT: 7.51 min Scan# 922
 Delta R.T. -0.01 min
 Lab File: BF110634.D
 Acq: 9 Nov 2018 18:25




Instrument :
 BNA_F
 ClientSampleId :
 EP2-EB-01-1118


Tot Ion	82	Resp	526705
Ion Ratio	100		
Lower	34.2		
Upper	51.2		
54	53.1	38.6	58.0

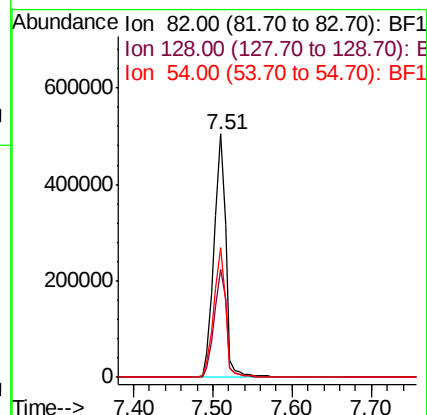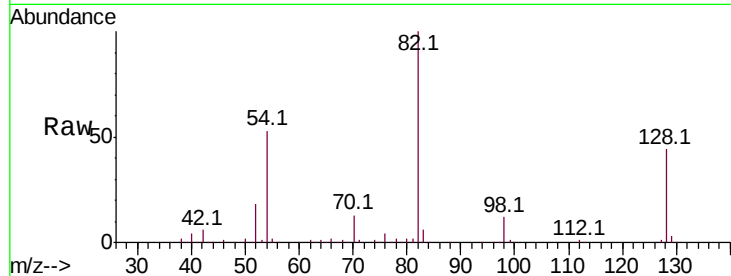

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.99 min Scan# 1343
 Delta R.T. -0.01 min
 Lab File: BF110634.D
 Acq: 9 Nov 2018 18:25

Tgt Ion	164	Resp	170376
Ion Ratio <td>100</td> <td></td> <td></td>	100		
Lower <td>83.0</td> <td></td> <td></td>	83.0		
Upper <td>124.6</td> <td></td> <td></td>	124.6		
162	106.1	37.0	55.6

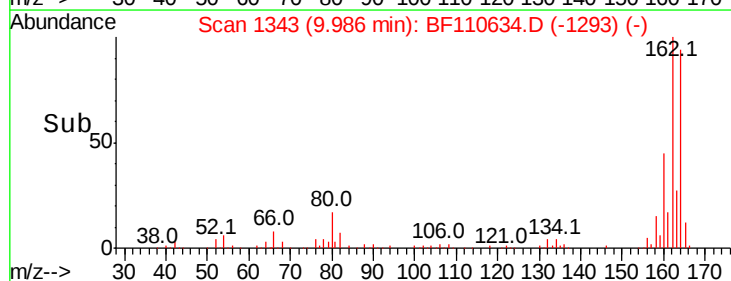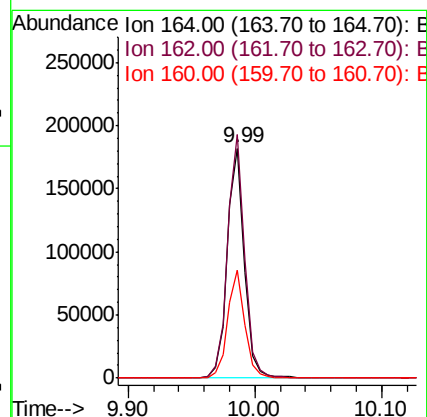

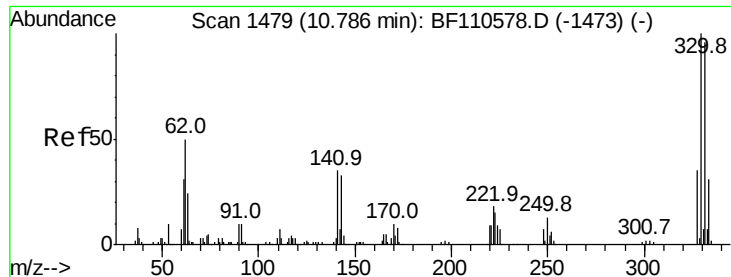

#42

2,4,6-Tribromophenol

Concen: 106.568 ng

RT: 10.78 min Scan# 1478

Delta R.T. -0.01 min

Lab File: BF110634.D

Acq: 9 Nov 2018 18:25

Instrument :

BNA_F

ClientSampleId :

EP2-EB-01-1118


Tot Ion:330 Resp: 182950

Ion Ratio Lower Upper

330 100

332 96.1 77.1 115.7




141 37.2 27.0 40.4

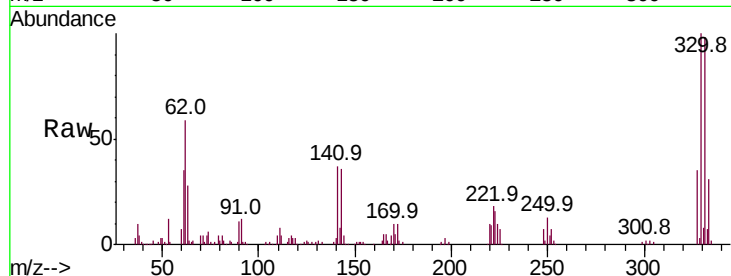

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

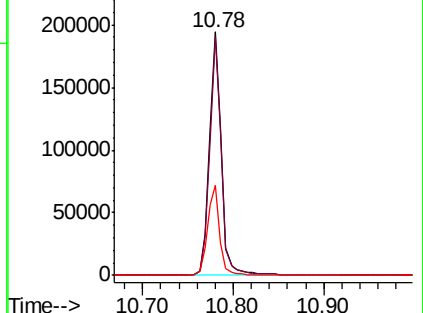

#45

2-Fluorobiphenyl

Concen: 80.289 ng

RT: 9.30 min Scan# 1226

Delta R.T. -0.01 min

Lab File: BF110634.D

Acq: 9 Nov 2018 18:25


Tgt Ion:172 Resp: 957809

Ion Ratio Lower Upper

172 100

171 36.0 28.6 43.0



170 23.4 19.7 29.5




Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

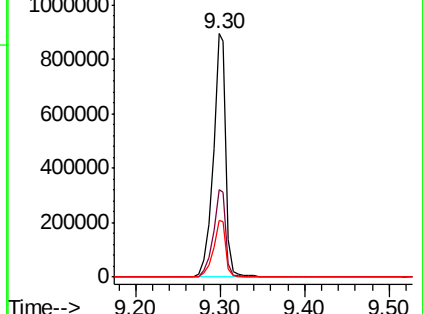







#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.48 min Scan# 1597
Delta R.T. -0.01 min
Lab File: BF110634.D
Acq: 9 Nov 2018 18:25

Instrument :
BNA_F
ClientSampleId :
EP2-EB-01-1118

Tot Ion:188 Resp: 340784
Ion Ratio Lower Upper
188 100
94 8.8 7.2 10.8
80 9.3 7.9 11.9

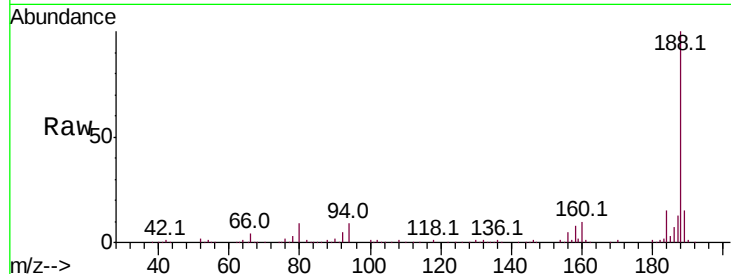


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1


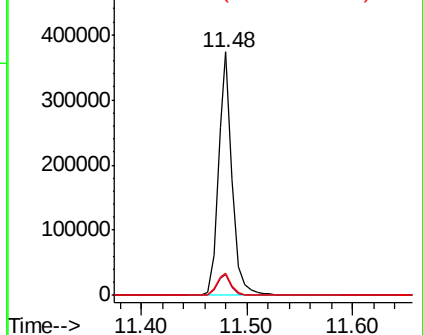



#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.13 min Scan# 2047
Delta R.T. -0.01 min
Lab File: BF110634.D
Acq: 9 Nov 2018 18:25

Tgt Ion:240 Resp: 269380
Ion Ratio Lower Upper
240 100
120 12.6 8.3 12.5#
236 26.9 21.2 31.8



Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

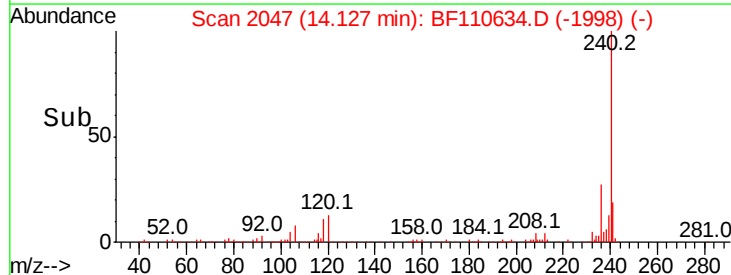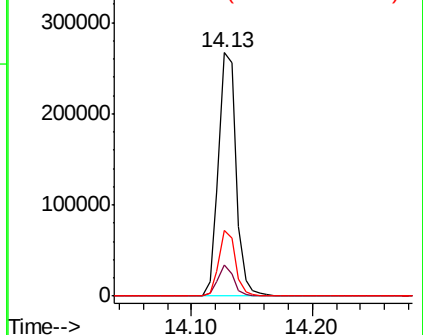

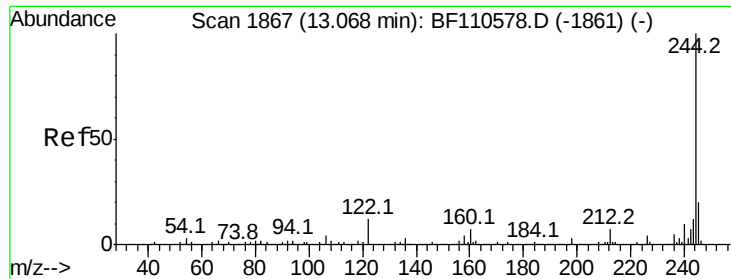

#79

Terphenyl-d14

Concen: 76.940 ng

RT: 13.07 min Scan# 1867

Delta R.T. 0.00 min

Lab File: BF110634.D

Acq: 9 Nov 2018 18:25

Instrument :

BNA_F

ClientSampleId :

EP2-EB-01-1118


Tot Ion:244 Resp: 1106709

Ion Ratio Lower Upper

244 100

212 7.0 5.8 8.8




122 12.2 8.7 13.1



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

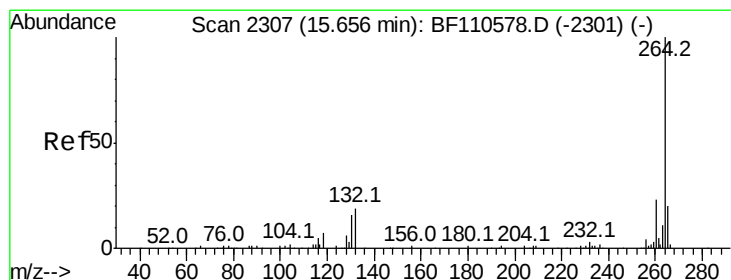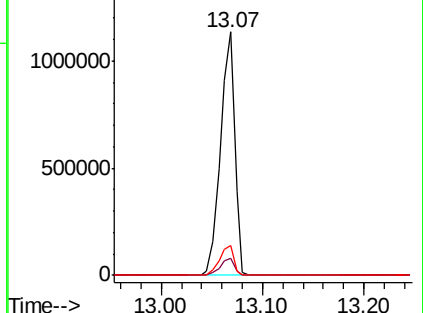

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.66 min Scan# 2307

Delta R.T. 0.00 min

Lab File: BF110634.D

Acq: 9 Nov 2018 18:25


Tgt Ion:264 Resp: 168827

Ion Ratio Lower Upper

264 100

260 22.8 18.7 28.1

265 21.6 16.7 25.1



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

