

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF110918\
 Data File : BF110636.D
 Acq On : 9 Nov 2018 19:20
 Operator : JU/SJ
 Sample : J5864-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OLDMANS-1

Quant Time: Nov 11 03:40:31 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF110818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 09 15:13:13 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.95	152	74371	20.00	ng	0.00
21) Naphthalene-d8	8.23	136	304553	20.00	ng	0.00
39) Acenaphthene-d10	9.99	164	151027	20.00	ng	0.00
64) Phenanthrene-d10	11.48	188	305586	20.00	ng	0.00
76) Chrysene-d12	14.13	240	242609	20.00	ng	-0.01
87) Perylene-d12	15.66	264	148782	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.57	112	606763	132.52	ng	0.00
7) Phenol-d6	6.57	99	768084	131.19	ng	0.00
23) Nitrobenzene-d5	7.51	82	483525	91.43	ng	0.00
42) 2,4,6-Tribromophenol	10.78	330	187810	123.41	ng	0.00
45) 2-Fluorobiphenyl	9.30	172	885788	83.76	ng	0.00
79) Terphenyl-d14	13.06	244	948344	73.21	ng	0.00
Target Compounds						
10) Phenol	6.58	94	50192	7.393	ng	Qvalue # 69
50) Dimethylphthalate	9.69	163	56200	4.987	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF110918\
Data File : BF110636.D
Acq On : 9 Nov 2018 19:20
Operator : JU/SJ
Sample : J5864-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OLDMANS-1

Quant Time: Nov 11 03:40:31 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF110818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 09 15:13:13 2018
Response via : Initial Calibration

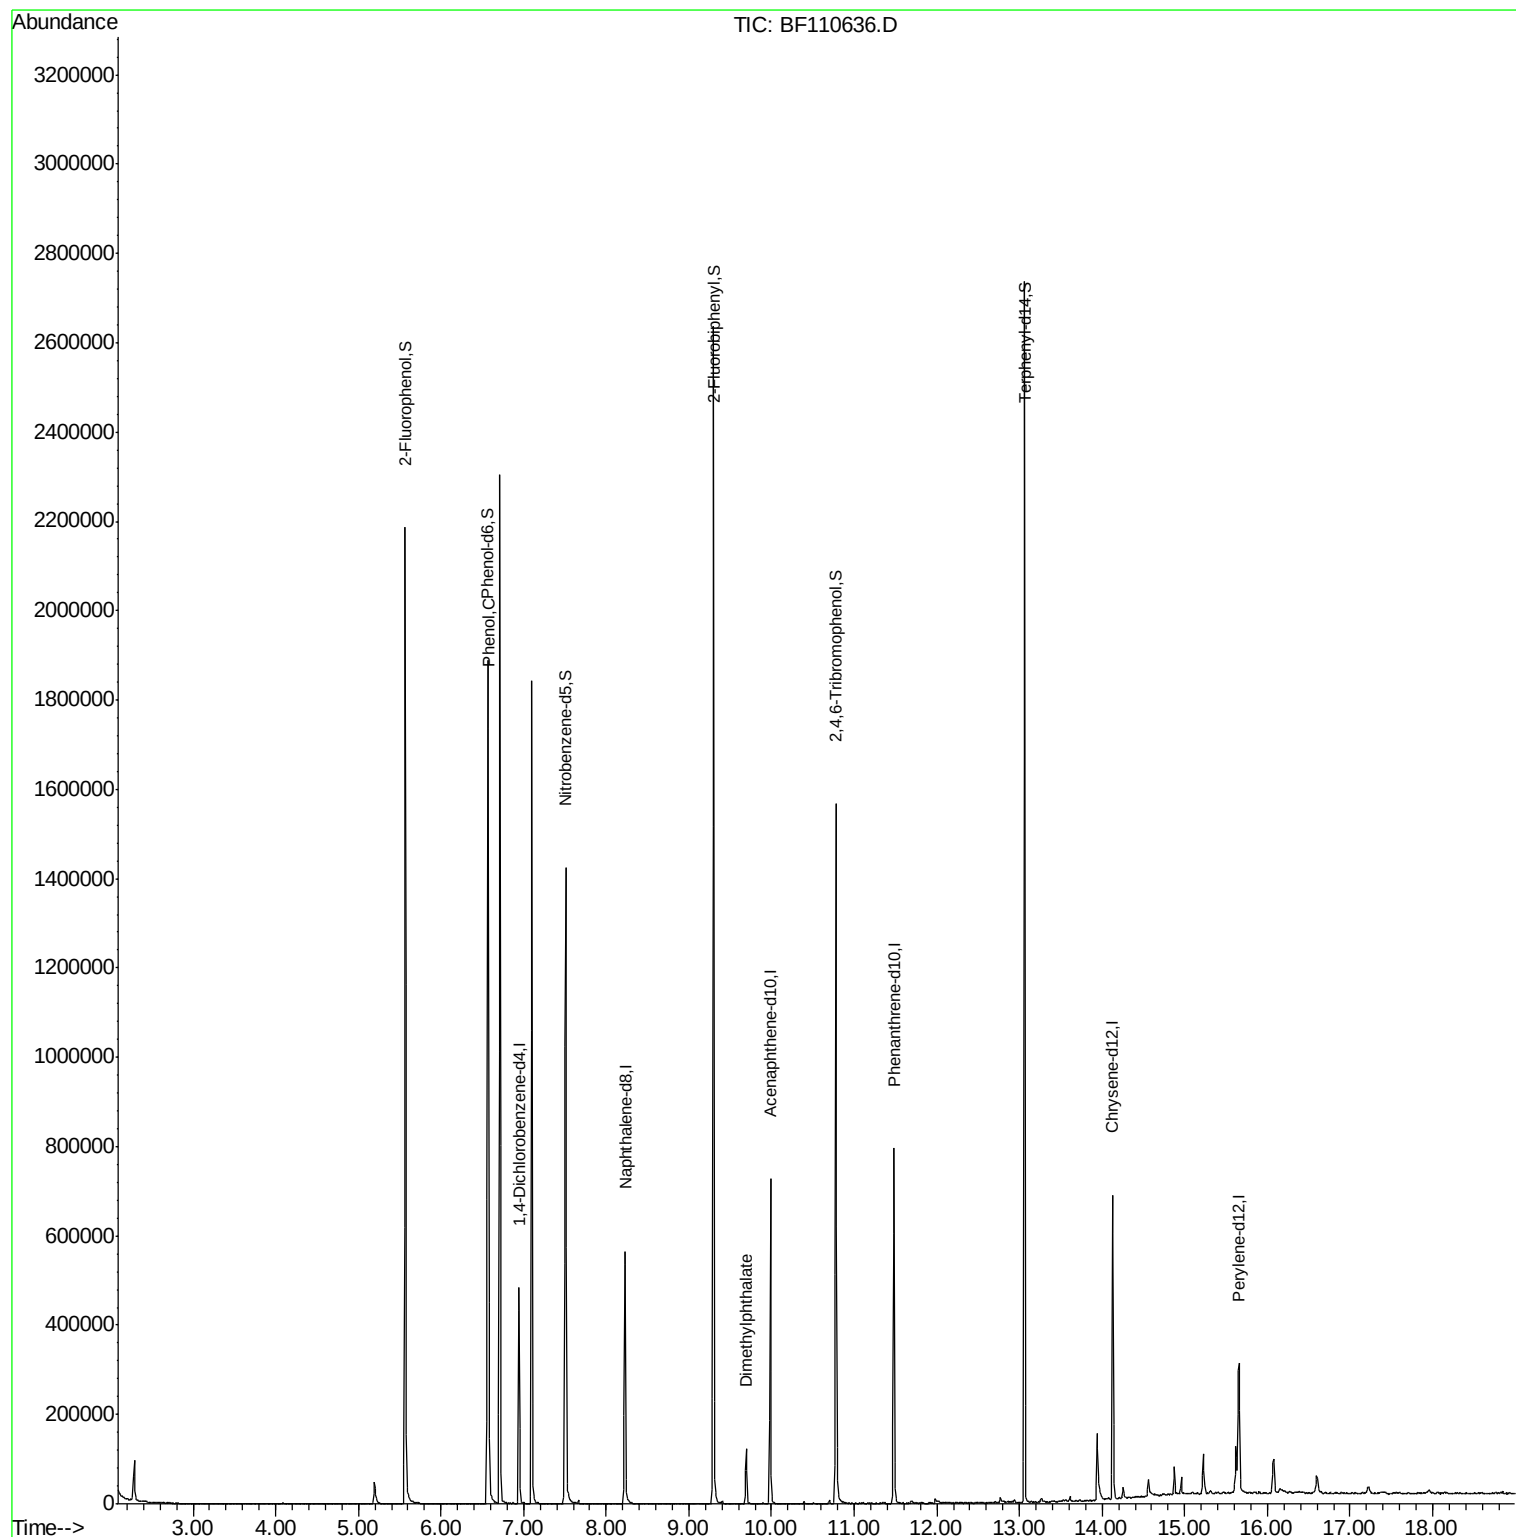

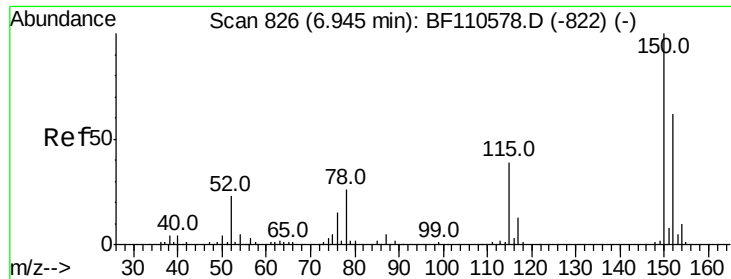


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.95 min Scan# 826
Delta R.T. 0.00 min
Lab File: BF110636.D
Acq: 9 Nov 2018 19:20

Instrument :
BNA_F
ClientSampleId :
OLDMANS-1

Tot Ion:152 Resp: 74371
Ion Ratio Lower Upper
152 100
150 158.4 122.7 184.1
115 61.9 49.1 73.7

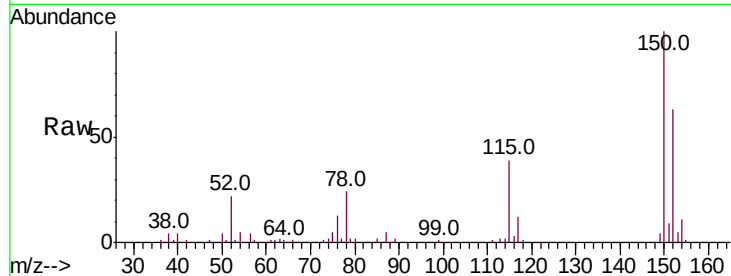


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

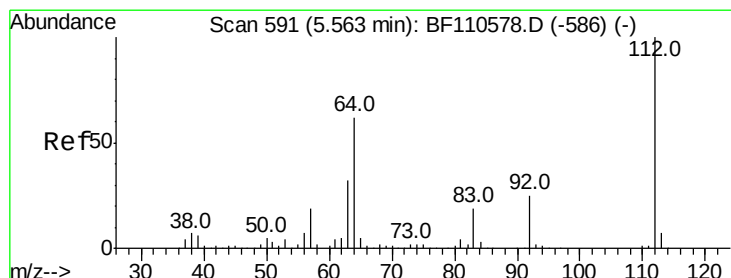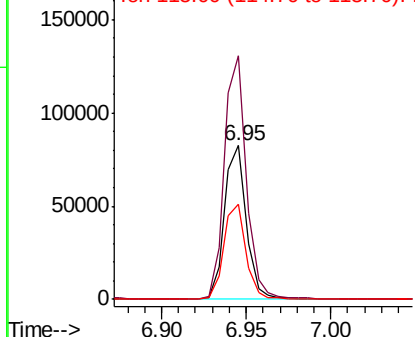



#5




2-Fluorophenol
Concen: 132.521 ng
RT: 5.57 min Scan# 592
Delta R.T. 0.01 min
Lab File: BF110636.D
Acq: 9 Nov 2018 19:20

Tgt Ion:112 Resp: 606763
Ion Ratio Lower Upper
112 100
64 60.5 44.1 66.1
63 32.0 23.7 35.5

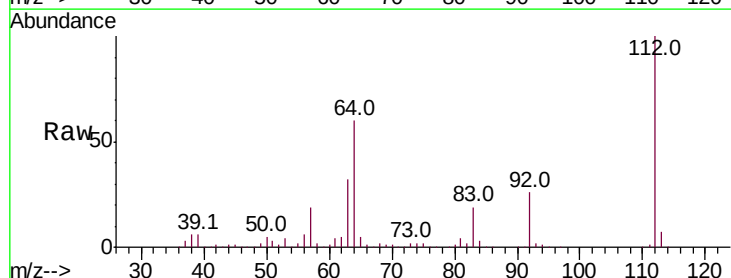

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

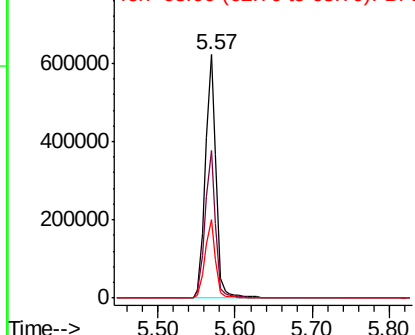

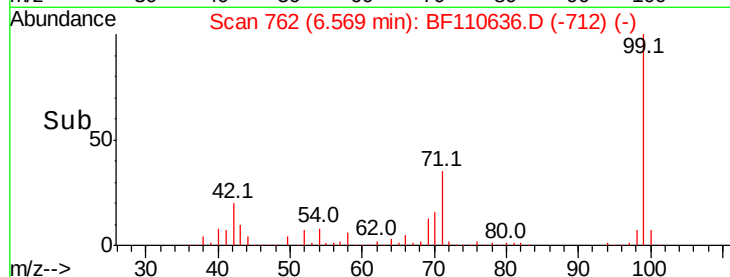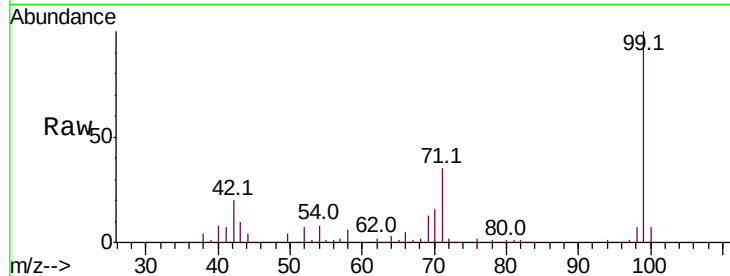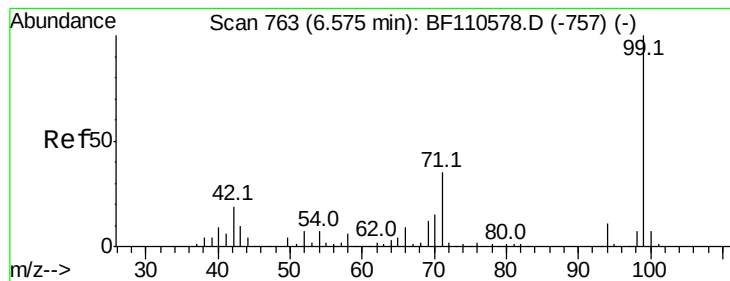

#7

Phenol-d6

Concen: 131.186 ng

RT: 6.57 min Scan# 762

Delta R.T. -0.01 min

Lab File: BF110636.D

Acq: 9 Nov 2018 19:20

Instrument :

BNA_F

ClientSampleId :

OLDMANS-1





Tot Ion: 99 Resp: 768084

Ion Ratio Lower Upper

99 100

42 19.8 15.8 23.6

71 34.9 28.0 42.0

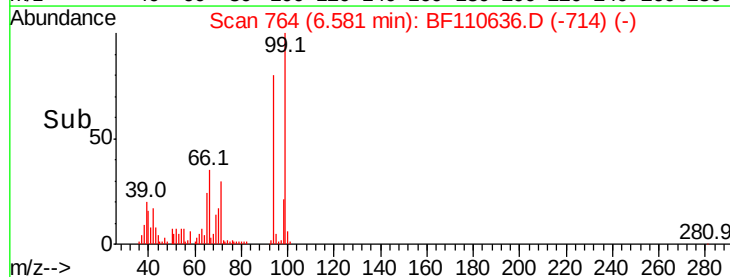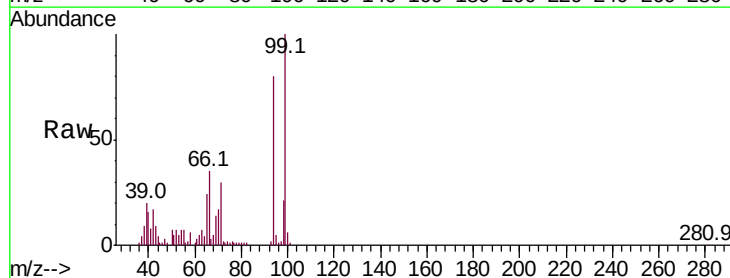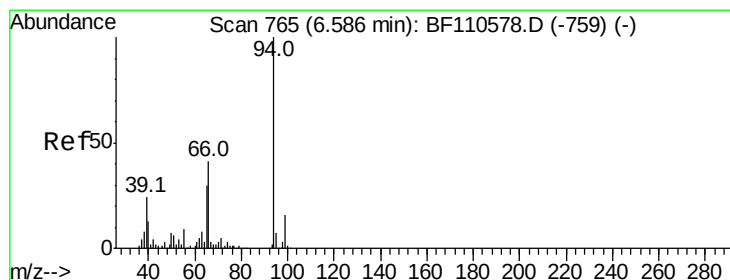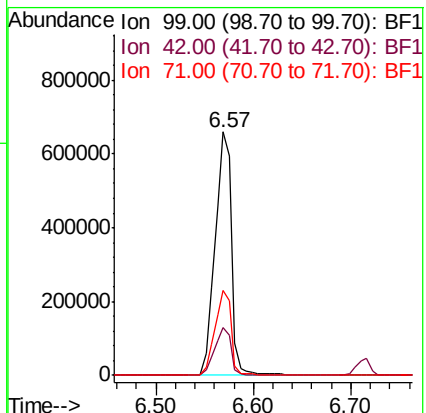

#10

Phenol

Concen: 7.393 ng

RT: 6.58 min Scan# 764

Delta R.T. -0.01 min

Lab File: BF110636.D

Acq: 9 Nov 2018 19:20


Tgt Ion: 94 Resp: 50192


Ion Ratio Lower Upper

94 100

65 30.3 25.3 65.3

66 43.7 54.5 94.5#




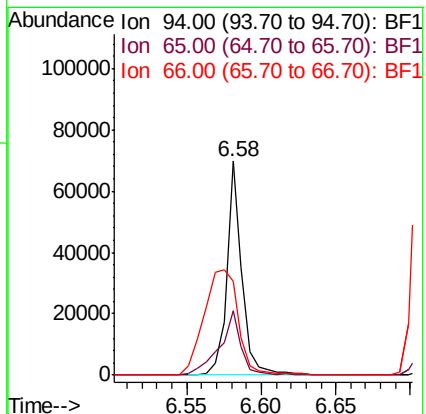


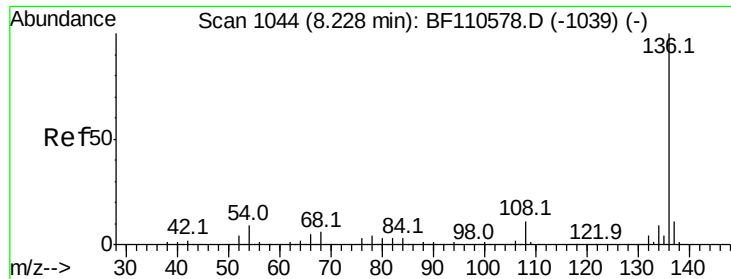

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.23 min Scan# 1044
Delta R.T. 0.00 min
Lab File: BF110636.D
Acq: 9 Nov 2018 19:20




Instrument :
BNA_F
ClientSampleId :
OLDMANS-1


Tot Ion:	136	Resp:	304553
Ion	Ratio	Lower	Upper
136	100		
137	10.7	8.8	13.2
54	7.2	5.4	8.2
68	4.7	4.2	6.2

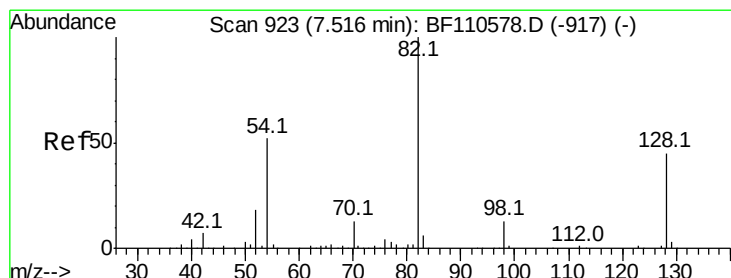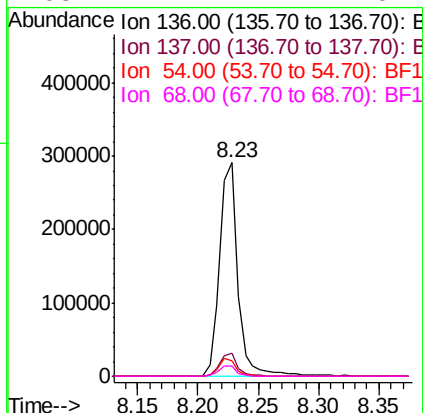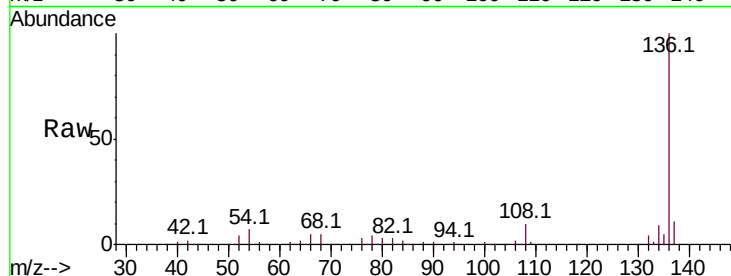

#23
Nitrobenzene-d5
Concen: 91.432 ng
RT: 7.51 min Scan# 922
Delta R.T. -0.01 min
Lab File: BF110636.D
Acq: 9 Nov 2018 19:20

Tgt Ion:	82	Resp:	483525
Ion	Ratio	Lower	Upper
82	100		
128	45.0	34.2	51.2
54	52.3	38.6	58.0

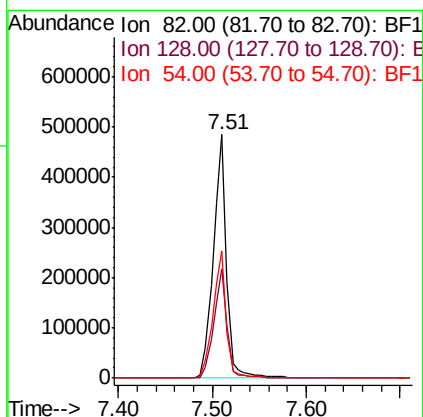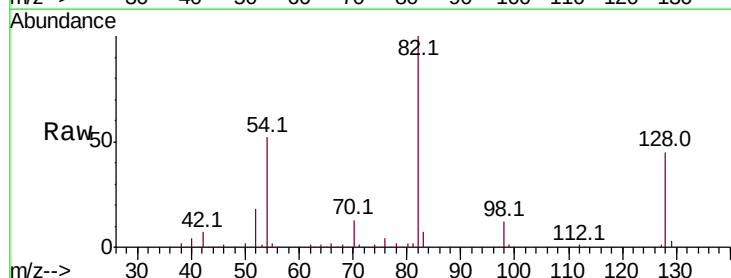


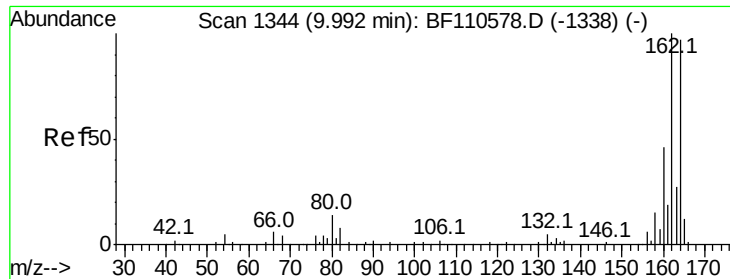




#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.99 min Scan# 1343
Delta R.T. -0.01 min
Lab File: BF110636.D
Acq: 9 Nov 2018 19:20

Instrument :
BNA_F
ClientSampleId :
OLDMANS-1

Tot Ion:164 Resp: 151027
Ion Ratio Lower Upper
164 100
162 102.5 83.0 124.6
160 47.1 37.0 55.6

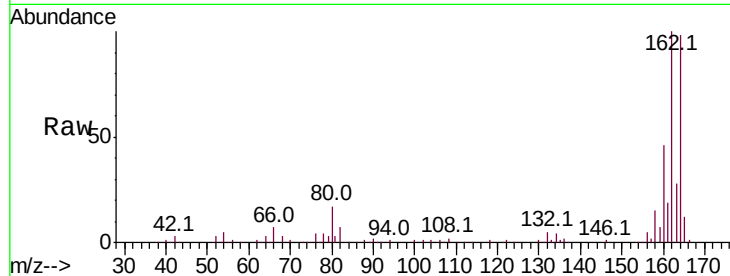


Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

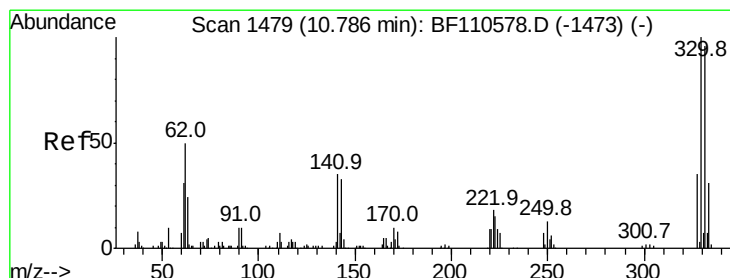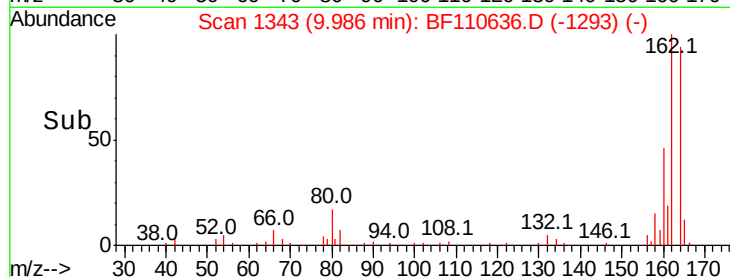
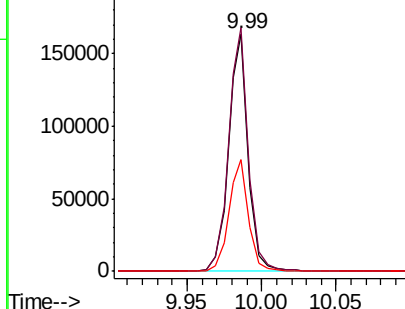



#42
2,4,6-Tribromophenol
Concen: 123.414 ng
RT: 10.78 min Scan# 1478
Delta R.T. -0.01 min
Lab File: BF110636.D
Acq: 9 Nov 2018 19:20

Tgt Ion:330 Resp: 187810
Ion Ratio Lower Upper
330 100
332 95.8 77.1 115.7
141 37.8 27.0 40.4

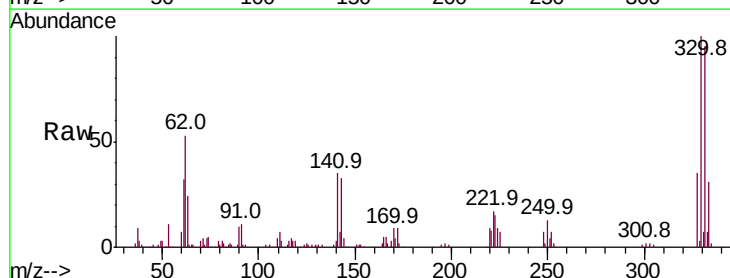

Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

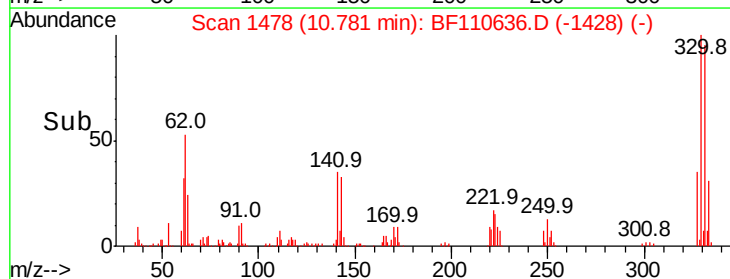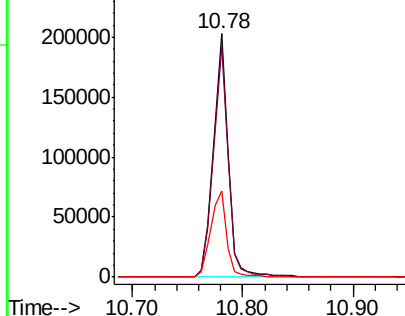







#45
2-Fluorobiphenyl
Concen: 83.764 ng
RT: 9.30 min Scan# 1226
Delta R.T. -0.01 min
Lab File: BF110636.D
Acq: 9 Nov 2018 19:20

Instrument :
BNA_F
ClientSampleId :
OLDMANS-1

Tot Ion:172 Resp: 885788
Ion Ratio Lower Upper
172 100
171 36.3 28.6 43.0
170 23.6 19.7 29.5

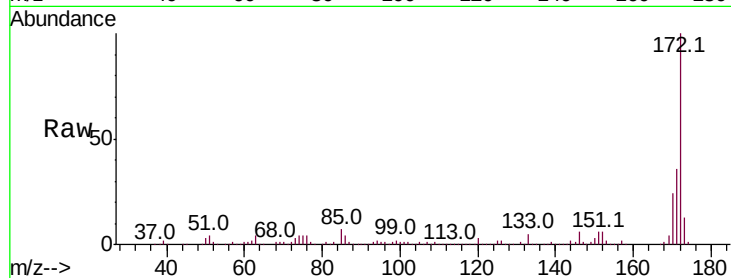


Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

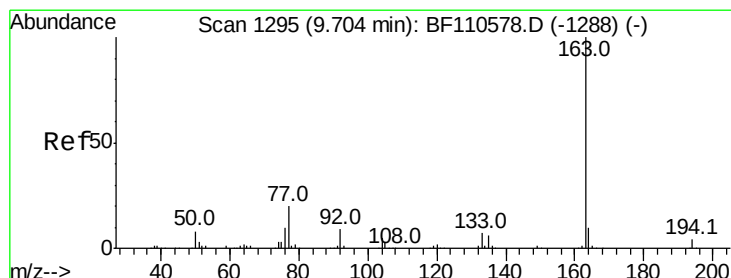
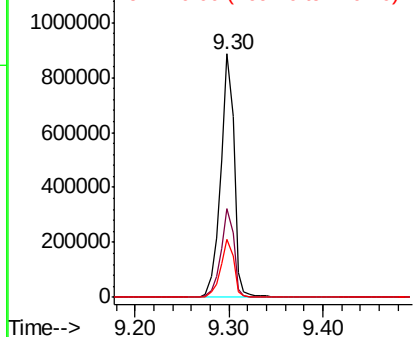



#50
Dimethylphthalate
Concen: 4.987 ng
RT: 9.69 min Scan# 1293
Delta R.T. -0.01 min
Lab File: BF110636.D
Acq: 9 Nov 2018 19:20

Tgt Ion:163 Resp: 56200
Ion Ratio Lower Upper
163 100
194 4.0 3.2 4.8
164 10.1 8.1 12.1

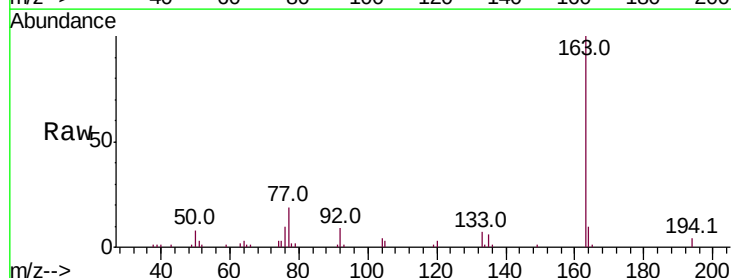

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E




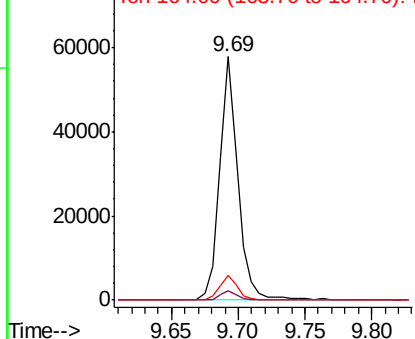


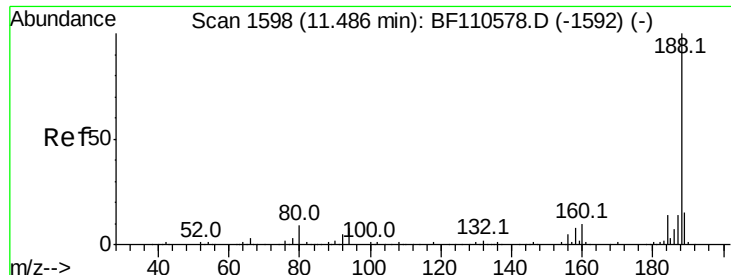

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.48 min Scan# 1597
Delta R.T. -0.01 min
Lab File: BF110636.D
Acq: 9 Nov 2018 19:20




Instrument :
BNA_F
ClientSampleId :
OLDMANS-1


Tot Ion:188 Resp: 305586
Ion Ratio Lower Upper
188 100
94 8.1 7.2 10.8
80 9.0 7.9 11.9

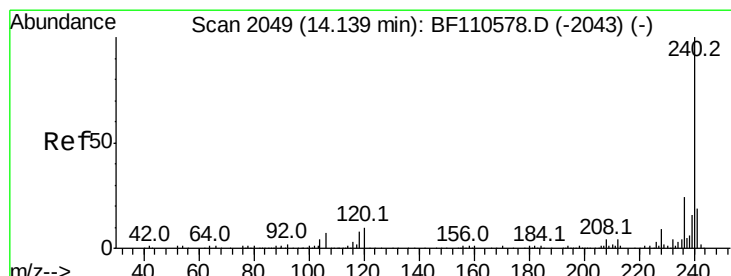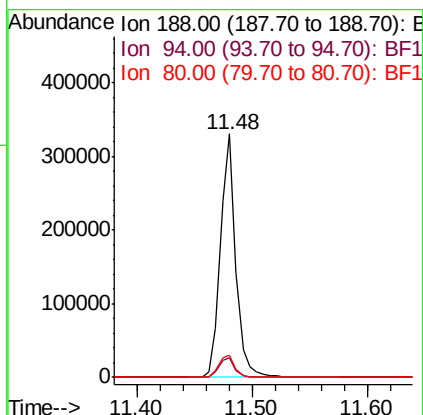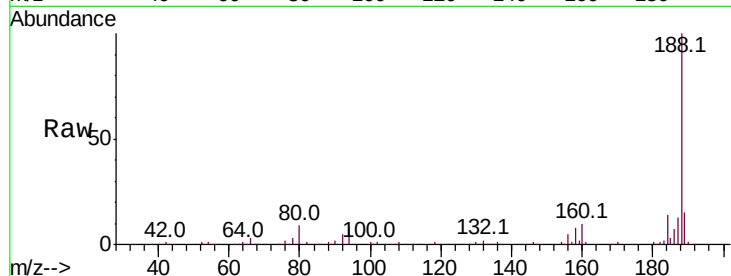

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.13 min Scan# 2047
Delta R.T. -0.01 min
Lab File: BF110636.D
Acq: 9 Nov 2018 19:20

Tgt Ion:240 Resp: 242609
Ion Ratio Lower Upper
240 100
120 12.4 8.3 12.5
236 25.8 21.2 31.8

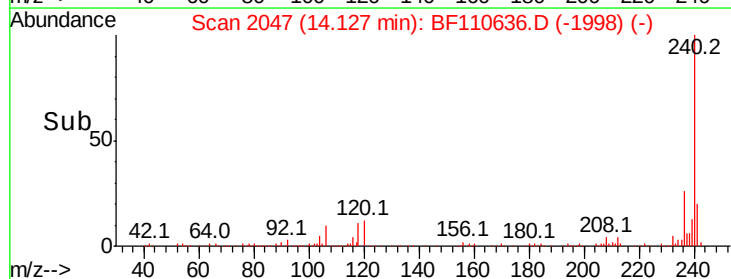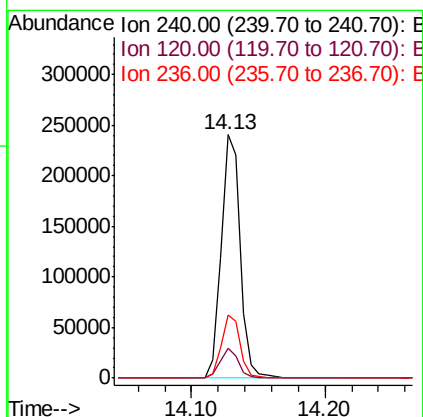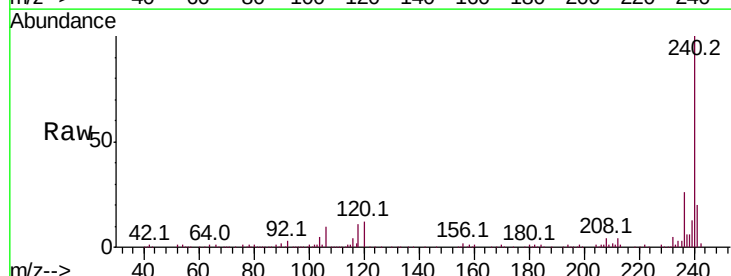



#79

Terphenyl-d14

Concen: 73.205 ng

RT: 13.06 min Scan# 1866

Delta R.T. -0.01 min

Lab File: BF110636.D

Acq: 9 Nov 2018 19:20

Instrument :

BNA_F

ClientSampleId :

OLDMANS-1


Tot Ion:244 Resp: 948344

Ion Ratio Lower Upper

244 100

212 6.9 5.8 8.8




122 13.2 8.7 13.1#

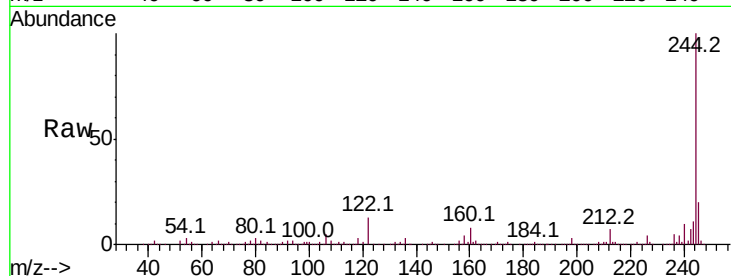

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

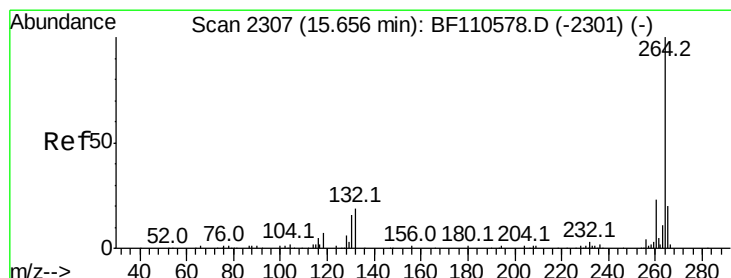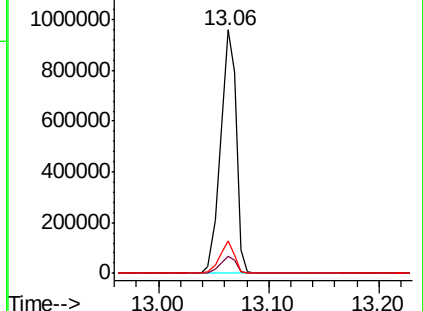

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.66 min Scan# 2307

Delta R.T. 0.00 min

Lab File: BF110636.D

Acq: 9 Nov 2018 19:20


Tgt Ion:264 Resp: 148782

Ion Ratio Lower Upper

264 100

260 24.1 18.7 28.1

265 20.9 16.7 25.1

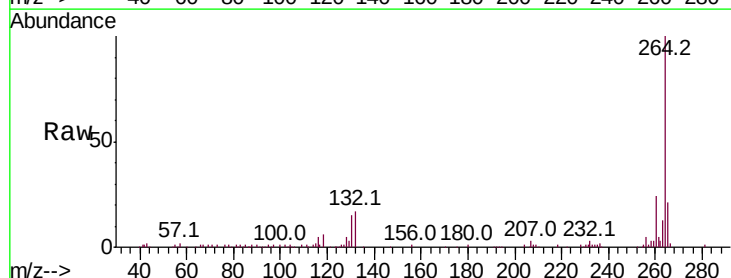

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

