

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF110918\
 Data File : BF110668.D
 Acq On : 10 Nov 2018 10:17
 Operator : JU/SJ
 Sample : J5881-19
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 110718-SIDI-E-U-B

Quant Time: Nov 11 04:28:48 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF110818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 09 15:13:13 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.95	152	71809	20.00	ng	0.00
21) Naphthalene-d8	8.23	136	295925	20.00	ng	0.00
39) Acenaphthene-d10	9.99	164	123111	20.00	ng	0.00
64) Phenanthrene-d10	11.48	188	184399	20.00	ng	0.00
76) Chrysene-d12	14.13	240	141232	20.00	ng	-0.01
87) Perylene-d12	15.66	264	103720	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.56	112	198287	44.85	ng	0.00
7) Phenol-d6	6.56	99	151643	26.82	ng	-0.01
23) Nitrobenzene-d5	7.51	82	518835	100.97	ng	0.00
42) 2,4,6-Tribromophenol	10.78	330	98178	79.14	ng	0.00
45) 2-Fluorobiphenyl	9.30	172	948660	110.05	ng	0.00
79) Terphenyl-d14	13.06	244	571249	75.75	ng	0.00
Target Compounds						
50) Dimethylphthalate	9.69	163	20516	2.233	ng	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF110918\
Data File : BF110668.D
Acq On : 10 Nov 2018 10:17
Operator : JU/SJ
Sample : J5881-19
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
110718-SIDI-E-U-B

Quant Time: Nov 11 04:28:48 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF110818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 09 15:13:13 2018
Response via : Initial Calibration

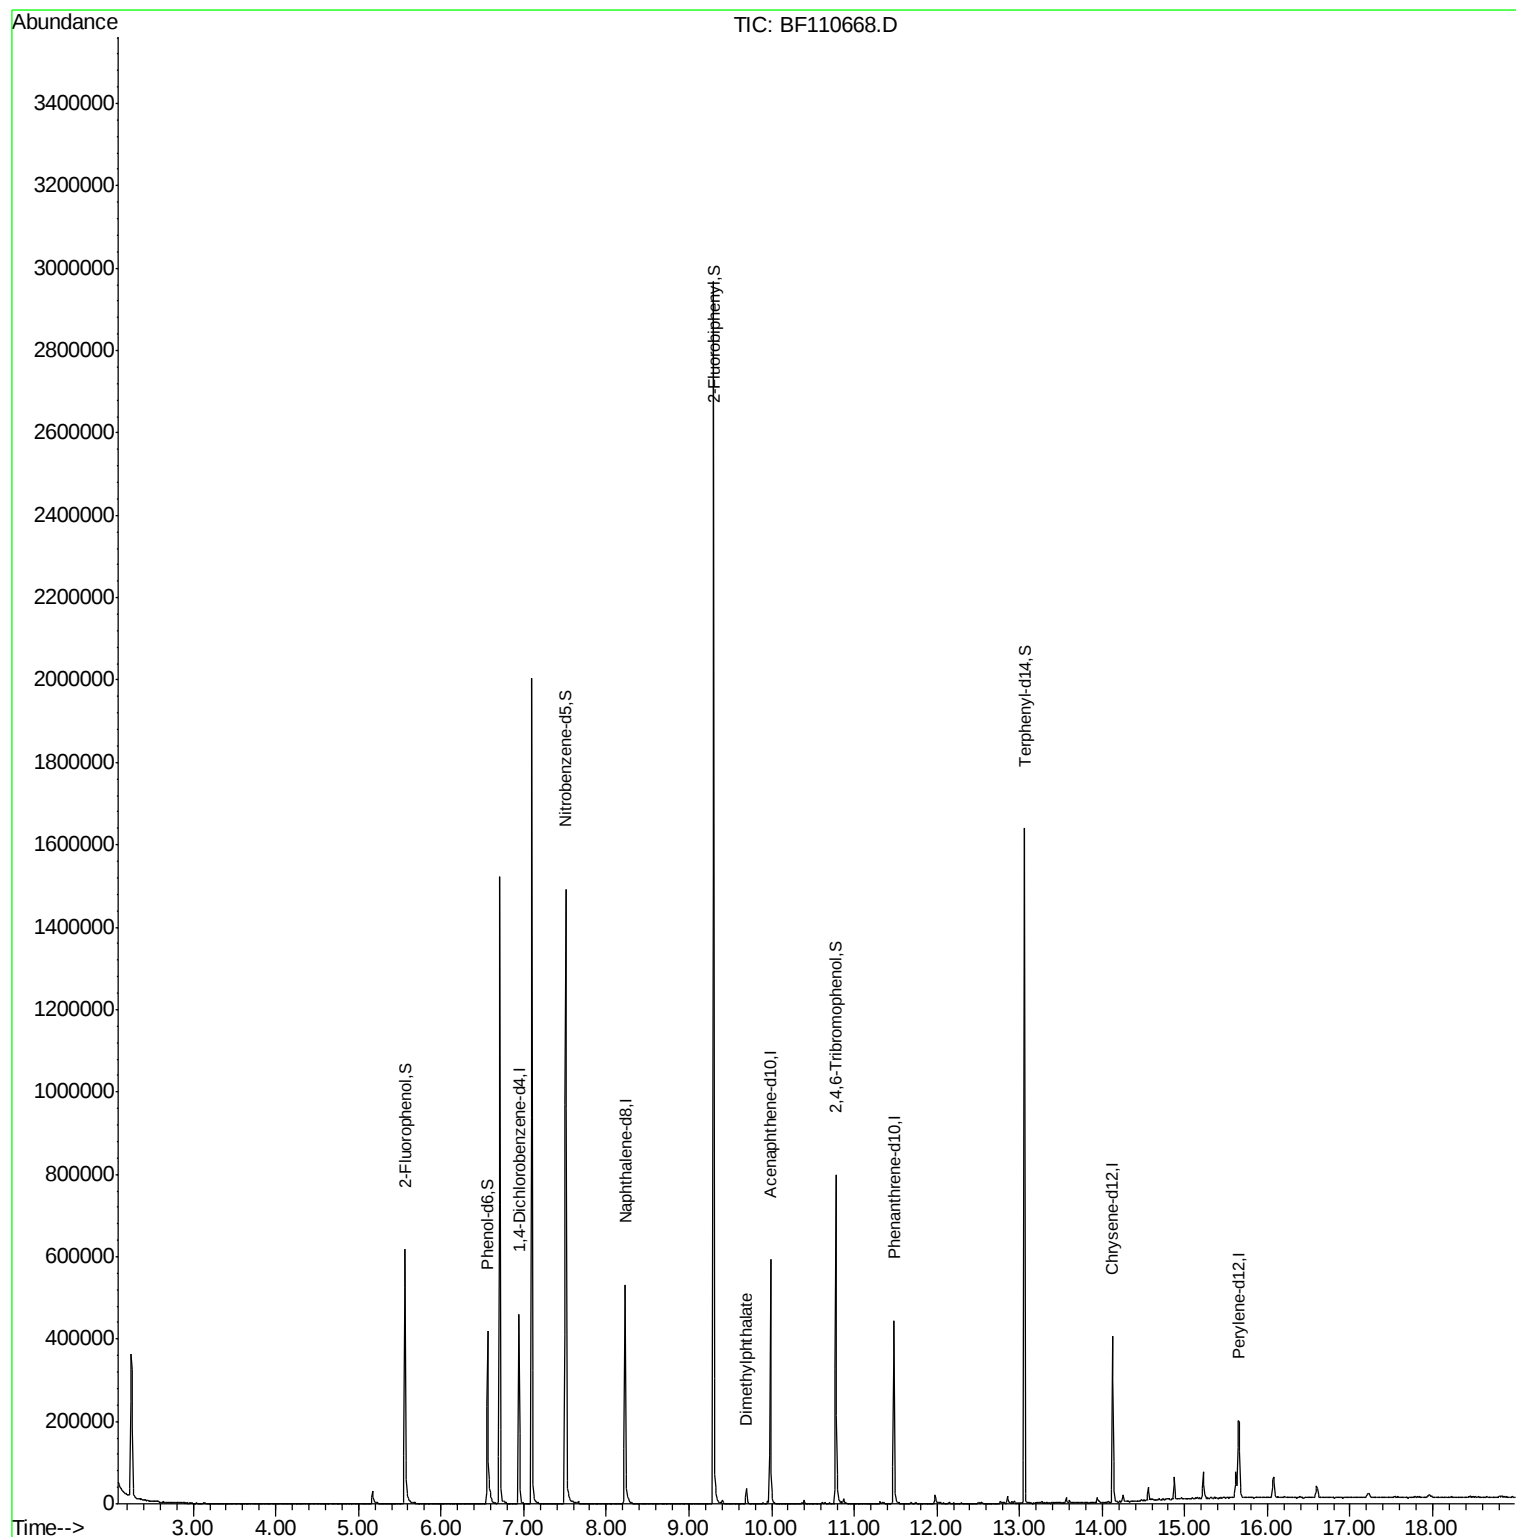

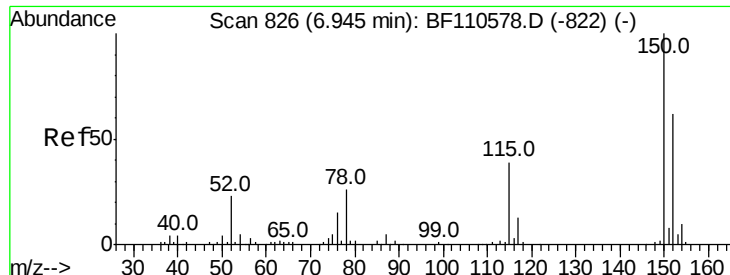


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.95 min Scan# 826
Delta R.T. 0.00 min
Lab File: BF110668.D
Acq: 10 Nov 2018 10:17

Instrument :
BNA_F
ClientSampleId :
110718-SIDI-E-U-B

Tot Ion:152 Resp: 71809
Ion Ratio Lower Upper
152 100
150 153.6 122.7 184.1
115 59.1 49.1 73.7

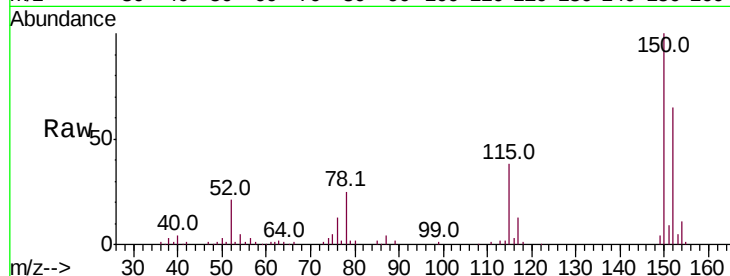


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

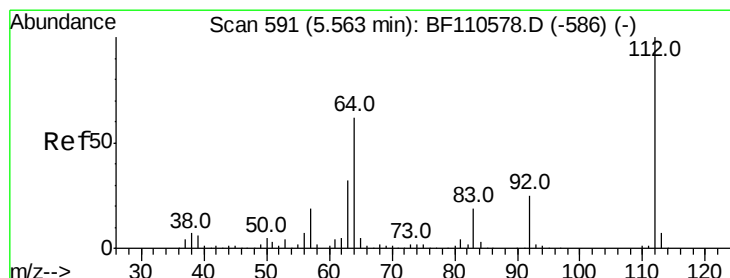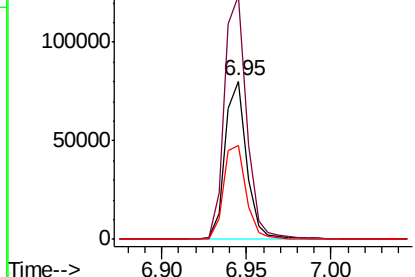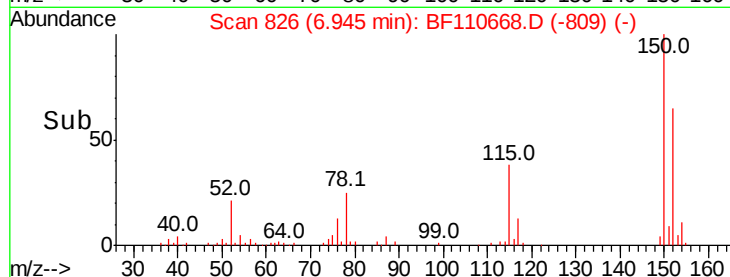



#5


2-Fluorophenol
Concen: 44.852 ng
RT: 5.56 min Scan# 591
Delta R.T. 0.00 min
Lab File: BF110668.D
Acq: 10 Nov 2018 10:17

Tgt Ion:112 Resp: 198287
Ion Ratio Lower Upper
112 100
64 57.5 44.1 66.1
63 30.2 23.7 35.5

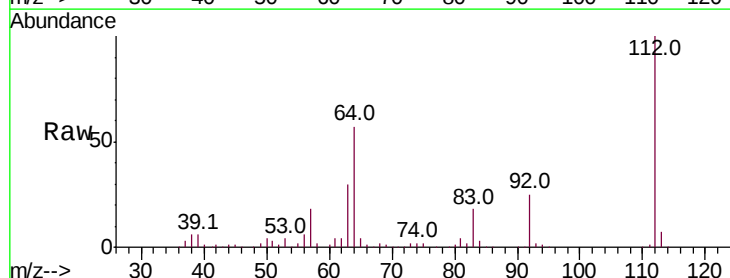

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

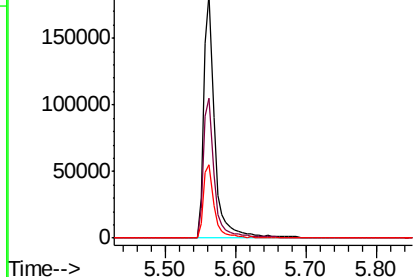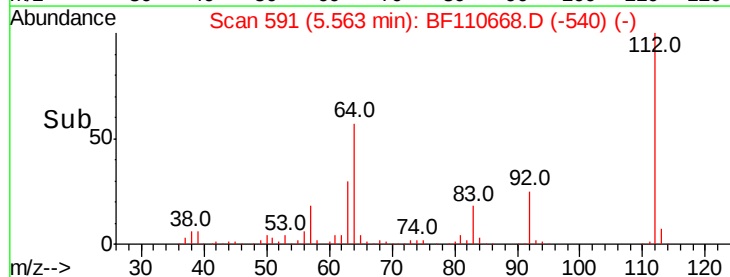

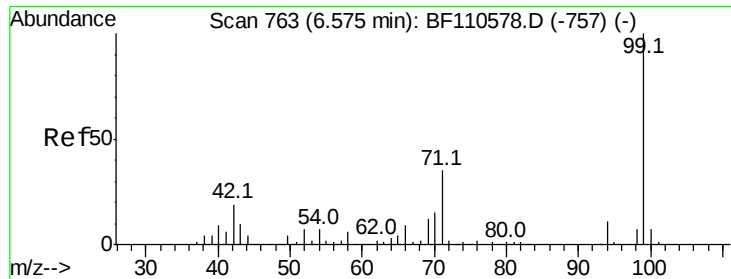

#7

Phenol-d6

Concen: 26.824 ng

RT: 6.56 min Scan# 761

Delta R.T. -0.01 min

Lab File: BF110668.D

Acq: 10 Nov 2018 10:17

Instrument :

BNA_F

ClientSampleId :

110718-SIDI-E-U-B


Tot Ion: 99 Resp: 151643

Ion Ratio Lower Upper




99 100

42 18.2 15.8 23.6

71 33.8 28.0 42.0



Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

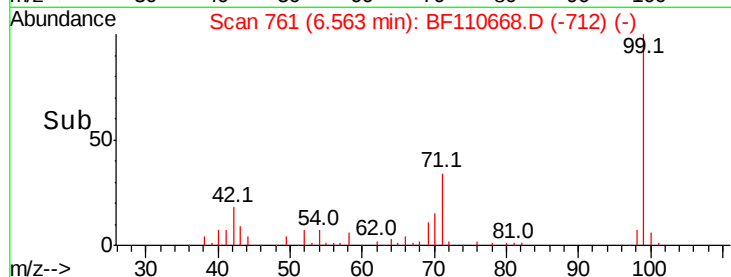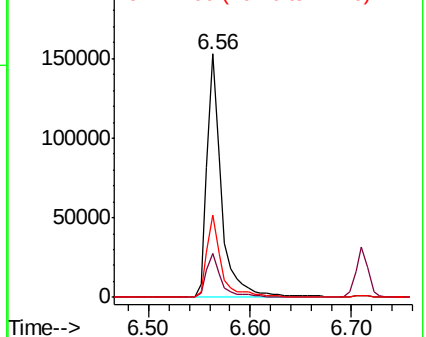

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.23 min Scan# 1044

Delta R.T. 0.00 min

Lab File: BF110668.D

Acq: 10 Nov 2018 10:17

Tgt Ion: 136 Resp: 295925


Ion Ratio Lower Upper

136 100



137 10.6 8.8 13.2


54 7.5 5.4 8.2

68 4.9 4.2 6.2



Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1



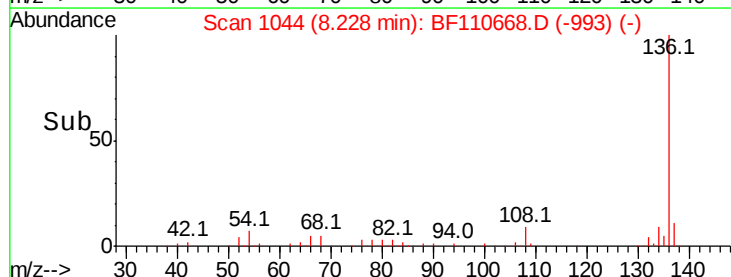
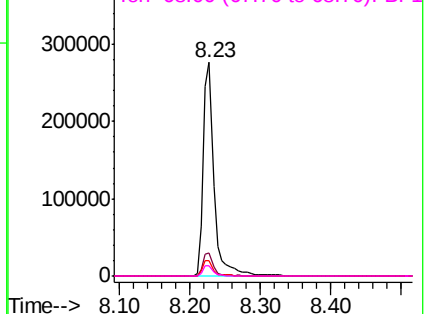


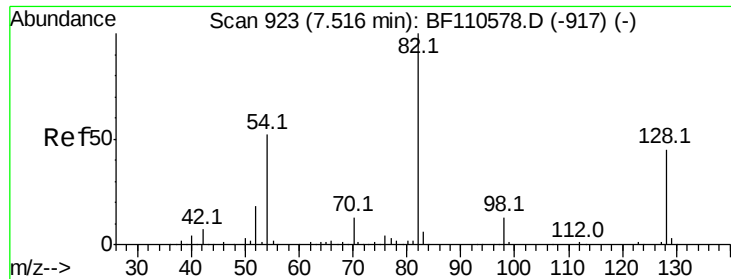

#23
 Nitrobenzene-d5
 Concen: 100.970 ng
 RT: 7.51 min Scan# 922
 Delta R.T. -0.01 min
 Lab File: BF110668.D
 Acq: 10 Nov 2018 10:17




Instrument :
 BNA_F
 ClientSampleId :
 110718-SIDI-E-U-B


Tot Ion: 82 Resp: 518835
 Ion Ratio Lower Upper
 82 100
 128 45.0 34.2 51.2
 54 52.9 38.6 58.0

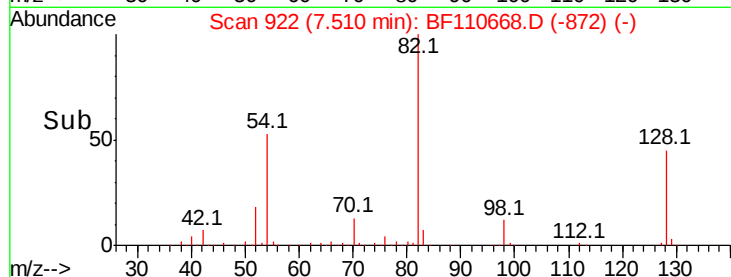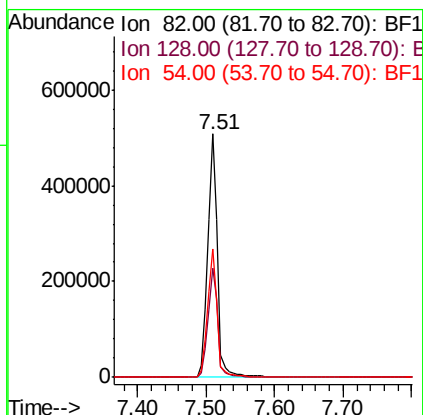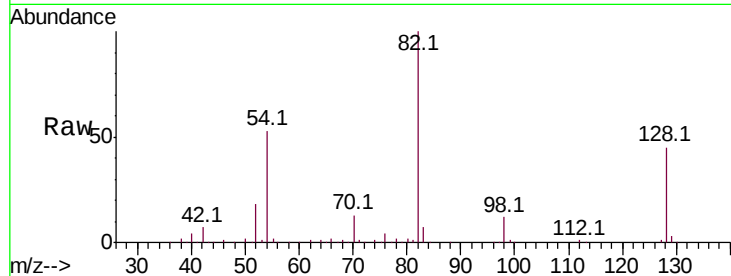

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.99 min Scan# 1343
 Delta R.T. -0.01 min
 Lab File: BF110668.D
 Acq: 10 Nov 2018 10:17

Tgt Ion: 164 Resp: 123111
 Ion Ratio Lower Upper
 164 100
 162 107.3 83.0 124.6
 160 47.6 37.0 55.6

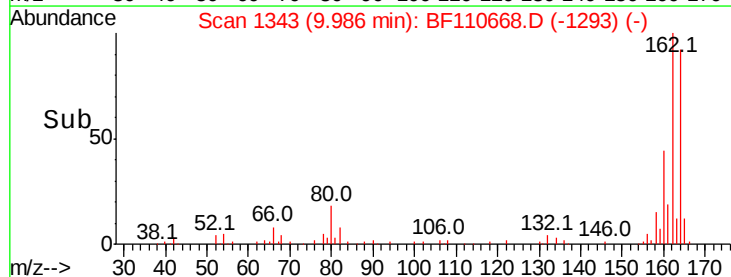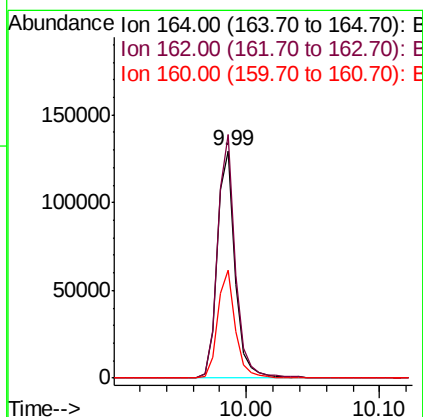


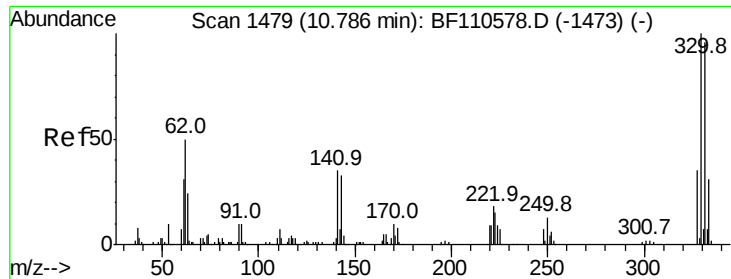

#42
 2,4,6-Tribromophenol
 Concen: 79.144 ng
 RT: 10.78 min Scan# 1478
 Delta R.T. -0.01 min
 Lab File: BF110668.D
 Acq: 10 Nov 2018 10:17

Instrument :
 BNA_F
 ClientSampleId :
 110718-SIDI-E-U-B

Tot Ion	Ratio	Lower	Upper
330	100		
332	95.2	77.1	115.7
141	37.2	27.0	40.4



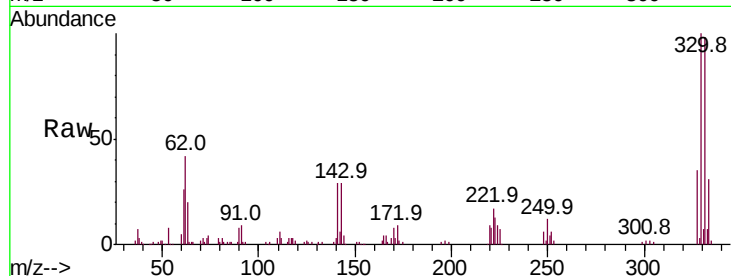


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

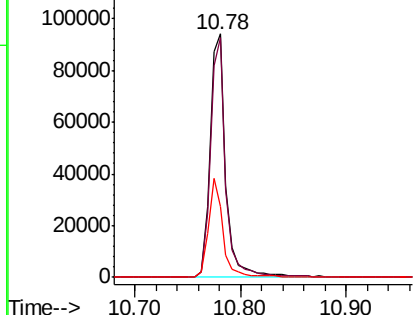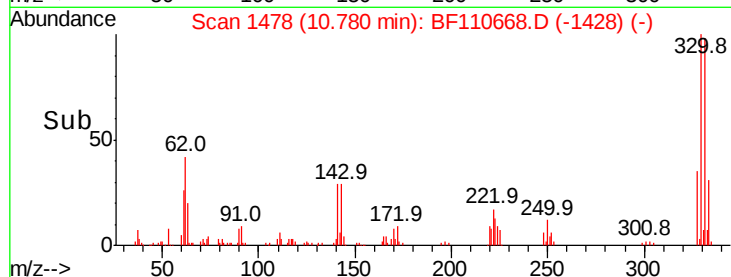

#45
 2-Fluorobiphenyl
 Concen: 110.052 ng
 RT: 9.30 min Scan# 1226
 Delta R.T. -0.01 min
 Lab File: BF110668.D
 Acq: 10 Nov 2018 10:17

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.3	28.6	43.0
170	23.6	19.7	29.5






Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

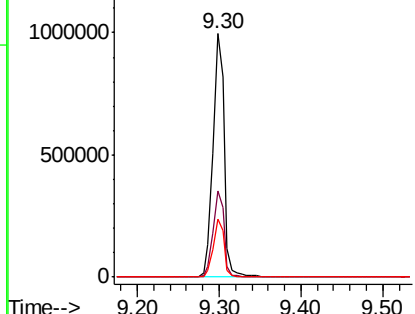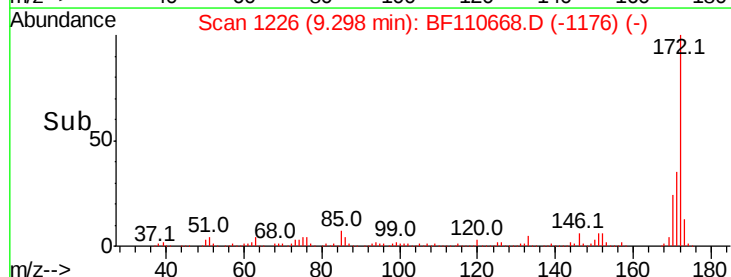

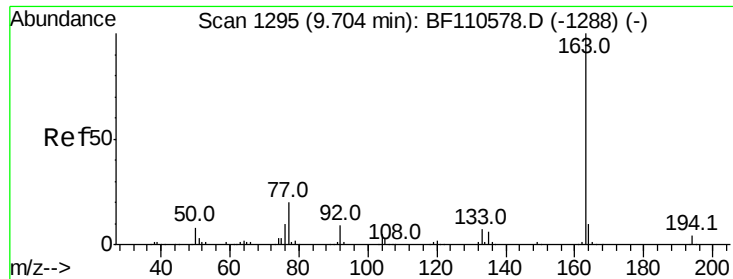

#50

Dimethylphthalate

Concen: 2.233 ng

RT: 9.69 min Scan# 1293

Delta R.T. -0.01 min

Lab File: BF110668.D

Acq: 10 Nov 2018 10:17

Instrument :

BNA_F

ClientSampleId :

110718-SIDI-E-U-B


Tot Ion:163 Resp: 20516

Ion Ratio Lower Upper

163 100

194 3.8 3.2 4.8




164 11.3 8.1 12.1

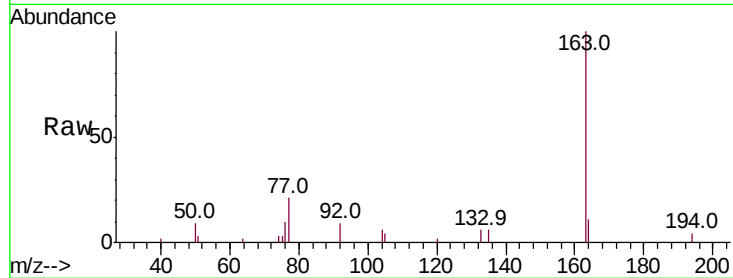

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

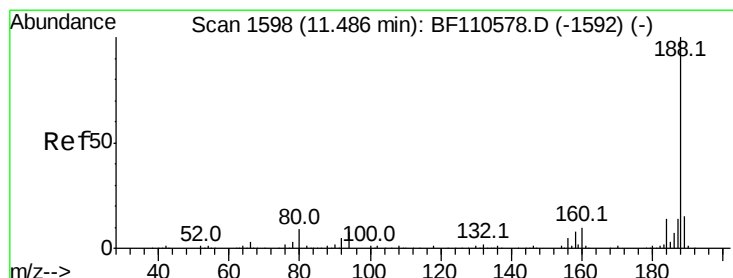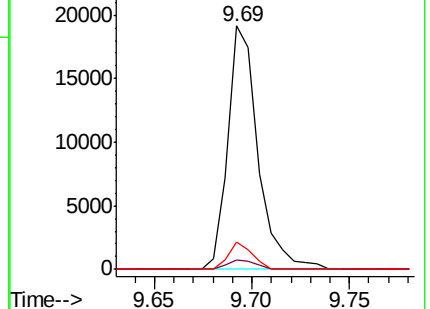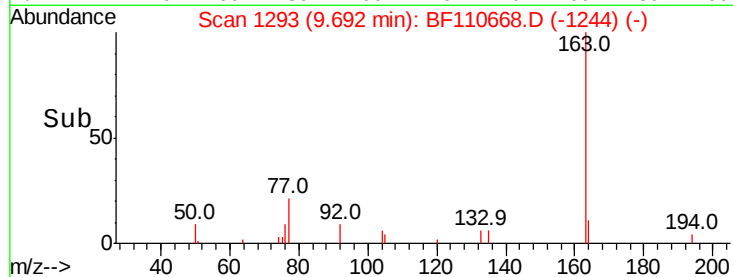

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.48 min Scan# 1597

Delta R.T. -0.01 min

Lab File: BF110668.D

Acq: 10 Nov 2018 10:17


Tgt Ion:188 Resp: 184399

Ion Ratio Lower Upper

188 100

94 8.6 7.2 10.8



80 9.2 7.9 11.9

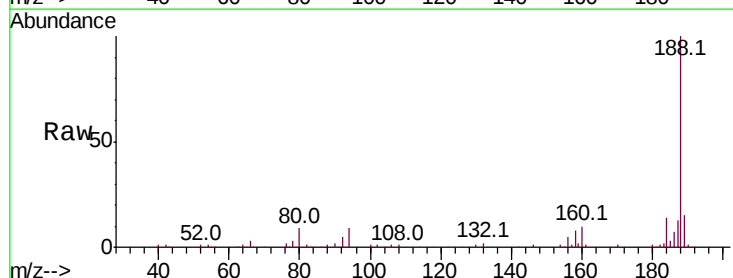


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

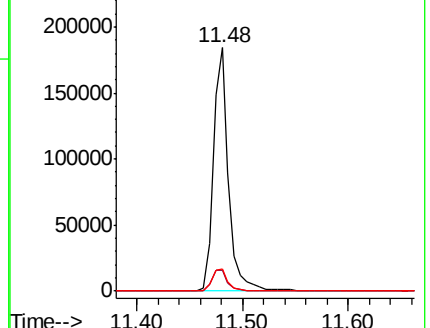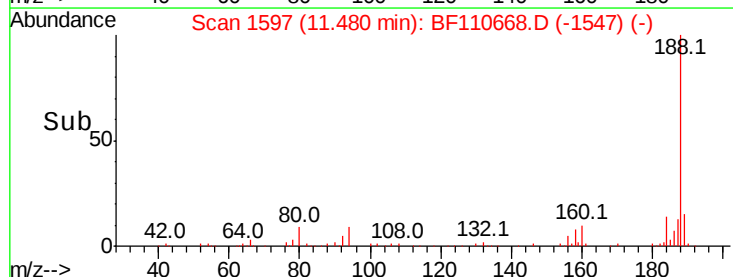


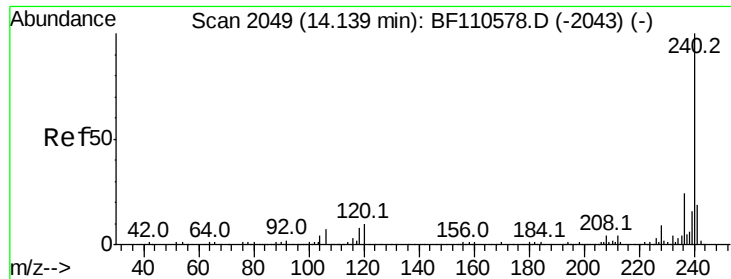




#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.13 min Scan# 2047
Delta R.T. -0.01 min
Lab File: BF110668.D
Acq: 10 Nov 2018 10:17

Instrument :
BNA_F
ClientSampleId :
110718-SIDI-E-U-B

Tot Ion	Ratio	Lower	Upper
240	100		
120	12.3	8.3	12.5
236	25.3	21.2	31.8




Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

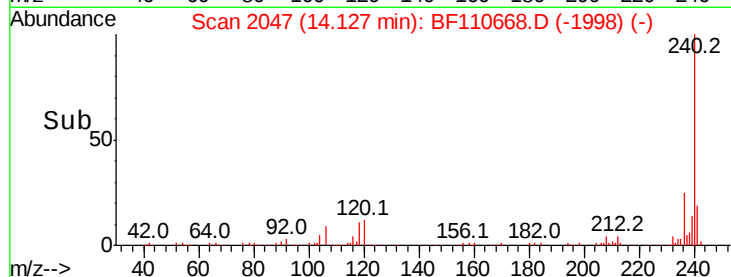
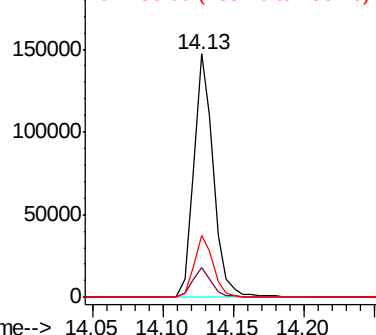



#79
Terphenyl-d14
Concen: 75.749 ng
RT: 13.06 min Scan# 1866
Delta R.T. -0.01 min
Lab File: BF110668.D
Acq: 10 Nov 2018 10:17

Tgt Ion	Ratio	Lower	Upper
244	100		
212	6.5	5.8	8.8
122	10.3	8.7	13.1



Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

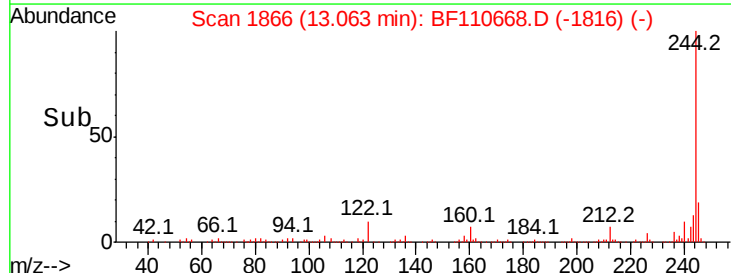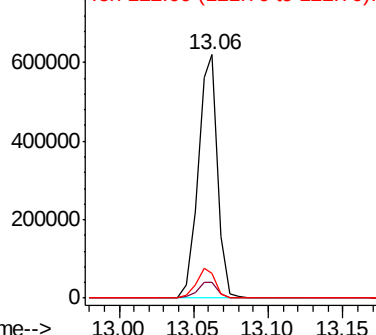

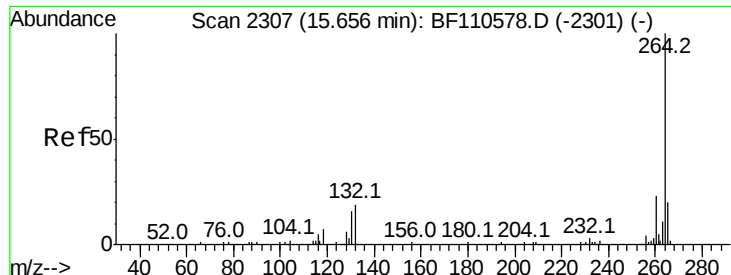

#87
Pervlene-d12
Concen: 20.000 ng
RT: 15.66 min Scan# 2307
Delta R.T. 0.00 min
Lab File: BF110668.D
Acq: 10 Nov 2018 10:17

Instrument :
BNA_F
ClientSampleId :
110718-SIDI-E-U-B

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.2	18.7	28.1
265	20.5	16.7	25.1

