

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF110918\
 Data File : BF110664.D
 Acq On : 10 Nov 2018 8:29
 Operator : JU/SJ
 Sample : J5881-15
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 110718-DBRI-E-U-M

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.246	22	27	42	rVB	318239	421216	16.02%	3.129%
2	5.169	520	524	534	rBV	34860	49074	1.87%	0.365%
3	5.563	587	591	604	rBV	455724	511261	19.45%	3.798%
4	6.563	758	761	782	rBV2	330598	403181	15.34%	2.995%
5	6.710	782	786	801	rVV	1277231	1080322	41.09%	8.025%
6	6.945	822	826	832	rBV	509295	443543	16.87%	3.295%
7	7.098	848	852	856	rBV	1846781	1789221	68.06%	13.290%
8	7.510	917	922	925	rBV	1505996	1409218	53.60%	10.468%
9	8.228	1040	1044	1057	rBV	600339	589577	22.43%	4.379%
10	9.298	1222	1226	1241	rBV	2808493	2628989	100.00%	19.528%
11	9.692	1290	1293	1302	rBV	70744	66105	2.51%	0.491%
12	9.986	1339	1343	1356	rVB	627457	576258	21.92%	4.280%
13	10.774	1474	1477	1491	rBV	645013	654042	24.88%	4.858%
14	11.480	1593	1597	1607	rBV	459113	452444	17.21%	3.361%
15	13.063	1861	1866	1869	rBV	1636502	1494729	56.86%	11.103%
16	13.939	2008	2015	2023	rBV2	21962	37542	1.43%	0.279%
17	14.127	2043	2047	2058	rBV	410301	400144	15.22%	2.972%
18	14.874	2171	2174	2179	rVB	31724	30290	1.15%	0.225%
19	15.221	2230	2233	2238	rVB	38209	46909	1.78%	0.348%
20	15.621	2297	2301	2303	rBV	41604	52216	1.99%	0.388%
21	15.656	2303	2307	2315	rVB2	199211	278424	10.59%	2.068%
22	16.074	2373	2378	2384	rVB2	29145	47942	1.82%	0.356%


Sum of corrected areas: 13462647

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF110918\
Data File : BF110664.D
Acq On : 10 Nov 2018 8:29
Operator : JU/SJ
Sample : J5881-15
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
110718-DBRI-E-U-M

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF110818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

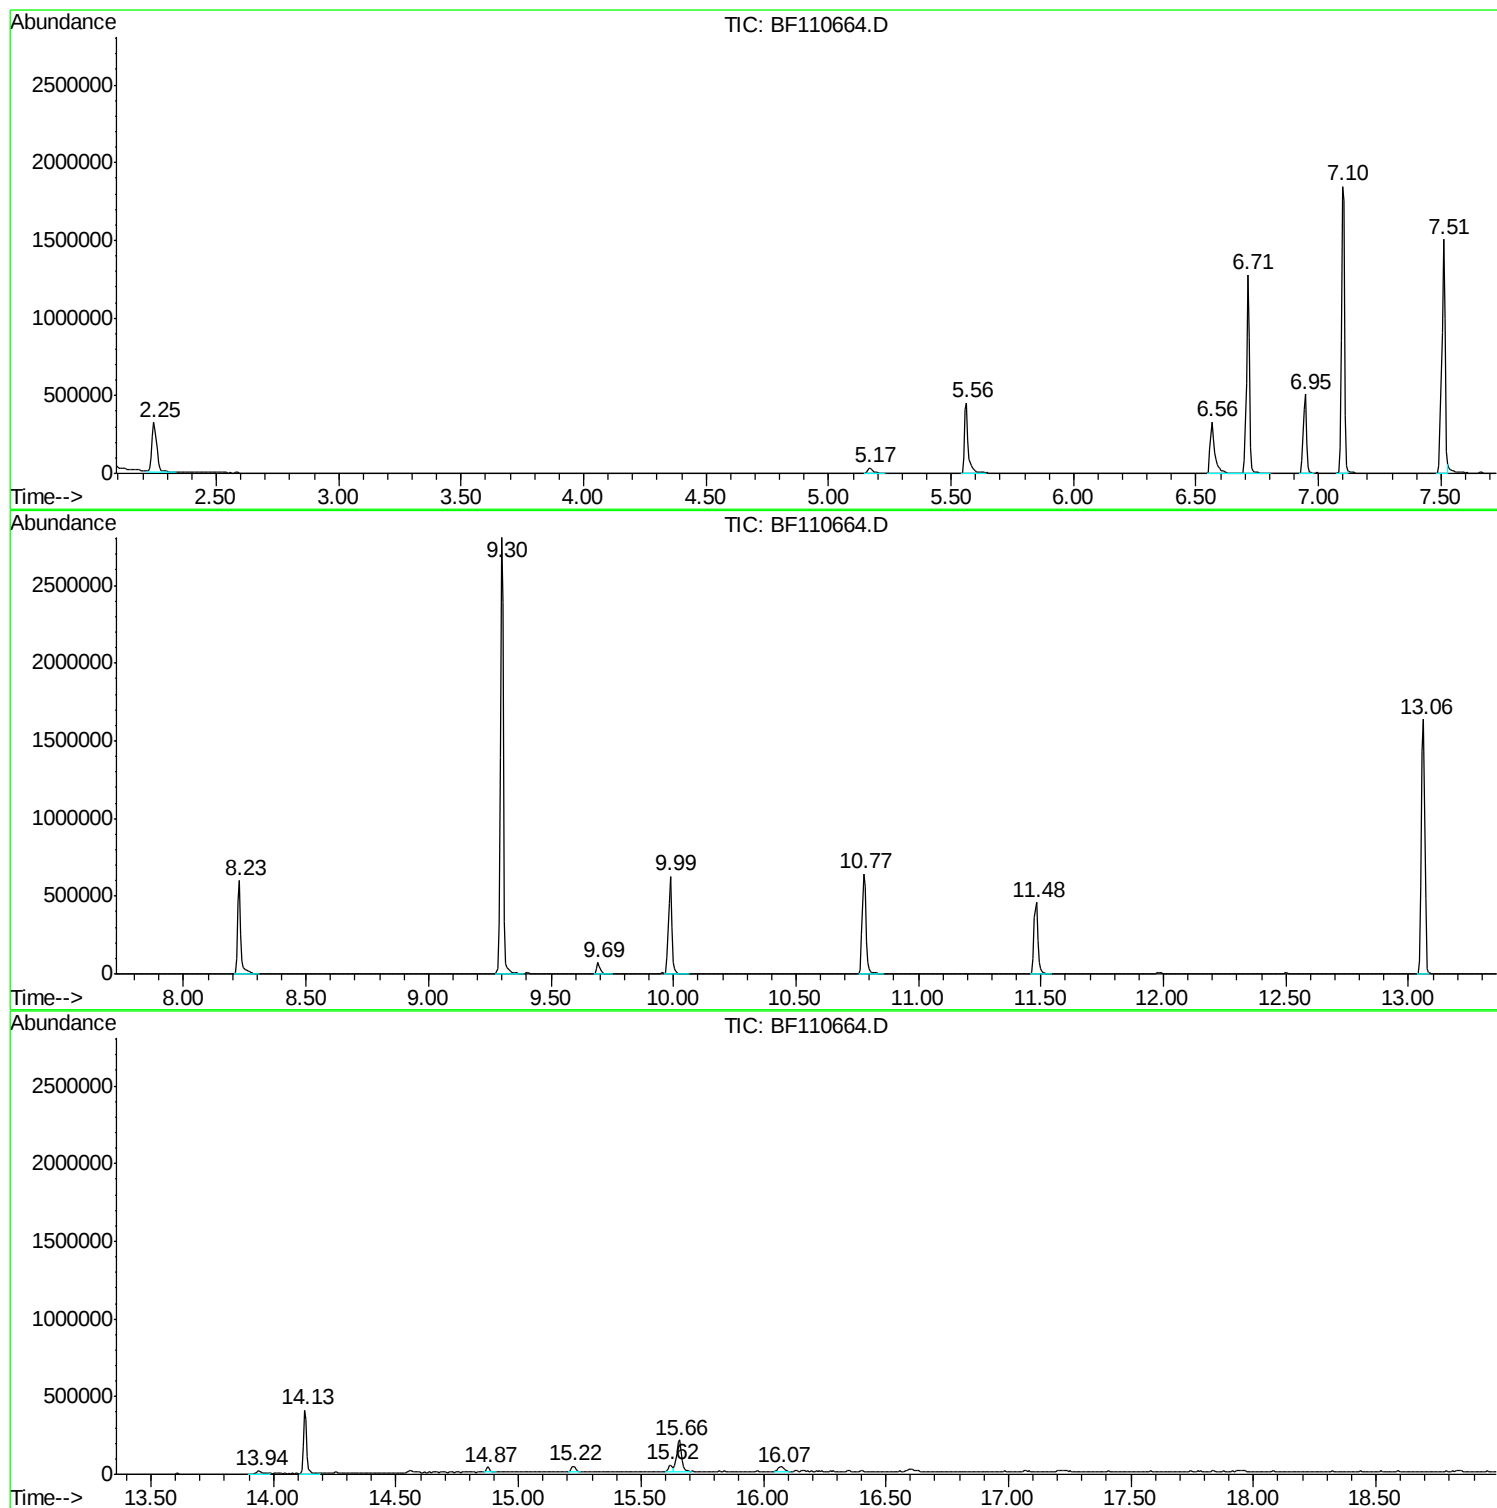

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF110918\
Data_File : BF110664.D
Acq_On : 10 Nov 2018 8:299
Operator : JU/SJJ
Sample : J5881-155
Misc :
ALS_Vial : 33 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
110718-DBRI-E-U-M

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110818.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
