

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111120\
 Data File : BF122305.D
 Acq On : 11 Nov 2020 10:09
 Operator : JU/CG
 Sample : PB132419BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB132419BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF122305.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.493	572	579	582	rBV	7349071	8759968	76.74%	13.232%
2	6.487	741	748	751	rBV	6840301	9014903	78.97%	13.617%
3	6.863	809	812	816	rVB	2093532	1723939	15.10%	2.604%
4	7.428	902	908	911	rBV	5330454	5817421	50.96%	8.787%
5	8.151	1026	1031	1034	rVB	2256499	2273541	19.92%	3.434%
6	9.228	1208	1214	1217	rBV	8971003	10289089	90.13%	15.542%
7	9.904	1323	1329	1332	rBV	2956609	2601095	22.79%	3.929%
8	10.692	1456	1463	1466	rBV	6160312	6587109	57.70%	9.950%
9	11.386	1575	1581	1585	rBV	2969595	2663729	23.33%	4.024%
10	12.980	1845	1852	1856	rBV	9583790	11415754	100.00%	17.244%
11	14.027	2026	2030	2033	rBV	3057168	2627870	23.02%	3.969%
12	15.498	2274	2280	2286	rBV	2003969	2427827	21.27%	3.667%




Sum of corrected areas: 66202245

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111120\
Data File : BF122305.D
Acq On : 11 Nov 2020 10:09
Operator : JU/CG
Sample : PB132419BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB132419BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

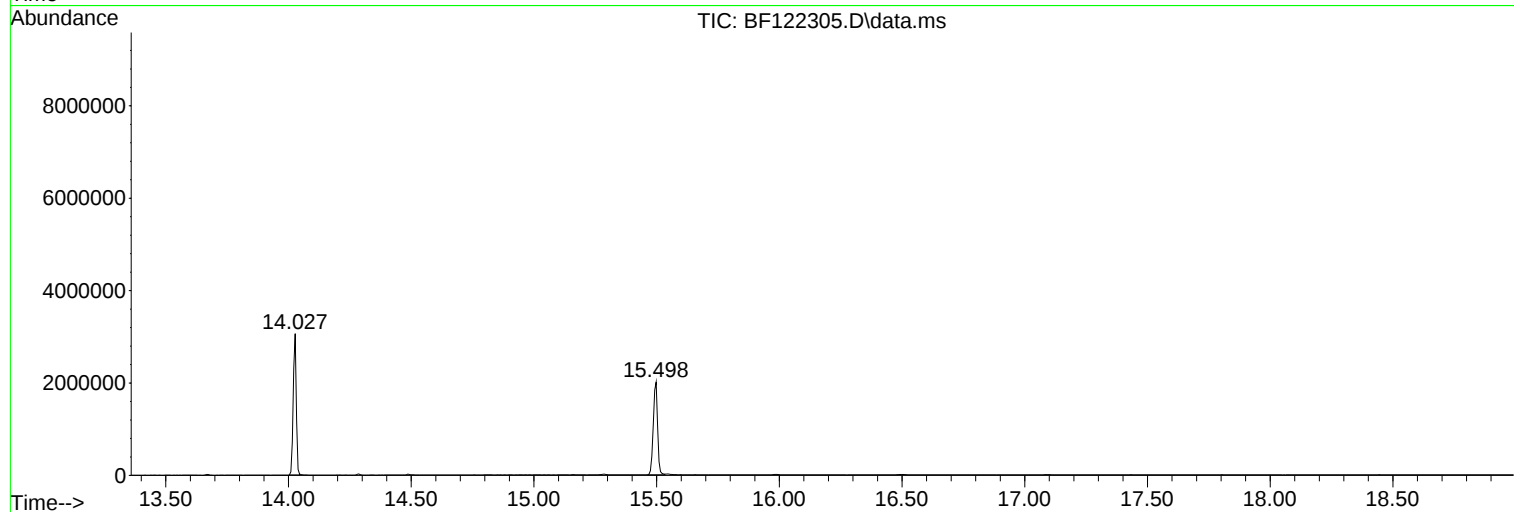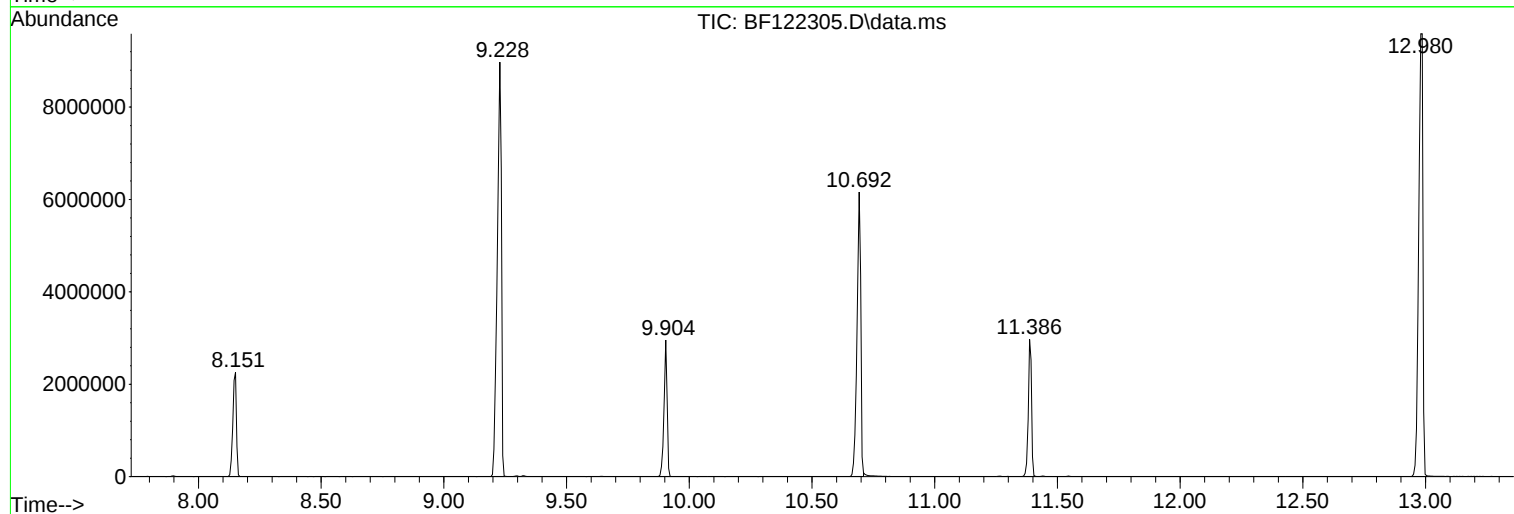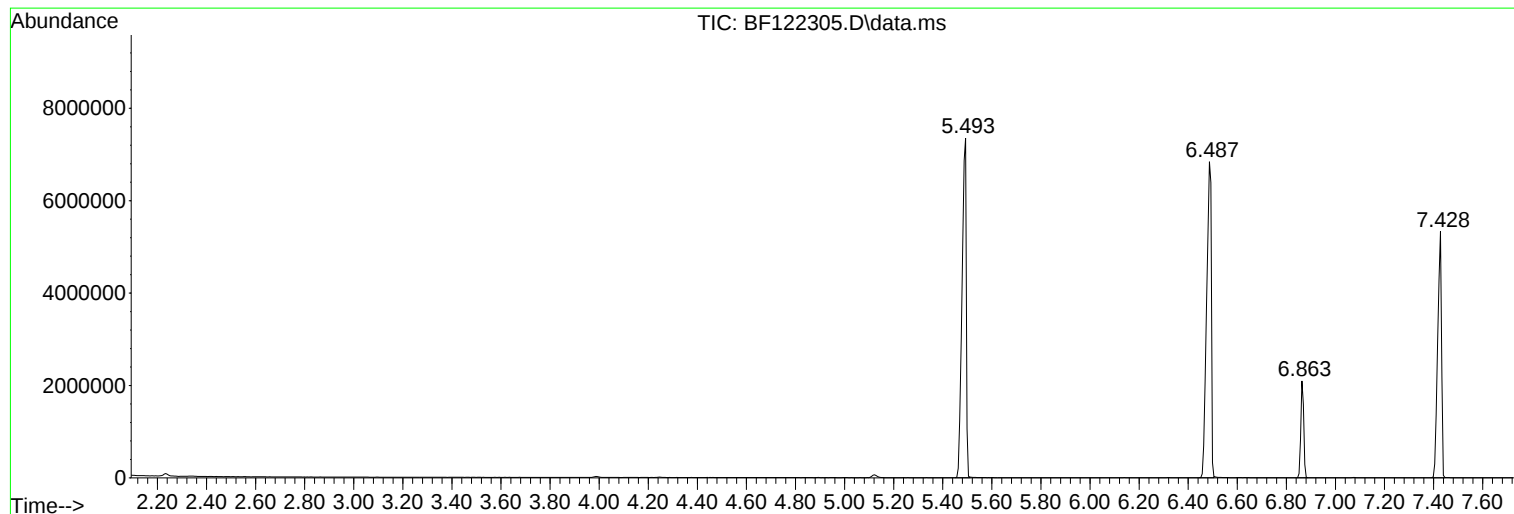

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111120\
Data File : BF122305.D
Acq On : 11 Nov 2020 10:09
Operator : JU/CG
Sample : PB132419BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB132419BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111120\
Data File : BF122305.D
Acq On : 11 Nov 2020 10:09
Operator : JU/CG
Sample : PB132419BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB132419BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------