
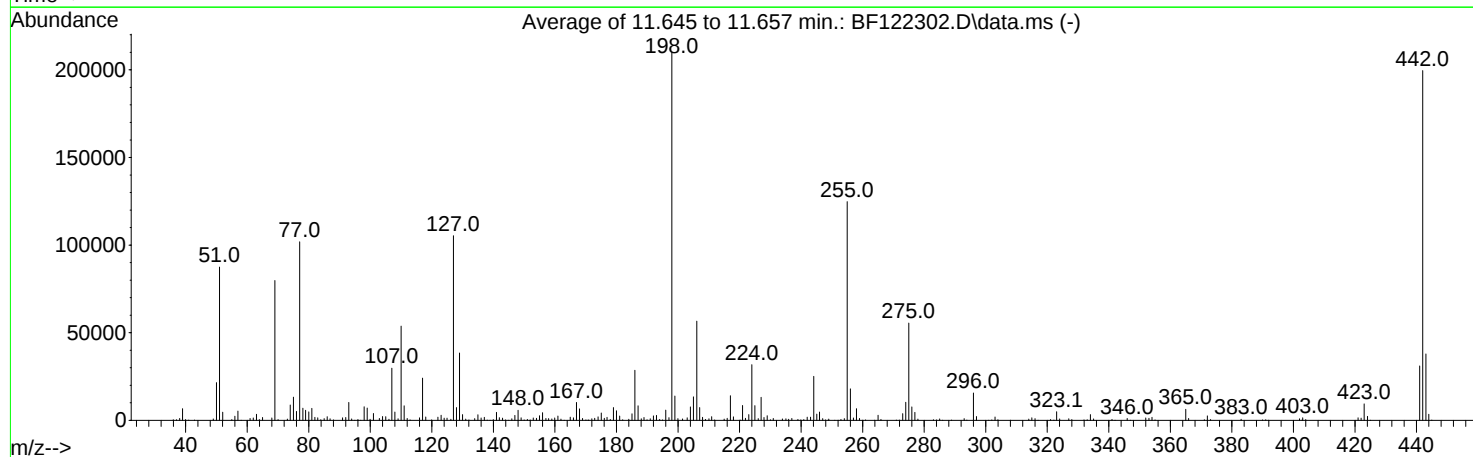


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111120\
 Data File : BF122302.D
 Acq On : 11 Nov 2020 8:37
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 10 12:25:42 2020

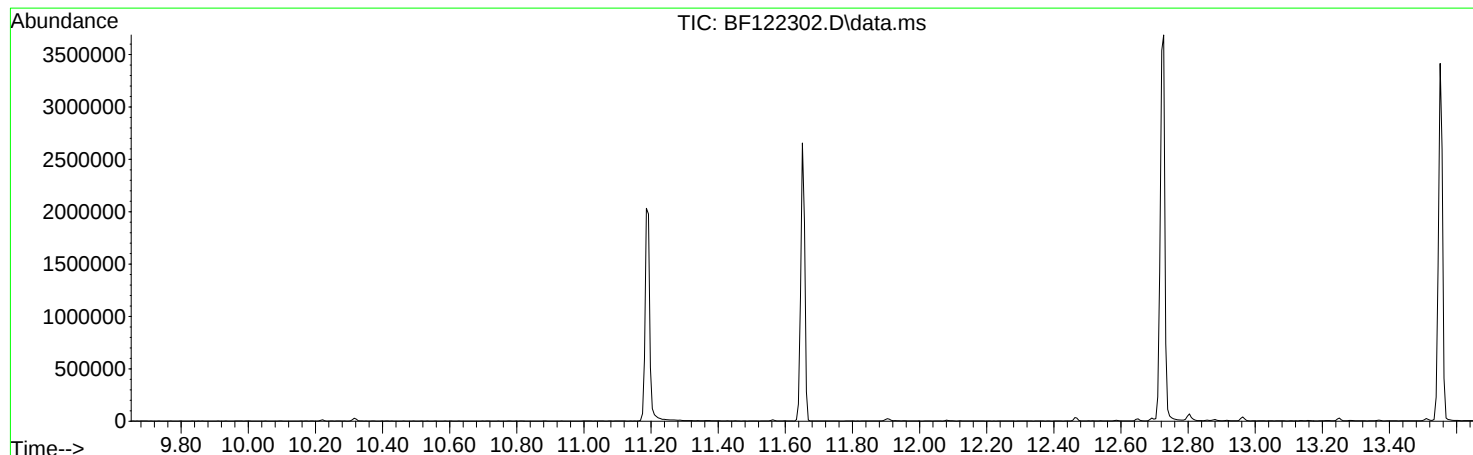

AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.7	87437	PASS
68	69	0.00	2	1.7	1381	PASS
69	198	0.00	100	38.0	79789	PASS
70	69	0.00	2	0.6	459	PASS
127	198	10	80	50.2	105387	PASS
197	198	0.00	2	0.7	1570	PASS
198	198	100	100	100.0	209899	PASS
199	198	5	9	6.6	13845	PASS
275	198	10	60	26.4	55472	PASS
365	198	1	100	3.0	6309	PASS
441	198	0.01	100	14.8	31034	PASS
442	442	100	100	100.0	199597	PASS
443	442	15	24	19.0	37905	PASS