
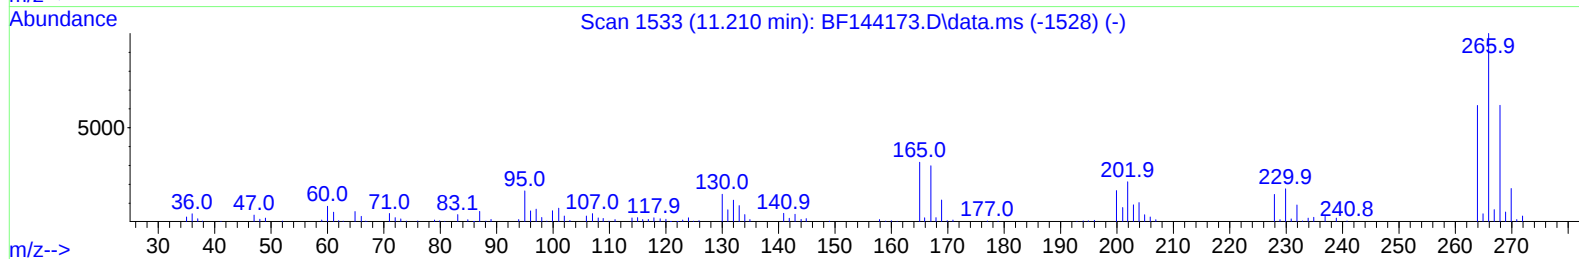
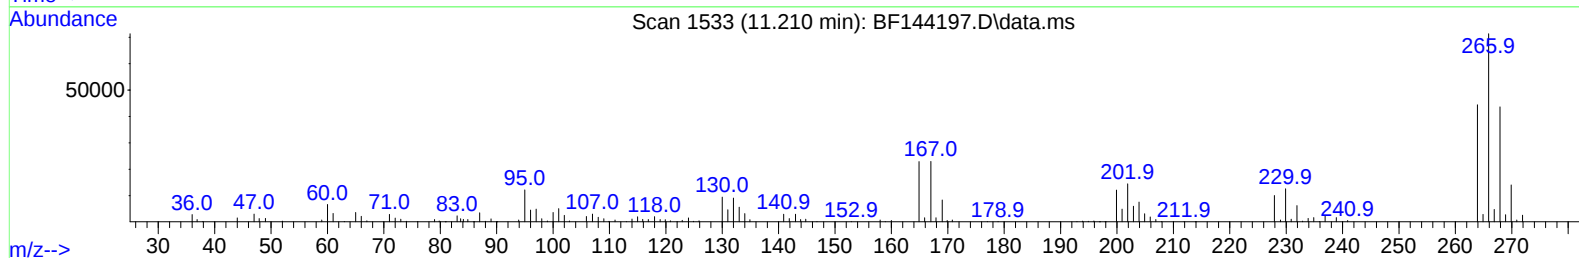


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111125\
Data File : BF144197.D
Acq On : 11 Nov 2025 09:40
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 11 10:42:04 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 05 18:37:33 2025
Response via : Initial Calibration

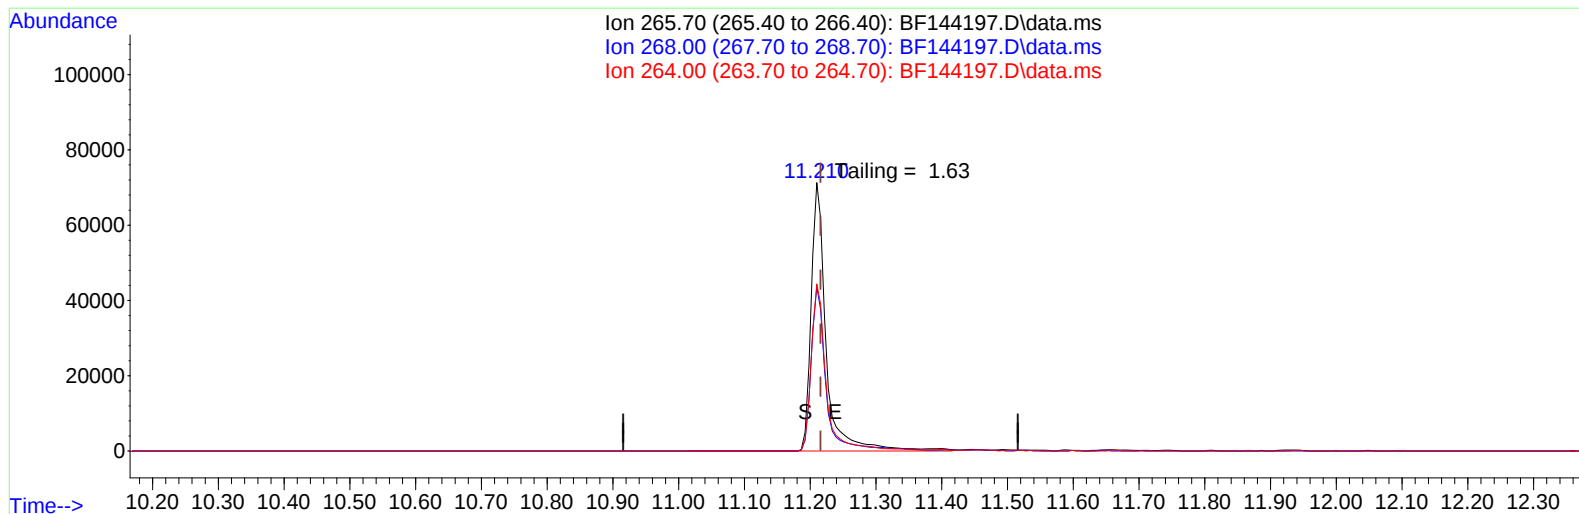

TIC: BF144197.D\data.ms

(70) Pentachlorophenol (C)




11.210min (-0.006) 27091.68 ng

response 112364

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	61.18
264.00	61.80	62.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111125\
Data File : BF144197.D
Acq On : 11 Nov 2025 09:40
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 11 10:42:04 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 05 18:37:33 2025
Response via : Initial Calibration

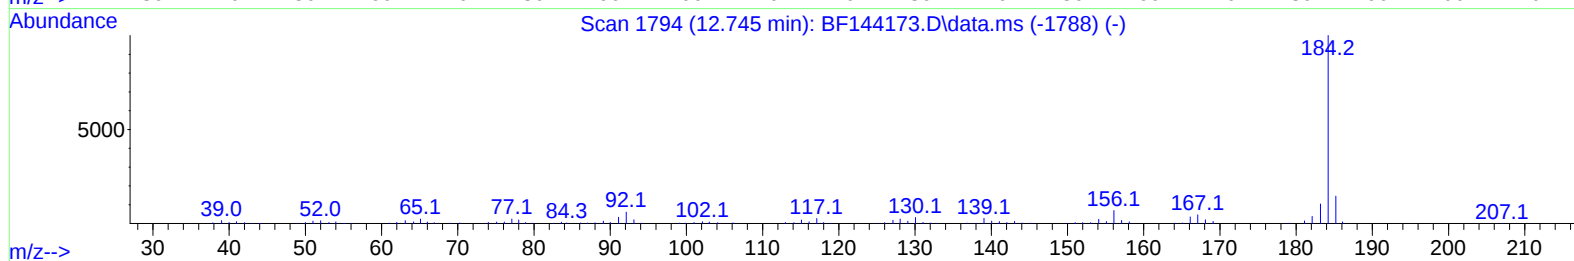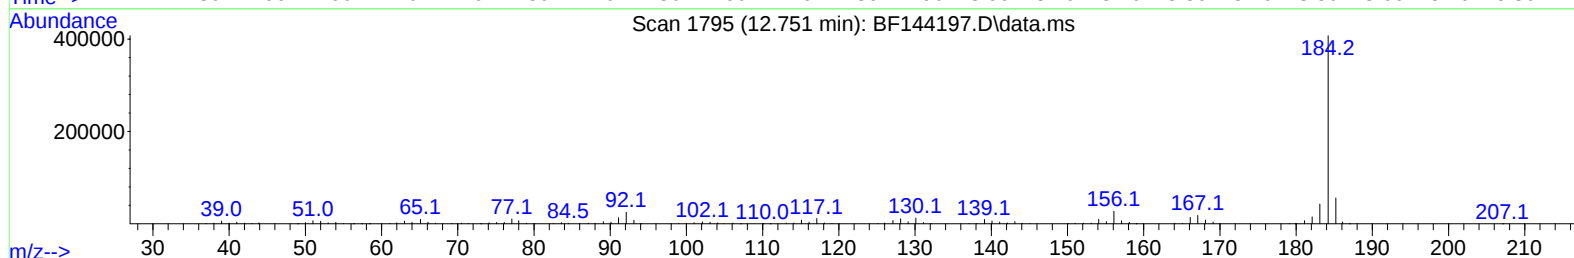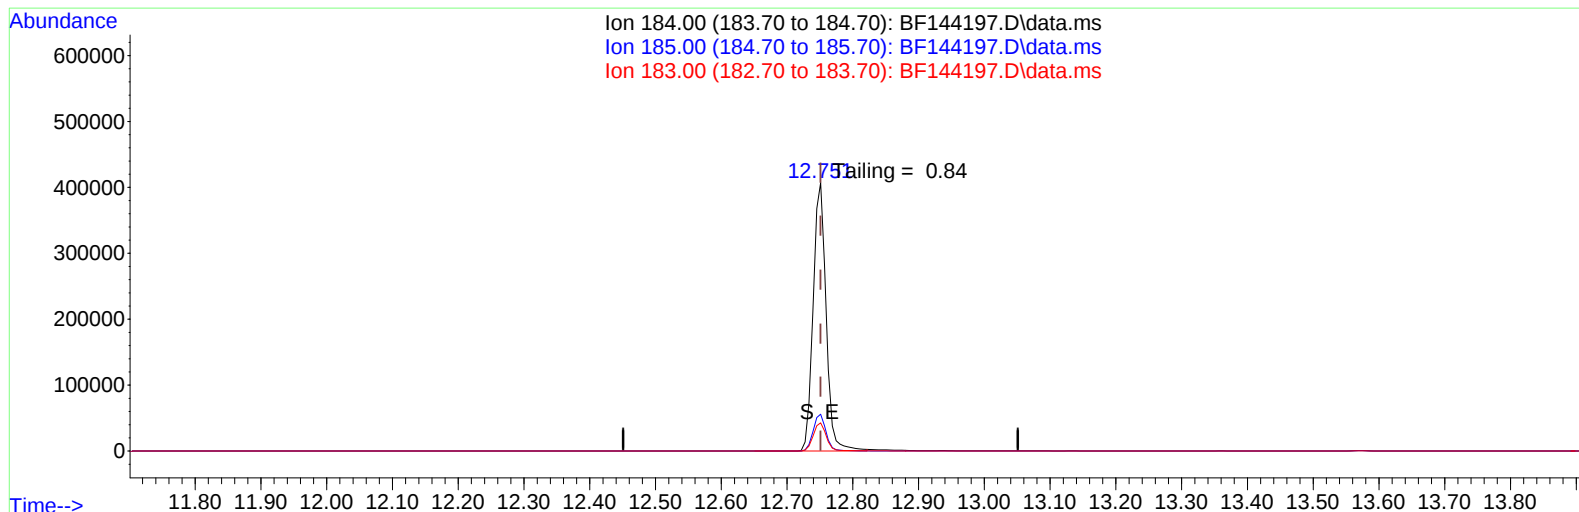

TIC: BF144197.D\data.ms

(77) Benzidine

12.751min (+ 0.000) 0.00 ng

response 562470

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	13.73
183.00	10.40	10.51
0.00	0.00	0.00