

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111125\
 Data File : BF144226.D
 Acq On : 12 Nov 2025 02:52
 Operator : RC/JU
 Sample : Q3582-04 5X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 RT4912

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF144226.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.492	556	561	572	rBV	122493	188731	6.05%	1.327%
2	6.504	727	733	750	rBV	136331	234140	7.51%	1.646%
3	6.875	791	796	812	rVB	297292	384123	12.32%	2.700%
4	7.433	886	891	901	rBV	91293	130609	4.19%	0.918%
5	8.157	1008	1014	1019	rBV	351327	454859	14.59%	3.198%
6	8.616	1086	1092	1096	rBV3	86713	159342	5.11%	1.120%
7	8.845	1128	1131	1136	rBV5	69916	99237	3.18%	0.698%
8	9.151	1180	1183	1186	rBV3	204933	264165	8.47%	1.857%
9	9.227	1192	1196	1201	rBV2	398455	685761	21.99%	4.821%
10	9.310	1207	1210	1214	rBV2	491148	720651	23.11%	5.066%
11	9.627	1260	1264	1269	rBV2	1910595	2836360	90.97%	19.939%
12	9.792	1288	1292	1295	rBV3	1326601	2080505	66.73%	14.625%
13	9.839	1296	1300	1304	rVB	2252390	3117919	100.00%	21.918%
14	9.910	1309	1312	1318	rVB6	1107193	2240878	71.87%	15.753%
15	15.551	2266	2271	2289	rVB	307918	628082	20.14%	4.415%




Sum of corrected areas: 14225362

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111125\
Data File : BF144226.D
Acq On : 12 Nov 2025 02:52
Operator : RC/JU
Sample : Q3582-04 5X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RT4912

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

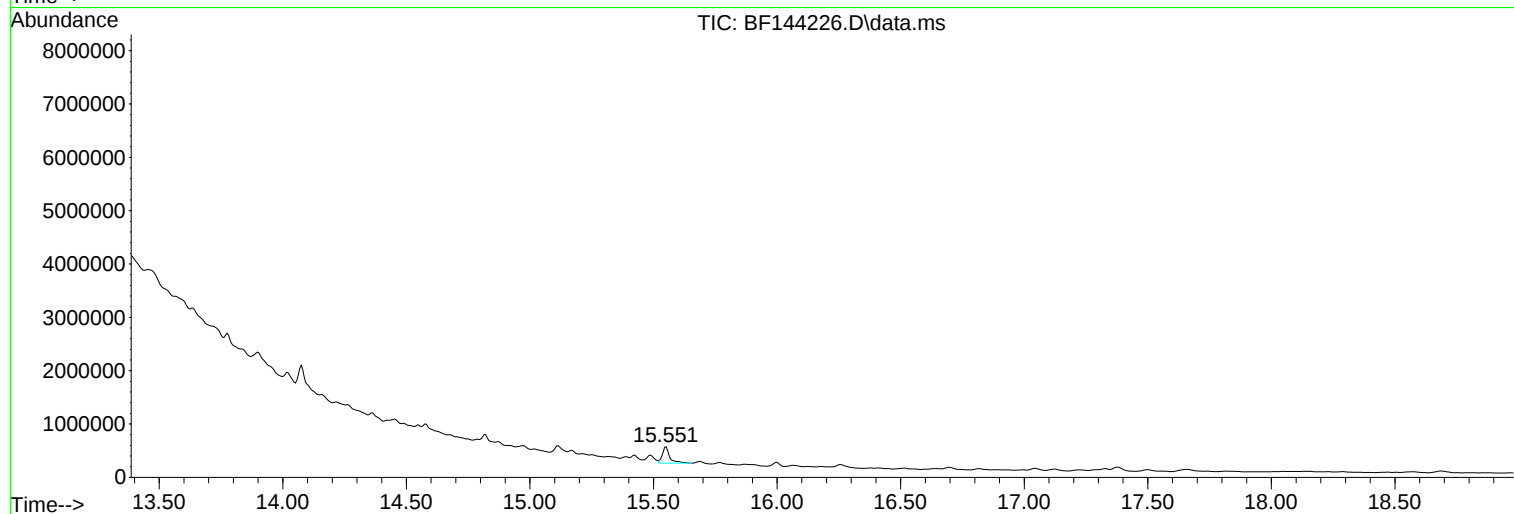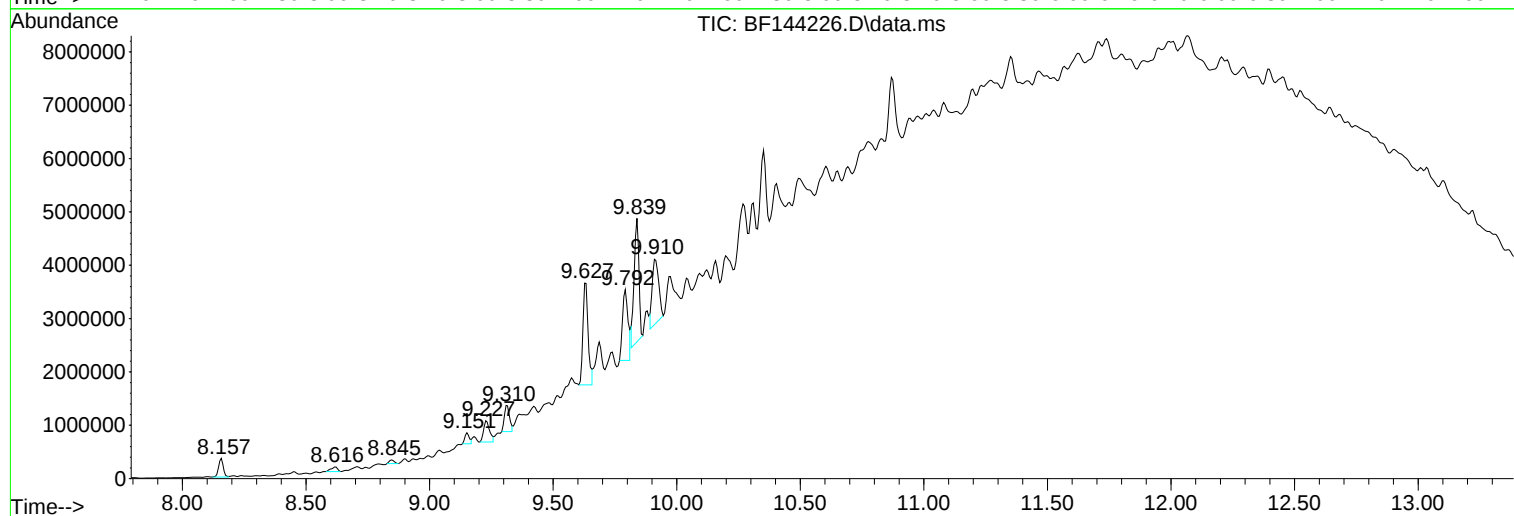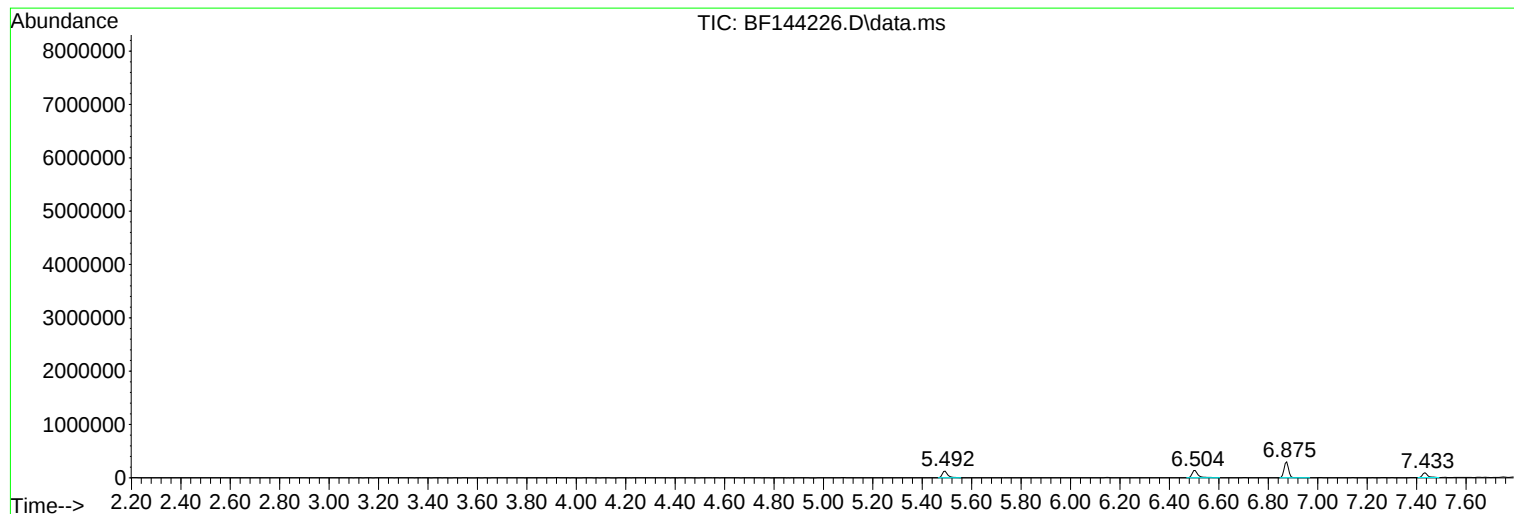

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111125\
Data File : BF144226.D
Acq On : 12 Nov 2025 02:52
Operator : RC/JU
Sample : Q3582-04 5X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RT4912

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111125\
Data File : BF144226.D
Acq On : 12 Nov 2025 02:52
Operator : RC/JU
Sample : Q3582-04 5X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RT4912

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------