

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111125\
Data File : BF144227.D
Acq On : 12 Nov 2025 03:22
Operator : RC/JU
Sample : Q3593-04 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
A-LAW-25-0167-0175-COMP

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF144227.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.493	550	561	577	rBV	153336	254437	29.53%	8.442%
2	6.504	727	733	750	rBV	151406	254948	29.59%	8.459%
3	6.875	791	796	802	rBV	351034	449346	52.15%	14.909%
4	7.434	886	891	900	rBV	91319	127835	14.84%	4.242%
5	8.157	1007	1014	1018	rBV	417100	568547	65.98%	18.864%
6	8.445	1059	1063	1066	rBV5	84943	123641	14.35%	4.102%
7	8.598	1086	1089	1095	rVB4	94154	125574	14.57%	4.166%
8	8.663	1096	1100	1102	rBV2	98149	133028	15.44%	4.414%
9	8.692	1102	1105	1108	rBV4	86403	114911	13.34%	3.813%
10	15.551	2266	2271	2289	rVB	429131	861638	100.00%	28.589%




Sum of corrected areas: 3013905

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111125\
Data File : BF144227.D
Acq On : 12 Nov 2025 03:22
Operator : RC/JU
Sample : Q3593-04 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
A-LAW-25-0167-0175-COMP

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

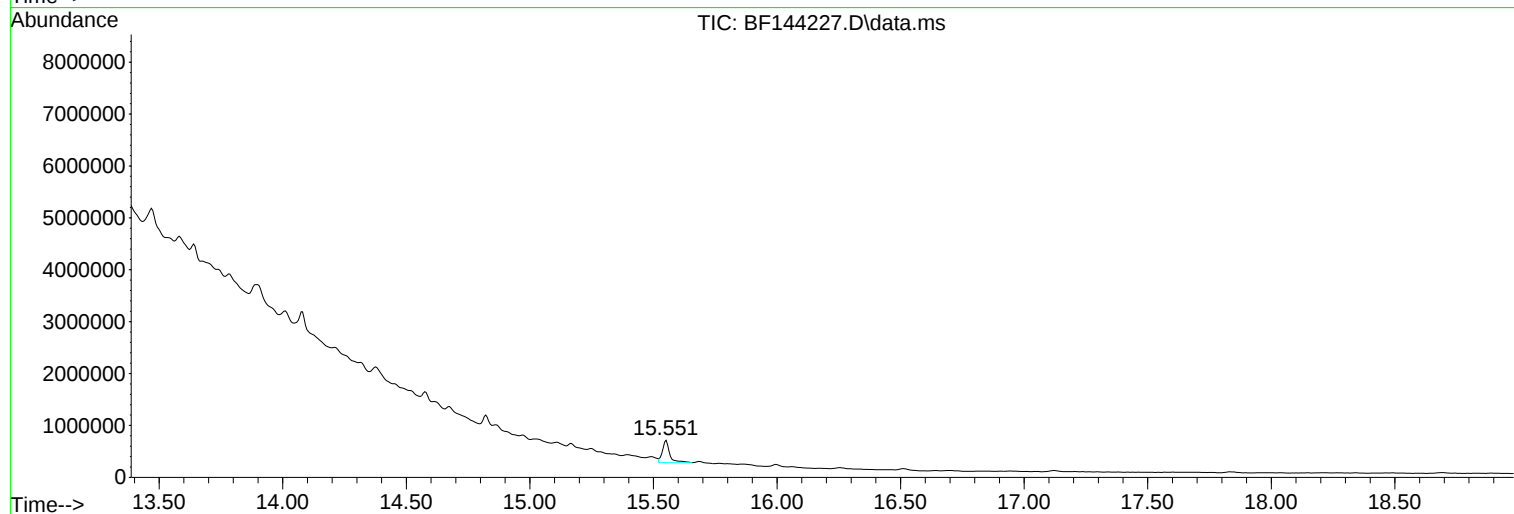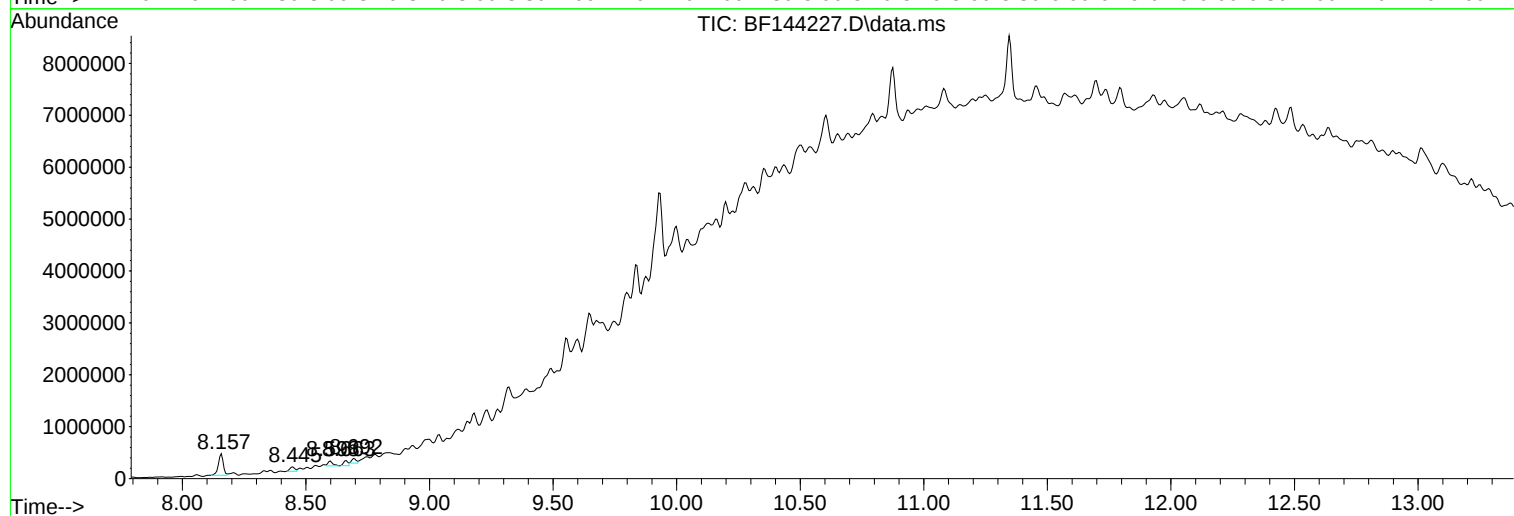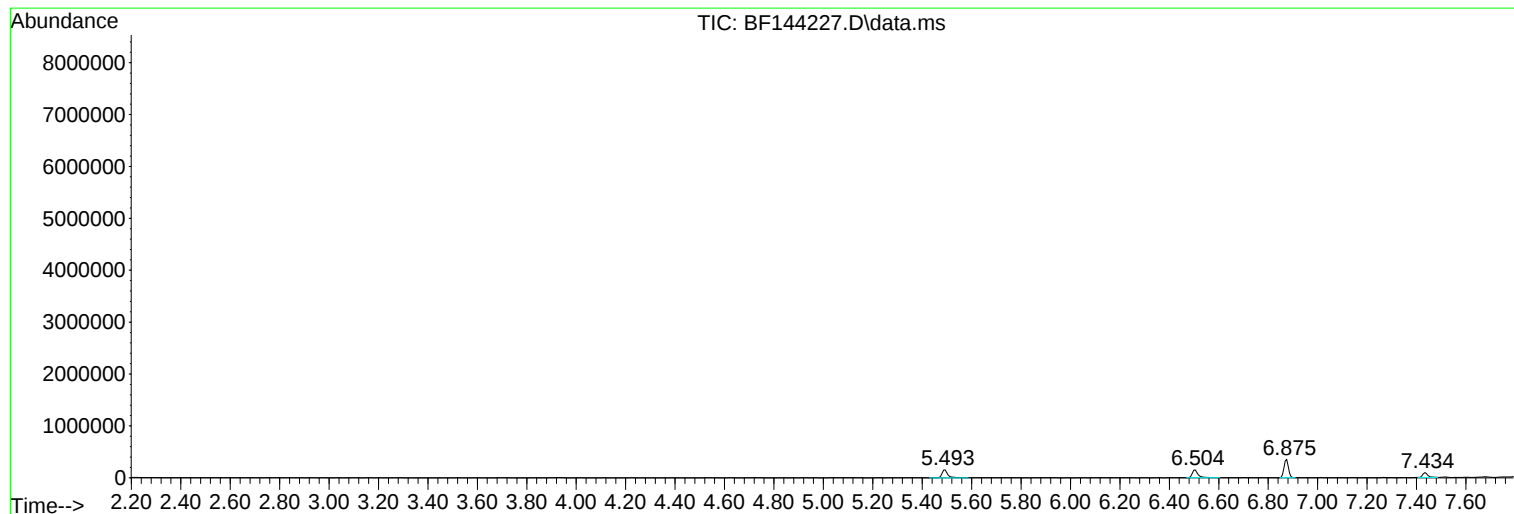

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111125\
Data File : BF144227.D
Acq On : 12 Nov 2025 03:22
Operator : RC/JU
Sample : Q3593-04 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
A-LAW-25-0167-0175-COMP

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111125\
Data File : BF144227.D
Acq On : 12 Nov 2025 03:22
Operator : RC/JU
Sample : Q3593-04 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
A-LAW-25-0167-0175-COMP

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
