

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111125\
 Data File : BF144228.D
 Acq On : 12 Nov 2025 03:52
 Operator : RC/JU
 Sample : Q3593-06 10X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 B-LAW-25-0167-0175-COMP

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF144228.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.493	556	561	578	rVB	155394	252007	29.15%	6.414%
2	6.504	728	733	748	rBV	165487	280939	32.50%	7.151%
3	6.875	791	796	803	rBV	517710	667158	77.17%	16.981%
4	7.434	887	891	900	rBV	105207	151864	17.57%	3.865%
5	8.157	1007	1014	1018	rBV	642054	864485	100.00%	22.003%
6	8.210	1020	1023	1026	rVB2	66669	83511	9.66%	2.126%
7	8.245	1026	1029	1034	rBV6	37900	82360	9.53%	2.096%
8	8.334	1040	1044	1045	rBV3	65625	84499	9.77%	2.151%
9	8.445	1059	1063	1066	rBV3	116917	171395	19.83%	4.362%
10	8.539	1076	1079	1081	rBV3	71649	92505	10.70%	2.354%
11	8.598	1086	1089	1095	rVB4	129856	178372	20.63%	4.540%
12	8.663	1096	1100	1102	rBV2	130353	176412	20.41%	4.490%
13	8.692	1102	1105	1108	rBV2	121133	165058	19.09%	4.201%
14	15.551	2266	2271	2279	rVB	393446	678324	78.47%	17.265%




Sum of corrected areas: 3928889

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111125\
Data File : BF144228.D
Acq On : 12 Nov 2025 03:52
Operator : RC/JU
Sample : Q3593-06 10X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
B-LAW-25-0167-0175-COMP

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

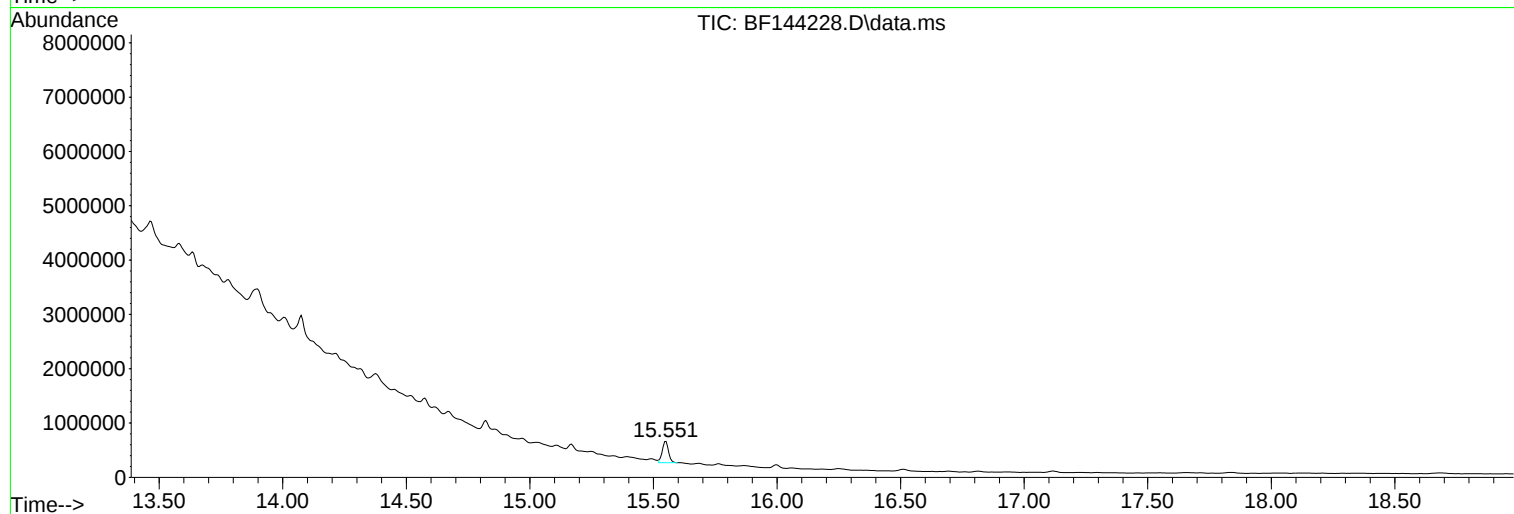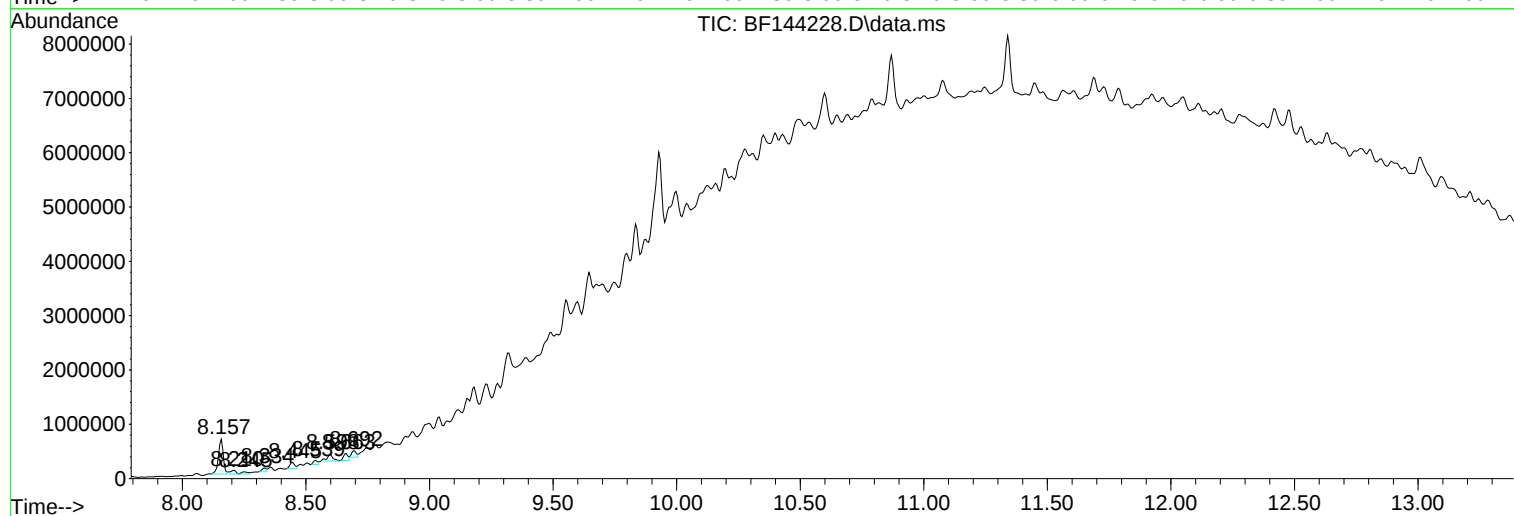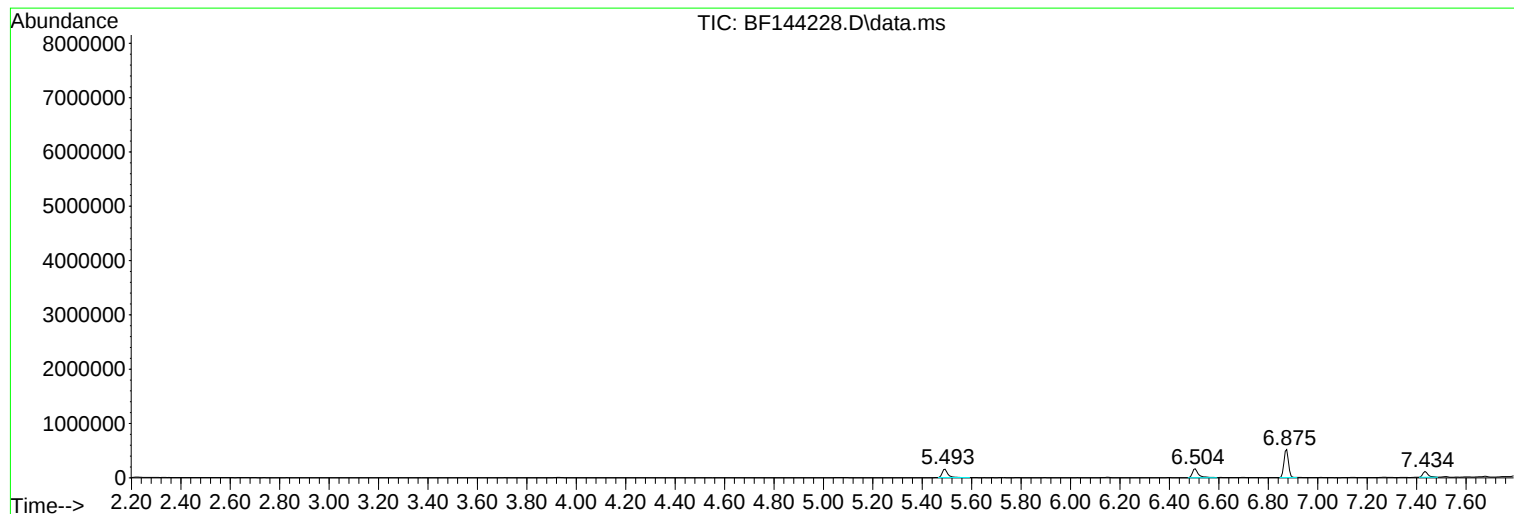

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111125\
Data File : BF144228.D
Acq On : 12 Nov 2025 03:52
Operator : RC/JU
Sample : Q3593-06 10X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
B-LAW-25-0167-0175-COMP

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111125\
Data File : BF144228.D
Acq On : 12 Nov 2025 03:52
Operator : RC/JU
Sample : Q3593-06 10X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
B-LAW-25-0167-0175-COMP

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc