
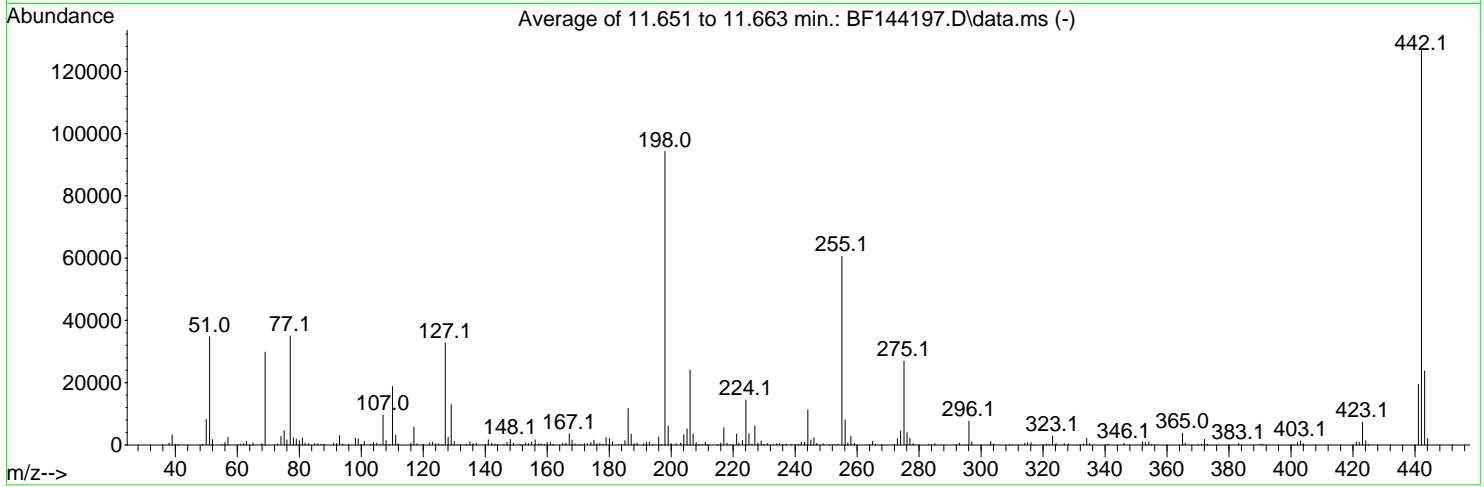


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111125\
 Data File : BF144197.D
 Acq On : 11 Nov 2025 09:40
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 05 18:37:33 2025

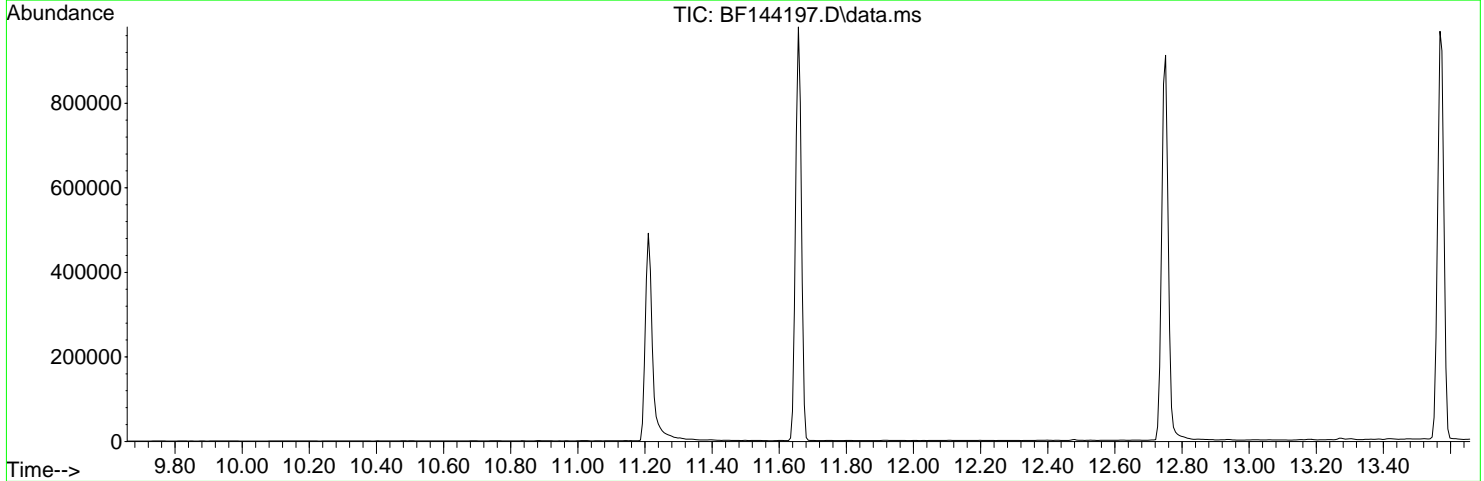




AutoFind: Scans 1608, 1609, 1610; Background Corrected with Scan 1602

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.2	373	PASS
69	69	100	100	100.0	29859	PASS
70	69	0.00	2	0.0	0	PASS
197	198	0.00	2	0.1	96	PASS
198	198	100	100	100.0	94299	PASS
199	198	5	9	6.5	6095	PASS
365	198	1	100	4.0	3780	PASS
441	443	0.01	150	81.9	19483	PASS
442	442	100	100	100.0	126867	PASS
443	442	15	24	18.7	23781	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111125\
 Data File : BF144197.D
 Acq On : 11 Nov 2025 09:40
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
ClientSampleId :
 DFTPP

Quant Time: Nov 11 10:42:04 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 05 18:37:33 2025
 Response via : Initial Calibration

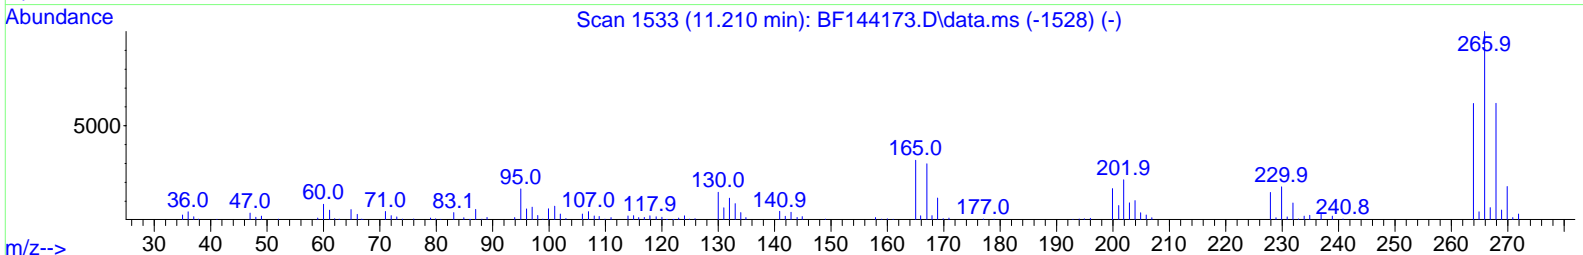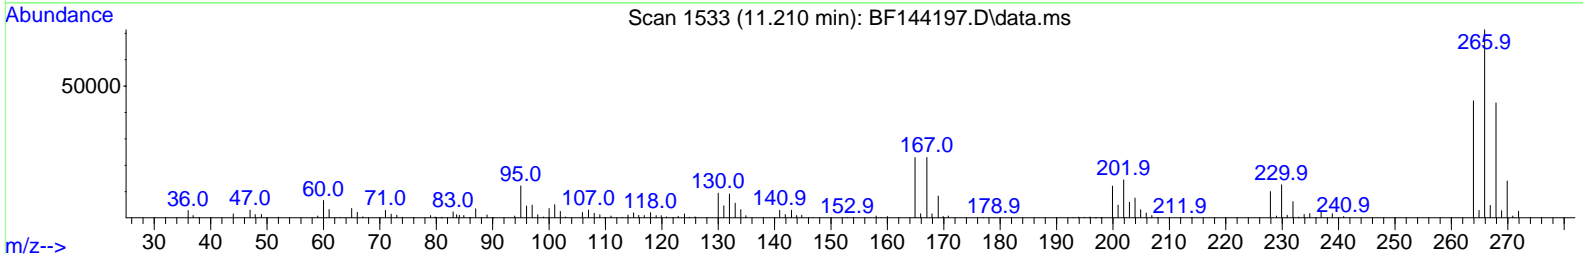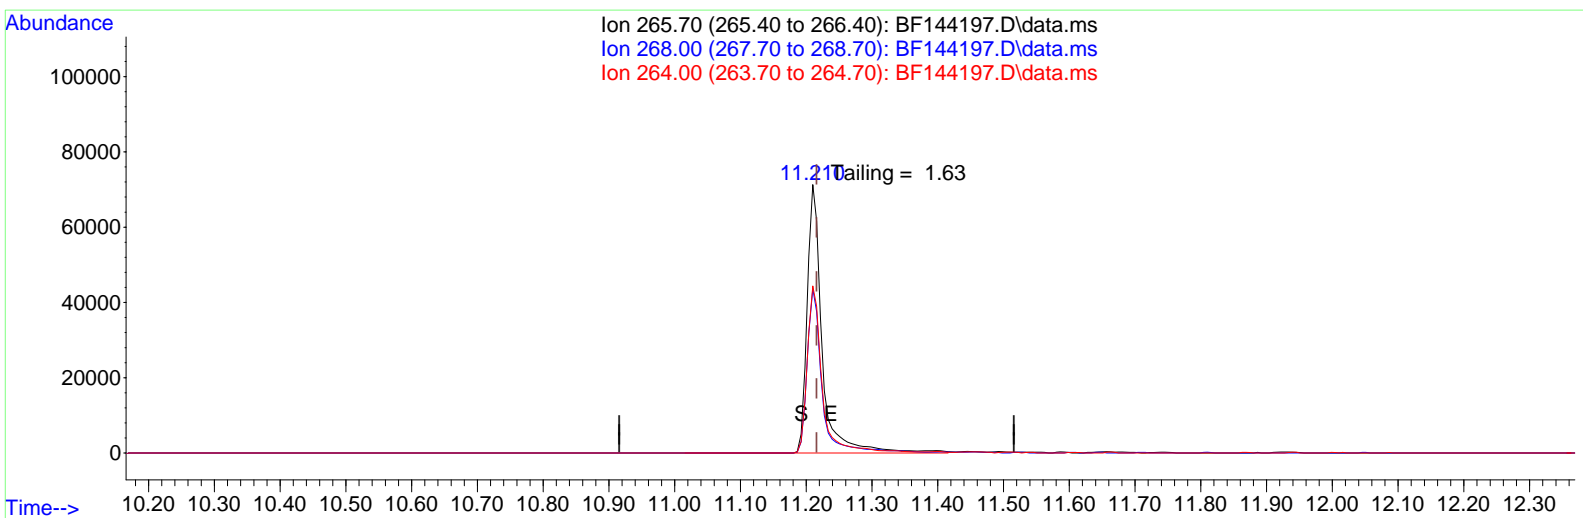

TIC: BF144197.D\data.ms

(70) Pentachlorophenol (C)




11.210min (-0.006) 27091.68 ng

response	112364
Ion	Exp% Act%
265.70	100.00 100.00
268.00	61.90 61.18
264.00	61.80 62.26
0.00	0.00 0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111125\
 Data File : BF144197.D
 Acq On : 11 Nov 2025 09:40
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Nov 11 10:42:04 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 05 18:37:33 2025
 Response via : Initial Calibration

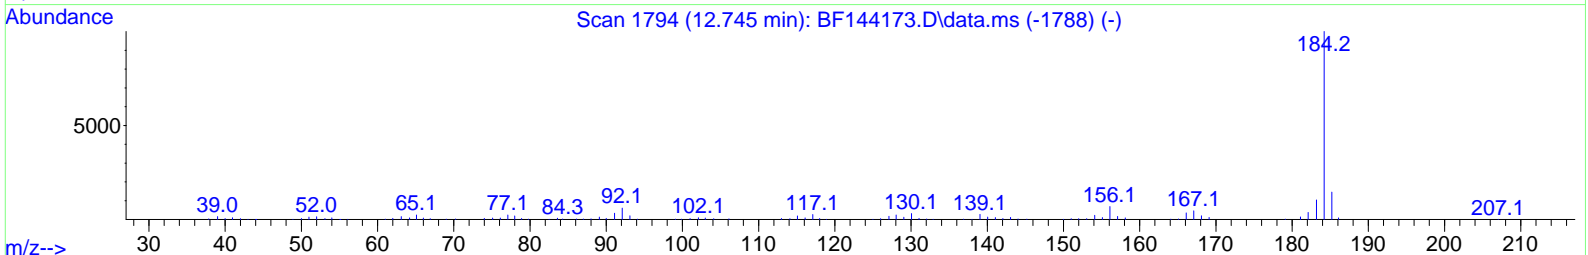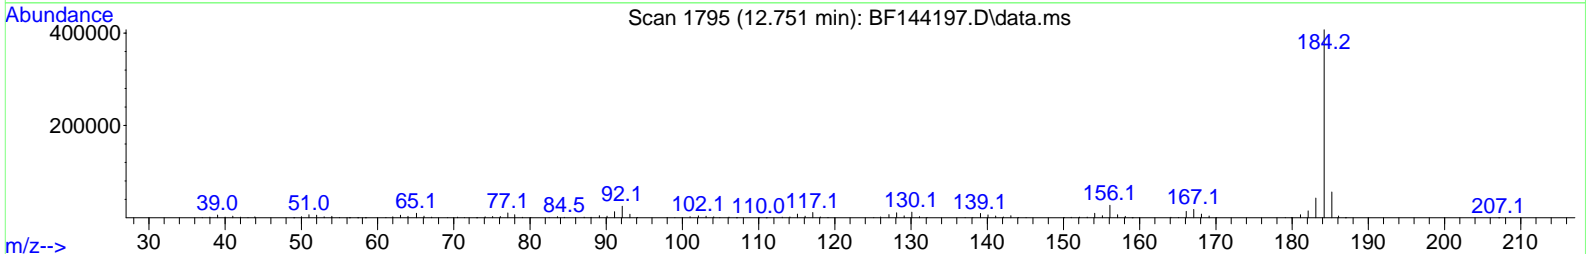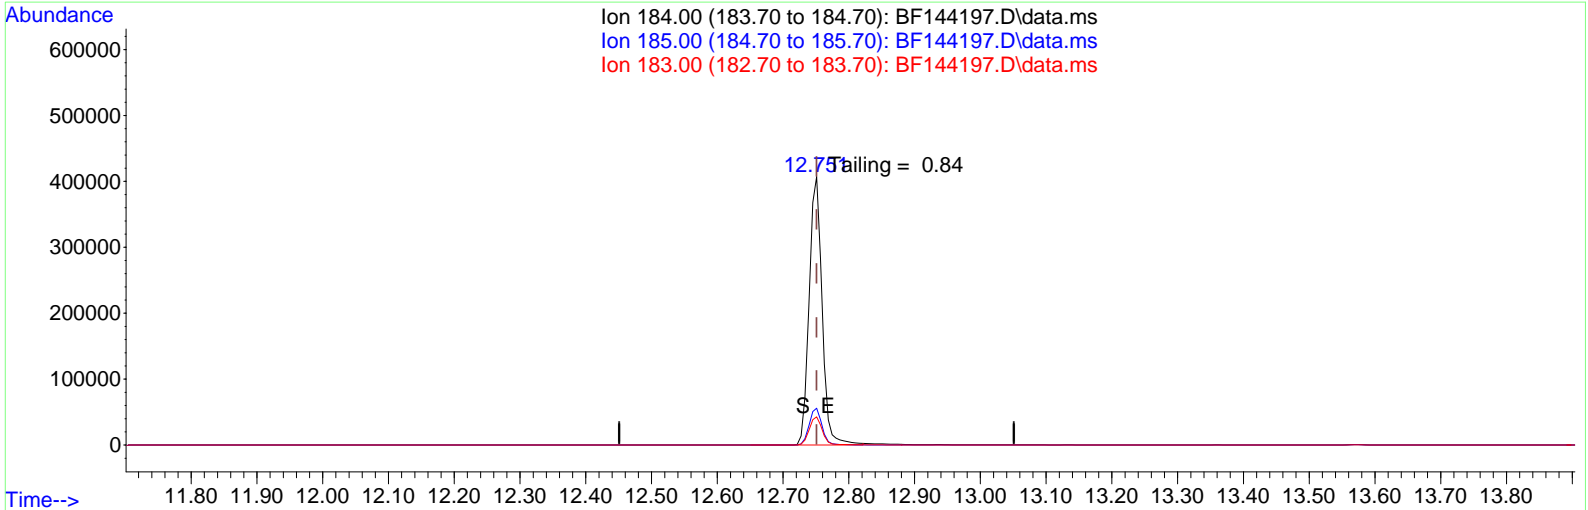

TIC: BF144197.D\data.ms

(77) Benzidine

12.751min (+ 0.000) 0.00 ng

response 562470

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	13.73
183.00	10.40	10.51
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/11/2025	BNA_F	<u>BF144197.D</u>
Compound Name	Response	Retention Time
DDT	273985	13.569
DDD	2952	13.274
DDE	571	12.933
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3523	277508	1.27

Instrument :
 BNA_F
 ClientSampled :
 DFTPP