
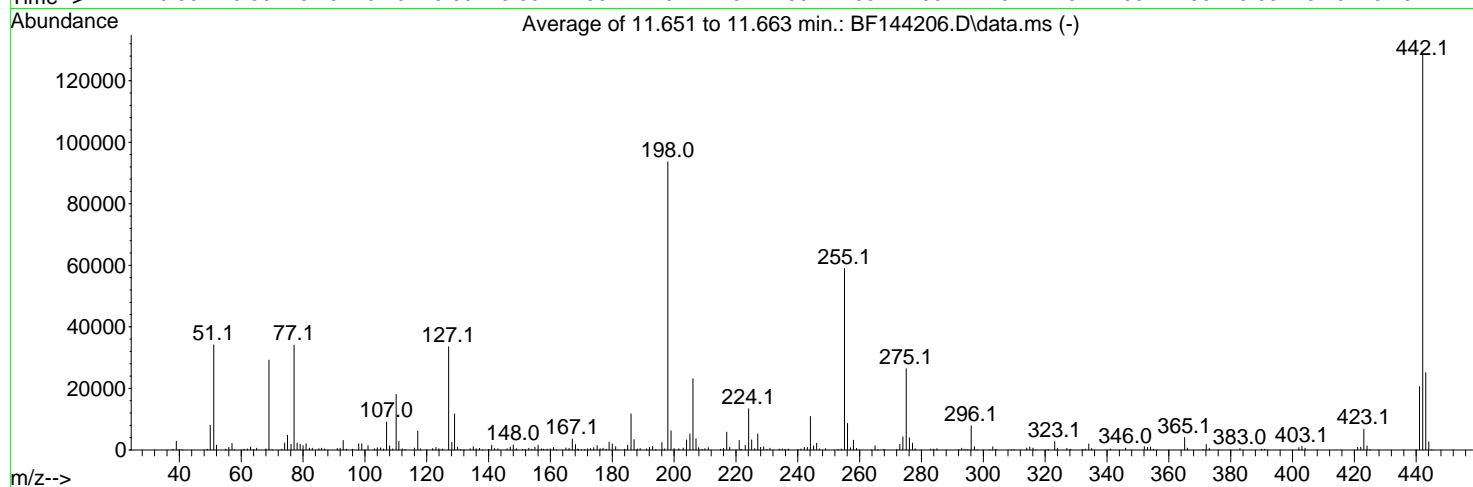


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF111125\  
 Data File : BF144206.D  
 Acq On : 11 Nov 2025 17:03  
 Operator : RC/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF110525.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed Nov 05 18:37:33 2025

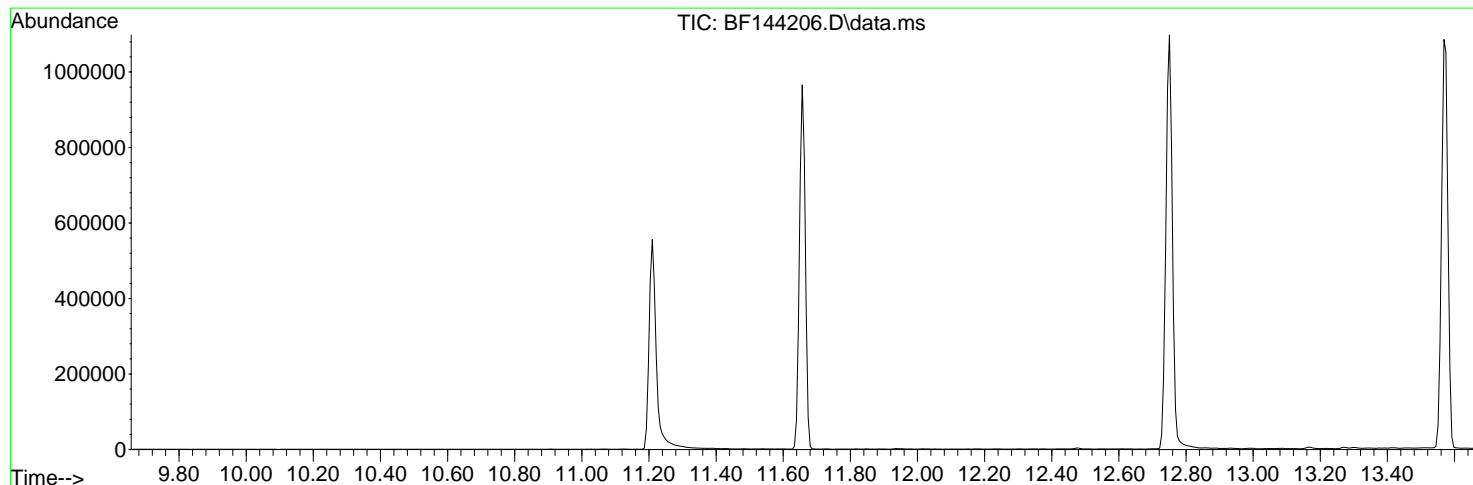




AutoFind: Scans 1608, 1609, 1610; Background Corrected with Scan 1602

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.2	346	PASS
69	69	100	100	100.0	29195	PASS
70	69	0.00	2	0.5	142	PASS
197	198	0.00	2	0.4	354	PASS
198	198	100	100	100.0	93635	PASS
199	198	5	9	6.7	6236	PASS
365	198	1	100	4.4	4077	PASS
441	443	0.01	150	81.9	20588	PASS
442	442	100	100	100.0	128341	PASS
443	442	15	24	19.6	25141	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF111125\  
 Data File : BF144206.D  
 Acq On : 11 Nov 2025 17:03  
 Operator : RC/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

**Instrument :**  
 BNA\_F  
**ClientSampleId :**  
 DFTPP

Quant Time: Nov 11 17:43:39 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF110525.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Nov 05 18:37:33 2025  
 Response via : Initial Calibration

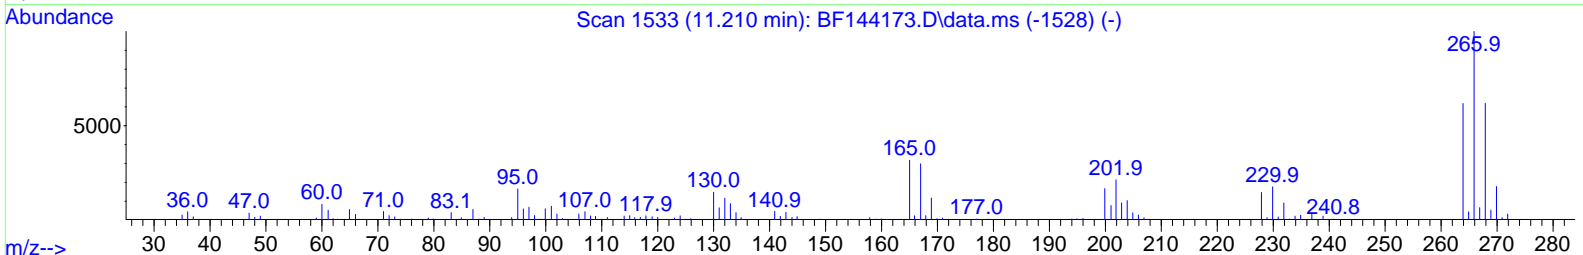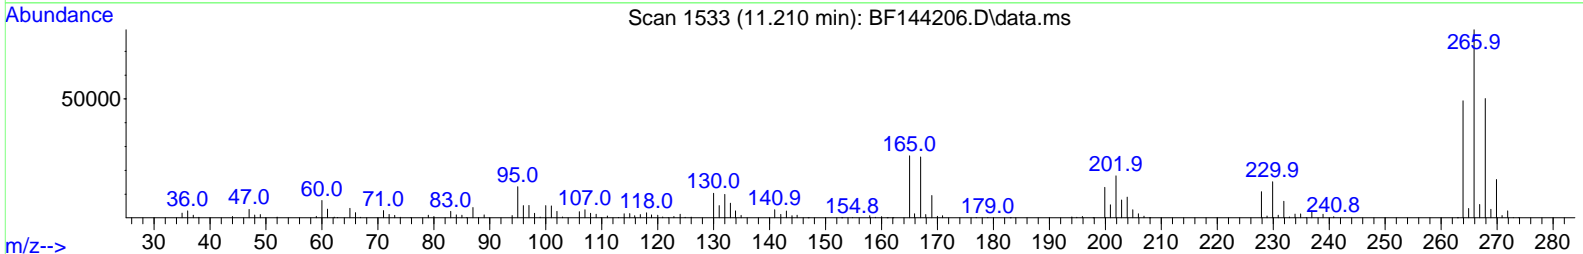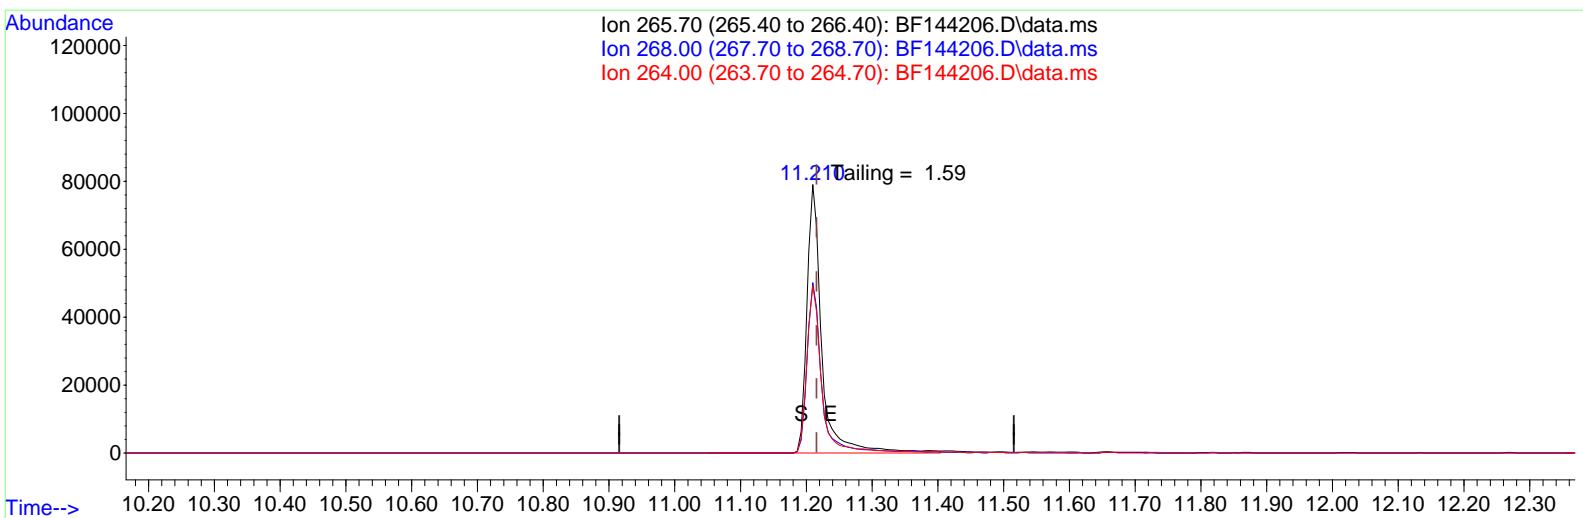

TIC: BF144206.D\data.ms

(70) Pentachlorophenol (C)




11.210min (-0.006) 122536.22 ng

response	122928	
Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	63.47
264.00	61.80	62.28
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF111125\  
 Data File : BF144206.D  
 Acq On : 11 Nov 2025 17:03  
 Operator : RC/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Quant Time: Nov 11 17:43:39 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF110525.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Nov 05 18:37:33 2025  
 Response via : Initial Calibration

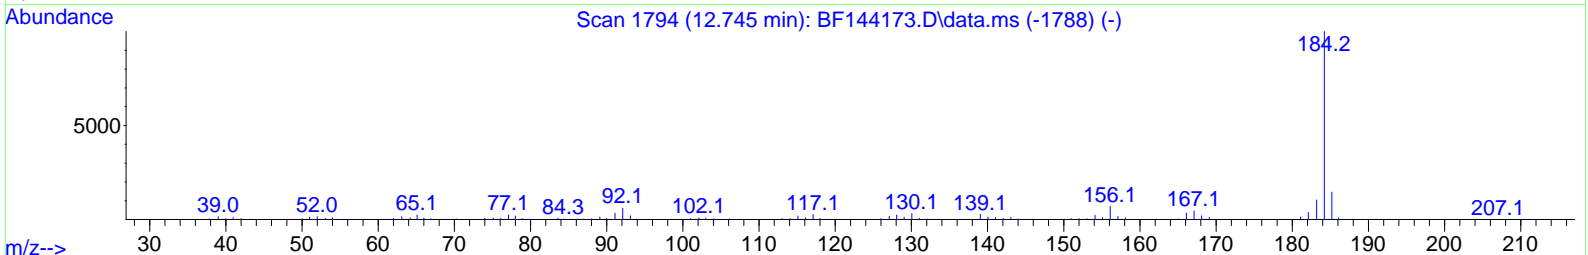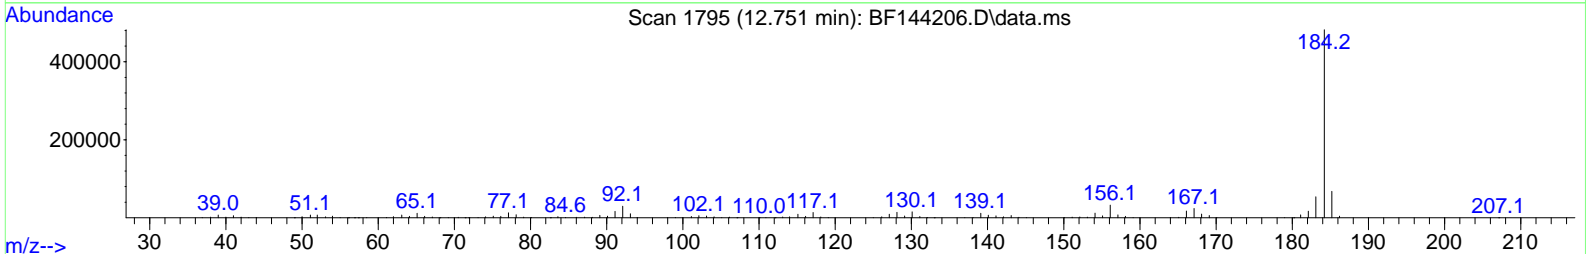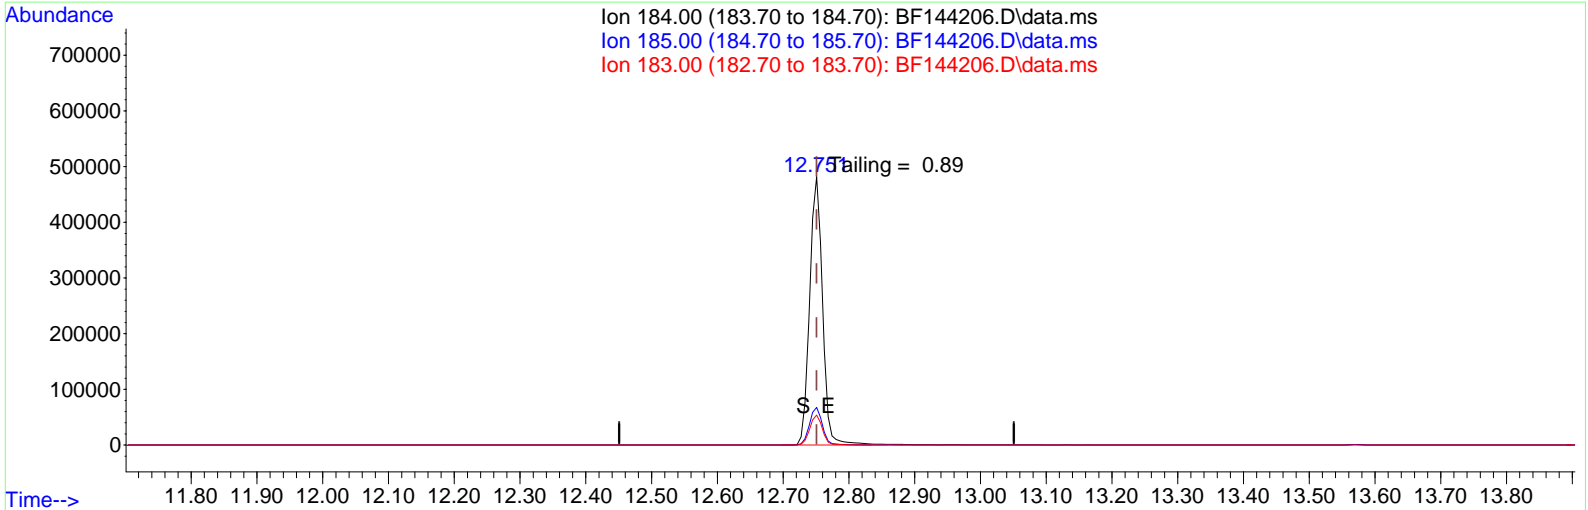

TIC: BF144206.D\data.ms

(77) Benzidine

12.751min ( 0.000) 0.00 ng

response 658432

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.05
183.00	10.40	11.15
0.00	0.00	0.00

**DDT Breakdown**

<b>Date</b>	<b>Instrument Name</b>	<b>DFTPP Data File</b>
11/11/2025	BNA_F	<u>BF144206.D</u>
<b>Compound Name</b>	<b>Response</b>	<b>Retention Time</b>
DDT	309734	13.574
DDD	4786	13.274
DDE	688	12.933
<b>SUM(DDD+DDE)</b>	<b>SUM(DDT+DDD+DDE)</b>	<b>% Breakdown Of DDT</b>
5474	315208	1.74

Instrument :  
 BNA\_F  
 ClientSampled :  
 DFTPP