
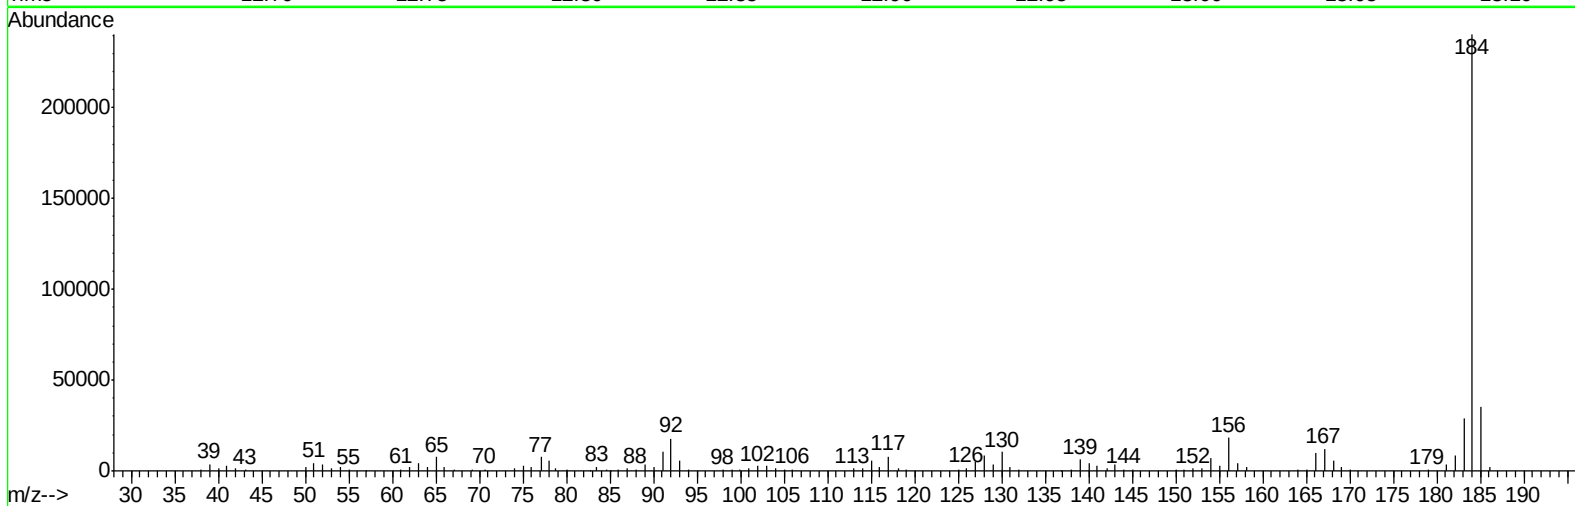


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF111218\
Data File : BF110696.D
Acq On : 13 Nov 2018 2:06
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 13 07:51:12 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF110818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 09 15:13:13 2018
Response via : Initial Calibration

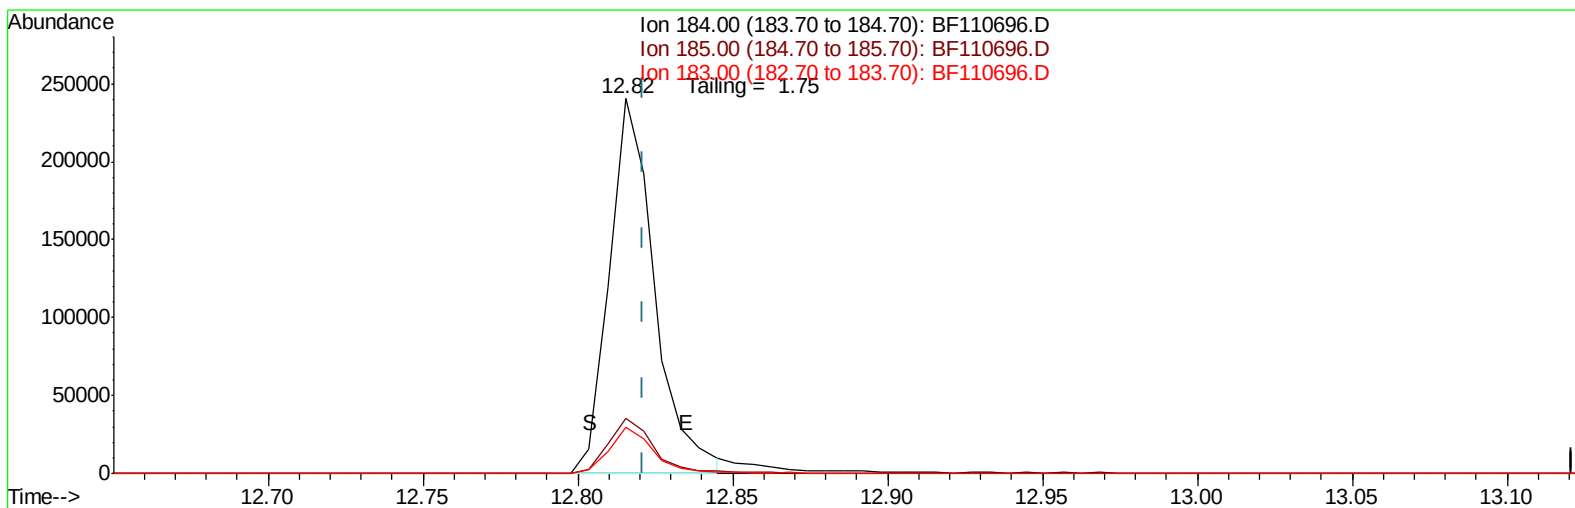

TIC: BF110696.D

(77) Benzidine



12.815min (-0.006) 0.00ng

response 255498

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	14.71
183.00	11.80	12.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF111218\
Data File : BF110696.D
Acq On : 13 Nov 2018 2:06
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 13 07:51:12 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF110818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 09 15:13:13 2018
Response via : Initial Calibration

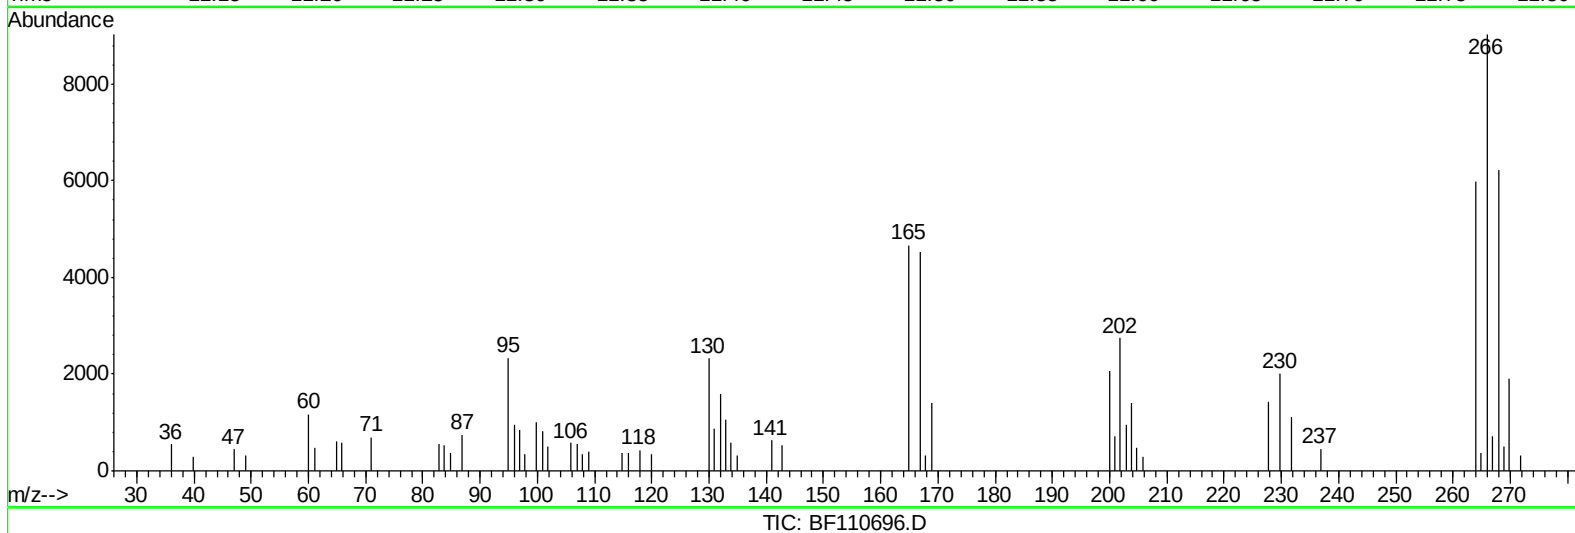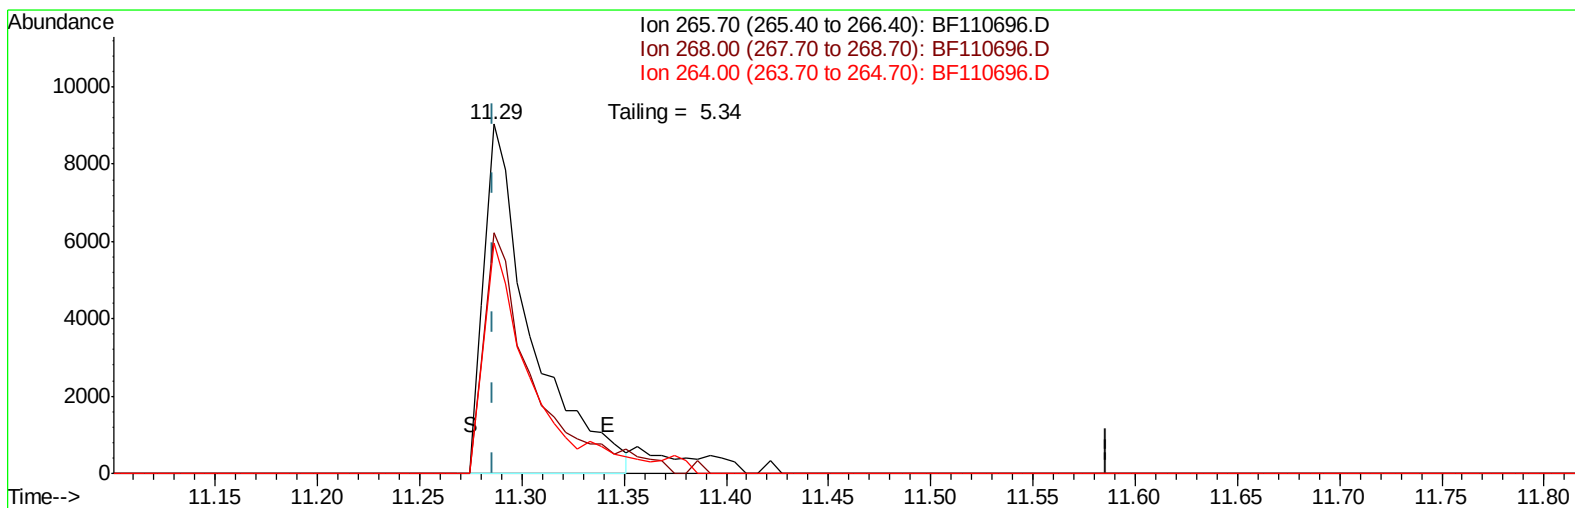

TIC: BF110696.D

(70) Pentachlorophenol (C)

11.286min (-0.000) 22199.64ng

response 15597

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	68.88
264.00	63.20	66.18
0.00	0.00	0.00