

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF111218\
 Data File : BF110711.D
 Acq On : 13 Nov 2018 9:00
 Operator : JU/SJ
 Sample : J5904-22
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 110818-JETT-E-U-S

Quant Time: Nov 13 10:47:38 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF110818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 09 15:13:13 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.95	152	78974	20.00	ng	0.00
21) Naphthalene-d8	8.23	136	328565	20.00	ng	0.00
39) Acenaphthene-d10	9.99	164	149006	20.00	ng	0.00
64) Phenanthrene-d10	11.48	188	245993	20.00	ng	0.00
76) Chrysene-d12	14.13	240	161772	20.00	ng	-0.01
87) Perylene-d12	15.66	264	129519	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.56	112	179818	36.98	ng	0.00
7) Phenol-d6	6.56	99	140227	22.55	ng	-0.01
23) Nitrobenzene-d5	7.51	82	508806	89.18	ng	0.00
42) 2,4,6-Tribromophenol	10.79	330	4345	2.89	ng	0.00
45) 2-Fluorobiphenyl	9.30	172	929075	89.05	ng	0.00
79) Terphenyl-d14	13.06	244	639213	74.00	ng	0.00
Target Compounds						
50) Dimethylphthalate	9.69	163	25670	2.309	ng	Qvalue 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF111218\
Data File : BF110711.D
Acq On : 13 Nov 2018 9:00
Operator : JU/SJ
Sample : J5904-22
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
110818-JETT-E-U-S

Quant Time: Nov 13 10:47:38 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF110818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 09 15:13:13 2018
Response via : Initial Calibration

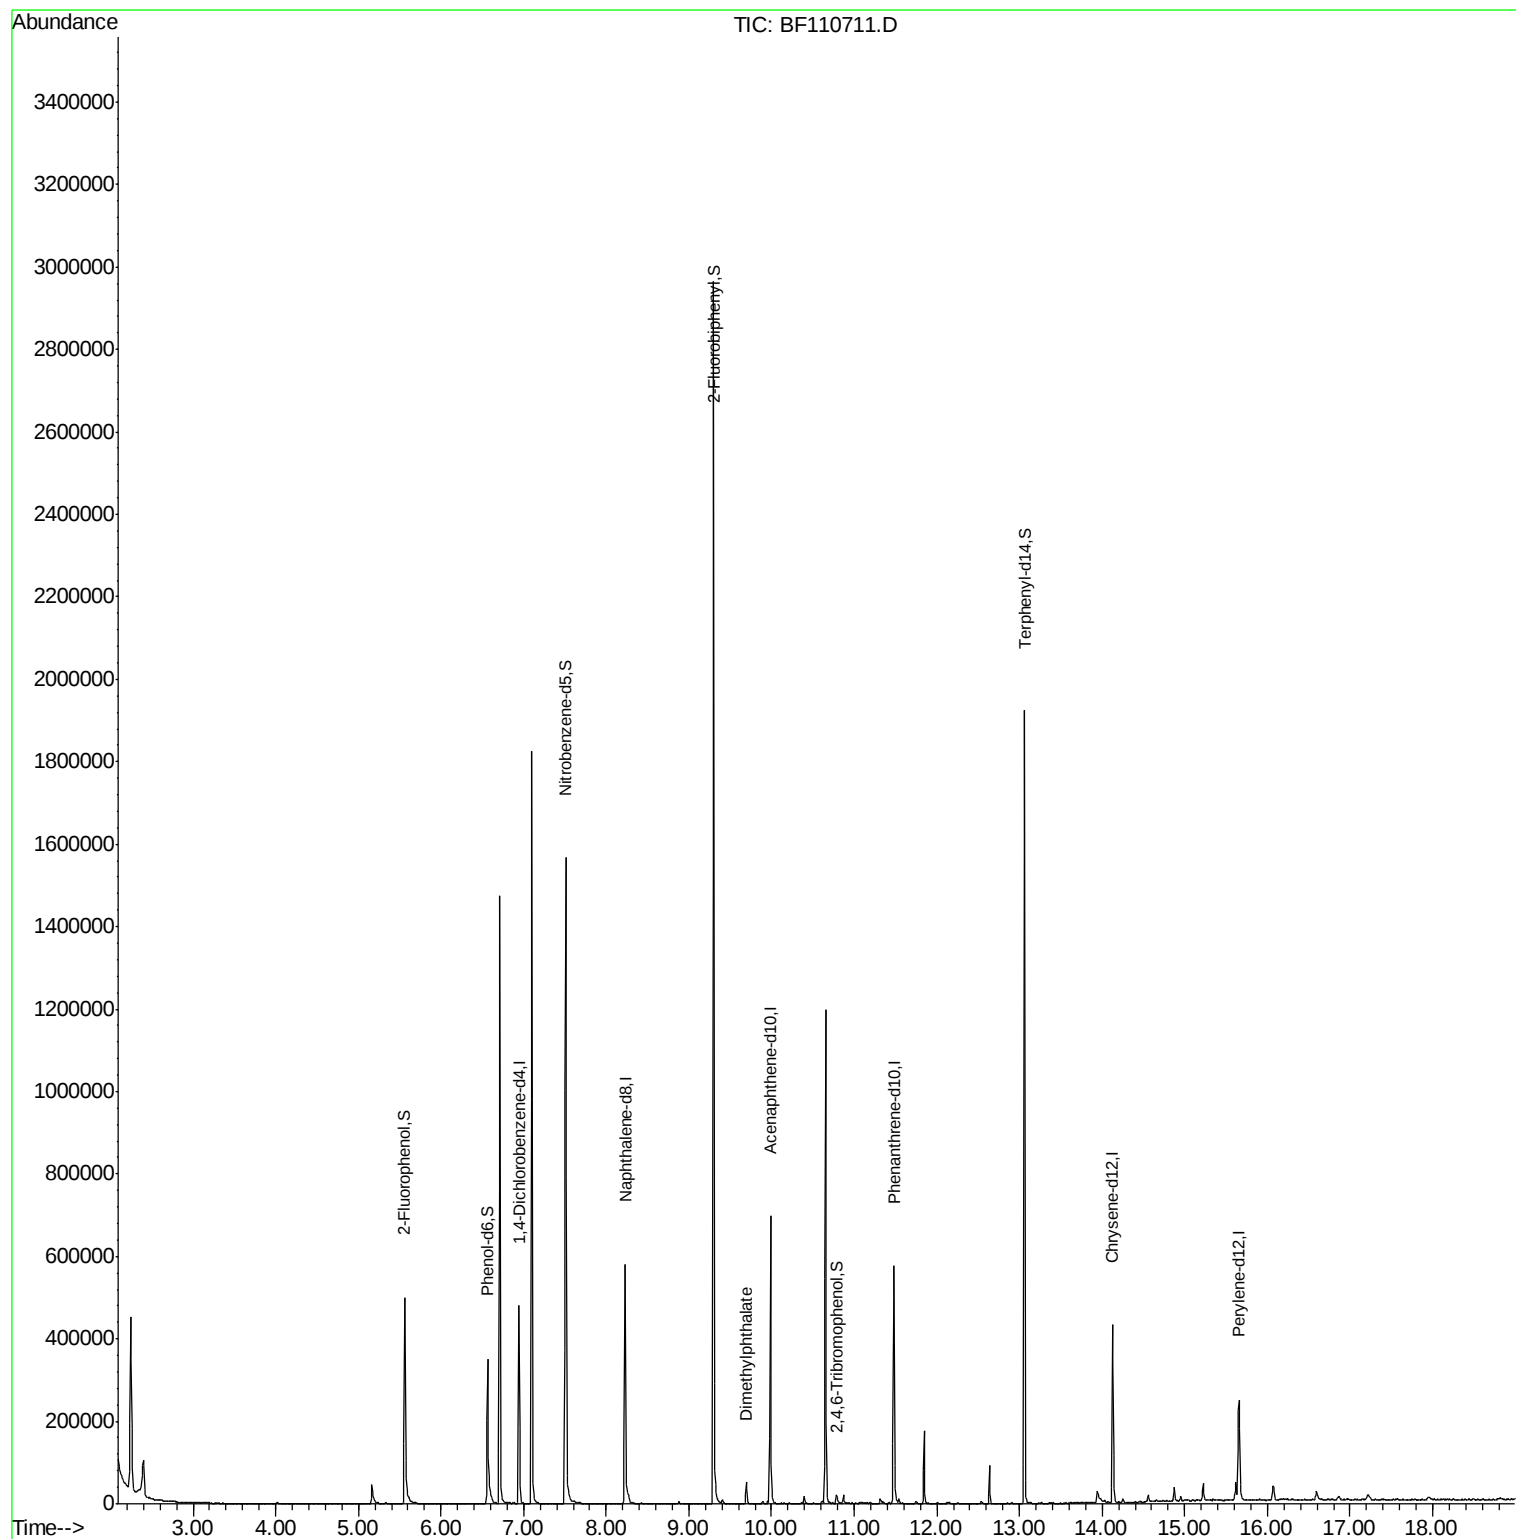




#1



1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.95 min Scan# 826
 Delta R.T. 0.00 min
 Lab File: BF110711.D
 Acq: 13 Nov 2018 9:00

Instrument :
 BNA_F
 ClientSampleId :
 110818-JETT-E-U-S

Tot Ion:152 Resp: 78974
 Ion Ratio Lower Upper
 152 100
 150 152.6 122.7 184.1
 115 60.7 49.1 73.7

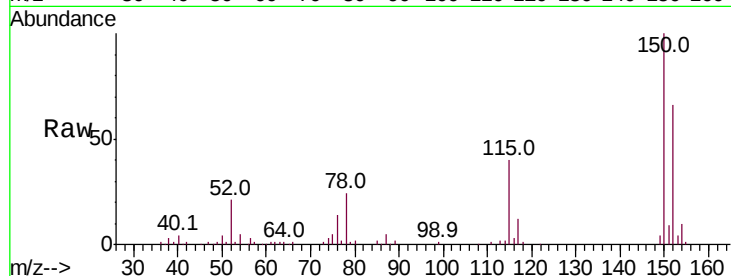


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

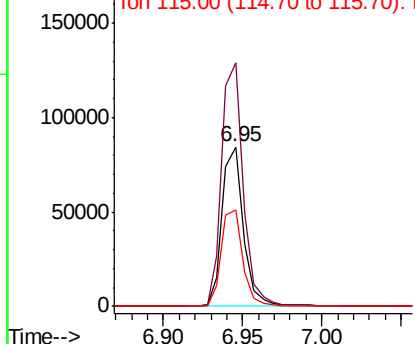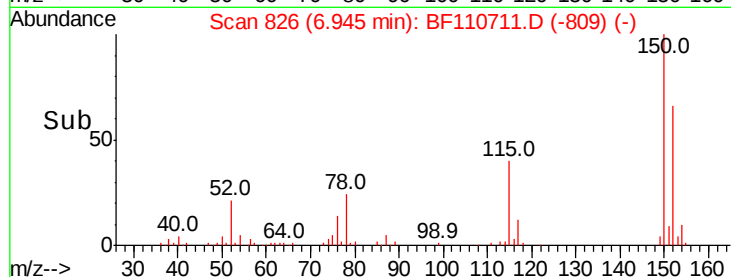



#5


2-Fluorophenol
 Concen: 36.984 ng
 RT: 5.56 min Scan# 591
 Delta R.T. 0.00 min
 Lab File: BF110711.D
 Acq: 13 Nov 2018 9:00

Tgt Ion:112 Resp: 179818
 Ion Ratio Lower Upper
 112 100
 64 58.0 44.1 66.1
 63 29.9 23.7 35.5

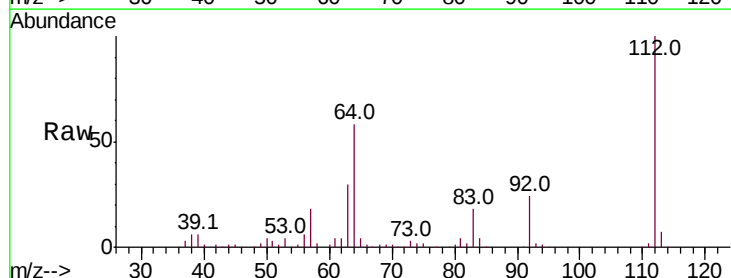

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF1
 Ion 63.00 (62.70 to 63.70): BF1

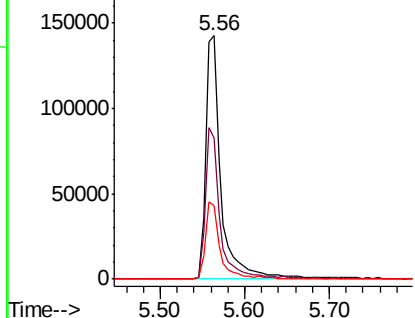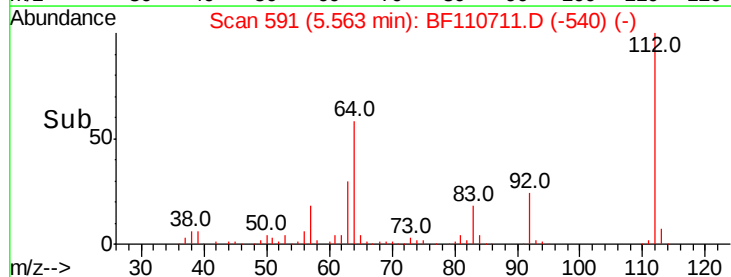

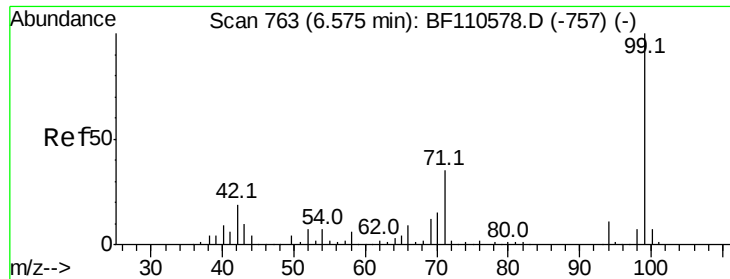

#7

Phenol-d6

Concen: 22.554 ng

RT: 6.56 min Scan# 761

Delta R.T. -0.01 min

Lab File: BF110711.D

Acq: 13 Nov 2018 9:00

Instrument :

BNA_F

ClientSampleId :

110818-JETT-E-U-S


Tot Ion: 99 Resp: 140227

Ion Ratio Lower Upper




99 100

42 18.4 15.8 23.6

71 34.4 28.0 42.0

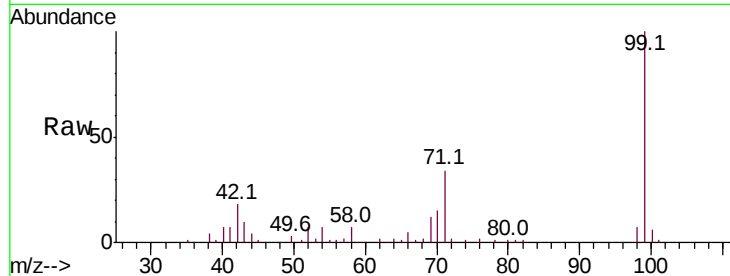

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

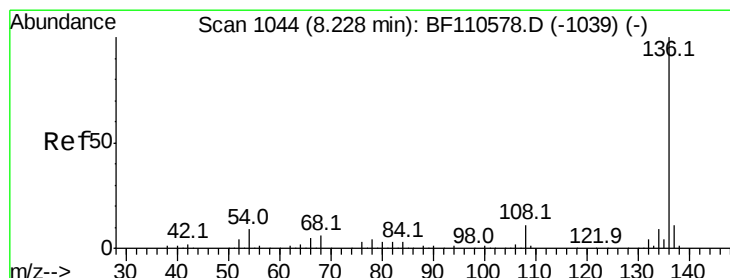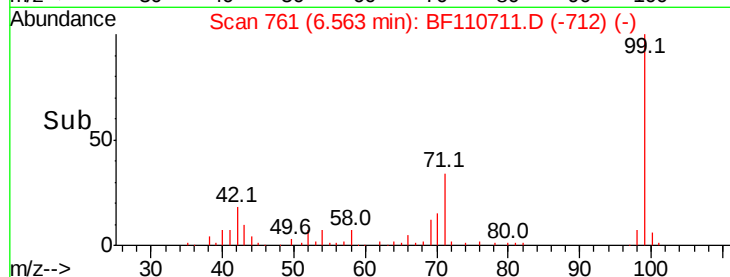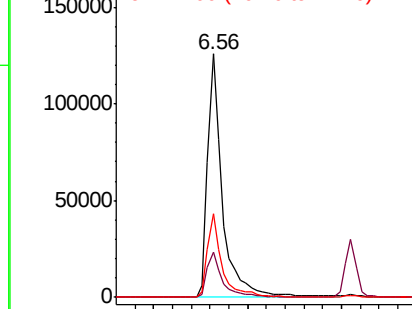

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.23 min Scan# 1044

Delta R.T. 0.00 min

Lab File: BF110711.D

Acq: 13 Nov 2018 9:00

Tgt Ion: 136 Resp: 328565


Ion Ratio Lower Upper

136 100



137 10.4 8.8 13.2

54 7.4 5.4 8.2

68 5.1 4.2 6.2

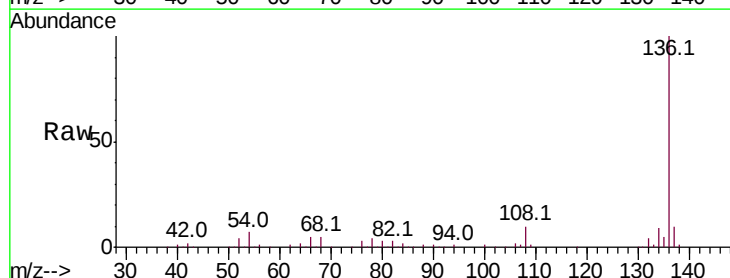

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

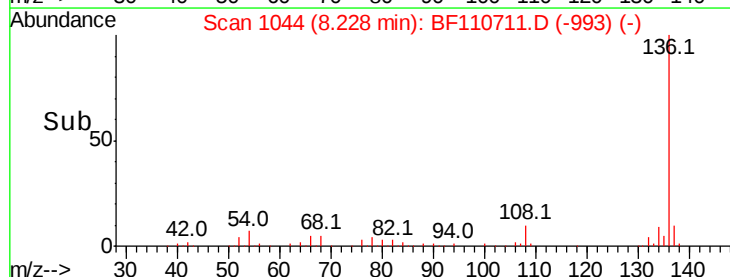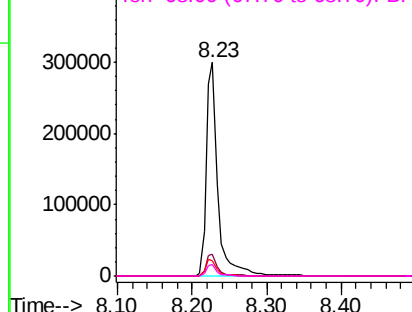







#23
 Nitrobenzene-d5
 Concen: 89.181 ng
 RT: 7.51 min Scan# 922
 Delta R.T. -0.01 min
 Lab File: BF110711.D
 Acq: 13 Nov 2018 9:00

Instrument :
 BNA_F
 ClientSampleId :
 110818-JETT-E-U-S

Tot Ion	Ratio	Lower	Upper
82	100		
128	44.8	34.2	51.2
54	53.0	38.6	58.0

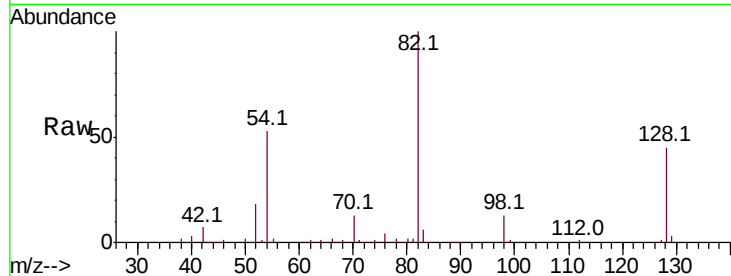


Abundance Ion 82.00 (81.70 to 82.70): BF1
 Ion 128.00 (127.70 to 128.70): BF1
 Ion 54.00 (53.70 to 54.70): BF1

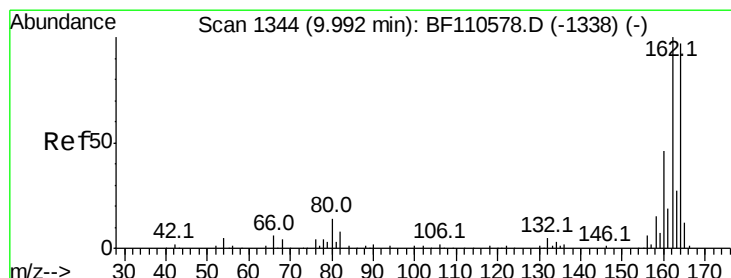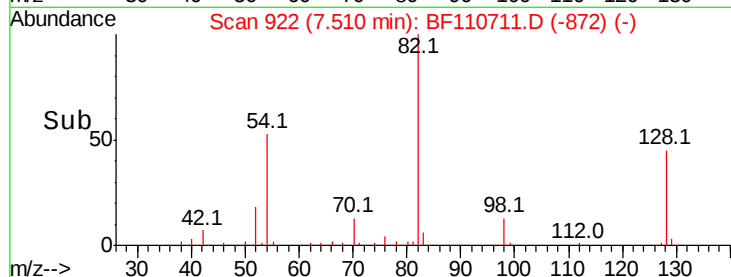
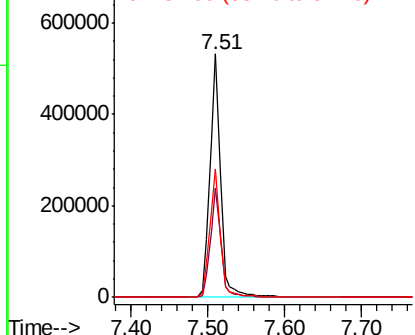


#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.99 min Scan# 1343
 Delta R.T. -0.01 min
 Lab File: BF110711.D
 Acq: 13 Nov 2018 9:00

Tgt Ion	Ratio	Lower	Upper
164	100		
162	105.4	83.0	124.6
160	47.6	37.0	55.6

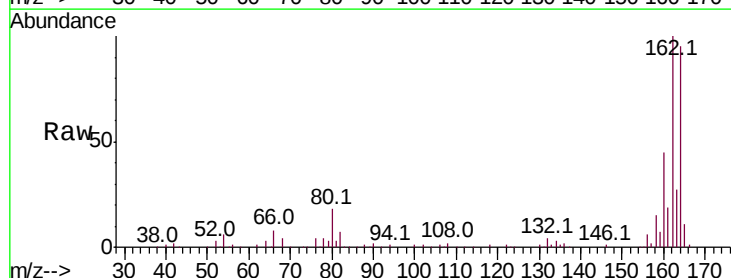

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

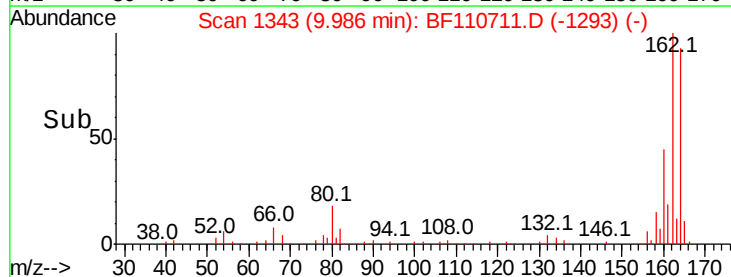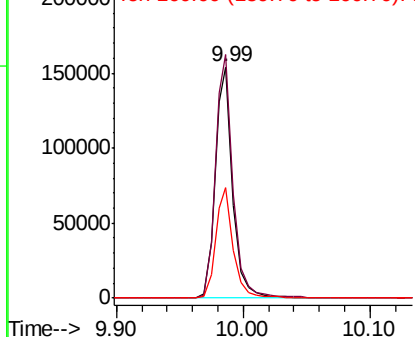



#42

2,4,6-Tribromophenol

Concen: 2.894 ng

RT: 10.79 min Scan# 1479

Delta R.T. 0.00 min

Lab File: BF110711.D

Acq: 13 Nov 2018 9:00

Instrument :

BNA_F

ClientSampleId :

110818-JETT-E-U-S


Tot Ion:330 Resp: 4345

Ion Ratio Lower Upper

330 100

332 97.1 77.1 115.7




141 36.6 27.0 40.4

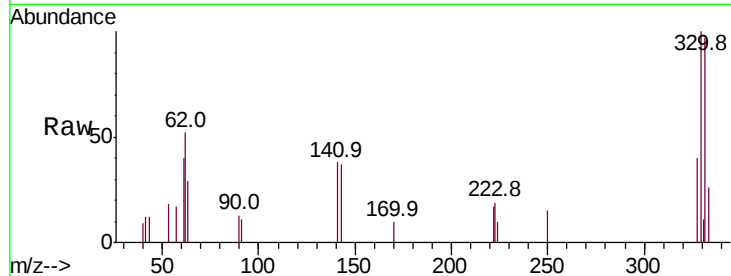

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

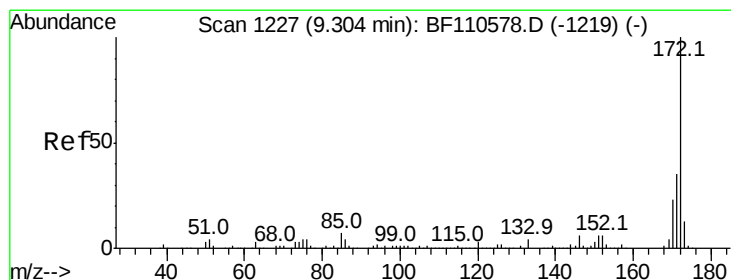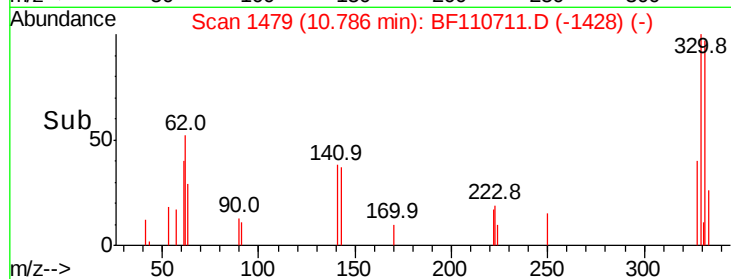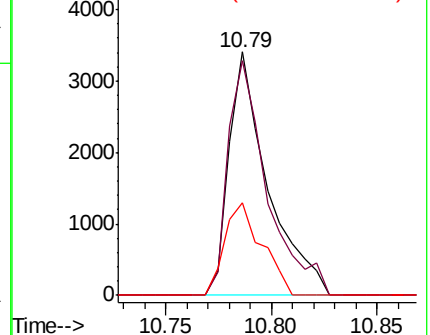

#45

2-Fluorobiphenyl

Concen: 89.049 ng

RT: 9.30 min Scan# 1226

Delta R.T. -0.01 min

Lab File: BF110711.D

Acq: 13 Nov 2018 9:00


Tgt Ion:172 Resp: 929075

Ion Ratio Lower Upper

172 100

171 35.1 28.6 43.0



170 24.2 19.7 29.5

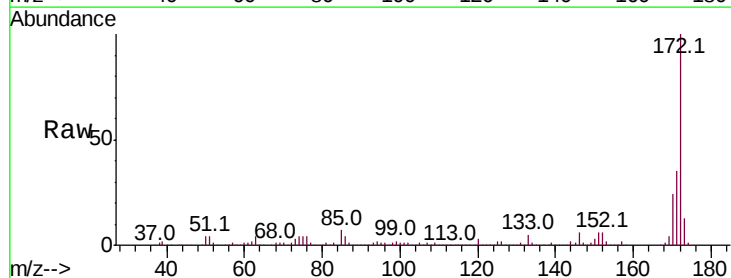


Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E



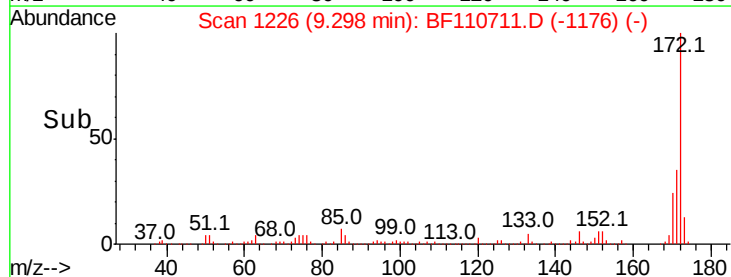
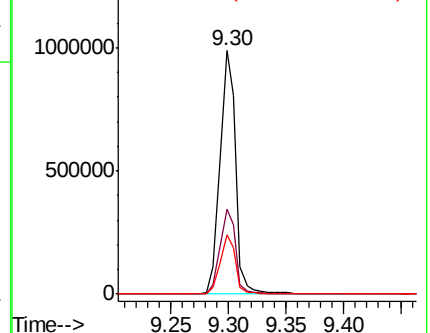


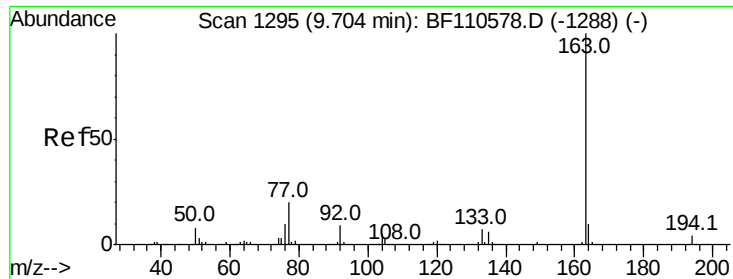

#50
Dimethylphthalate
Concen: 2.309 ng
RT: 9.69 min Scan# 1293
Delta R.T. -0.01 min
Lab File: BF110711.D
Acq: 13 Nov 2018 9:00




Instrument :
BNA_F
ClientSampleId :
110818-JETT-E-U-S


Tot Ion:163 Resp: 25670
Ion Ratio Lower Upper
163 100
194 3.8 3.2 4.8
164 11.2 8.1 12.1

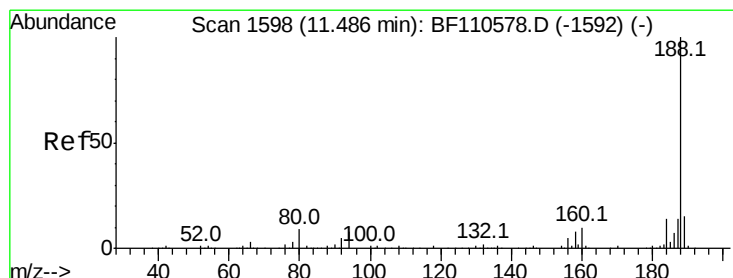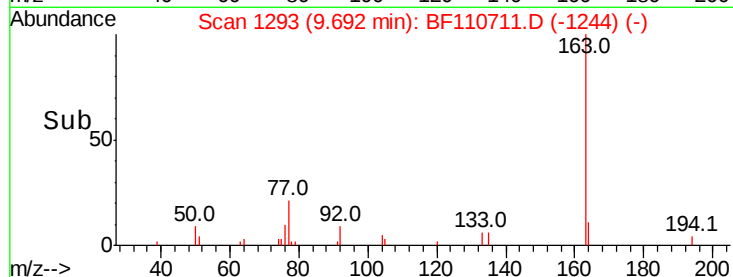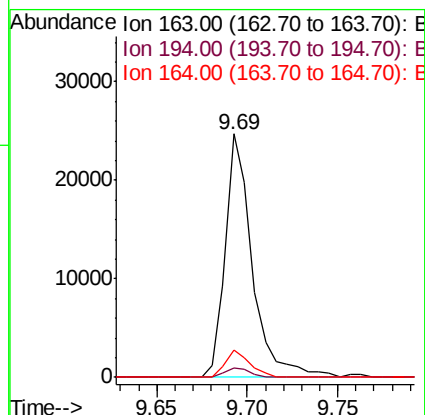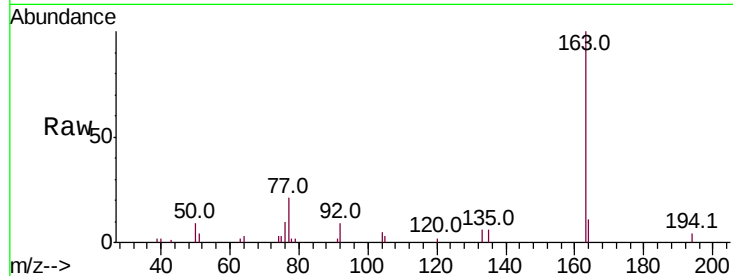

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.48 min Scan# 1597
Delta R.T. -0.01 min
Lab File: BF110711.D
Acq: 13 Nov 2018 9:00

Tgt Ion:188 Resp: 245993
Ion Ratio Lower Upper
188 100
94 8.2 7.2 10.8
80 9.4 7.9 11.9

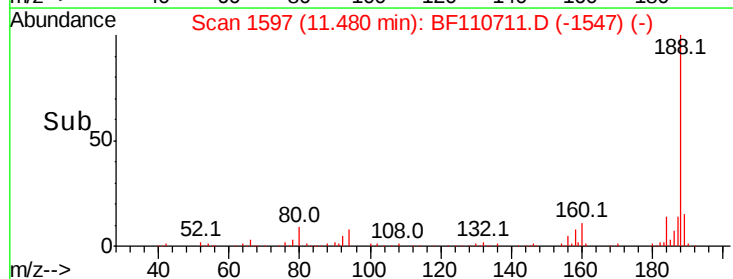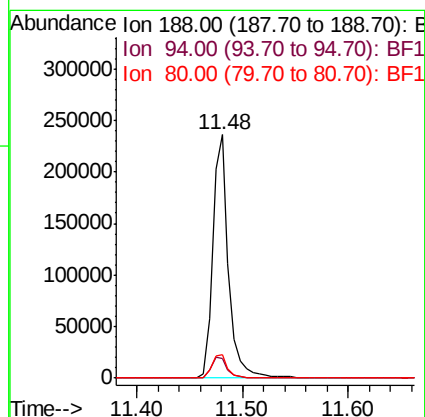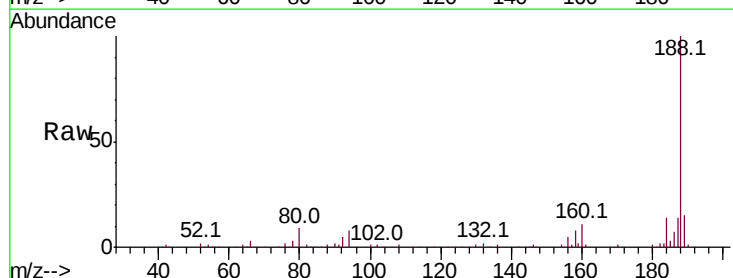


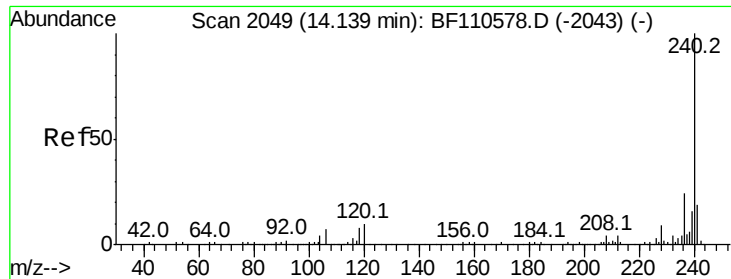




#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.13 min Scan# 2047
Delta R.T. -0.01 min
Lab File: BF110711.D
Acq: 13 Nov 2018 9:00

Instrument :
BNA_F
ClientSampleId :
110818-JETT-E-U-S

Tot Ion:240 Resp: 161772
Ion Ratio Lower Upper
240 100
120 12.5 8.3 12.5#
236 25.5 21.2 31.8

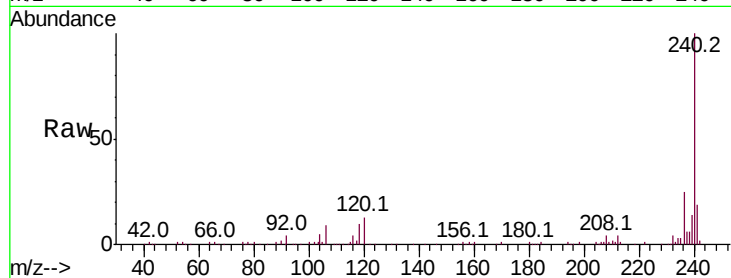


Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

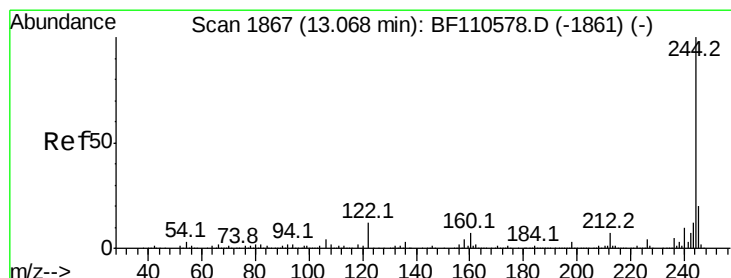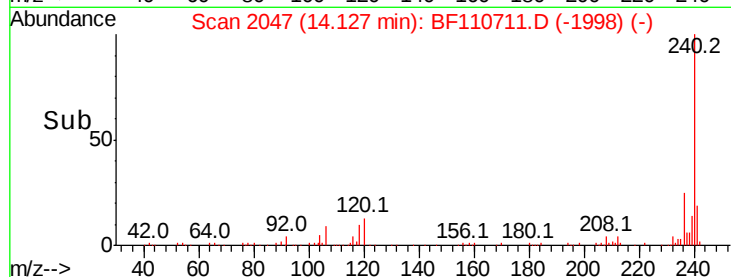
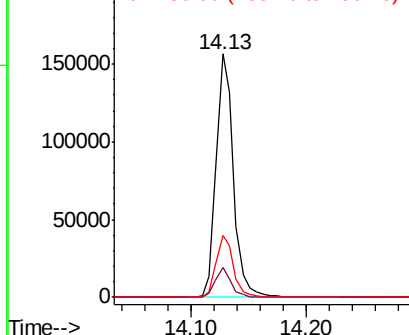



#79
Terphenyl-d14
Concen: 73.999 ng
RT: 13.06 min Scan# 1866
Delta R.T. -0.01 min
Lab File: BF110711.D
Acq: 13 Nov 2018 9:00

Tgt Ion:244 Resp: 639213
Ion Ratio Lower Upper
244 100
212 6.5 5.8 8.8
122 11.0 8.7 13.1

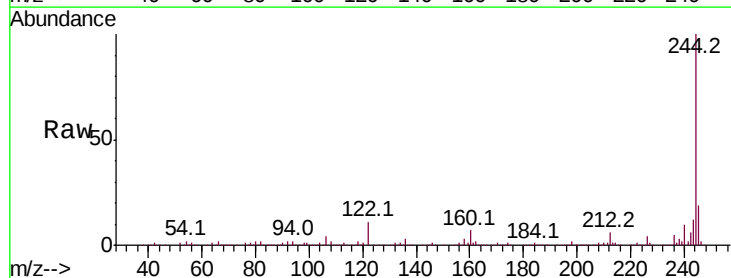

Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

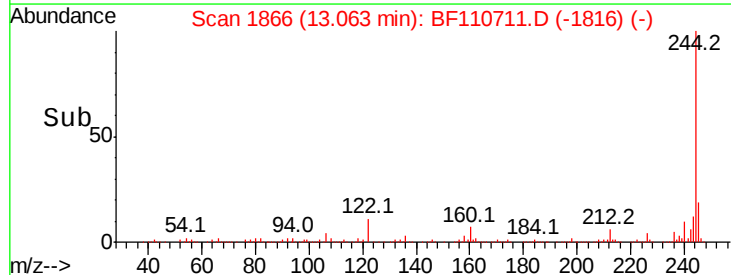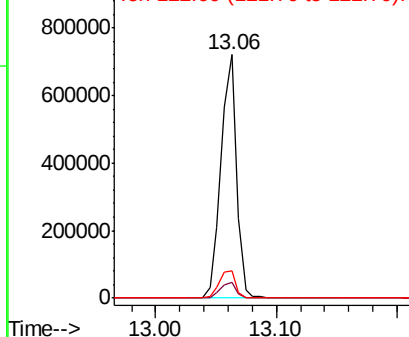

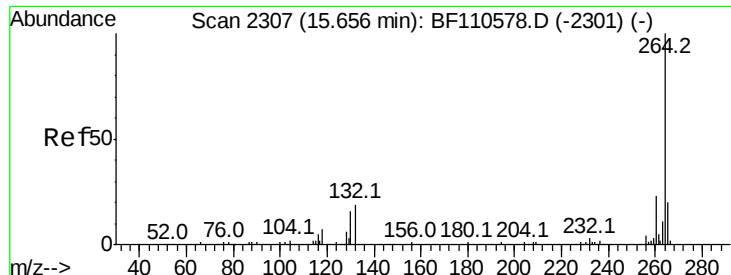

#87
 Pervlene-d12
 Concen: 20.000 ng
 RT: 15.66 min Scan# 2307
 Delta R.T. 0.00 min
 Lab File: BF110711.D
 Acq: 13 Nov 2018 9:00

Instrument :
 BNA_F
 ClientSampleId :
 110818-JETT-E-U-S

Tot Ion:	264	Resp:	129519
Ion	Ratio	Lower	Upper
264	100		
260	22.2	18.7	28.1
265	21.7	16.7	25.1

