


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111218\
 Data File : BF110696.D
 Acq On : 13 Nov 2018 2:06
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 09 15:13:13 2018

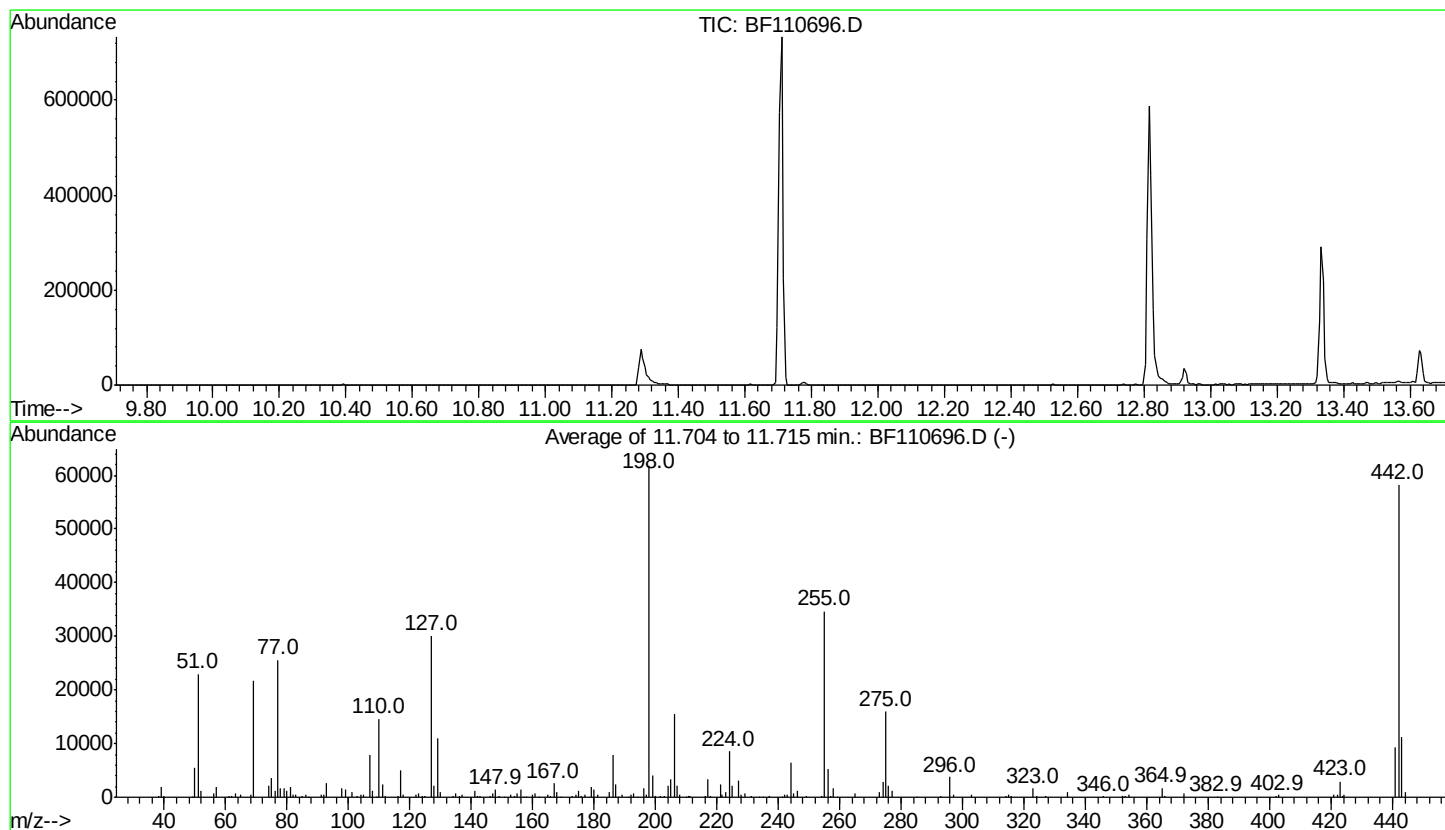

AutoFind: Scans 1635, 1636, 1637; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.2	22980	PASS
68	69	0.00	2	1.8	390	PASS
69	198	0.00	100	35.2	21767	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.8	30186	PASS
197	198	0.00	2	0.7	417	PASS
198	198	100	100	100.0	61813	PASS
199	198	5	9	6.7	4143	PASS
275	198	10	60	25.8	15933	PASS
365	198	1	100	2.7	1683	PASS
441	198	0.01	100	15.0	9265	PASS
442	198	50	100	94.3	58301	PASS
443	442	15	24	19.2	11221	PASS