
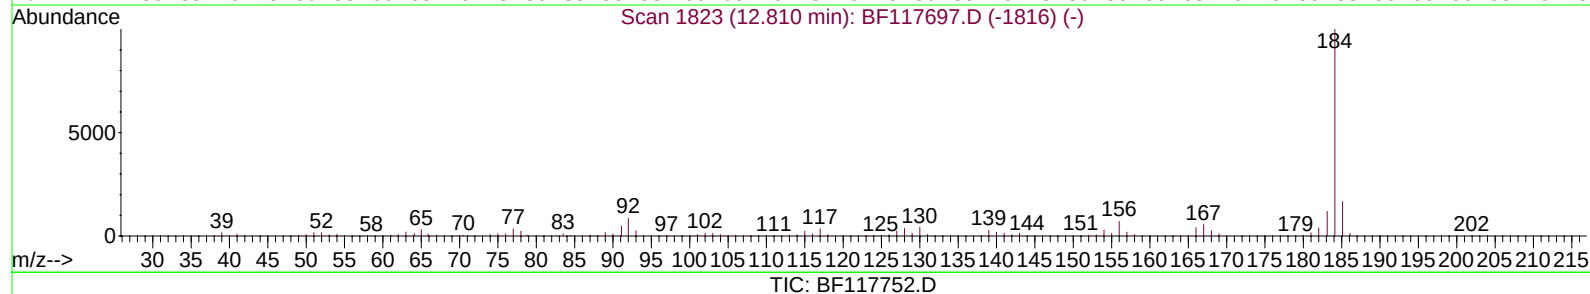
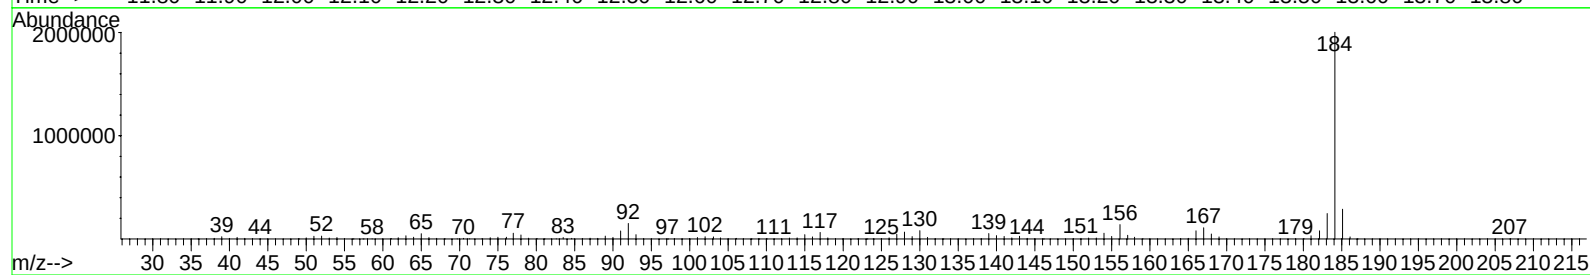


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF111219\
Data File : BF117752.D
Acq On : 12 Nov 2019 10:33
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 12 17:34:29 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF110619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 12 13:32:26 2019
Response via : Initial Calibration

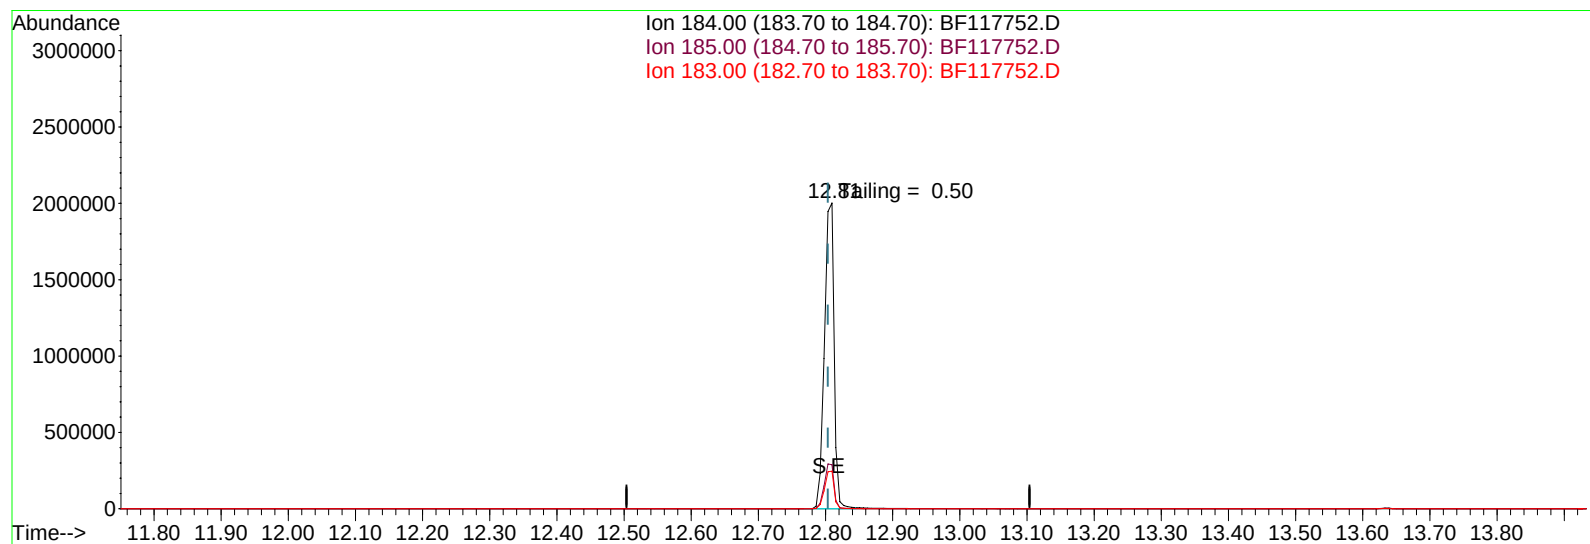

(77) Benzidine




12.810min (+0.006) 0.00ng

response 2020789

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	14.40
183.00	12.20	12.29
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF111219\
Data File : BF117752.D
Acq On : 12 Nov 2019 10:33
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 12 17:34:29 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF110619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 12 13:32:26 2019
Response via : Initial Calibration

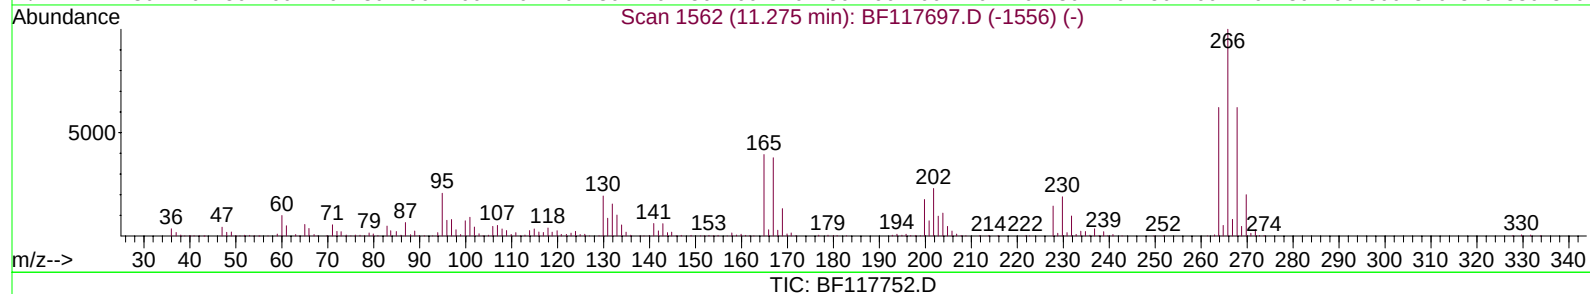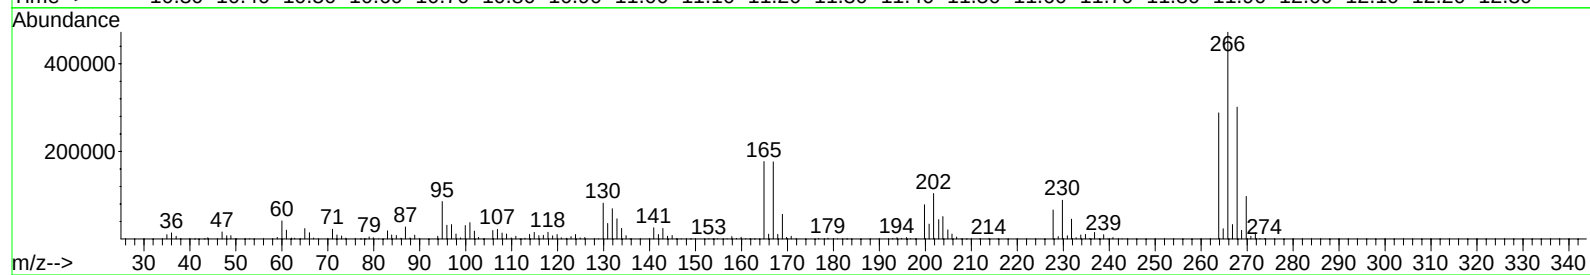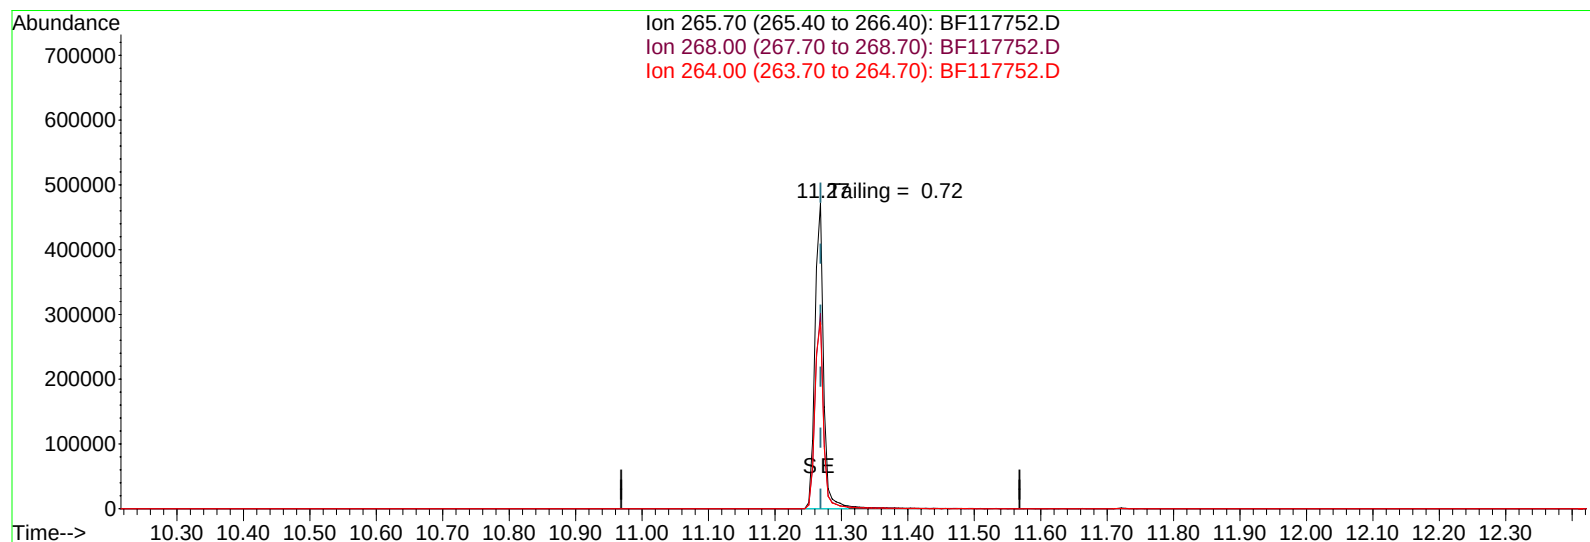

(70) Pentachlorophenol (C)

11.268min (-0.000) 40762.06ng

response 430939

Ion	Exp%	Act%
265.70	100	100
268.00	62.60	63.82
264.00	62.20	61.01
0.00	0.00	0.00