


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF111219\
 Data File : BF117752.D
 Acq On : 12 Nov 2019 10:33
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 12 13:32:26 2019

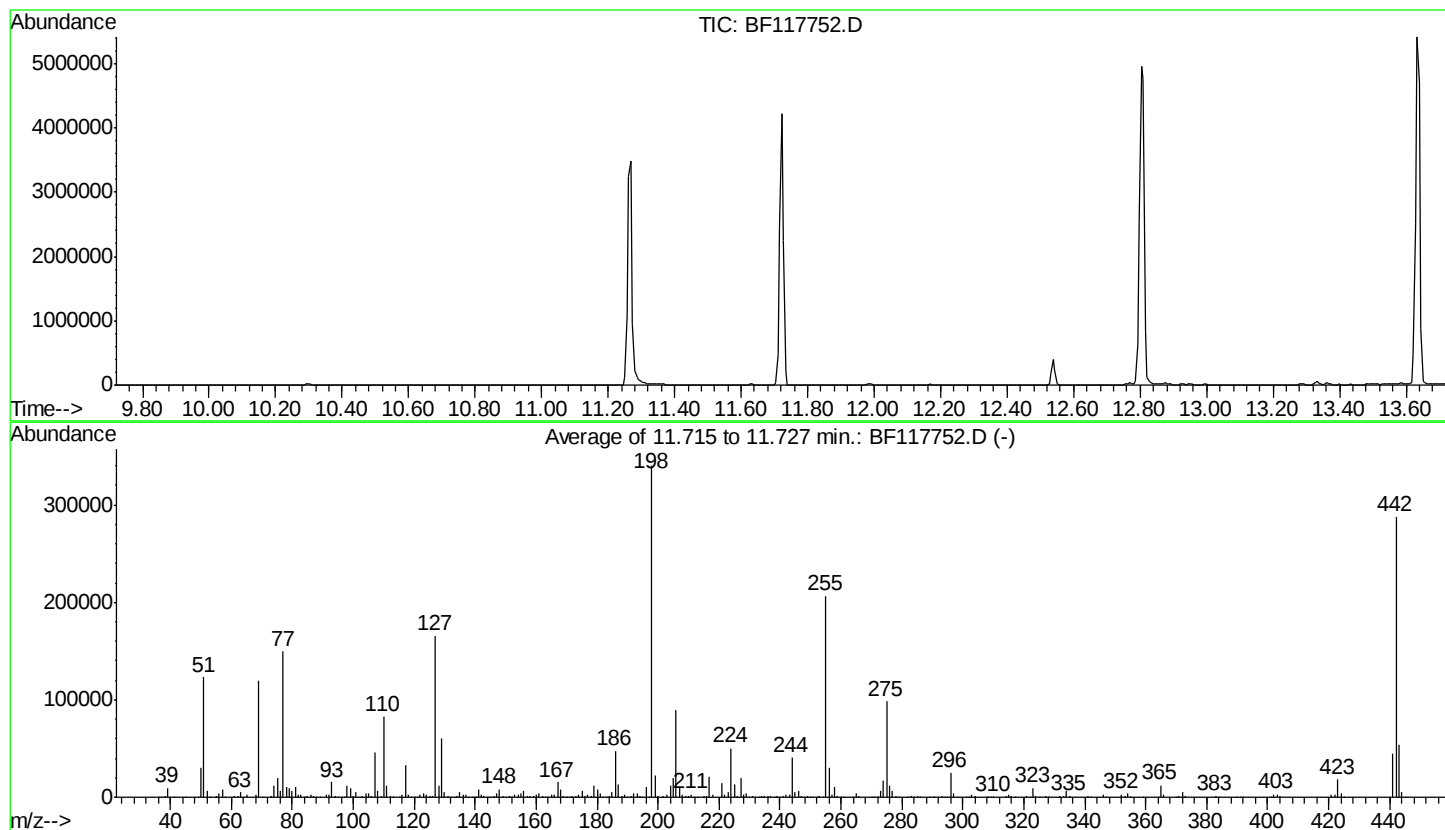

AutoFind: Scans 1637, 1638, 1639; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.3	123482	PASS
68	69	0.00	2	1.8	2200	PASS
69	198	0.00	100	35.2	119680	PASS
70	69	0.00	2	0.4	468	PASS
127	198	10	80	48.7	165890	PASS
197	198	0.00	2	0.2	593	PASS
198	198	100	100	100.0	340352	PASS
199	198	5	9	6.7	22819	PASS
275	198	10	60	28.9	98464	PASS
365	198	1	100	3.6	12153	PASS
441	198	0.01	100	13.3	45336	PASS
442	198	50	100	84.7	288298	PASS
443	442	15	24	18.6	53754	PASS