
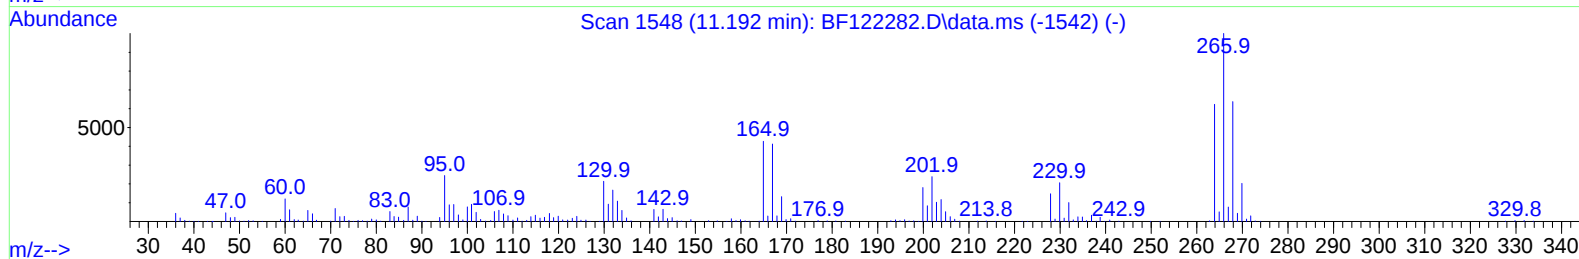
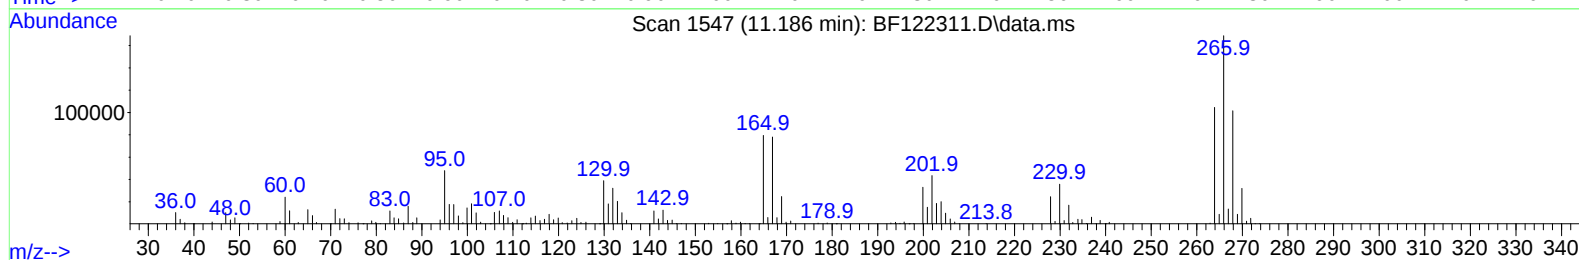


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111220\
Data File : BF122311.D
Acq On : 12 Nov 2020 12:36
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 13 02:12:31 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 10 12:25:42 2020
Response via : Initial Calibration

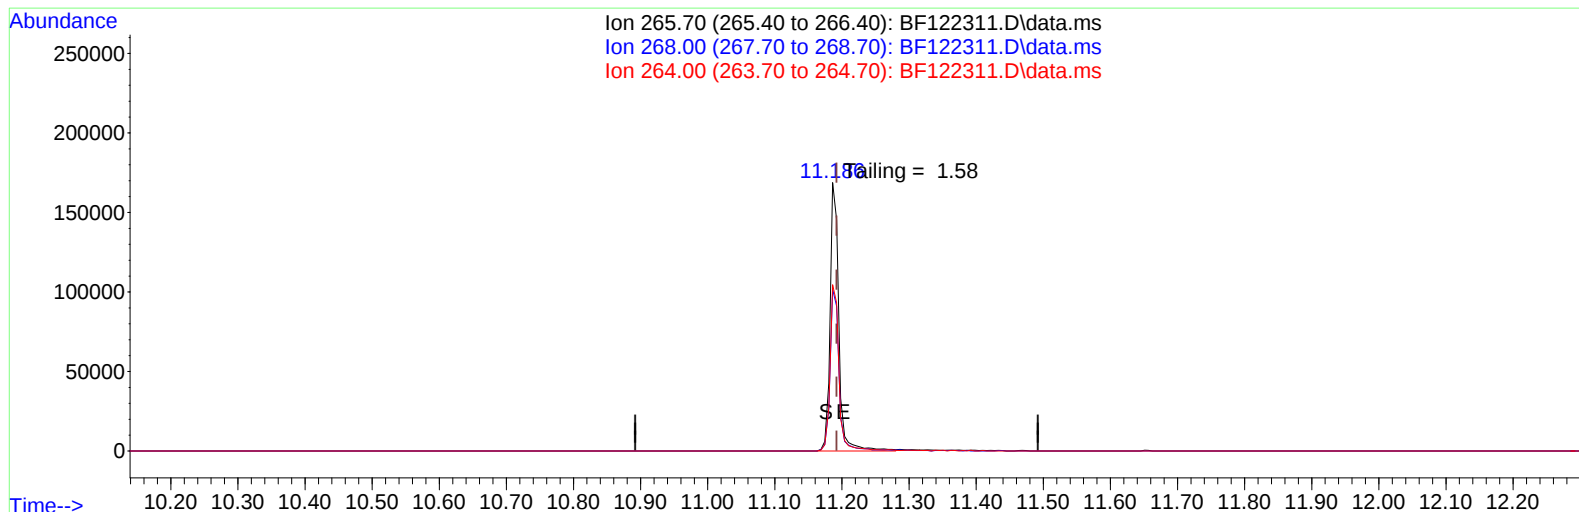

TIC: BF122311.D\data.ms

(70) Pentachlorophenol (C)




11.186min (-0.006) 91075.82 ng

response 153891

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.50	60.20
264.00	62.40	61.97
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111220\
Data File : BF122311.D
Acq On : 12 Nov 2020 12:36
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 13 02:12:31 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 10 12:25:42 2020
Response via : Initial Calibration

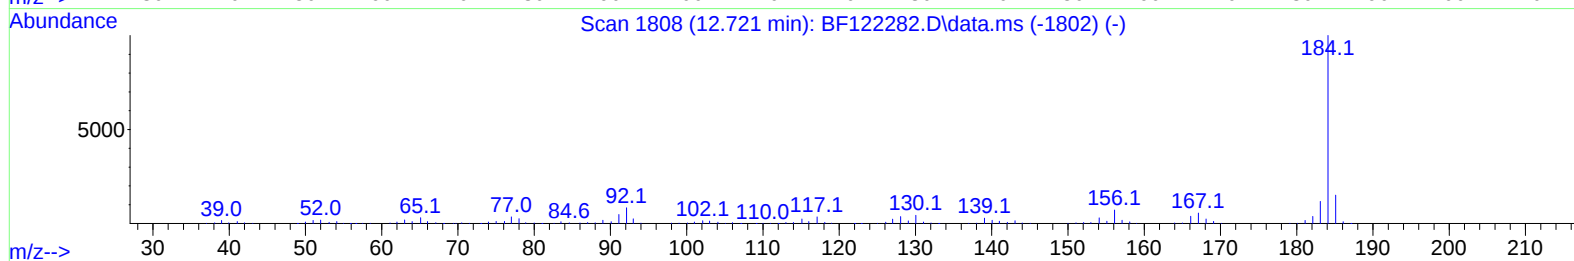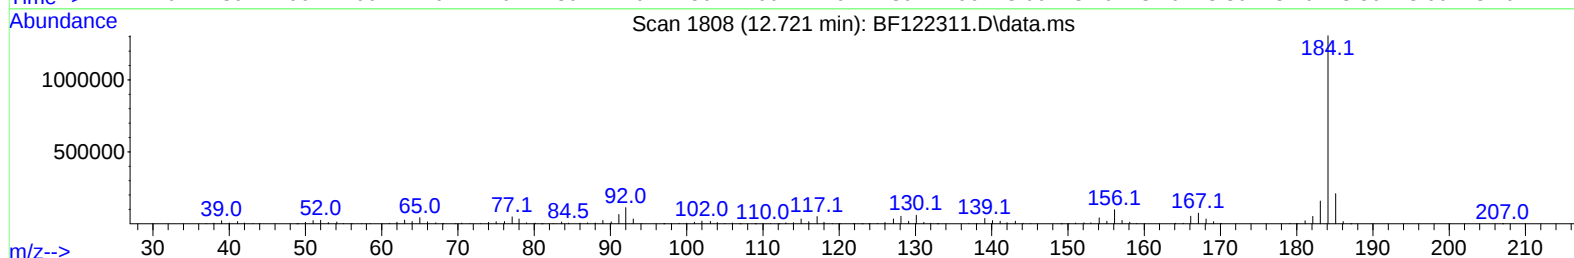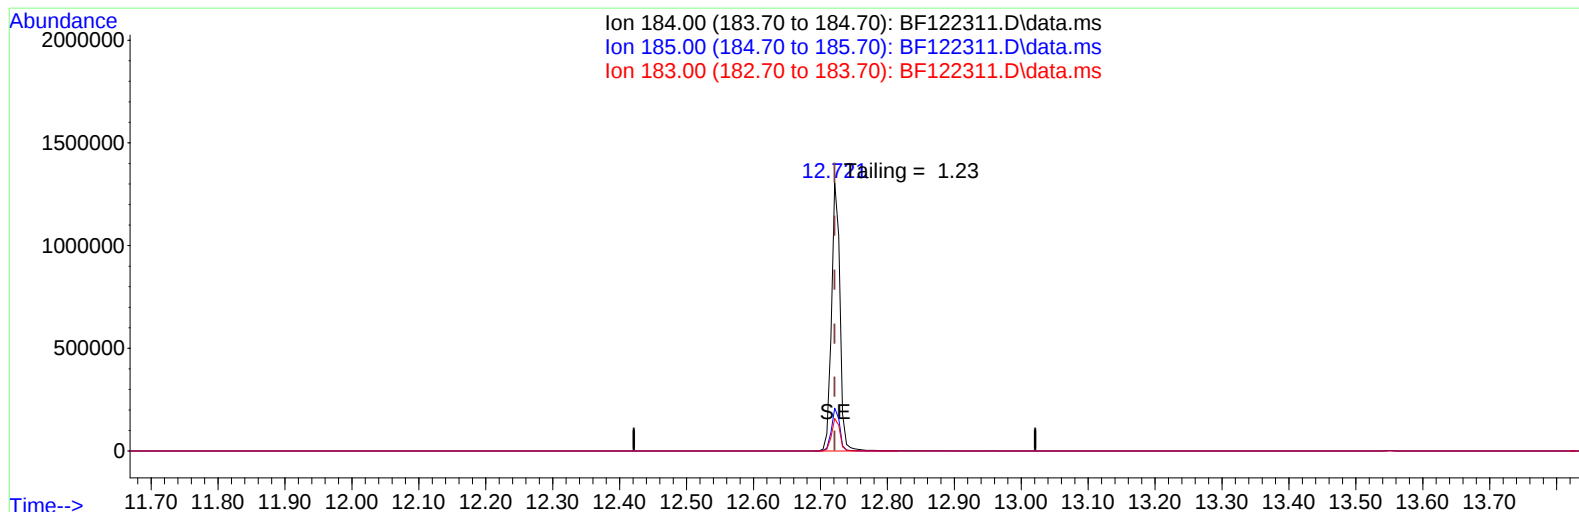

TIC: BF122311.D\data.ms

(77) Benzidine

12.721min (+ 0.000) 20254.85 ng

response 1156161

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	16.01
183.00	11.70	12.09
0.00	0.00	0.00