

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111220\
 Data File : BF122313.D
 Acq On : 12 Nov 2020 13:38
 Operator : JU/CG
 Sample : PB132953BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB132953BL

Quant Time: Nov 12 14:05:16 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 10 12:25:42 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.863	152	307248	20.00	ng	0.00
21) Naphthalene-d8	8.151	136	1183913	20.00	ng	0.00
39) Acenaphthene-d10	9.904	164	609707	20.00	ng	0.00
64) Phenanthrene-d10	11.386	188	1111402	20.00	ng	0.00
76) Chrysene-d12	14.027	240	985964	20.00	ng	0.00
86) Perylene-d12	15.498	264	946175	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.493	112	2479782	123.93	ng	0.02
7) Phenol-d6	6.487	99	3185719	121.70	ng	0.00
23) Nitrobenzene-d5	7.428	82	1984008	102.59	ng	0.00
42) 2,4,6-Tribromophenol	10.692	330	857718	131.07	ng	0.00
45) 2-Fluorobiphenyl	9.228	172	3380154	86.62	ng	0.00
79) Terphenyl-d14	12.980	244	3599994	77.35	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111220\
Data File : BF122313.D
Acq On : 12 Nov 2020 13:38
Operator : JU/CG
Sample : PB132953BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB132953BL

Quant Time: Nov 12 14:05:16 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 10 12:25:42 2020
Response via : Initial Calibration




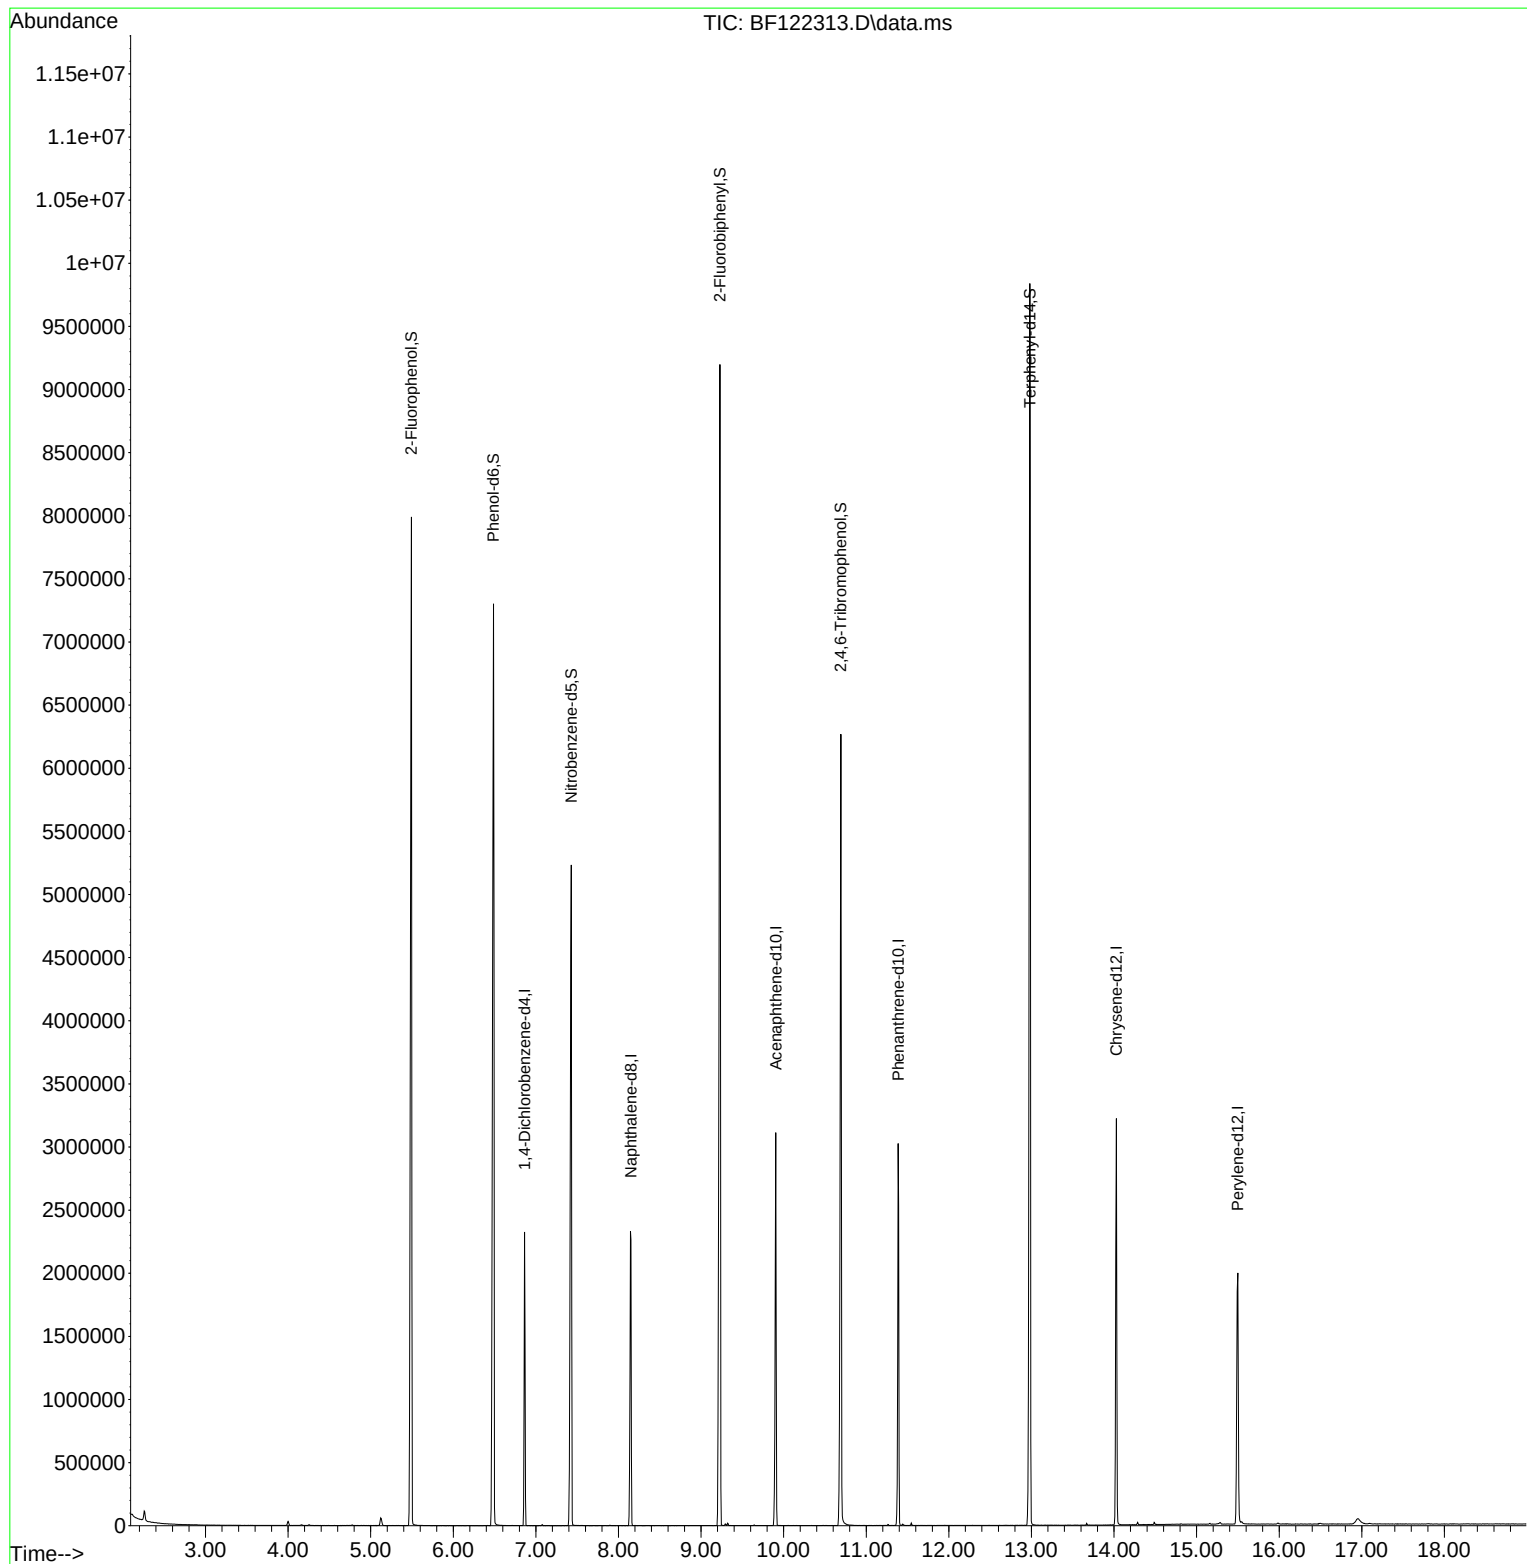




#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.863 min Scan# 812
Delta R.T. -0.006 min
Lab File: BF122313.D
Acq: 12 Nov 2020 13:38




Instrument :
BNA_F
ClientSampleId :
PB132953BL


Tgt Ion:152 Resp: 307248
Ion Ratio Lower Upper
152 100
150 155.9 125.3 187.9
115 62.2 51.9 77.9

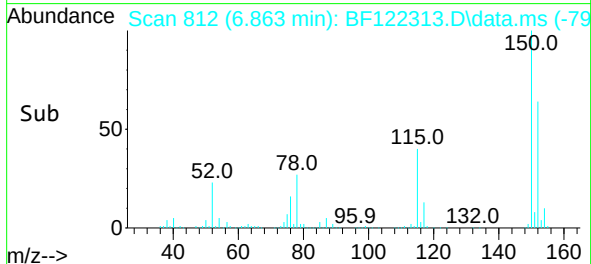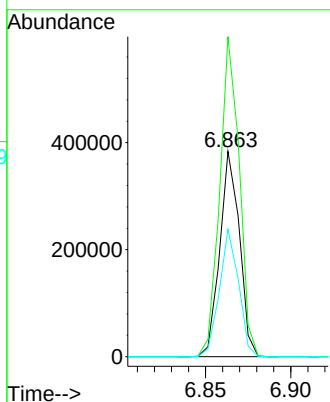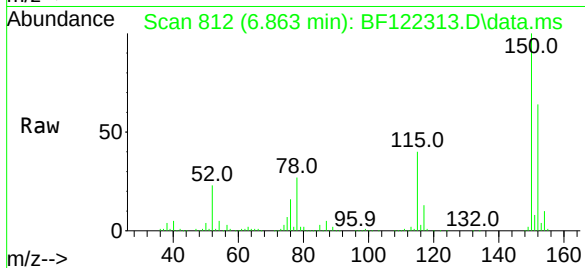

#5
2-Fluorophenol
Concen: 123.93 ng
RT: 5.493 min Scan# 579
Delta R.T. 0.018 min
Lab File: BF122313.D
Acq: 12 Nov 2020 13:38

Tgt Ion:112 Resp: 2479782
Ion Ratio Lower Upper
112 100
64 60.0 50.4 75.6
63 32.0 25.8 38.6


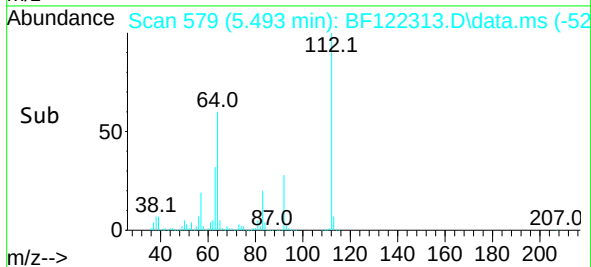
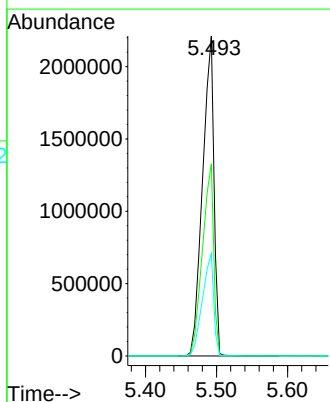
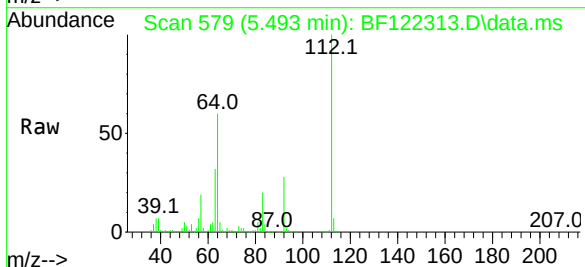


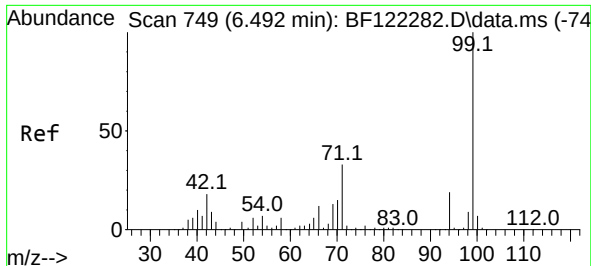

#7
Phenol-d6
Concen: 121.70 ng
RT: 6.487 min Scan# 748
Delta R.T. -0.005 min
Lab File: BF122313.D
Acq: 12 Nov 2020 13:38




Instrument :
BNA_F
ClientSampleId :
PB132953BL


Tgt Ion: 99 Resp: 3185719
Ion Ratio Lower Upper
99 100
42 19.9 15.9 23.9
71 35.3 27.1 40.7

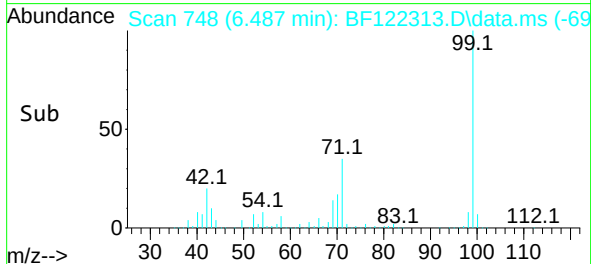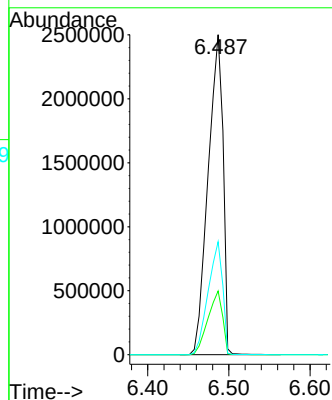

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.151 min Scan# 1031
Delta R.T. 0.000 min
Lab File: BF122313.D
Acq: 12 Nov 2020 13:38

Tgt Ion:136 Resp: 1183913
Ion Ratio Lower Upper
136 100
137 11.2 8.6 13.0
54 7.4 7.1 10.7
68 5.6 5.0 7.4

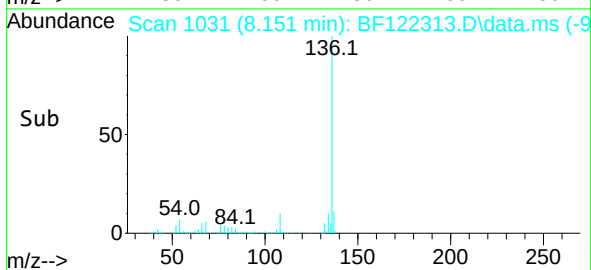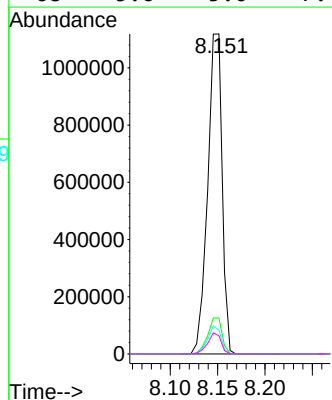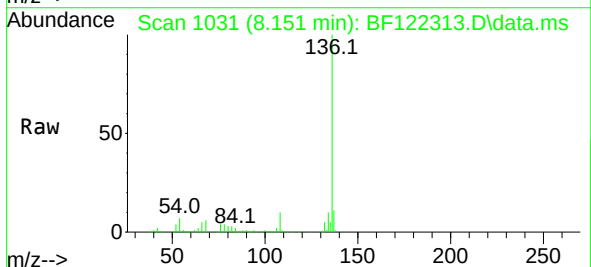

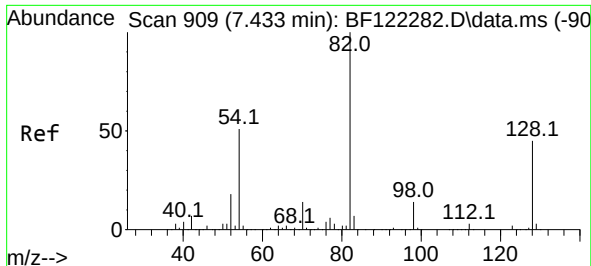

#23

Nitrobenzene-d5

Concen: 102.59 ng

RT: 7.428 min Scan# 908

Delta R.T. -0.005 min

Lab File: BF122313.D

Acq: 12 Nov 2020 13:38

Tgt Ion: 82 Resp: 1984008





Ion	Ratio	Lower	Upper
82	100		
128	45.6	35.0	52.4
54	50.8	43.9	65.9

Instrument :

BNA_F

ClientSampleId :

PB132953BL

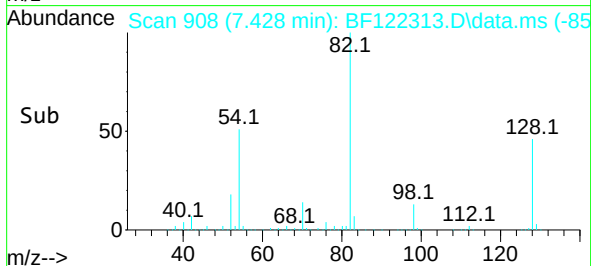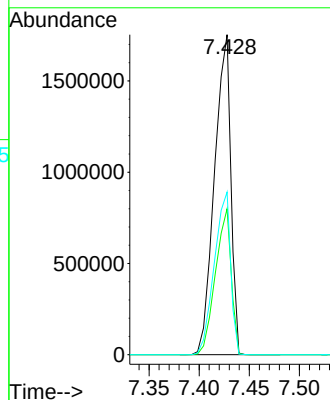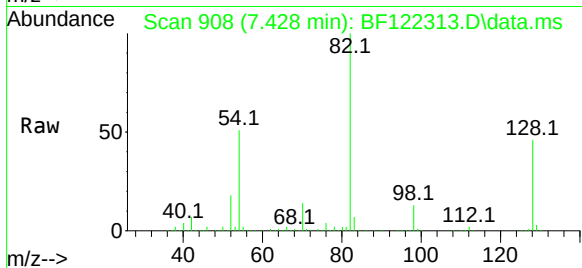

#39

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.904 min Scan# 1329




Delta R.T. -0.006 min


Lab File: BF122313.D

Acq: 12 Nov 2020 13:38

Tgt Ion:164 Resp: 609707

Ion	Ratio	Lower	Upper
164	100		
162	102.5	83.2	124.8
160	47.3	37.5	56.3


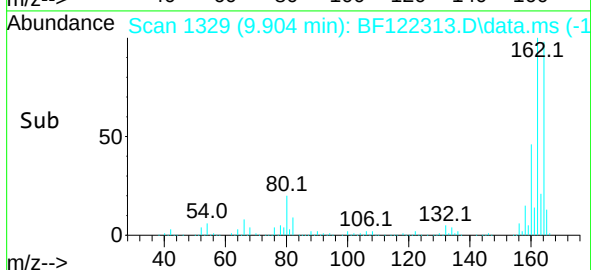
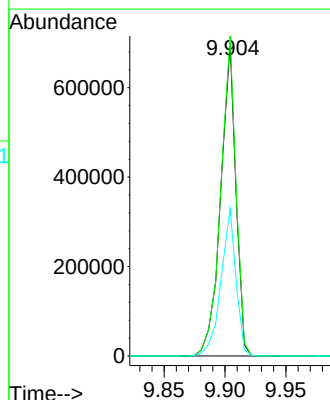
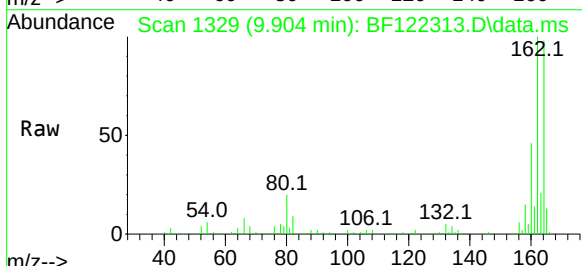


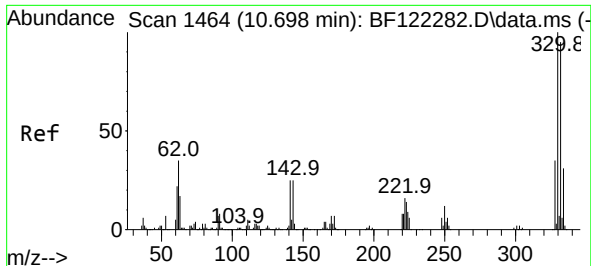

#42
2,4,6-Tribromophenol
Concen: 131.07 ng
RT: 10.692 min Scan# 1463
Delta R.T. -0.005 min
Lab File: BF122313.D
Acq: 12 Nov 2020 13:38




Instrument :
BNA_F
ClientSampleId :
PB132953BL


Tgt Ion: 330 Resp: 857718
Ion Ratio Lower Upper
330 100
332 96.5 77.3 115.9
141 30.6 22.3 33.5

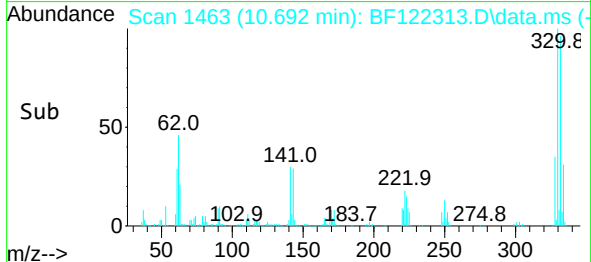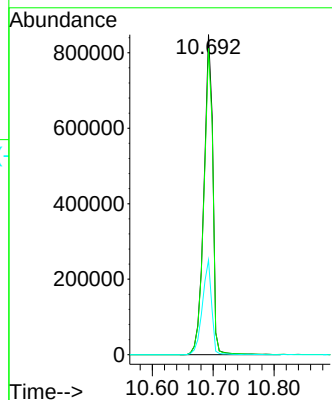

#45
2-Fluorobiphenyl
Concen: 86.62 ng
RT: 9.228 min Scan# 1214
Delta R.T. -0.005 min
Lab File: BF122313.D
Acq: 12 Nov 2020 13:38

Tgt Ion: 172 Resp: 3380154
Ion Ratio Lower Upper
172 100
171 38.1 29.1 43.7
170 25.7 19.8 29.6


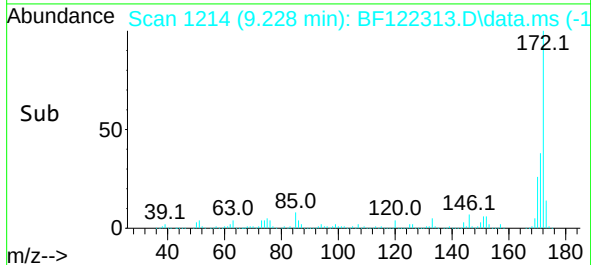
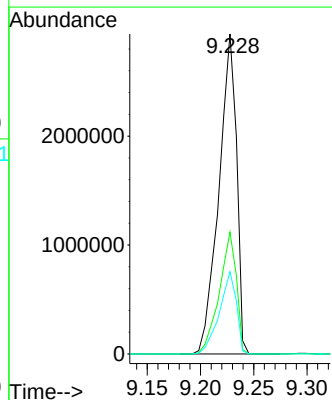
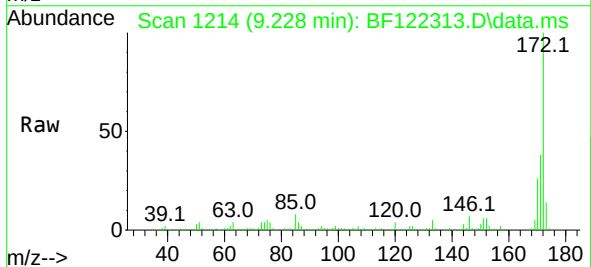


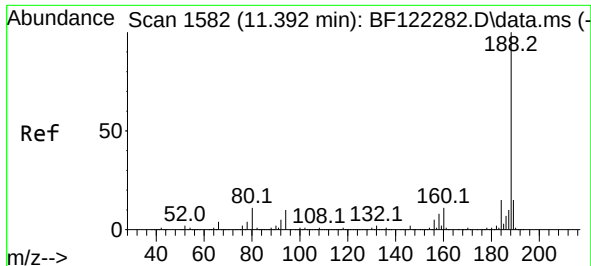

#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.386 min Scan# 1581
Delta R.T. -0.006 min
Lab File: BF122313.D
Acq: 12 Nov 2020 13:38




Instrument :
BNA_F
ClientSampleId :
PB132953BL


Tgt Ion:188 Resp: 1111402
Ion Ratio Lower Upper
188 100
94 10.6 8.3 12.5
80 11.5 9.1 13.7

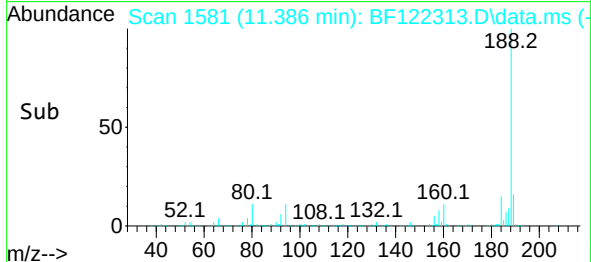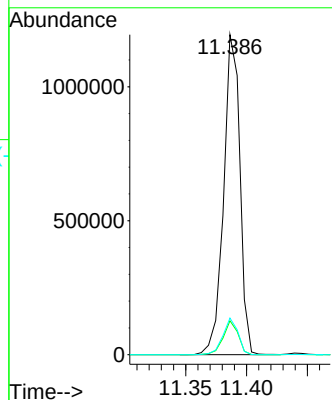

#76
Chrysene-d12
Concen: 20.00 ng
RT: 14.027 min Scan# 2030
Delta R.T. -0.006 min
Lab File: BF122313.D
Acq: 12 Nov 2020 13:38

Tgt Ion:240 Resp: 985964
Ion Ratio Lower Upper
240 100
120 10.4 9.2 13.8
236 26.5 20.9 31.3


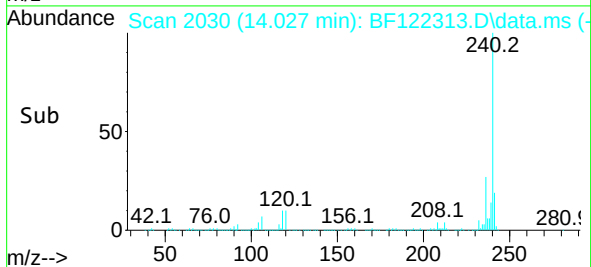
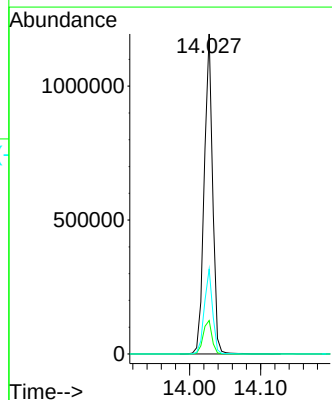
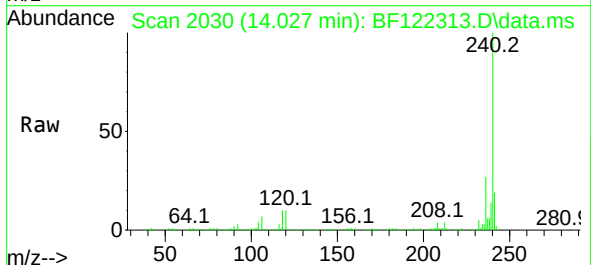




#79
 Terphenyl-d14
 Concen: 77.35 ng
 RT: 12.980 min Scan# 1852
 Delta R.T. 0.000 min
 Lab File: BF122313.D
 Acq: 12 Nov 2020 13:38

Instrument :
 BNA_F
 ClientSampleId :
 PB132953BL

Tgt Ion:244 Resp: 3599994
 Ion Ratio Lower Upper
 244 100
 212 7.5 5.4 8.2
 122 11.4 8.1 12.1

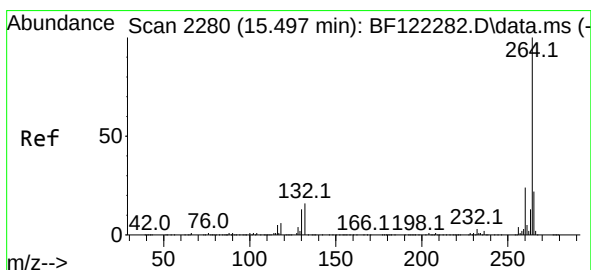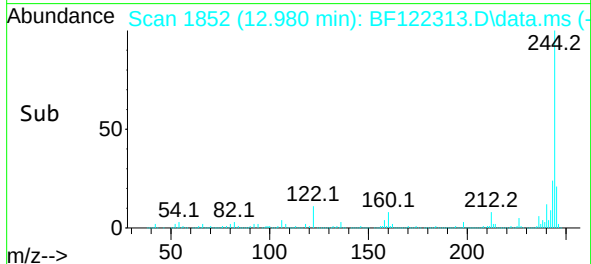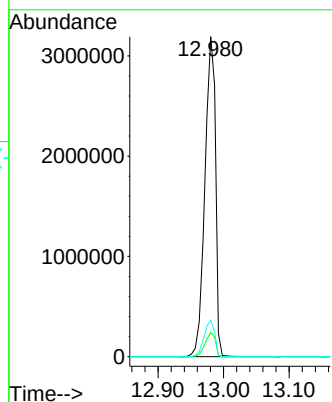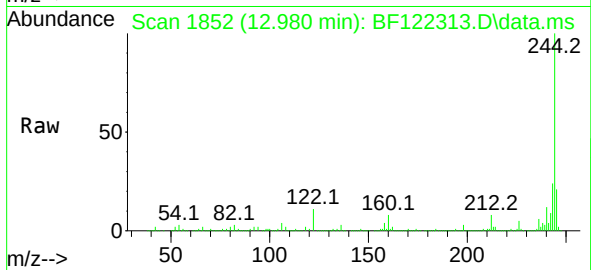

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.498 min Scan# 2280
 Delta R.T. 0.000 min
 Lab File: BF122313.D
 Acq: 12 Nov 2020 13:38

Tgt Ion:264 Resp: 946175
 Ion Ratio Lower Upper
 264 100
 260 24.0 18.7 28.1
 265 21.6 17.3 25.9

