

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111220\
 Data File : BF122315.D
 Acq On : 12 Nov 2020 15:00
 Operator : JU/CG
 Sample : L4702-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 M-5(10-20)

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF122315.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.163	8	13	20	rVB	1416110	1845390	22.58%	2.475%
2	5.087	501	510	516	rBV	56888	83764	1.02%	0.112%
3	5.481	571	577	580	rBV	6652117	6872040	84.07%	9.218%
4	6.486	741	748	751	rBV	6313008	7107721	86.95%	9.534%
5	6.686	779	782	784	rBV	401037	291009	3.56%	0.390%
6	6.863	809	812	816	rVB	2132829	1671034	20.44%	2.242%
7	7.428	902	908	911	rBV	4653722	4583030	56.07%	6.148%
8	8.145	1026	1030	1034	rBV	2346579	2249315	27.52%	3.017%
9	8.745	1128	1132	1135	rBV	139437	112413	1.38%	0.151%
10	9.227	1208	1214	1217	rBV	8055840	7829436	95.78%	10.503%
11	9.310	1223	1228	1231	rBV	268042	243729	2.98%	0.327%
12	9.616	1276	1280	1283	rBV	1527385	1264094	15.46%	1.696%
13	9.839	1315	1318	1322	rVB	409963	327486	4.01%	0.439%
14	9.904	1322	1329	1333	rVV	2981838	2631833	32.20%	3.530%
15	10.339	1400	1403	1406	rVB	222674	181049	2.21%	0.243%
16	10.692	1457	1463	1466	rBV	5532677	5618706	68.74%	7.537%
17	11.386	1577	1581	1585	rBV	2979456	2654004	32.47%	3.560%
18	11.921	1666	1672	1680	rBV	1417191	1899489	23.24%	2.548%
19	12.704	1800	1805	1815	rBV	796392	918324	11.23%	1.232%
20	12.798	1818	1821	1824	rVB3	110009	117194	1.43%	0.157%
21	12.980	1847	1852	1855	rBV	8368469	8174263	100.00%	10.965%
22	13.121	1864	1876	1877	rBV4	165562	523401	6.40%	0.702%
23	13.457	1927	1933	1940	rBV	1783273	1757671	21.50%	2.358%
24	13.521	1940	1944	1948	rVV3	88133	112167	1.37%	0.150%
25	13.821	1990	1995	1999	rBV	636078	918489	11.24%	1.232%
26	13.868	1999	2003	2005	rVV	960612	1503624	18.39%	2.017%
27	13.898	2005	2008	2012	rVV	2491397	2840367	34.75%	3.810%
28	13.951	2012	2017	2026	rVV2	408776	942653	11.53%	1.264%
29	14.027	2026	2030	2033	rVB	3070398	2701389	33.05%	3.624%
30	14.204	2056	2060	2066	rVB	120773	149398	1.83%	0.200%
31	14.380	2082	2090	2101	rBV2	267432	821699	10.05%	1.102%
32	14.504	2109	2111	2123	rVB	161642	220394	2.70%	0.296%
33	14.627	2125	2132	2136	rVV3	141131	368092	4.50%	0.494%
34	14.662	2136	2138	2141	rVB	109240	100869	1.23%	0.135%
35	14.786	2152	2159	2162	rBV3	138183	333113	4.08%	0.447%
36	14.815	2162	2164	2172	rVB	151869	169663	2.08%	0.228%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111220\
Data File : BF122315.D
Acq On : 12 Nov 2020 15:00
Operator : JU/CG
Sample : L4702-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
M-5(10-20)

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	15.156	2219	2222	2229	rVB	118866	151627	1.85%	0.203%
38	15.262	2233	2240	2251	rVB4	135679	452426	5.53%	0.607%
39	15.492	2274	2279	2284	rBV	1909507	2387555	29.21%	3.203%
40	15.545	2284	2288	2295	rVB	101317	131759	1.61%	0.177%
41	16.039	2368	2372	2381	rVB	42007	102570	1.25%	0.138%
42	16.133	2385	2388	2395	rVB6	46028	82249	1.01%	0.110%
43	16.321	2413	2420	2431	rVB4	71803	212386	2.60%	0.285%
44	16.498	2446	2450	2456	rVB	51777	87817	1.07%	0.118%
45	17.268	2570	2581	2597	rVB6	137889	571329	6.99%	0.766%
46	17.568	2625	2632	2644	rVB6	78217	229732	2.81%	0.308%




Sum of corrected areas: 74547762

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111220\
Data File : BF122315.D
Acq On : 12 Nov 2020 15:00
Operator : JU/CG
Sample : L4702-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
M-5(10-20)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

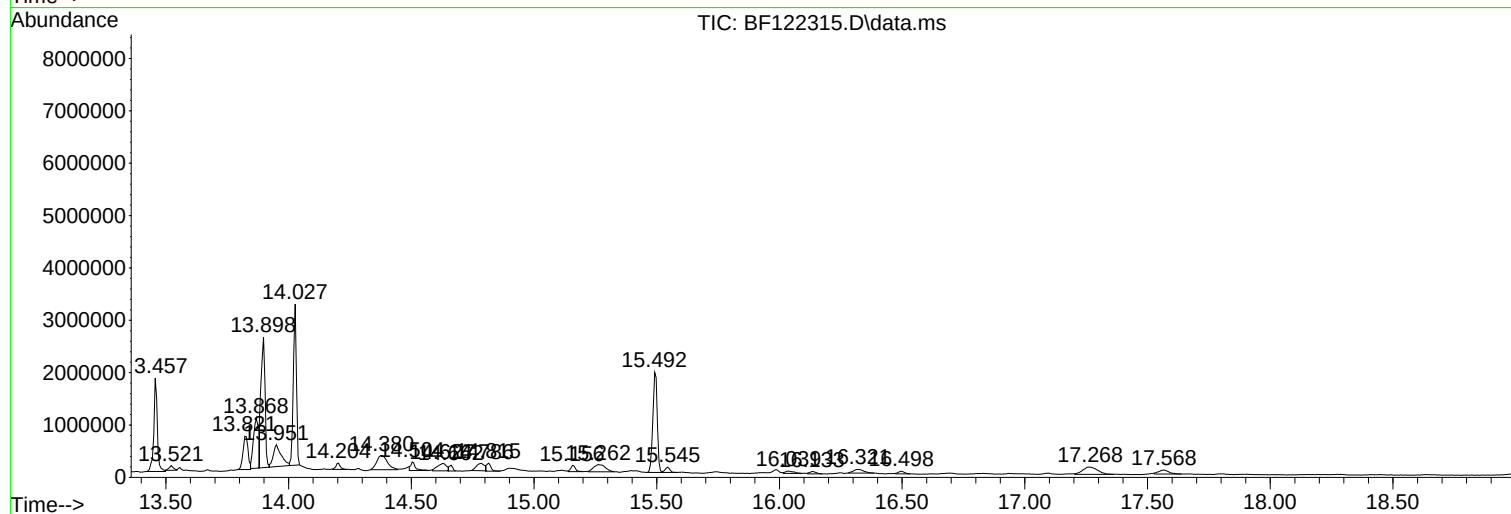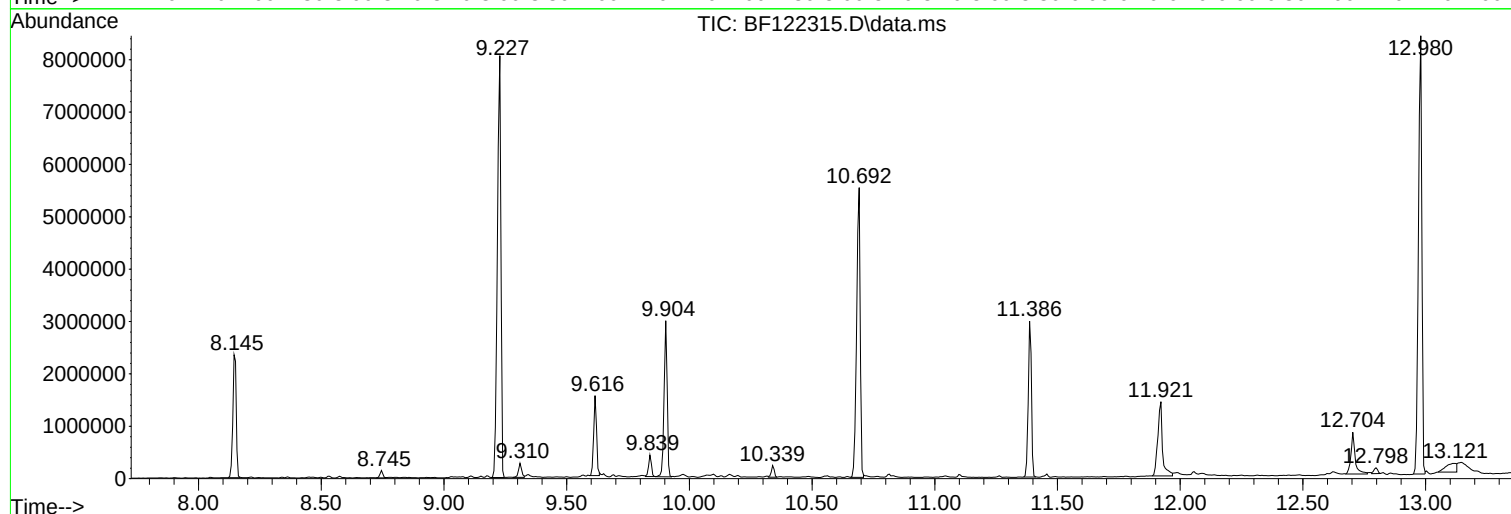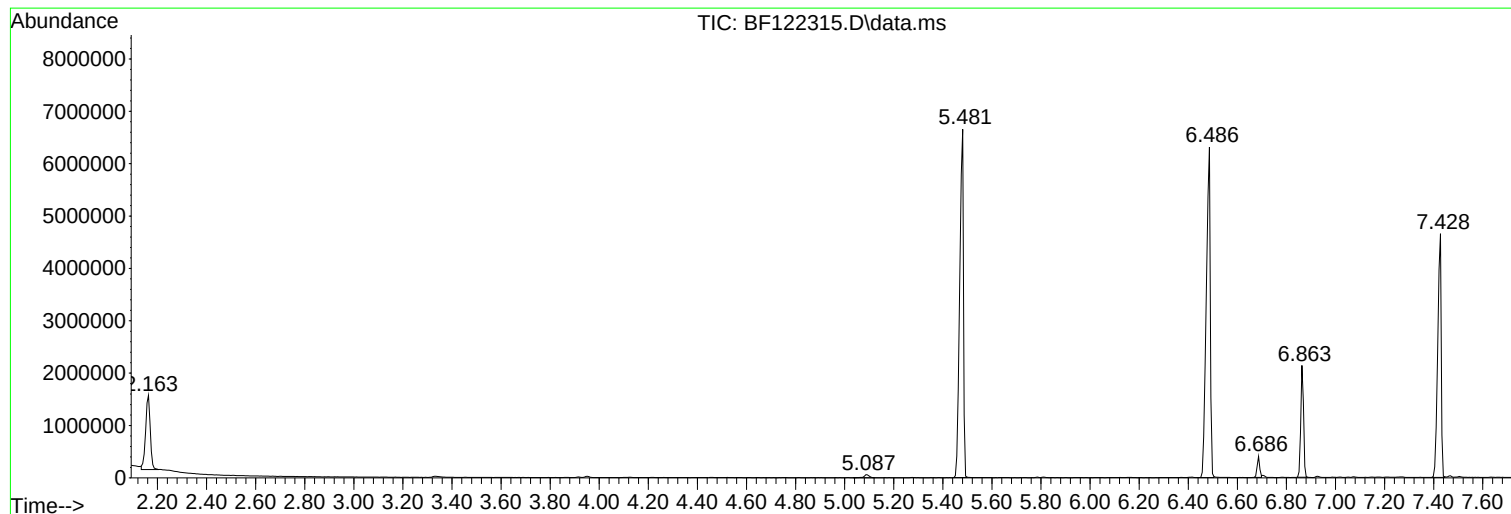

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111220\
Data File : BF122315.D
Acq On : 12 Nov 2020 15:00
Operator : JU/CG
Sample : L4702-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
M-5(10-20)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111220\
Data File : BF122315.D
Acq On : 12 Nov 2020 15:00
Operator : JU/CG
Sample : L4702-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
M-5(10-20)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------