

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111220\
 Data File : BF122318.D
 Acq On : 12 Nov 2020 16:35
 Operator : JU/CG
 Sample : L4717-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 R-LA-35-3-WC

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF122318.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.163	8	13	18	rVB	756269	958271	13.73%	1.885%
2	5.081	502	509	516	rVB	75854	91844	1.32%	0.181%
3	5.475	571	576	579	rBV	5660459	5342564	76.52%	10.507%
4	6.481	741	747	750	rBV	5353029	5554581	79.56%	10.924%
5	6.681	779	781	788	rVB	158698	145659	2.09%	0.286%
6	6.863	808	812	815	rBV	2020552	1538254	22.03%	3.025%
7	7.422	902	907	910	rBV	3792962	3571702	51.16%	7.024%
8	8.145	1026	1030	1034	rBV	2109934	2021499	28.96%	3.976%
9	9.227	1208	1214	1217	rBV	6568494	6241424	89.40%	12.275%
10	9.616	1276	1280	1283	rBV	1354766	1051181	15.06%	2.067%
11	9.904	1323	1329	1332	rBV	2678283	2277780	32.63%	4.480%
12	10.686	1457	1462	1466	rBV	4334407	4117980	58.98%	8.099%
13	11.386	1576	1581	1584	rBV	2869641	2339757	33.51%	4.602%
14	11.921	1666	1672	1680	rBV	854549	897875	12.86%	1.766%
15	12.374	1745	1749	1752	rBV	150784	126979	1.82%	0.250%
16	12.598	1783	1787	1790	rBV	139669	134163	1.92%	0.264%
17	12.704	1801	1805	1811	rBV	346260	359596	5.15%	0.707%
18	12.827	1821	1826	1829	rVB	109358	104515	1.50%	0.206%
19	12.974	1846	1851	1855	rBV	7170028	6981513	100.00%	13.730%
20	13.598	1954	1957	1960	rBV	155583	126837	1.82%	0.249%
21	13.874	1999	2004	2015	rBV2	872351	1092935	15.65%	2.149%
22	14.027	2021	2030	2033	rBV	2449773	2367269	33.91%	4.656%
23	14.198	2051	2059	2065	rBV	81723	121425	1.74%	0.239%
24	14.509	2106	2112	2119	rBV2	148510	211931	3.04%	0.417%
25	14.815	2160	2164	2169	rBV	58949	71492	1.02%	0.141%
26	14.962	2185	2189	2192	rVB	93965	93954	1.35%	0.185%
27	15.156	2218	2222	2225	rBV	127026	163116	2.34%	0.321%
28	15.186	2225	2227	2233	rVB2	76784	102063	1.46%	0.201%
29	15.492	2273	2279	2285	rBV	1533451	1878154	26.90%	3.694%
30	15.986	2358	2363	2367	rBV	113661	171282	2.45%	0.337%
31	16.033	2367	2371	2378	rVV4	58533	120625	1.73%	0.237%
32	16.386	2427	2431	2439	rBV10	37578	76086	1.09%	0.150%
33	16.498	2444	2450	2465	rVB10	53038	179664	2.57%	0.353%
34	17.180	2559	2566	2578	rVB10	25629	80418	1.15%	0.158%
35	17.568	2625	2632	2643	rBV10	48382	133041	1.91%	0.262%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111220\
Data File : BF122318.D
Acq On : 12 Nov 2020 16:35
Operator : JU/CG
Sample : L4717-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
R-LA-35-3-WC

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION




Sum of corrected areas: 50847429

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111220\
Data File : BF122318.D
Acq On : 12 Nov 2020 16:35
Operator : JU/CG
Sample : L4717-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
R-LA-35-3-WC

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

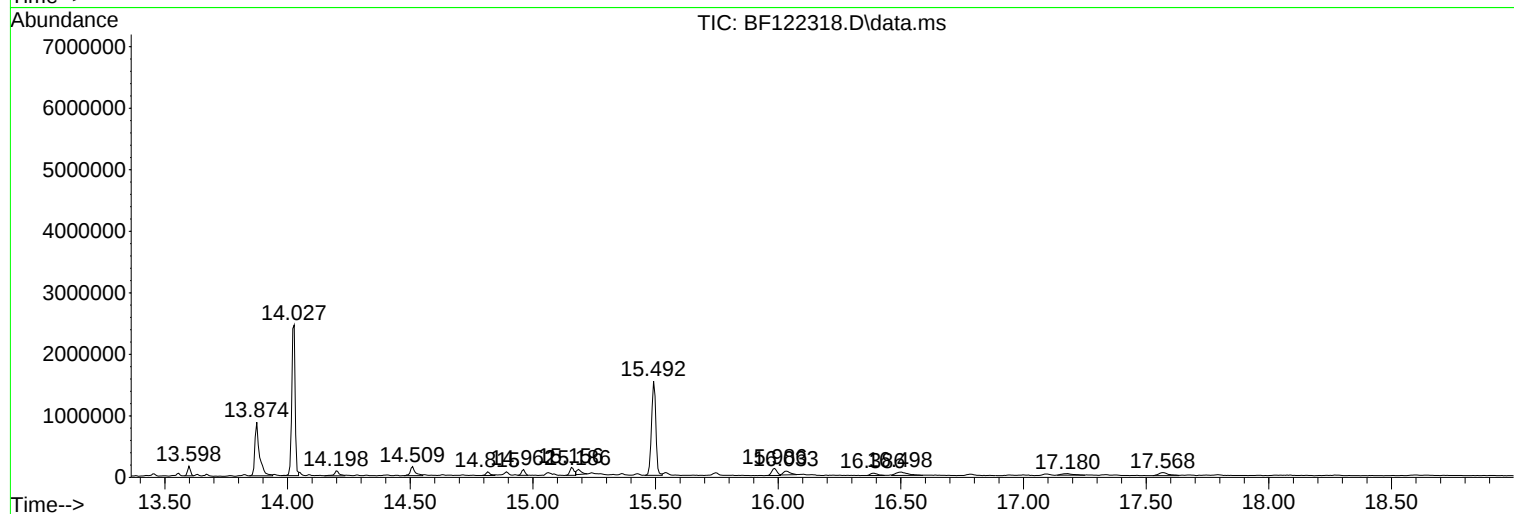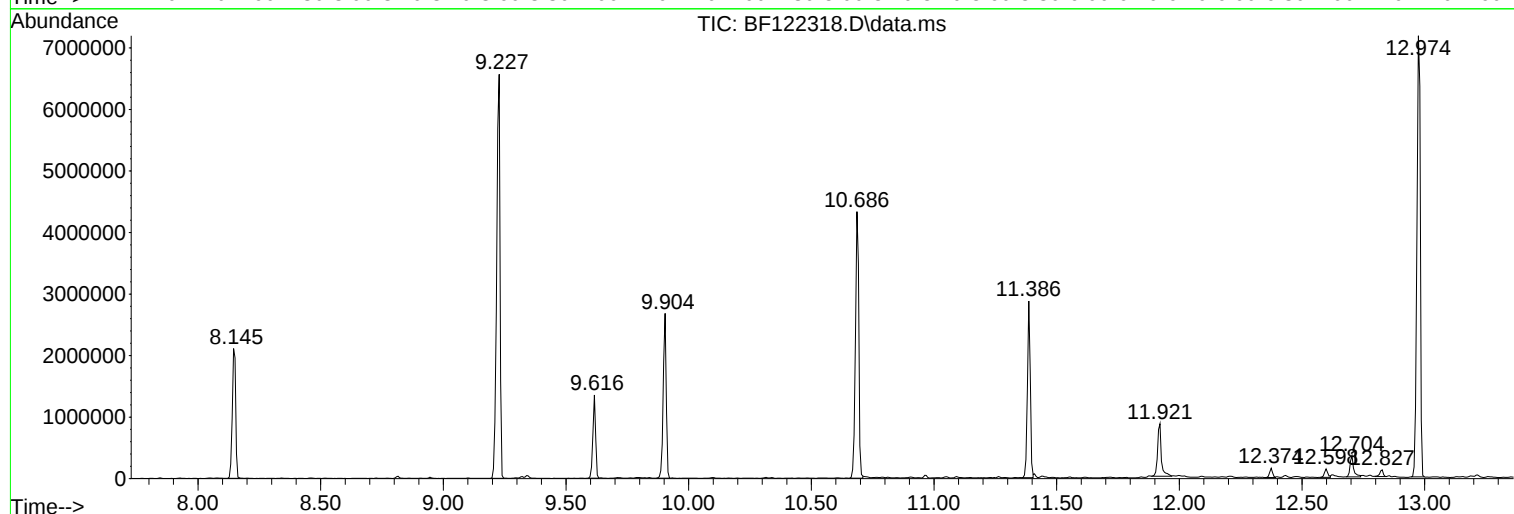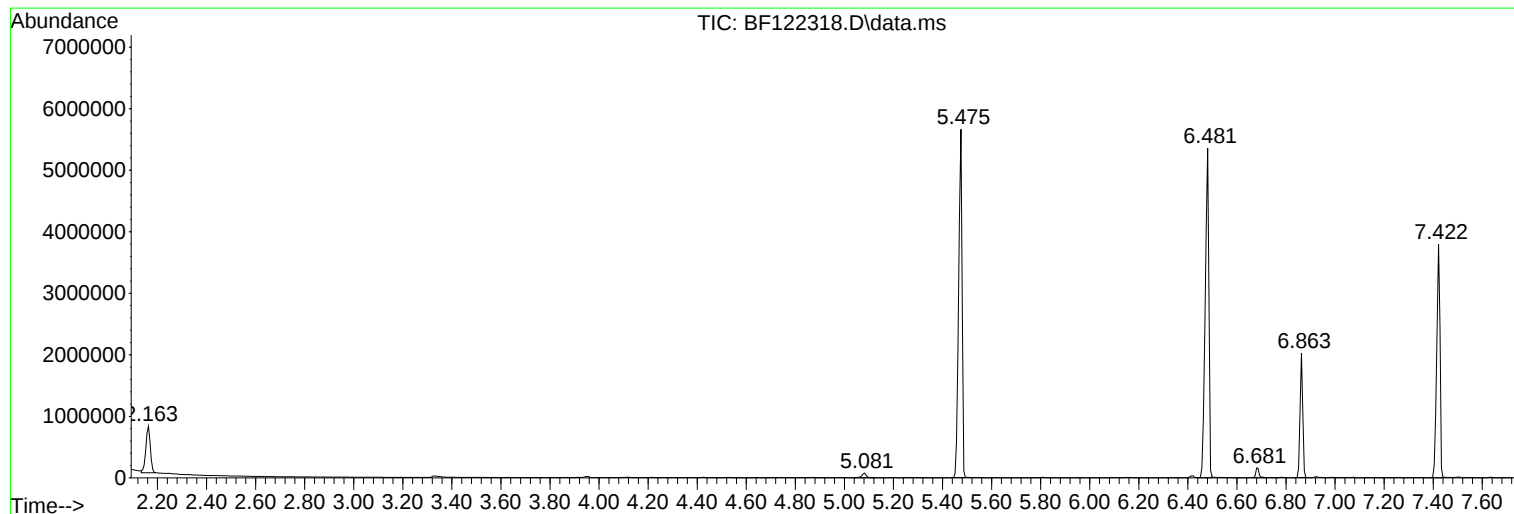

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111220\
Data File : BF122318.D
Acq On : 12 Nov 2020 16:35
Operator : JU/CG
Sample : L4717-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
R-LA-35-3-WC

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111220\
Data File : BF122318.D
Acq On : 12 Nov 2020 16:35
Operator : JU/CG
Sample : L4717-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
R-LA-35-3-WC

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc