

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111220\
 Data File : BF122322.D
 Acq On : 12 Nov 2020 18:40
 Operator : JU/CG
 Sample : L4702-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 M-5(0-10)

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF122322.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.169	9	14	26	rVB	1547877	2049173	19.88%	2.608%
2	3.340	209	213	226	rBV	83351	155162	1.51%	0.197%
3	5.481	571	577	580	rBV	7364745	7882589	76.46%	10.033%
4	6.487	741	748	751	rBV	7081498	8208080	79.62%	10.447%
5	6.687	779	782	785	rBV	505172	365452	3.55%	0.465%
6	6.863	808	812	815	rBV	2054486	1586251	15.39%	2.019%
7	7.428	902	908	911	rBV	5059442	5314745	51.56%	6.764%
8	8.145	1026	1030	1034	rBV	2327256	2101832	20.39%	2.675%
9	9.228	1208	1214	1217	rBV	9312971	9027442	87.57%	11.490%
10	9.310	1223	1228	1231	rBV	987113	833730	8.09%	1.061%
11	9.563	1263	1271	1274	rBV	216936	350931	3.40%	0.447%
12	9.616	1277	1280	1285	rVV	2000340	2028268	19.68%	2.582%
13	9.651	1285	1286	1290	rVV	359835	227880	2.21%	0.290%
14	9.692	1290	1293	1295	rVV	227190	198042	1.92%	0.252%
15	9.839	1314	1318	1322	rVB	2493955	2059626	19.98%	2.621%
16	9.904	1323	1329	1332	rVB	2849199	2605663	25.28%	3.316%
17	10.069	1353	1357	1360	rBV2	248626	350403	3.40%	0.446%
18	10.098	1360	1362	1365	rVV	236663	214739	2.08%	0.273%
19	10.128	1365	1367	1370	rVV	203836	180851	1.75%	0.230%
20	10.163	1370	1373	1376	rVV3	377028	409230	3.97%	0.521%
21	10.198	1376	1379	1382	rVB	206388	167619	1.63%	0.213%
22	10.339	1397	1403	1406	rBV	1680743	1402710	13.61%	1.785%
23	10.563	1435	1441	1443	rBV	229956	299378	2.90%	0.381%
24	10.692	1457	1463	1466	rBV	6353490	6230951	60.44%	7.931%
25	10.810	1480	1483	1493	rVB	387567	466217	4.52%	0.593%
26	11.386	1577	1581	1585	rBV	2880054	2507279	24.32%	3.191%
27	11.916	1667	1671	1681	rBV2	788599	901485	8.74%	1.147%
28	12.704	1801	1805	1817	rBV	318213	385609	3.74%	0.491%
29	12.798	1817	1821	1824	rBV2	105687	121930	1.18%	0.155%
30	12.980	1846	1852	1855	rBV	9737391	10308847	100.00%	13.121%
31	13.463	1927	1934	1940	rBV	3465054	3677099	35.67%	4.680%
32	13.521	1941	1944	1948	rVV2	122753	132836	1.29%	0.169%
33	13.874	2000	2004	2016	rBV	1196118	1344351	13.04%	1.711%
34	14.027	2025	2030	2033	rBV	2265938	2197173	21.31%	2.797%
35	14.198	2057	2059	2070	rVB	81727	115013	1.12%	0.146%
36	14.510	2109	2112	2117	rVB2	104111	108465	1.05%	0.138%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111220\
Data File : BF122322.D
Acq On : 12 Nov 2020 18:40
Operator : JU/CG
Sample : L4702-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
M-5(0-10)

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	15.492	2274	2279	2284	rBV2	1544653	1910610	18.53%	2.432%
38	16.033	2367	2371	2379	rVB3	77232	140879	1.37%	0.179%




Sum of corrected areas: 78568540

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111220\
Data File : BF122322.D
Acq On : 12 Nov 2020 18:40
Operator : JU/CG
Sample : L4702-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
M-5(0-10)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

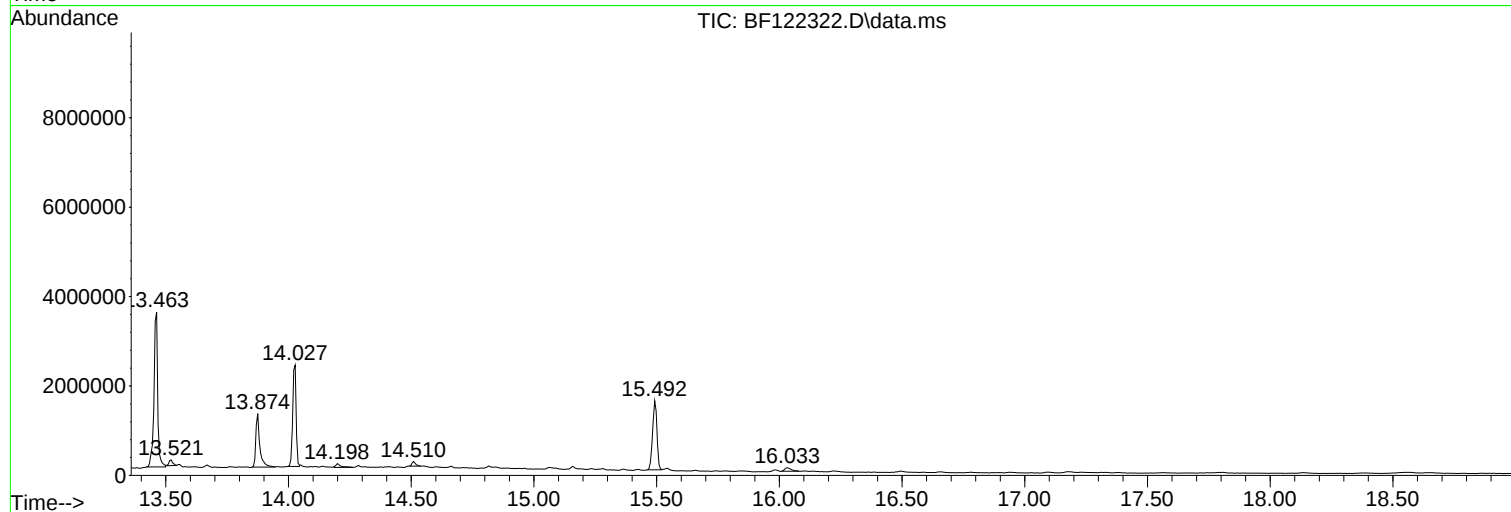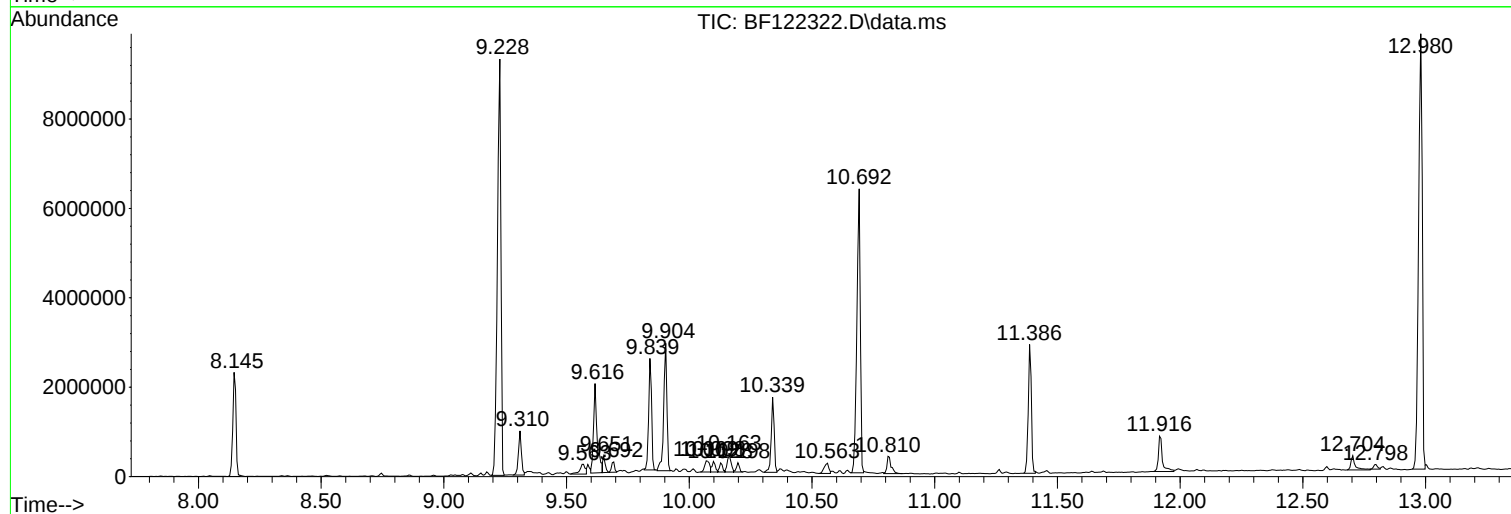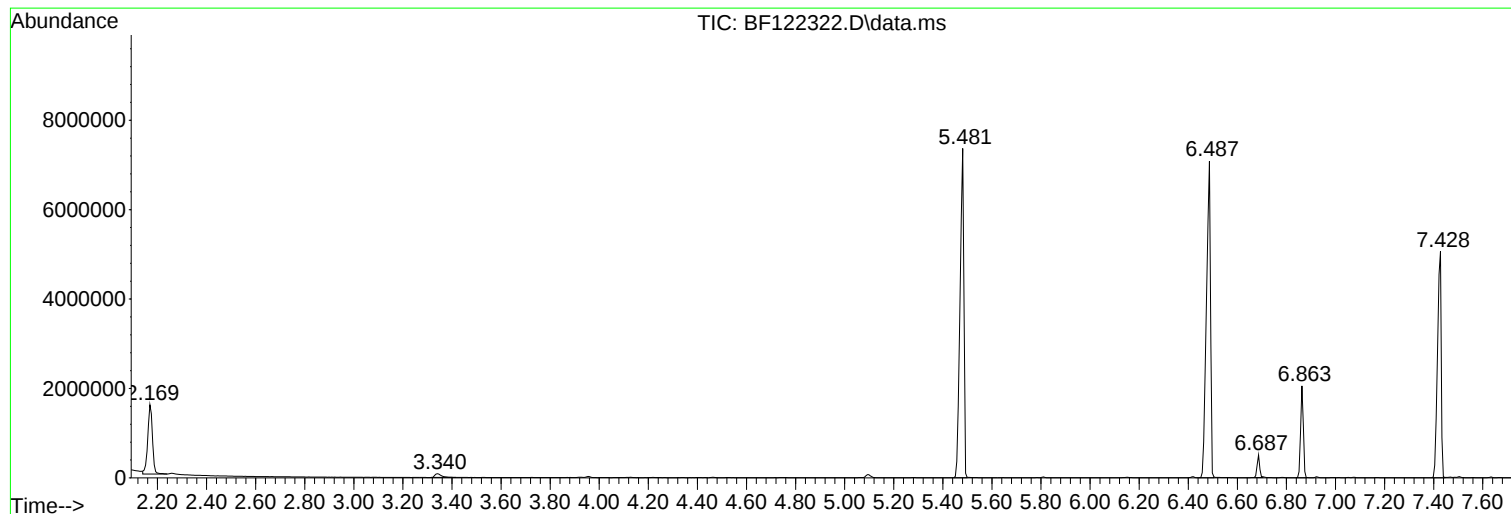

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111220\
Data File : BF122322.D
Acq On : 12 Nov 2020 18:40
Operator : JU/CG
Sample : L4702-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
M-5(0-10)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111220\
Data File : BF122322.D
Acq On : 12 Nov 2020 18:40
Operator : JU/CG
Sample : L4702-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
M-5(0-10)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
