


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111220\
Data File : BF122311.D
Acq On : 12 Nov 2020 12:36
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Nov 24 14:38:56 2020

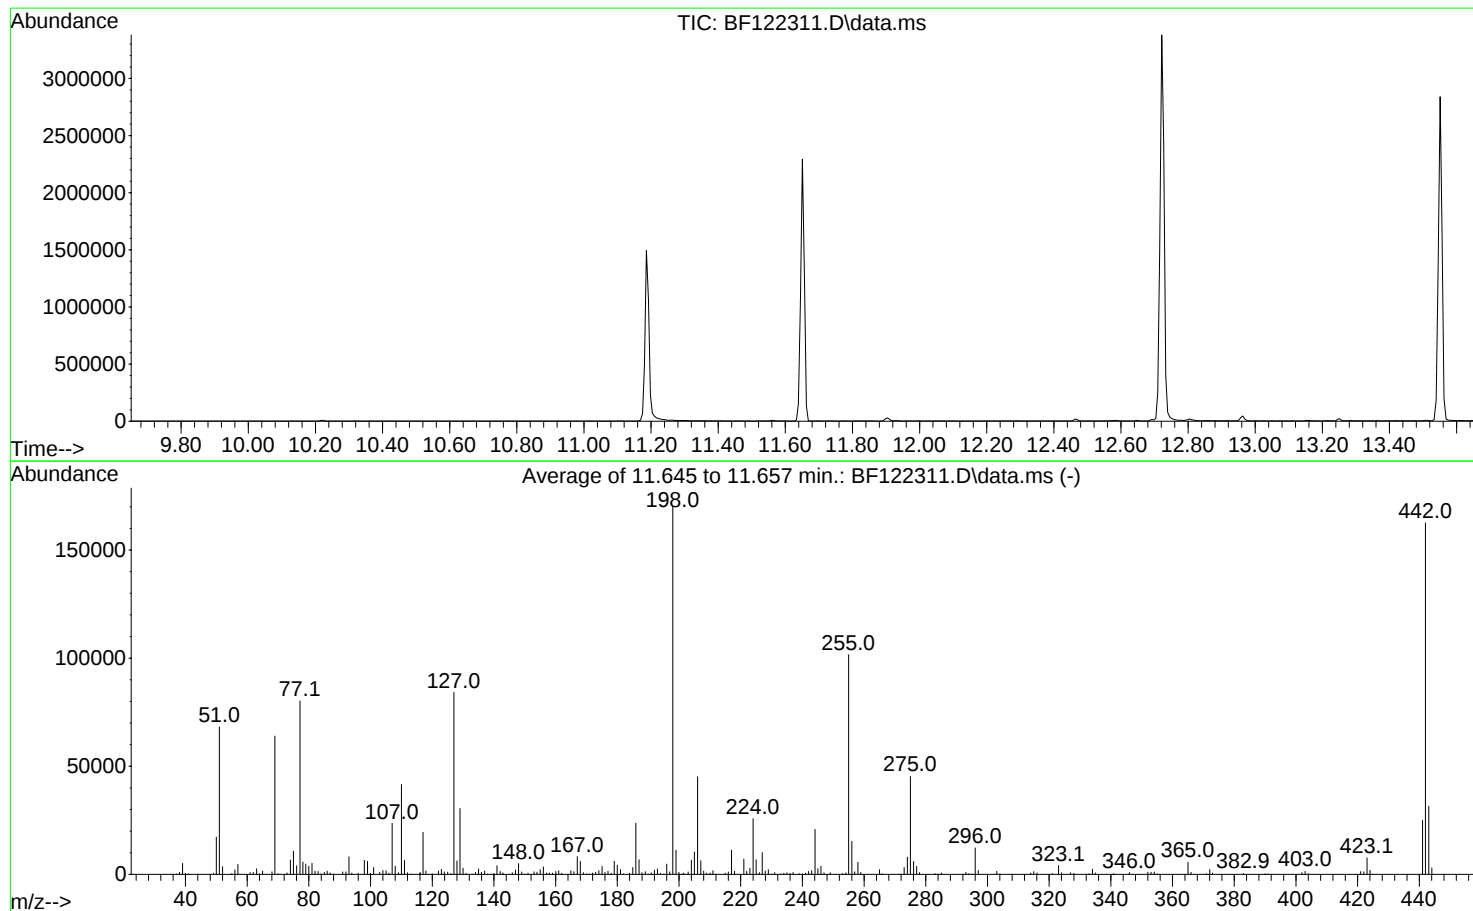

AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.0	68131	PASS
68	69	0.00	2	1.9	1219	PASS
69	198	0.00	100	37.6	63979	PASS
70	69	0.00	2	0.5	290	PASS
127	198	10	80	49.4	84123	PASS
197	198	0.00	2	0.7	1199	PASS
198	198	100	100	100.0	170133	PASS
199	198	5	9	6.6	11202	PASS
275	198	10	60	26.6	45317	PASS
365	198	1	100	3.3	5590	PASS
441	198	0.01	100	14.7	24994	PASS
442	198	50	100	95.5	162520	PASS
443	442	15	24	19.4	31505	PASS